

Data File : VR026191.D
Acq On : 6 Nov 2018 15:01
Operator : SY/MD
Sample : J5801-05
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
F9D04

Quant Time: Nov 06 15:57:02 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR101518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Nov 06 15:50:53 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	642996	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	553437	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.23	152	230752	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.15	65	233916	4.16	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.20%
7) Chloroethane-d5	2.62	69	229389	4.74	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.80%
11) 1,1-Dichloroethene-d2	3.61	63	460017	3.33	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.60%
20) 2-Butanone-d5	6.58	46	253457	54.86	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.72%
24) Chloroform-d	7.20	84	401765	4.49	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.80%
26) 1,2-Dichloroethane-d4	7.90	65	173579	4.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.40%
32) Benzene-d6	7.85	84	837259	4.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.20%
36) 1,2-Dichloropropane-d6	8.90	67	217538	4.74	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.80%
41) Toluene-d8	9.97	98	782621	4.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.20%
43) trans-1,3-Dichloropropene-	10.24	79	52081	4.33	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.60%
46) 2-Hexanone-d5	10.59	63	181417	52.17	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	104.34%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	84017	4.66	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.20%
64) 1,2-Dichlorobenzene-d4	13.52	152	207211	5.68	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	113.60%

Target Compounds

						Qvalue
13) Acetone	3.72	43	46360	9.707	ug/L	72
15) Methyl Acetate	3.94	43	29639	2.376	ug/L #	52
17) Methyl tert-butyl Ether	4.90	73	41741	0.735	ug/L #	1
18) trans-1,2-Dichloroethene	4.88	96	14163	0.300	ug/L	96
22) cis-1,2-Dichloroethene	6.67	96	71621	1.601	ug/L #	98
30) Cyclohexane	7.52	56	663654	8.742	ug/L	99
33) Benzene	7.90	78	743289	3.579	ug/L	100
35) Methylcyclohexane	8.95	83	535816	6.771	ug/L	96
37) 1,2-Dichloropropane	8.96	63	5847	0.133	ug/L	98
42) Toluene	10.03	91	90927	0.415	ug/L	96
44) trans-1,3-Dichloropropene	10.23	75	3398	0.097	ug/L	94
45) 1,1,2-Trichloroethane	10.41	97	17815	0.964	ug/L #	20
48) 2-Hexanone	10.59	43	26940	3.083	ug/L #	70
51) Chlorobenzene	11.32	112	4557903	37.565	ug/L	96
52) Ethylbenzene	11.39	91	6000728	23.809	ug/L	87
53) m,p-Xylene	11.50	106	3310970	36.056	ug/L	84
54) o-Xylene	11.83	106	581145	6.903	ug/L	98

Data File : VR026191.D
Acq On : 6 Nov 2018 15:01
Operator : SY/MD
Sample : J5801-05
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
F9D04

Quant Time: Nov 06 15:57:02 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR101518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Nov 06 15:50:53 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
55) Styrene	11.83	104	33281	0.257	ug/L #	1
56) Isopropylbenzene	12.13	105	509636	2.180	ug/L	99
62) 1,3-Dichlorobenzene	13.16	146	44835	0.585	ug/L	92
63) 1,4-Dichlorobenzene	13.24	146	172089	2.168	ug/L	89
65) 1,2-Dichlorobenzene	13.53	146	486183	7.902	ug/L	100
66) 1,2-Dibromo-3-chloropropan	14.16	75	24829	9.905	ug/L #	18
69) Naphthalene	15.00	128	7551862	285.257	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VR026191.D
Acq On : 6 Nov 2018 15:01
Operator : SY/MD
Sample : J5801-05
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
F9D04

Quant Time: Nov 06 15:57:02 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR101518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Nov 06 15:50:53 2018
Response via : Initial Calibration




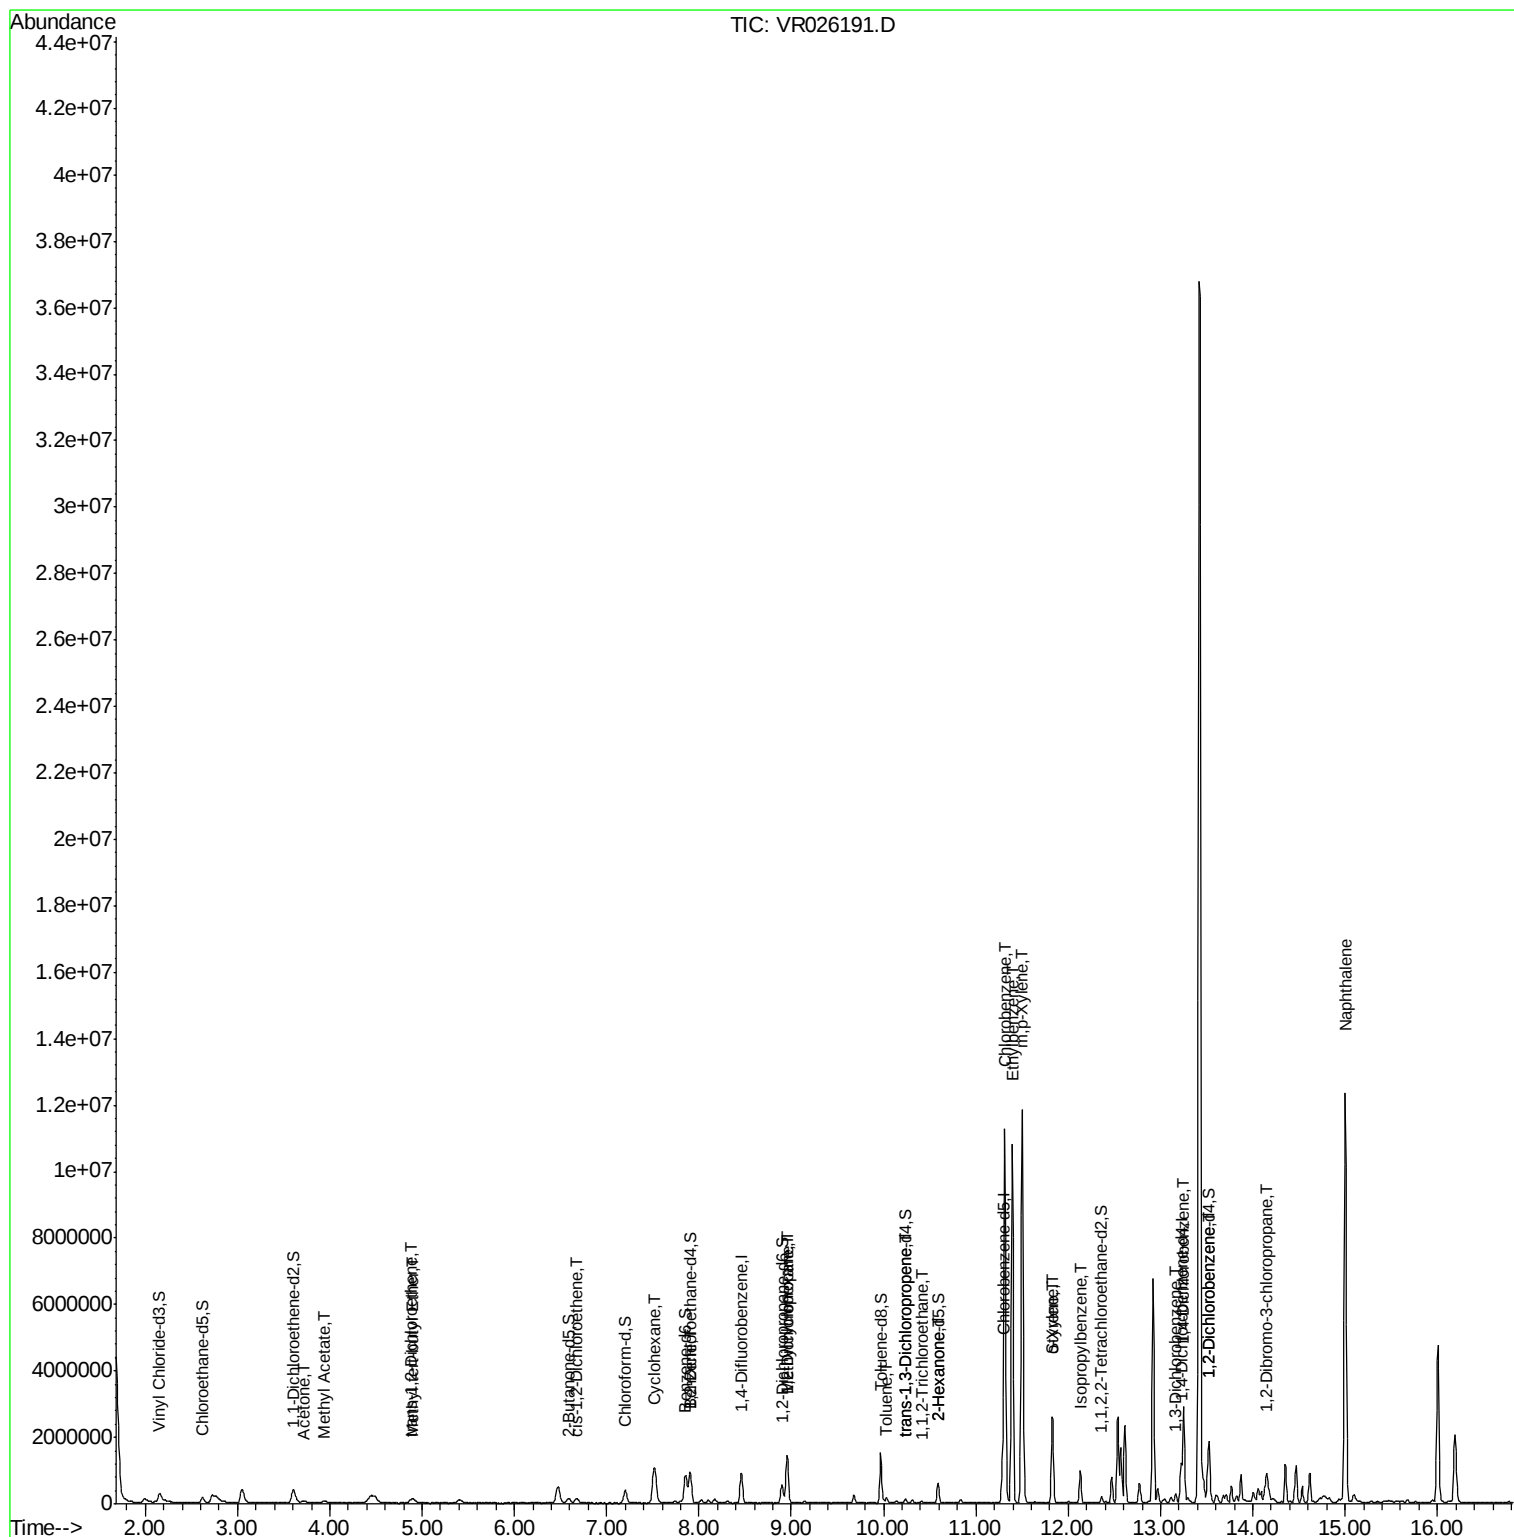


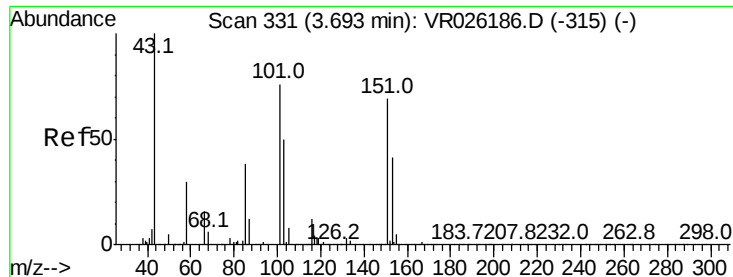

#13
Acetone
Concen: 9.707 ug/L
RT: 3.72 min Scan# 335
Delta R.T. 0.02 min
Lab File: VR026191.D
Acq: 6 Nov 2018 15:01




Instrument :
MSVOA_R
ClientSampleId :
F9D04


Tgt Ion: 43 Resp: 46360
Ion Ratio Lower Upper
43 100
58 12.8 0.0 55.4

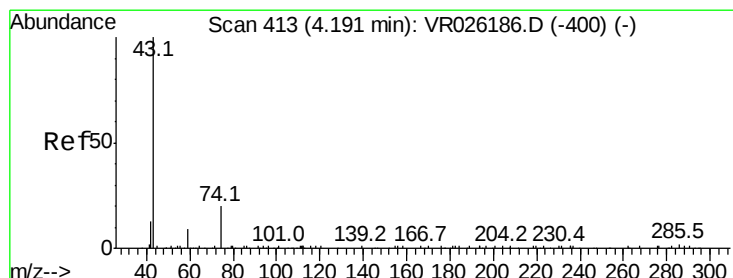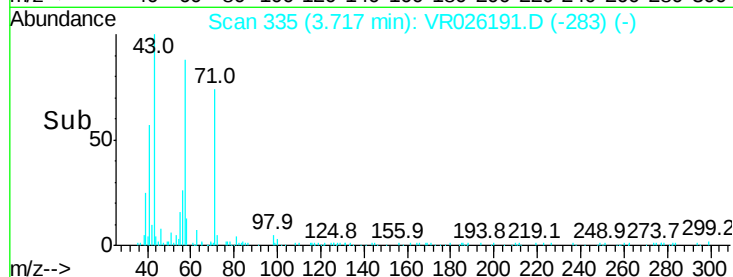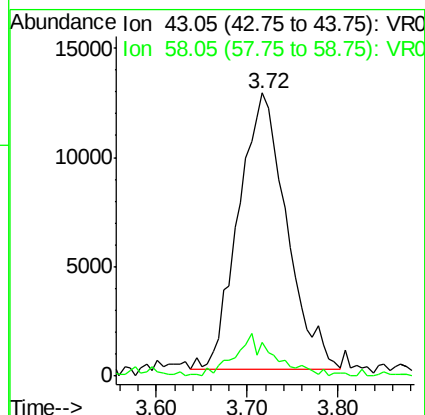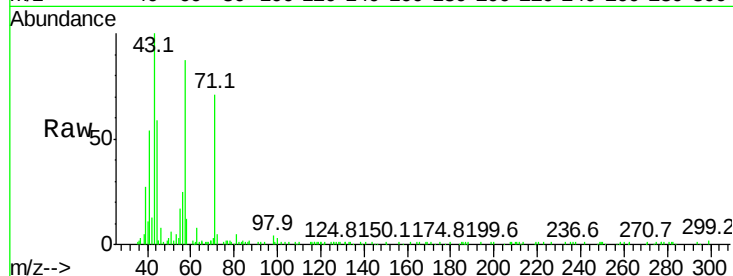

#15
Methyl Acetate
Concen: 2.376 ug/L
RT: 3.94 min Scan# 372
Delta R.T. -0.25 min
Lab File: VR026191.D
Acq: 6 Nov 2018 15:01

Tgt Ion: 43 Resp: 29639
Ion Ratio Lower Upper
43 100
74 0.6 19.8 29.8#

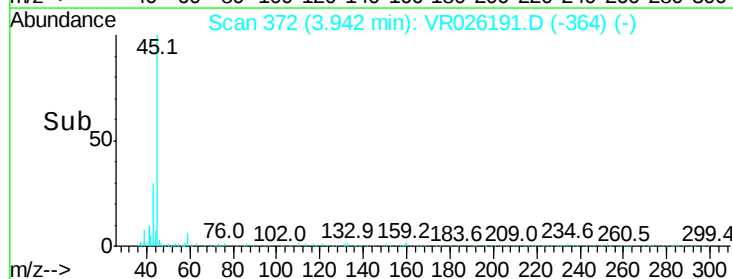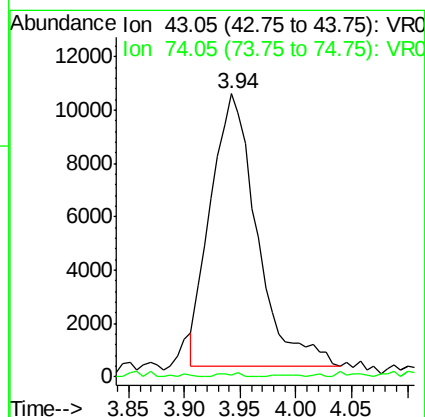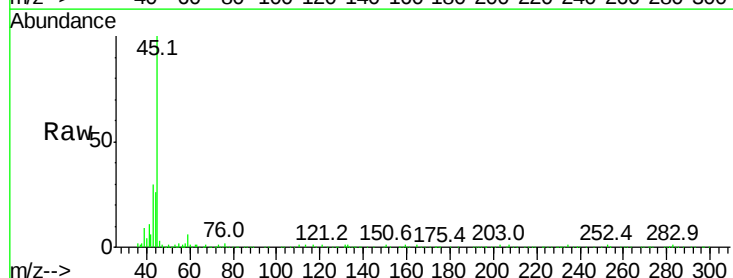

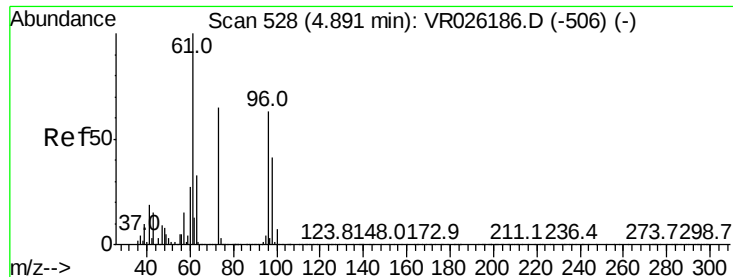

#17

Methyl tert-butyl Ether

Concen: 0.735 ug/L

RT: 4.90 min Scan# 529

Delta R.T. 0.01 min

Lab File: VR026191.D

Acq: 6 Nov 2018 15:01

Instrument :

MSVOA_R

ClientSampleId :

F9D04





Tgt Ion: 73 Resp: 41741

Ion Ratio Lower Upper

73 100

43 93.0 20.1 30.1#

57 273.7 19.0 28.4#

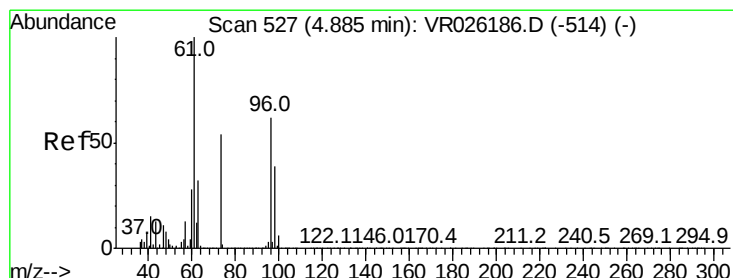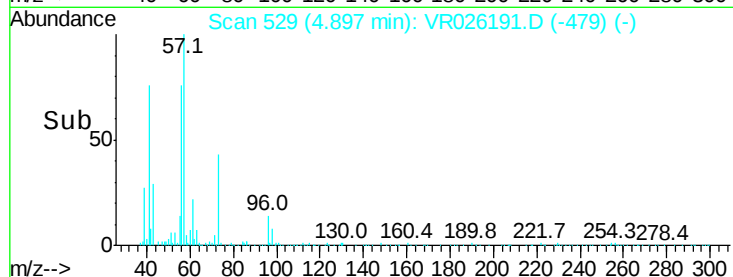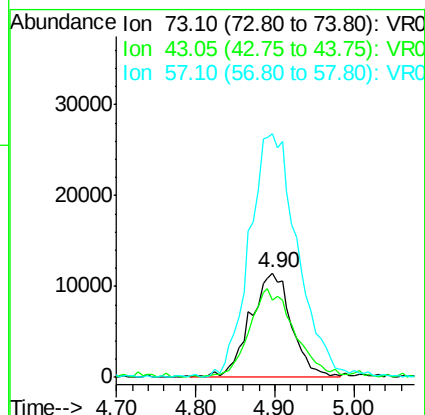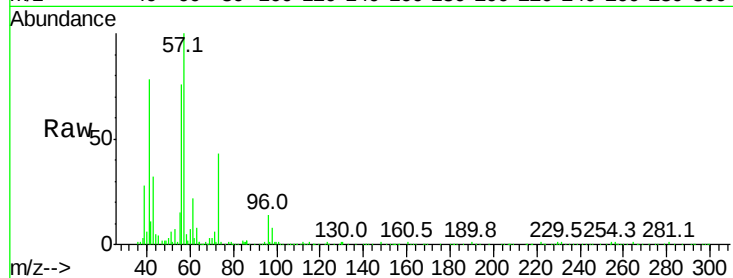

#18

trans-1,2-Dichloroethene

Concen: 0.300 ug/L

RT: 4.88 min Scan# 526

Delta R.T. -0.01 min

Lab File: VR026191.D

Acq: 6 Nov 2018 15:01




Tgt Ion: 96 Resp: 14163


Ion Ratio Lower Upper

96 100

61 152.4 111.4 206.8

98 58.4 41.4 77.0

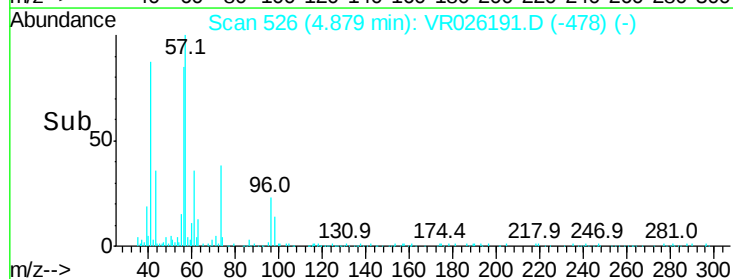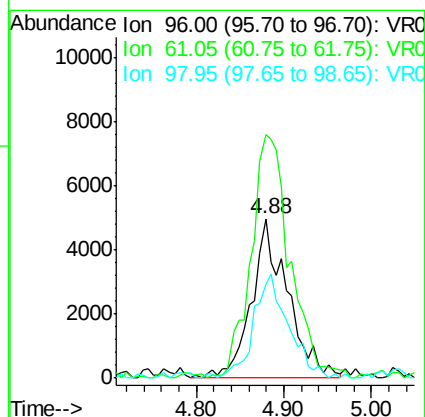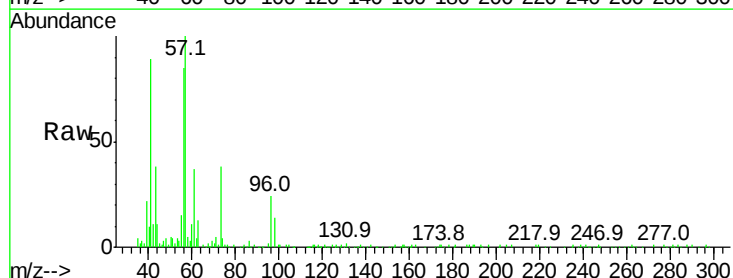




#22




cis-1,2-Dichloroethene
Concen: 1.601 ug/L
RT: 6.67 min Scan# 821
Delta R.T. 0.00 min
Lab File: VR026191.D
Acq: 6 Nov 2018 15:01

Instrument :
MSVOA_R
ClientSampled :
F9D04

Tgt Ion: 96 Resp: 71621
Ion Ratio Lower Upper
96 100
61 147.6 101.8 189.0
68 0.3 0.1 0.3#

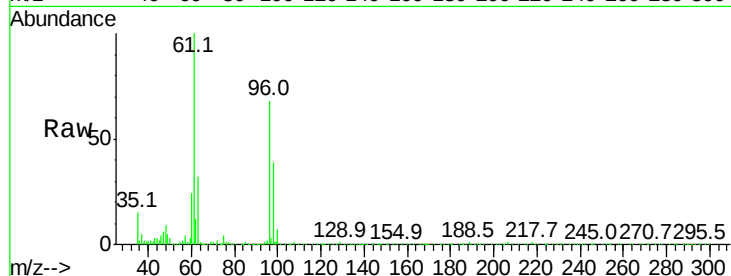


Abundance Ion 96.00 (95.70 to 96.70): VR0
Ion 61.05 (60.75 to 61.75): VR0
Ion 68.15 (67.85 to 68.85): VR0

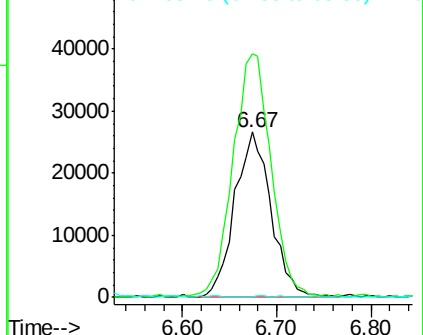



#30


Cyclohexane
Concen: 8.742 ug/L
RT: 7.52 min Scan# 960
Delta R.T. 0.00 min
Lab File: VR026191.D
Acq: 6 Nov 2018 15:01

Tgt Ion: 56 Resp: 663654
Ion Ratio Lower Upper
56 100
69 28.9 23.8 35.8
84 77.6 62.2 93.4



Abundance Ion 56.10 (55.80 to 56.80): VR0
Ion 69.15 (68.85 to 69.85): VR0
Ion 84.15 (83.85 to 84.85): VR0

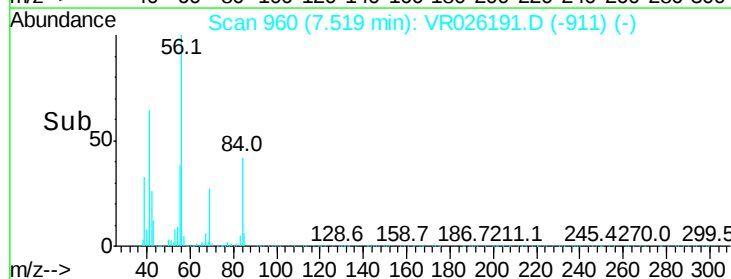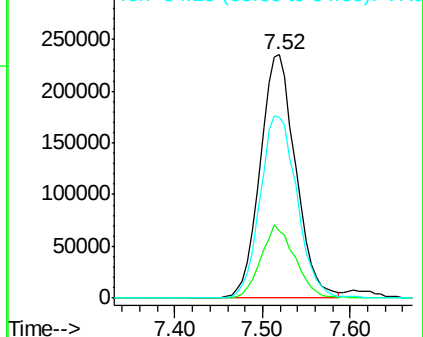



#33

Benzene

Concen: 3.579 ug/L

RT: 7.90 min Scan# 1023

Delta R.T. -0.01 min

Lab File: VR026191.D

Acq: 6 Nov 2018 15:01





Instrument :

MSVOA_R

ClientSampleId :

F9D04

Tgt Ion: 78 Resp: 743289

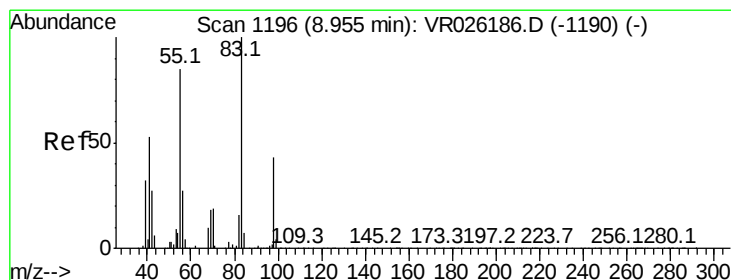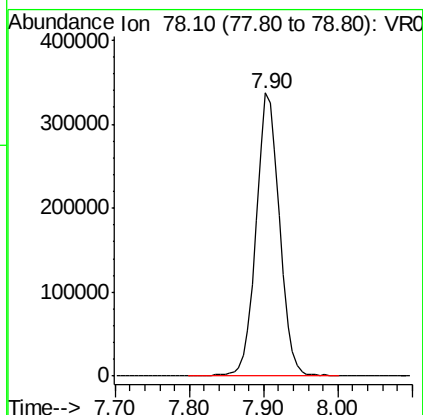

#35

Methylcyclohexane

Concen: 6.771 ug/L

RT: 8.95 min Scan# 1196




Delta R.T. 0.00 min


Lab File: VR026191.D

Acq: 6 Nov 2018 15:01

Tgt Ion: 83 Resp: 535816

Ion	Ratio	Lower	Upper
83	100		
55	87.9	66.8	100.2
98	43.3	35.2	52.8

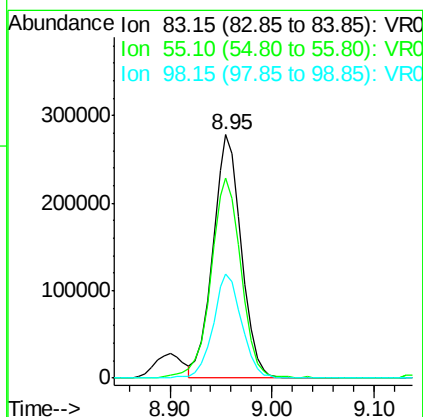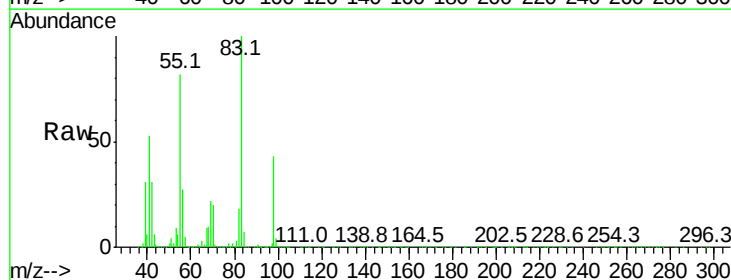

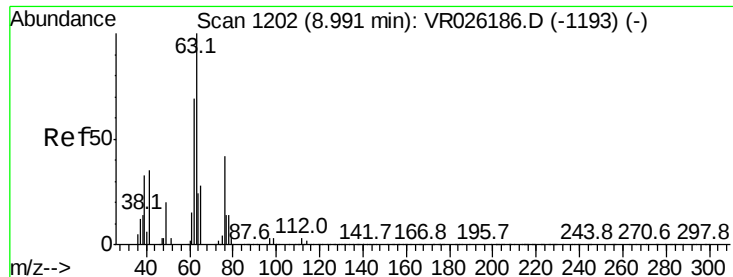

#37

1,2-Dichloropropane

Concen: 0.133 ug/L

RT: 8.96 min Scan# 1197

Delta R.T. -0.03 min

Lab File: VR026191.D

Acq: 6 Nov 2018 15:01

Instrument :

MSVOA_R

ClientSampleId :





F9D04

Tgt Ion: 63 Resp: 5847

Ion Ratio Lower Upper

63 100

112 3.9 2.7 4.1

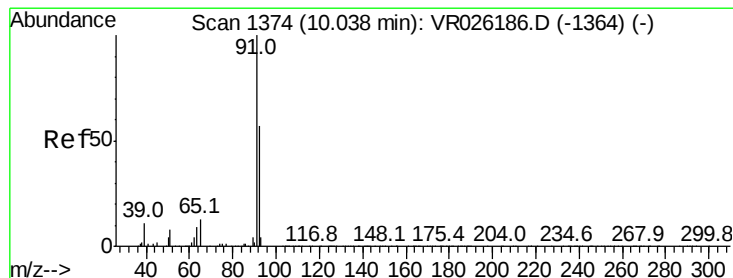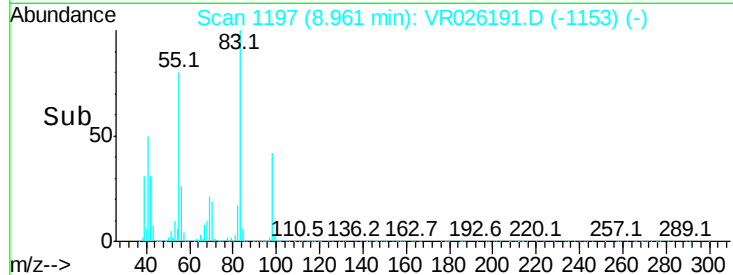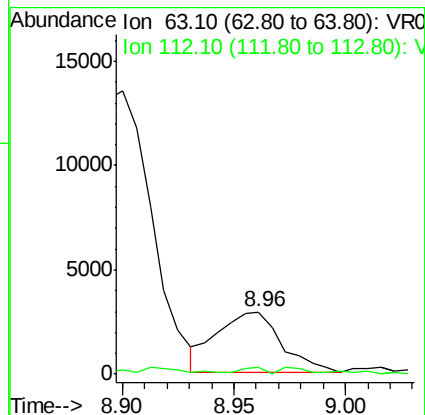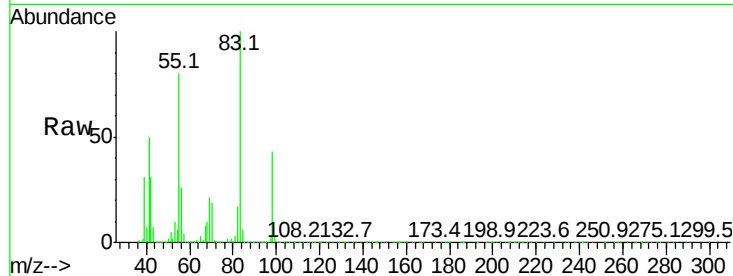

#42

Toluene

Concen: 0.415 ug/L

RT: 10.03 min Scan# 1373

Delta R.T. -0.01 min

Lab File: VR026191.D




Acq: 6 Nov 2018 15:01


Tgt Ion: 91 Resp: 90927

Ion Ratio Lower Upper

91 100

92 61.5 40.8 75.8

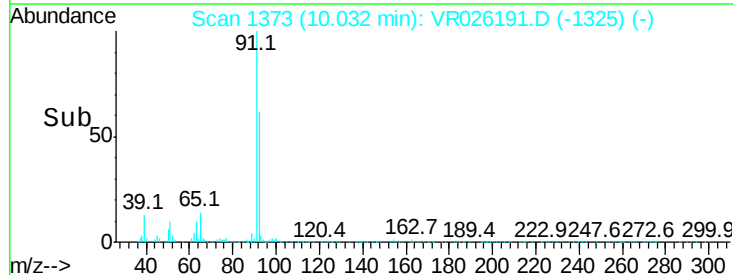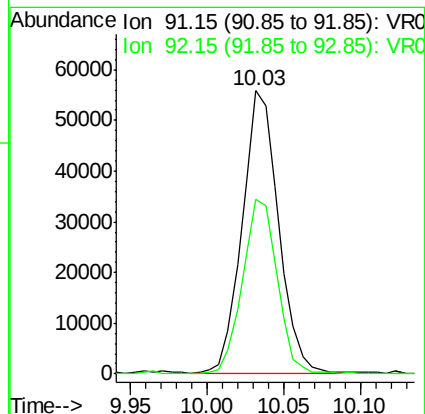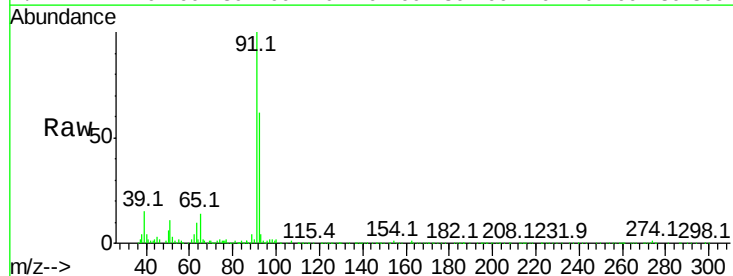

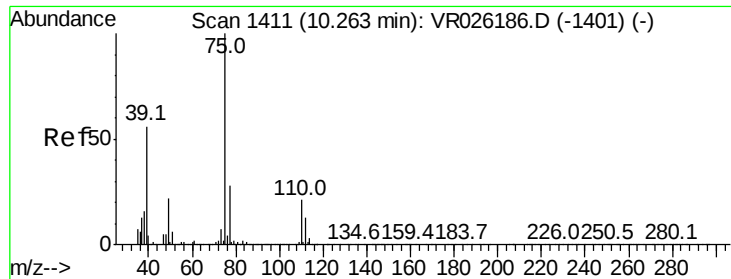

#44

trans-1,3-Dichloropropene

Concen: 0.097 ug/L

RT: 10.23 min Scan# 1406

Delta R.T. -0.03 min

Lab File: VR026191.D

Acq: 6 Nov 2018 15:01

Instrument :

MSVOA_R

ClientSampleId :


F9D04

Tgt Ion: 75 Resp: 3398

Ion Ratio Lower Upper




75 100

77 30.8 24.1 44.7

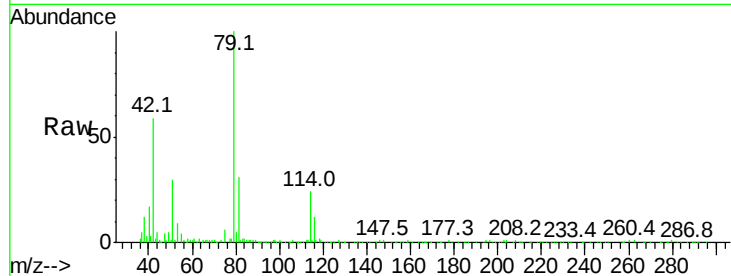

Abundance Ion 75.05 (74.75 to 75.75): VR0

Ion 77.05 (76.75 to 77.75): VR0

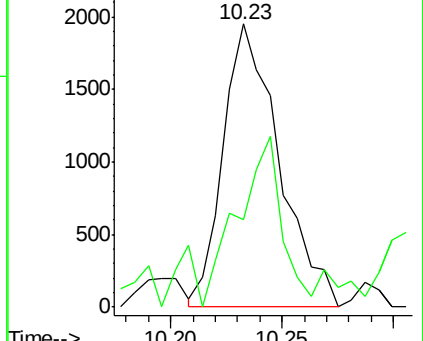

#45

1,1,2-Trichloroethane

Concen: 0.964 ug/L

RT: 10.41 min Scan# 1436

Delta R.T. -0.03 min

Lab File: VR026191.D

Acq: 6 Nov 2018 15:01

Tgt Ion: 97 Resp: 17815


Ion Ratio Lower Upper

97 100

99 1.3 42.8 79.4#

83 10.1 61.9 114.9#

85 0.0 39.3 72.9#






Abundance Ion 96.95 (96.65 to 97.65): VR0

Ion 99.05 (98.75 to 99.75): VR0

Ion 82.95 (82.65 to 83.65): VR0

Ion 85.00 (84.70 to 85.70): VR0




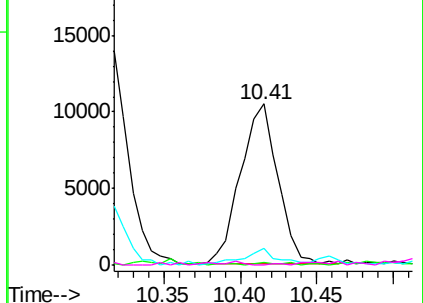


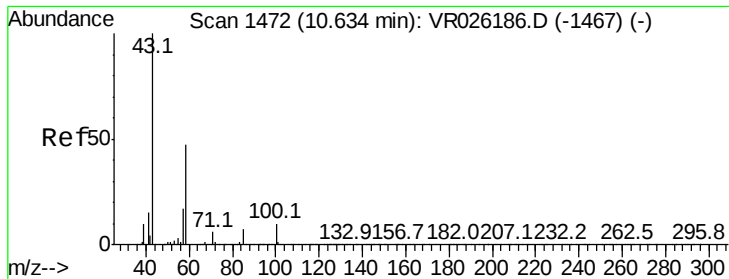

#48
2-Hexanone
Concen: 3.083 ug/L
RT: 10.59 min Scan# 1464
Delta R.T. -0.05 min
Lab File: VR026191.D
Acq: 6 Nov 2018 15:01




Instrument :
MSVOA_R
ClientSampleId :
F9D04


Tgt Ion:	43	Resp:	26940
Ion	Ratio	Lower	Upper
43	100		
58	26.3	39.6	59.4#
57	27.6	14.0	21.0#
100	1.1	7.0	10.6#

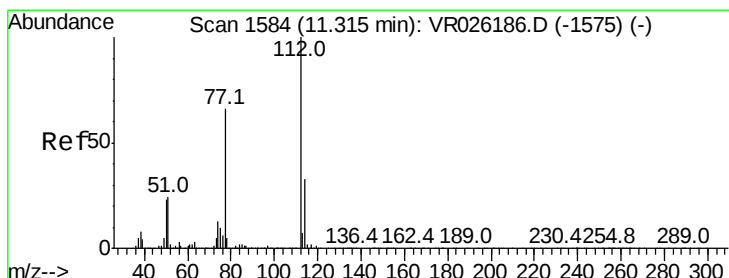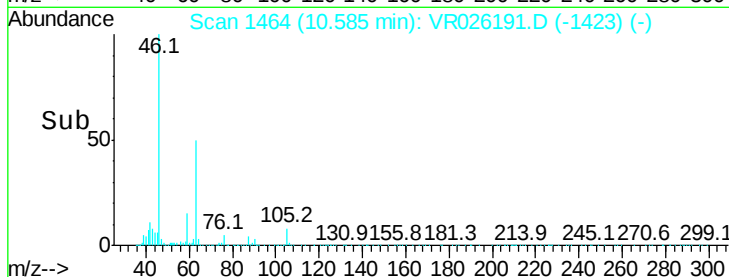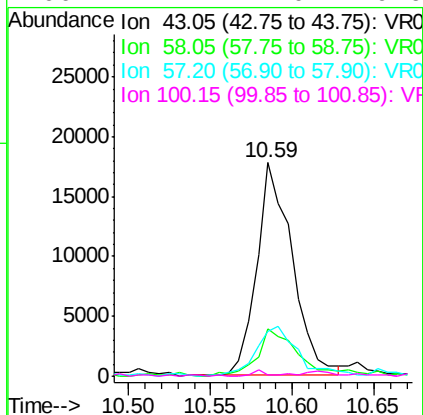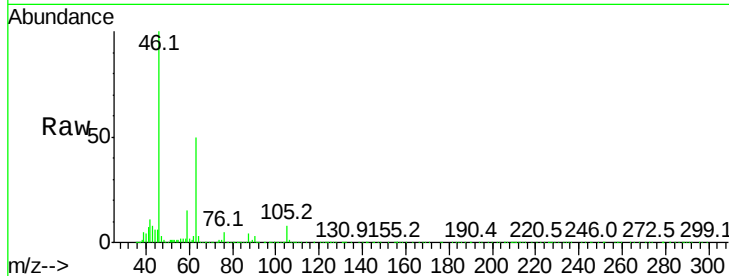

#51
Chlorobenzene
Concen: 37.565 ug/L
RT: 11.32 min Scan# 1584
Delta R.T. 0.00 min
Lab File: VR026191.D
Acq: 6 Nov 2018 15:01

Tgt Ion:	112	Resp:	4557903
Ion	Ratio	Lower	Upper
112	100		
114	35.3	22.8	42.4
77	67.3	51.5	77.3

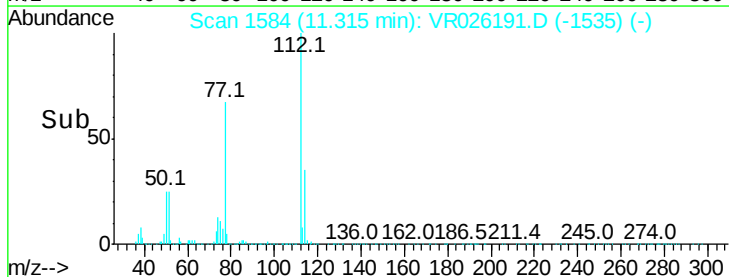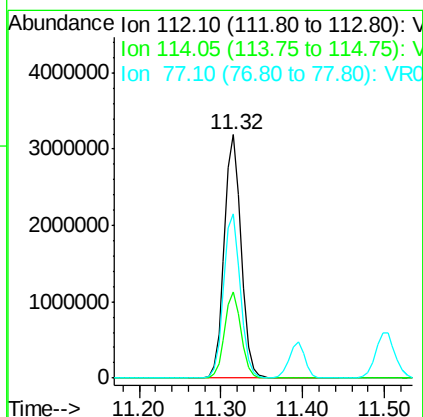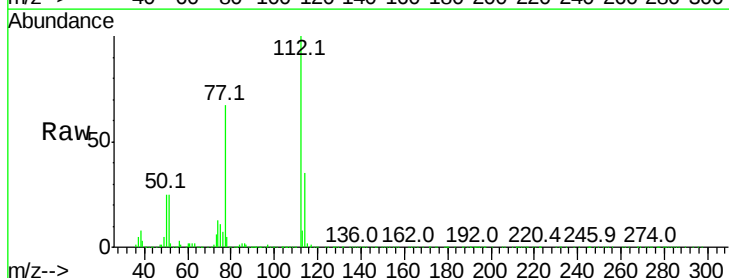



#52

Ethylbenzene

Concen: 23.809 ug/L

RT: 11.39 min Scan# 1597

Delta R.T. 0.00 min

Lab File: VR026191.D

Acq: 6 Nov 2018 15:01

Instrument :

MSVOA_R

ClientSampleId :





F9D04

Tgt Ion: 91 Resp: 6000728

Ion Ratio Lower Upper

91 100

106 37.3 21.2 39.4

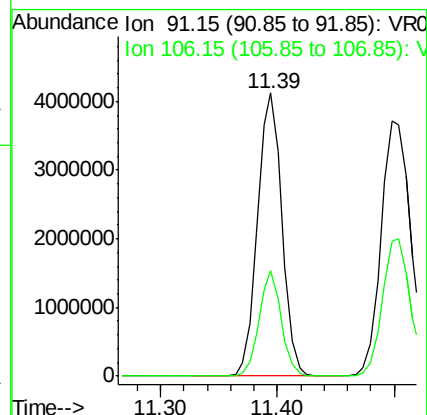

#53

m,p-Xylene

Concen: 36.056 ug/L

RT: 11.50 min Scan# 1615

Delta R.T. 0.00 min

Lab File: VR026191.D




Acq: 6 Nov 2018 15:01


Tgt Ion: 106 Resp: 3310970

Ion Ratio Lower Upper

106 100

91 182.6 145.3 269.8



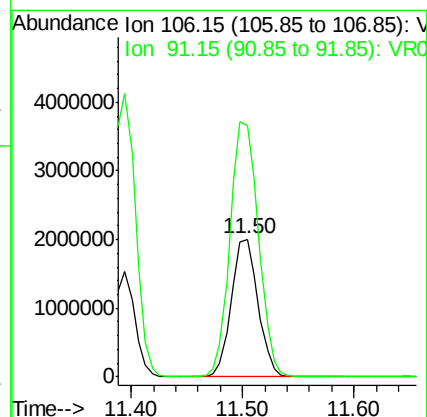





#54
o-Xylene
Concen: 6.903 ug/L
RT: 11.83 min Scan# 1668
Delta R.T. 0.00 min
Lab File: VR026191.D
Acq: 6 Nov 2018 15:01




Instrument :
MSVOA_R
ClientSampleId :
F9D04


Tgt Ion:106 Resp: 581145
Ion Ratio Lower Upper
106 100
91 225.8 155.8 289.3

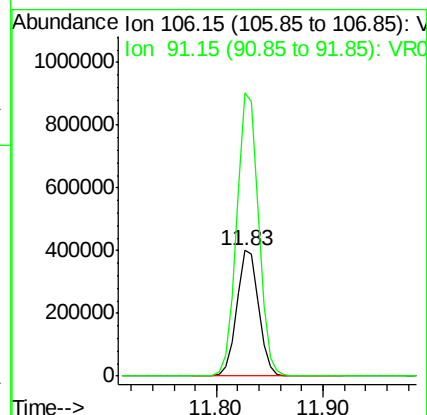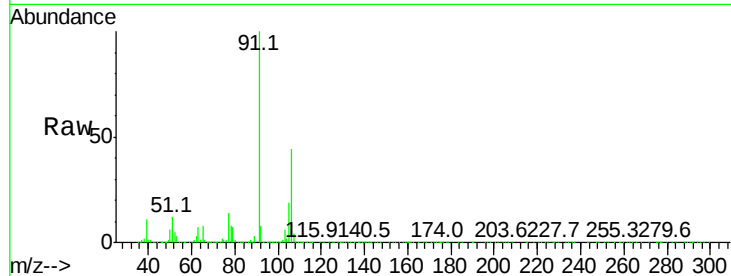

#55
Styrene
Concen: 0.257 ug/L
RT: 11.83 min Scan# 1669
Delta R.T. -0.01 min
Lab File: VR026191.D
Acq: 6 Nov 2018 15:01

Tgt Ion:104 Resp: 33281
Ion Ratio Lower Upper
104 100
78 338.7 34.7 64.5#

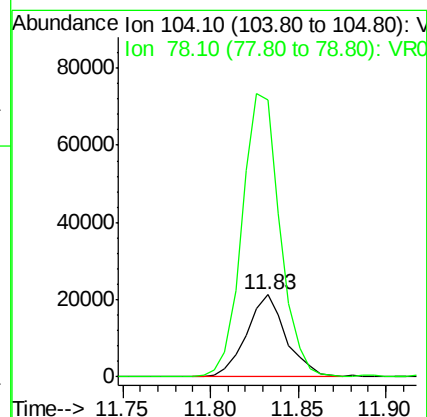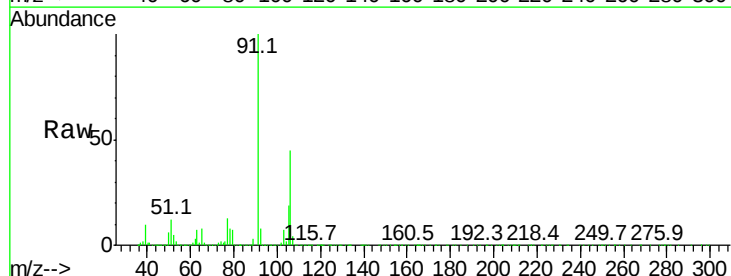

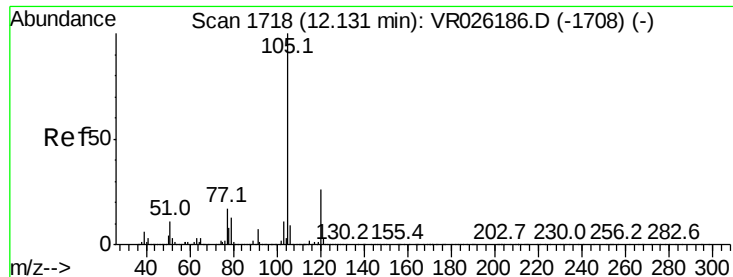

#56

Isopropylbenzene

Concen: 2.180 ug/L

RT: 12.13 min Scan# 1718

Delta R.T. 0.00 min

Lab File: VR026191.D

Acq: 6 Nov 2018 15:01

Instrument :

MSVOA_R

ClientSampleId :

F9D04


Tgt Ion:105 Resp: 509636

Ion Ratio Lower Upper

105 100

120 25.3 21.0 31.4




77 17.9 14.6 21.8

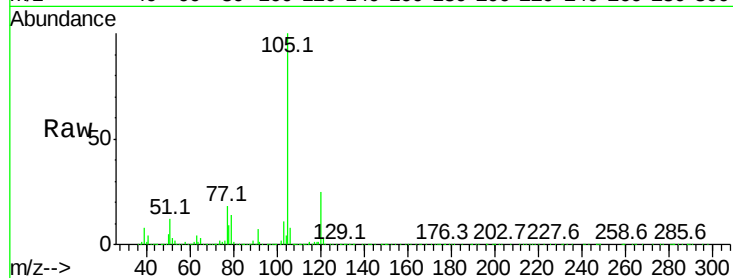

Abundance Ion 105.05 (104.75 to 105.75): V

Ion 120.10 (119.80 to 120.80): V

Ion 77.10 (76.80 to 77.80): VR0

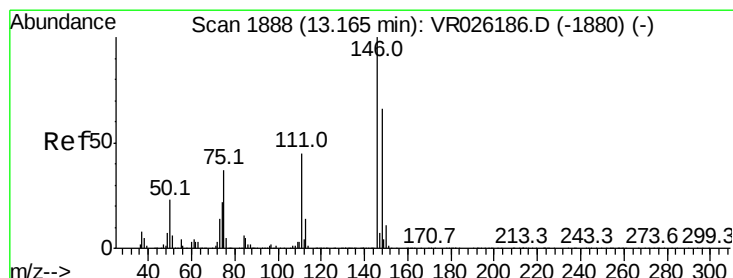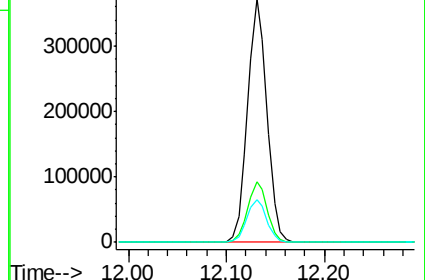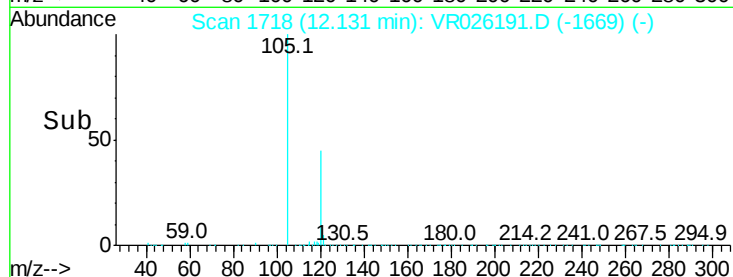

#62

1,3-Dichlorobenzene

Concen: 0.585 ug/L

RT: 13.16 min Scan# 1887

Delta R.T. 0.00 min

Lab File: VR026191.D

Acq: 6 Nov 2018 15:01


Tgt Ion:146 Resp: 44835

Ion Ratio Lower Upper

146 100

111 55.6 32.1 59.7



148 64.8 43.8 81.3

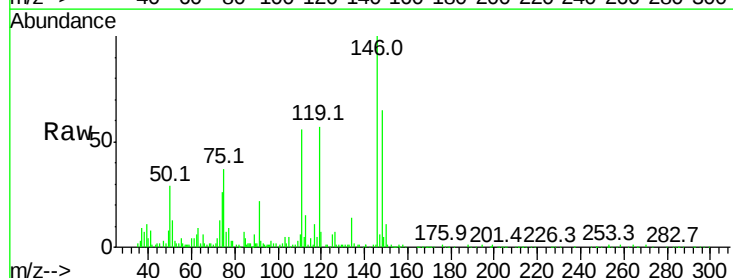


Abundance Ion 145.95 (145.65 to 146.65): V

Ion 111.00 (110.70 to 111.70): V

Ion 148.00 (147.70 to 148.70): V

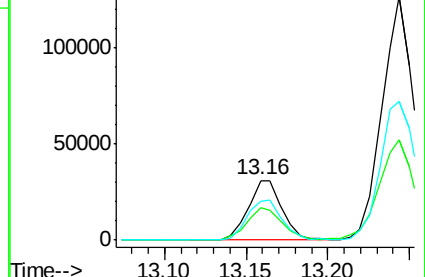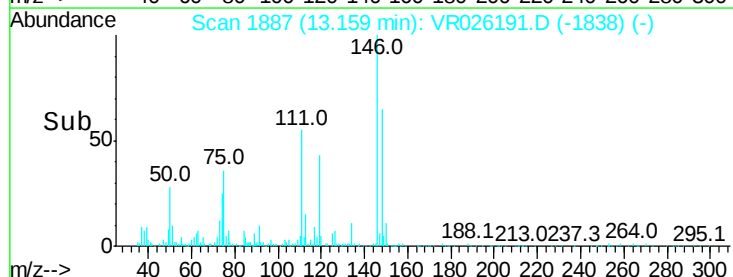



#63

1,4-Dichlorobenzene

Concen: 2.168 ug/L

RT: 13.24 min Scan# 1901

Delta R.T. 0.00 min

Lab File: VR026191.D

Acq: 6 Nov 2018 15:01

Instrument :

MSVOA_R

ClientSampleId :

F9D04


Tgt Ion:146 Resp: 172089

Ion Ratio Lower Upper

146 100

111 41.2 32.6 60.6




148 56.7 46.7 86.7

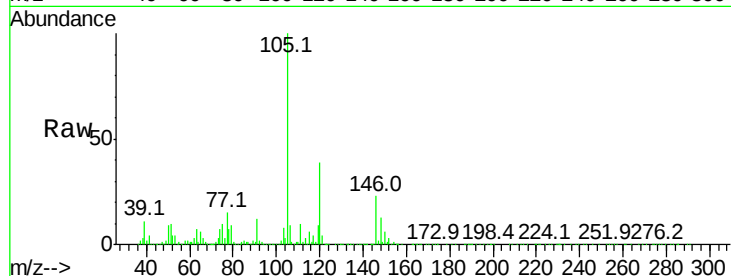

Abundance Ion 145.95 (145.65 to 146.65): V

Ion 111.00 (110.70 to 111.70): V

Ion 148.00 (147.70 to 148.70): V

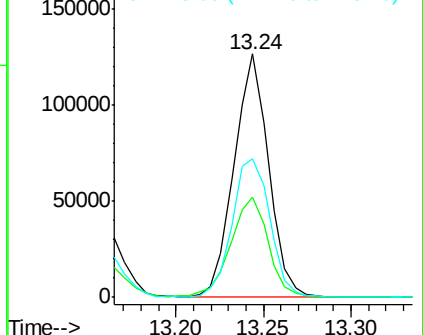

#65

1,2-Dichlorobenzene

Concen: 7.902 ug/L

RT: 13.53 min Scan# 1948

Delta R.T. 0.00 min

Lab File: VR026191.D

Acq: 6 Nov 2018 15:01


Tgt Ion:146 Resp: 486183

Ion Ratio Lower Upper

146 100

111 43.9 35.2 52.8



148 64.4 51.2 76.8




Abundance Ion 145.95 (145.65 to 146.65): V

Ion 111.00 (110.70 to 111.70): V

Ion 148.00 (147.70 to 148.70): V



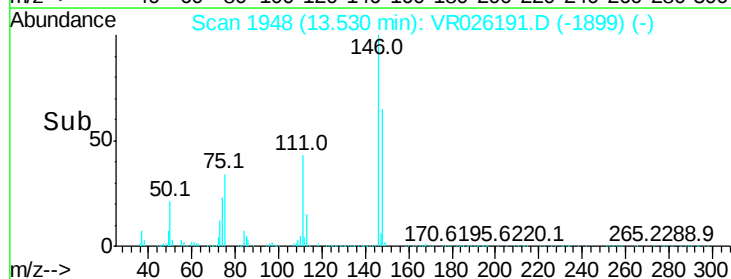
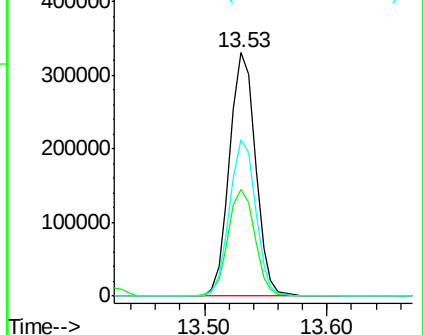




#66
 1,2-Dibromo-3-chloropropane
 Concen: 9.905 ug/L
 RT: 14.16 min Scan# 2051
 Delta R.T. 0.01 min
 Lab File: VR026191.D
 Acq: 6 Nov 2018 15:01

Instrument :
 MSVOA_R
 ClientSampleId :
 F9D04

Tgt Ion: 75 Resp: 24829
 Ion Ratio Lower Upper
 75 100
 155 5.8 40.9 61.3#
 157 0.8 67.3 100.9#

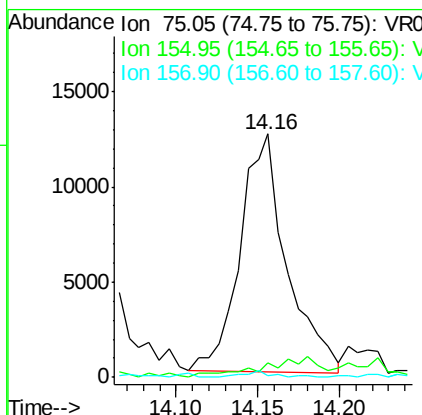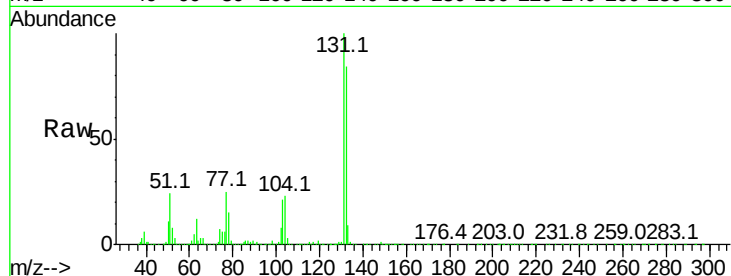

#69
 Naphthalene
 Concen: 285.257 ug/L
 RT: 15.00 min Scan# 2190
 Delta R.T. 0.00 min
 Lab File: VR026191.D
 Acq: 6 Nov 2018 15:01

Tgt Ion: 128 Resp: 7551862
 Ion Ratio Lower Upper
 128 100
 127 15.7 11.0 16.6
 129 13.5 9.1 13.7

