

Data File : VR026199.D
Acq On : 7 Nov 2018 11:18
Operator : SY/MD
Sample : J5801-03
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
F9D02

Quant Time: Nov 13 00:32:14 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR101518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Nov 07 12:50:17 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	655465	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	536346	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.23	152	193155	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.17	65	192475	3.36	ug/L	0.02
Spiked Amount	5.000	Range	40 - 130	Recovery	=	67.20%
7) Chloroethane-d5	2.62	69	199328	4.04	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	80.80%
11) 1,1-Dichloroethene-d2	3.61	63	400739	2.84	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	56.80%#
20) 2-Butanone-d5	6.58	46	220874	46.90	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.80%
24) Chloroform-d	7.20	84	360320	3.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	79.00%
26) 1,2-Dichloroethane-d4	7.90	65	159695	4.21	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.20%
32) Benzene-d6	7.85	84	718775	4.17	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.40%
36) 1,2-Dichloropropane-d6	8.90	67	192729	4.33	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	86.60%
41) Toluene-d8	9.97	98	677604	4.16	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.20%
43) trans-1,3-Dichloropropene-	10.24	79	47594	4.08	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.60%
46) 2-Hexanone-d5	10.59	63	188604	55.96	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	111.92%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	82359	4.72	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.40%
64) 1,2-Dichlorobenzene-d4	13.51	152	139200	4.56	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.20%


Target Compounds					Qvalue
13) Acetone	3.70	43	31451	6.460 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VR026199.D
Acq On : 7 Nov 2018 11:18
Operator : SY/MD
Sample : J5801-03
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
F9D02

Quant Time: Nov 13 00:32:14 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR101518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Nov 07 12:50:17 2018
Response via : Initial Calibration

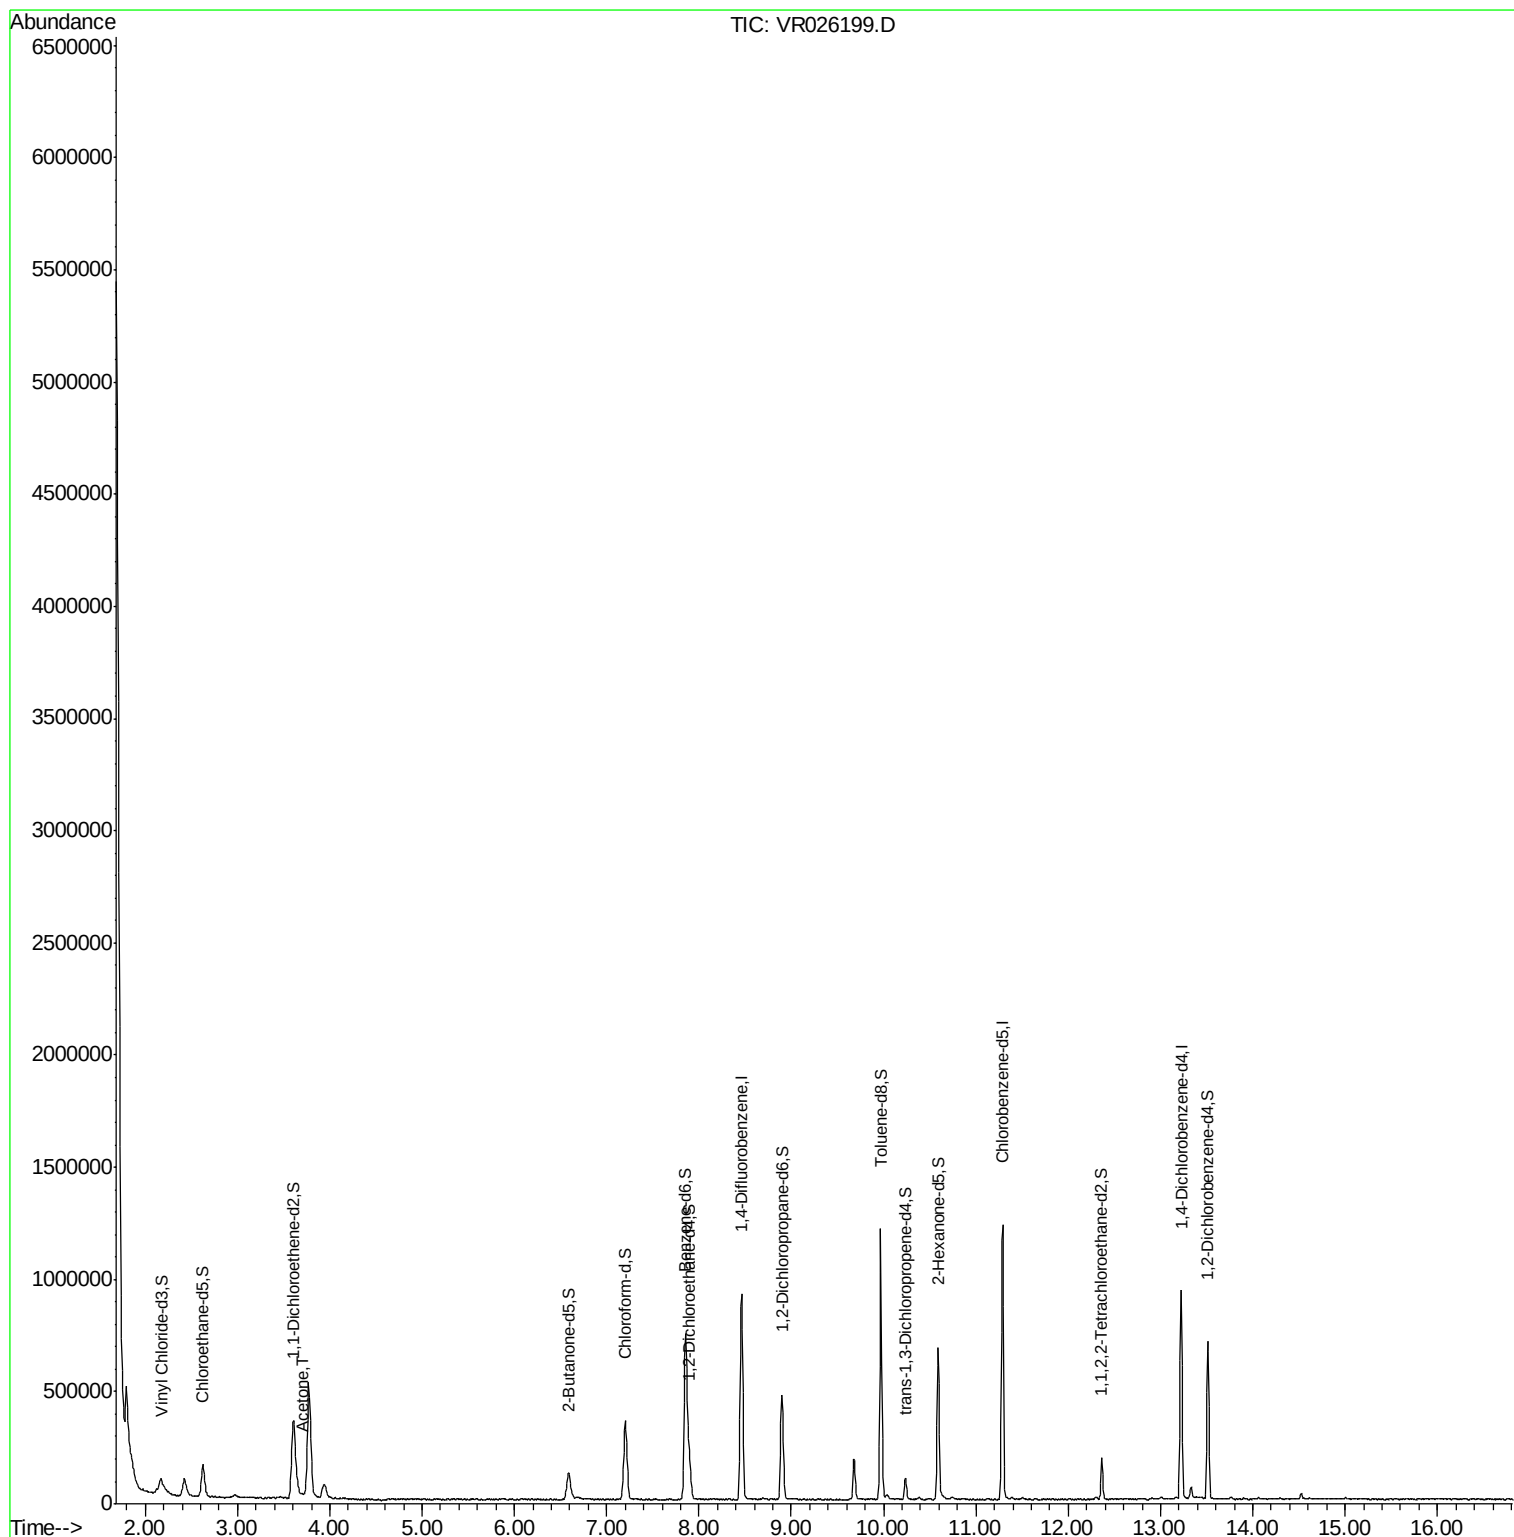

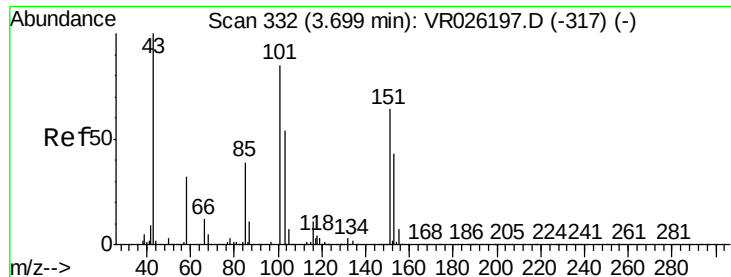

#13

Acetone

Concen: 6.460 ug/L

RT: 3.70 min Scan# 332

Delta R.T. -0.00 min

Lab File: VR026199.D

Acq: 7 Nov 2018 11:18

Instrument :
MSVOA_R
ClientSampleId :
F9D02

Tgt Ion: 43 Resp: 31451

Ion Ratio Lower Upper

43 100

58 25.3 0.0 55.4

