

Quantitation Report (LSC Reviewed)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR112018\
 Data File : VR026240.D
 Acq On : 20 Nov 2018 22:09
 Operator : SY/MD
 Sample : J6026-01
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_R
 Client Sample Id :
 H0FH2

Manual Integrations
 APPROVED

MMDadoda
 11/21/2018 5:40:10 PM

Quant Time: Nov 21 10:22:17 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR112018WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Nov 21 03:23:51 2018
 Response via : Initial Calibration

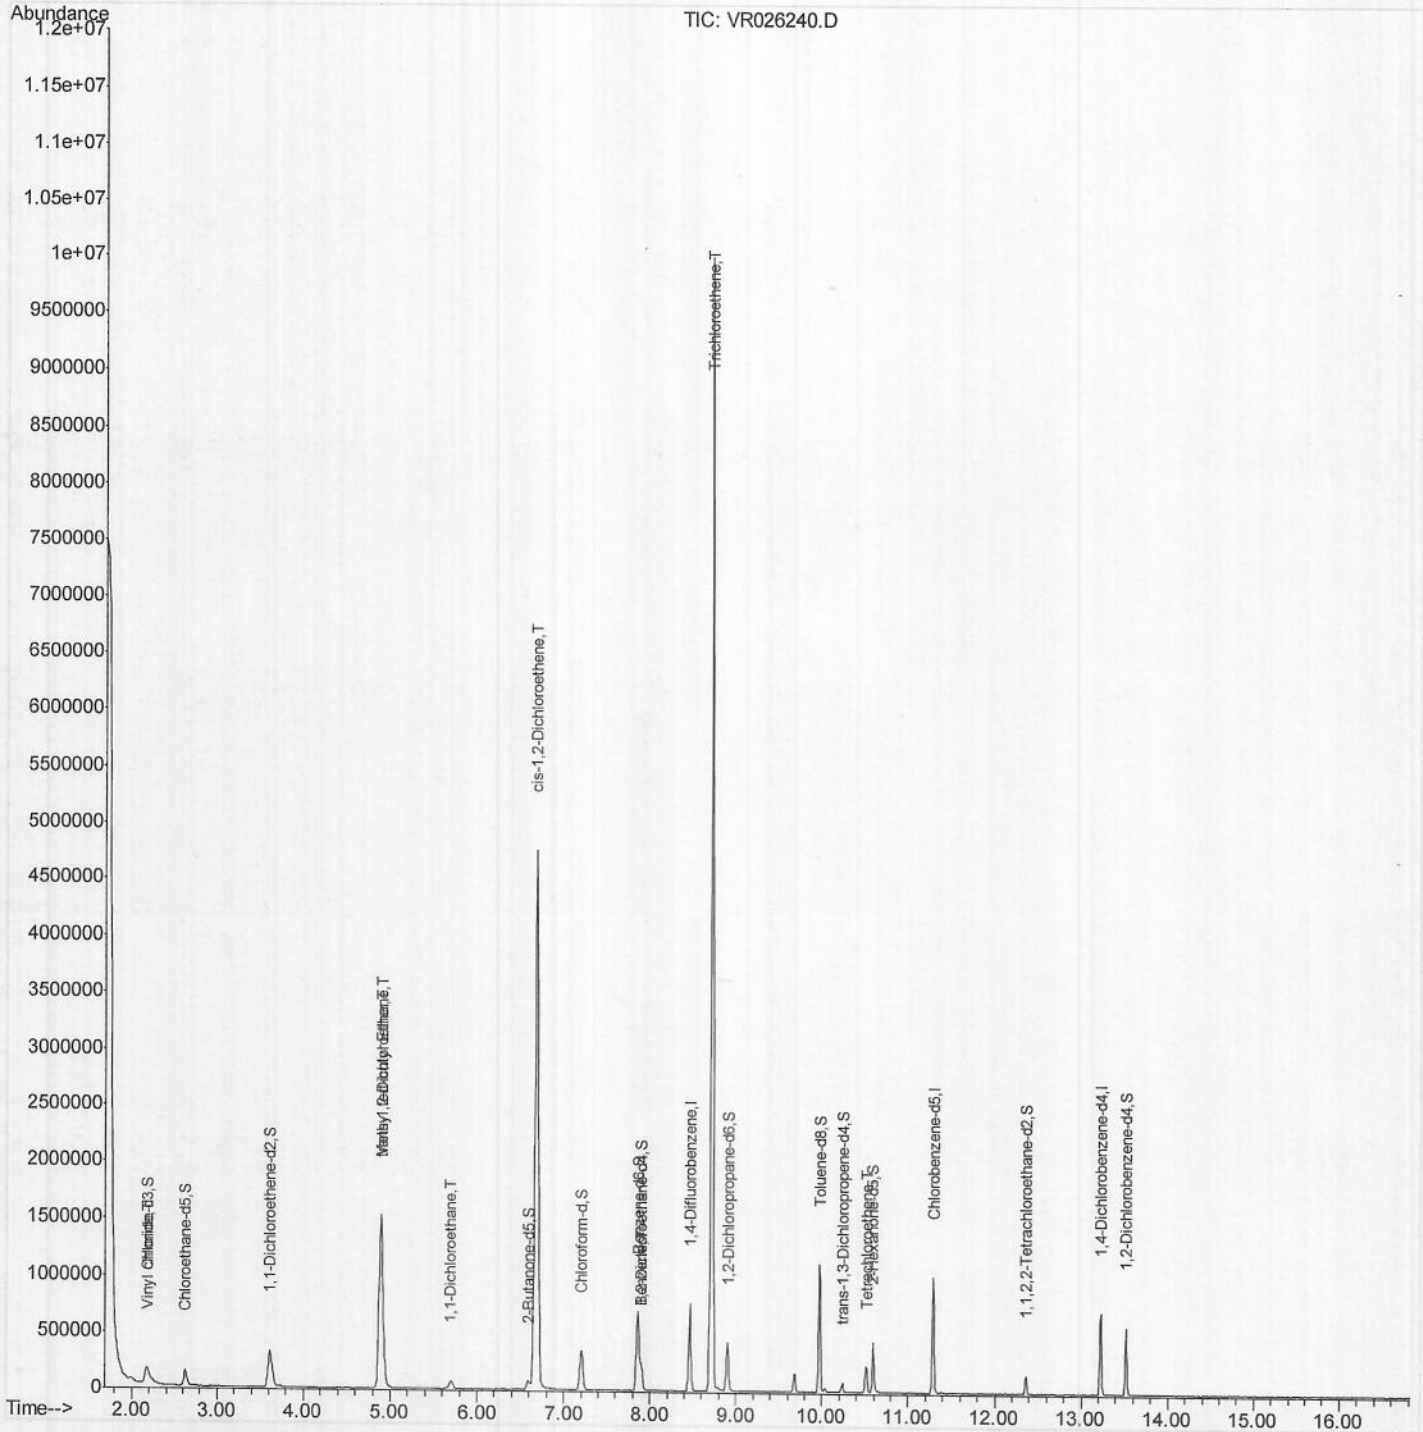

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR112018\
Quantitation Report (Qedit)




Data File : VR026240.D
Acq On : 20 Nov 2018 22:09
Operator : SY/MD
Sample : J6026-01
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
H0FH2

Manual Integrations
APPROVED

MMDadoda
11/21/2018 5:40:10 PM

Quant Time: Nov 21 03:27:01 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR112018WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Nov 21 03:23:51 2018
Response via : Initial Calibration

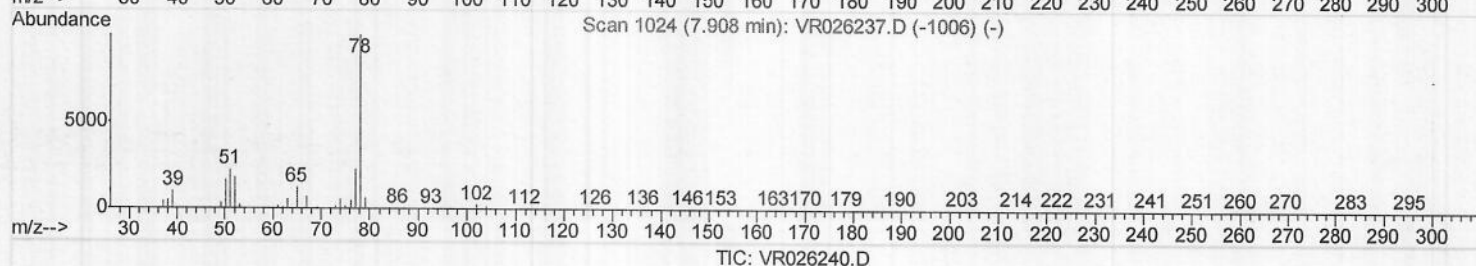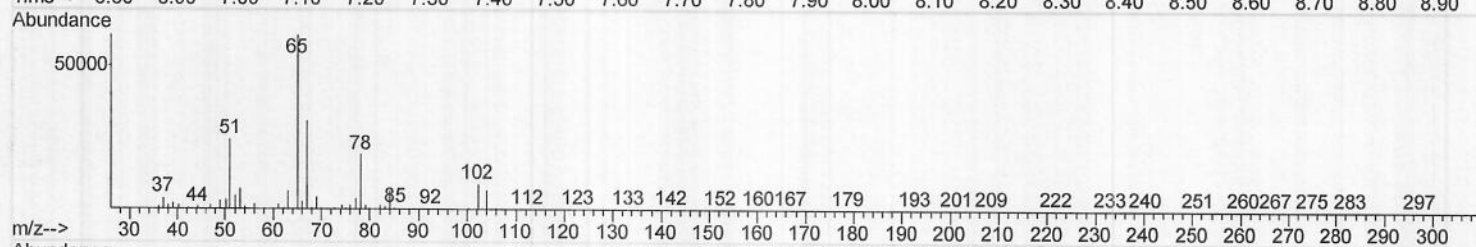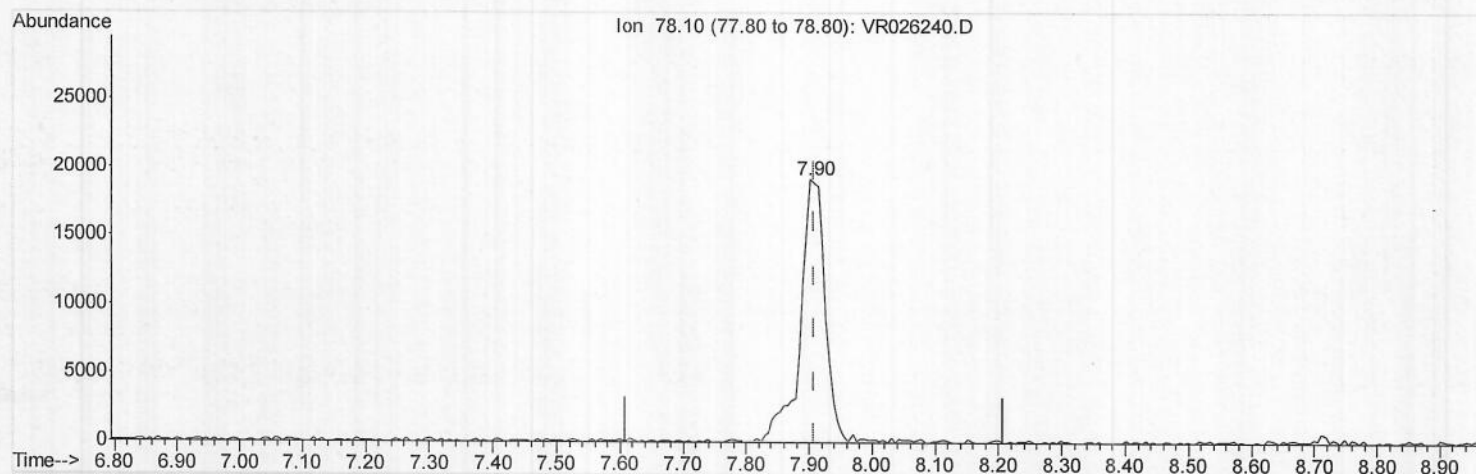

(33) Benzene (T)

7.902min (-0.006) 0.31ug/L

response 52058

Ion	Exp%	Act%
78.10	100	100
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR112018\
Quantitation Report (Qedit)




Data File : VR026240.D
Acq On : 20 Nov 2018 22:09
Operator : SY/MD
Sample : J6026-01
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
H0FH2

Manual Integrations
APPROVED

MMDadoda
11/21/2018 5:40:10 PM

Quant Time: Nov 21 03:27:01 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR112018WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Nov 21 03:23:51 2018
Response via : Initial Calibration

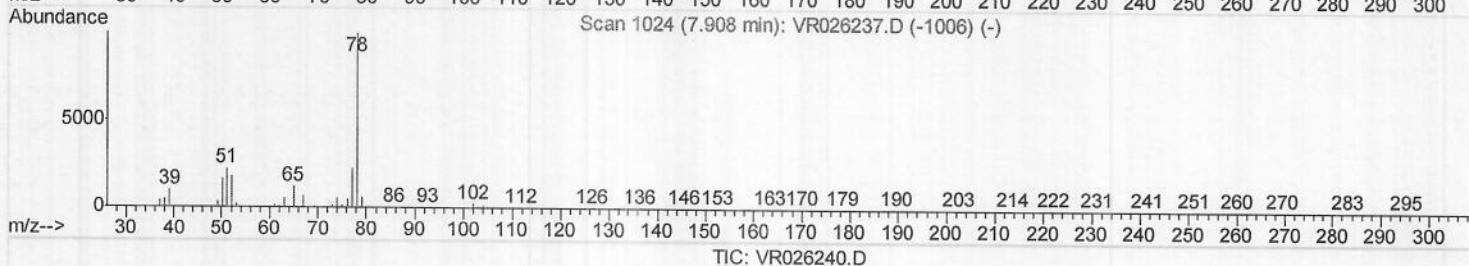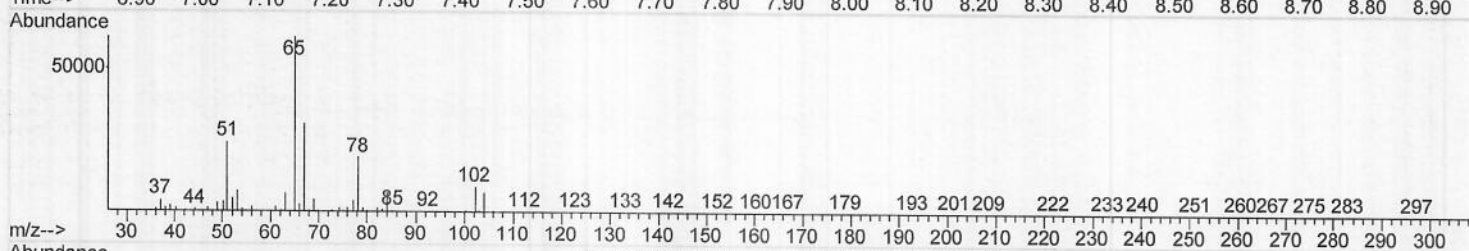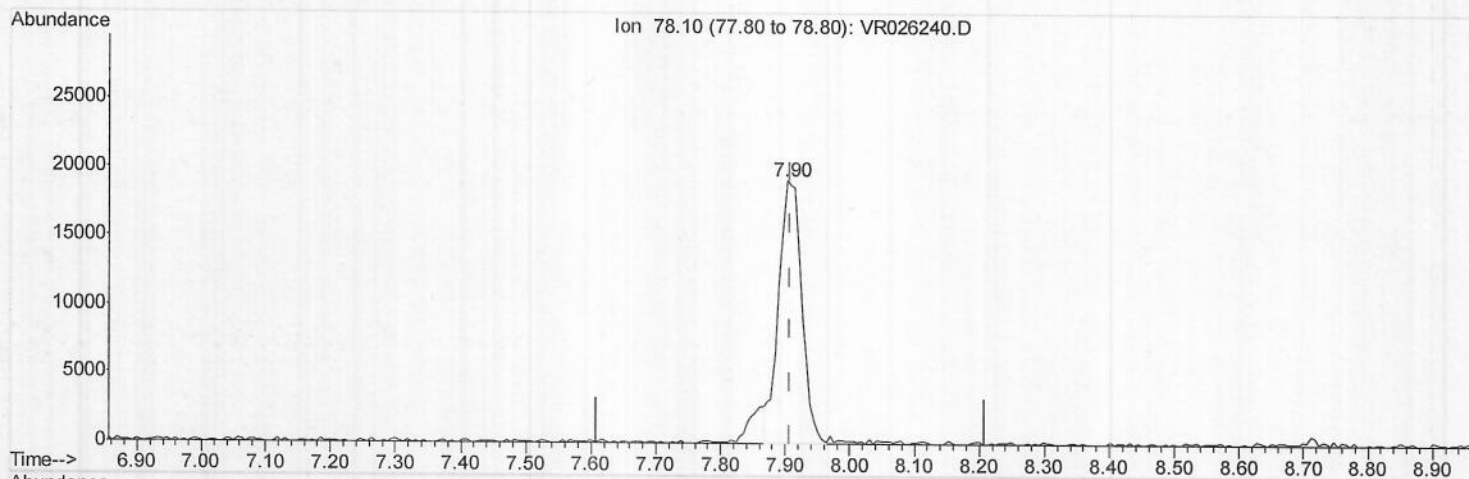

TIC: VR026240.D

(33) Benzene (T)

7.902min (-0.006) 0.29ug/L m) 11/26/18 SY

response 47765

Ion	Exp%	Act%
78.10	100	100
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (LSC Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR112018\
 Data File : VR026240.D
 Acq On : 20 Nov 2018 22:09
 Operator : SY/MD
 Sample : J6026-01
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_R
 Client Sampled :
 H0FH2

Manual Integrations
 APPROVED

MMDadoda
 11/21/2018 5:40:10 PM

Quant Time: Nov 21 10:22:17 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR112018WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Nov 21 03:23:51 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	544818	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	458385	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.23	152	147450	5.00	ug/L	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) Vinyl Chloride-d3	2.17	65	200955	4.84	ug/L	0.01
Spiked Amount 5.000	Range 40 - 130		Recovery =	96.80%		
7) Chloroethane-d5	2.63	69	186640	5.01	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	100.20%		
11) 1,1-Dichloroethene-d2	3.61	63	384906	3.65	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	73.00%		
20) 2-Butanone-d5	6.59	46	175341	45.58	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	91.16%		
24) Chloroform-d	7.20	84	358024	4.40	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	88.00%		
26) 1,2-Dichloroethane-d4	7.90	65	142308	4.49	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	89.80%		
32) Benzene-d6	7.85	84	704545	4.42	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	88.40%		
36) 1,2-Dichloropropane-d6	8.90	67	180939	4.52	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	90.40%		
41) Toluene-d8	9.97	98	625736	4.23	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	84.60%		
43) trans-1,3-Dichloropropene-	10.24	79	44022	4.03	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	80.60%		
46) 2-Hexanone-d5	10.59	63	124815	49.24	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	98.48%		
57) 1,1,2,2-Tetrachloroethane-	12.36	84	71710	4.39	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	87.80%		
64) 1,2-Dichlorobenzene-d4	13.52	152	127184	5.01	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	100.20%		

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
5) Vinyl chloride	2.18	62	159660	3.314	ug/L	93
17) Methyl tert-butyl Ether	4.90	73	549789	11.630	ug/L	99
18) trans-1,2-Dichloroethene	4.89	96	711845	16.949	ug/L	94
19) 1,1-Dichloroethane	5.69	63	105125	1.395	ug/L	96
22) cis-1,2-Dichloroethene	6.68	96	2798471	73.939	ug/L	99
33) Benzene	7.90	78	47765m)	0.285	ug/L	
34) Trichloroethene	8.71	95	3097721	69.828	ug/L	93
47) Tetrachloroethene	10.51	164	43704	1.341	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

) 11/26/18 SY