




Data File : VR026259.D
Acq On : 21 Nov 2018 13:50
Operator : SY/MD
Sample : VSTD02081
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
VSTD02081

Manual Integrations
APPROVED

MMDadoda
11/26/2018 9:21:24 AM

Quant Time: Nov 21 14:16:12 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR112118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Nov 21 13:44:11 2018
Response via : Initial Calibration

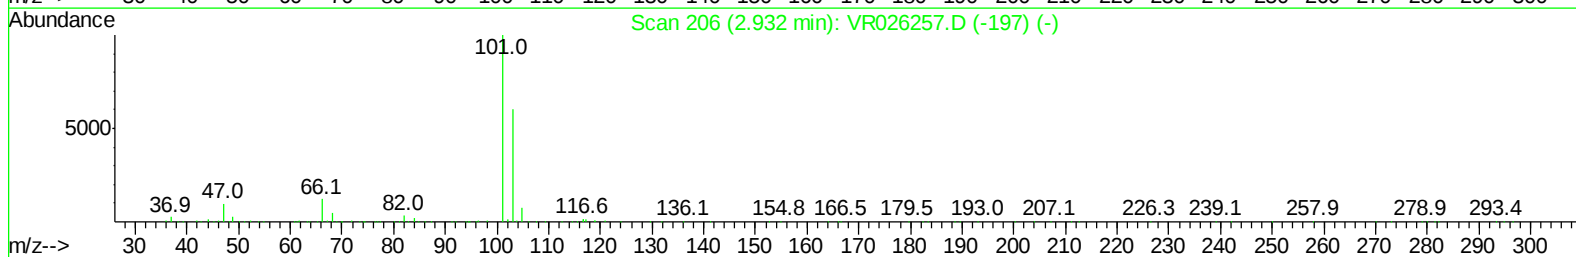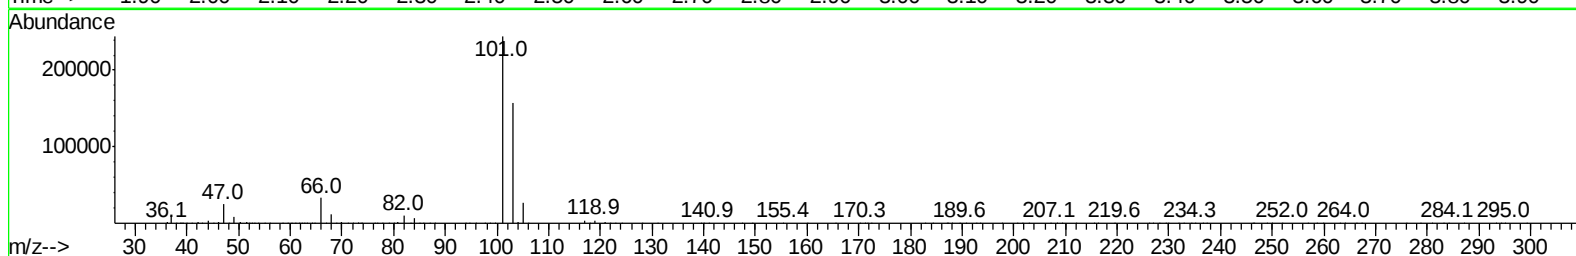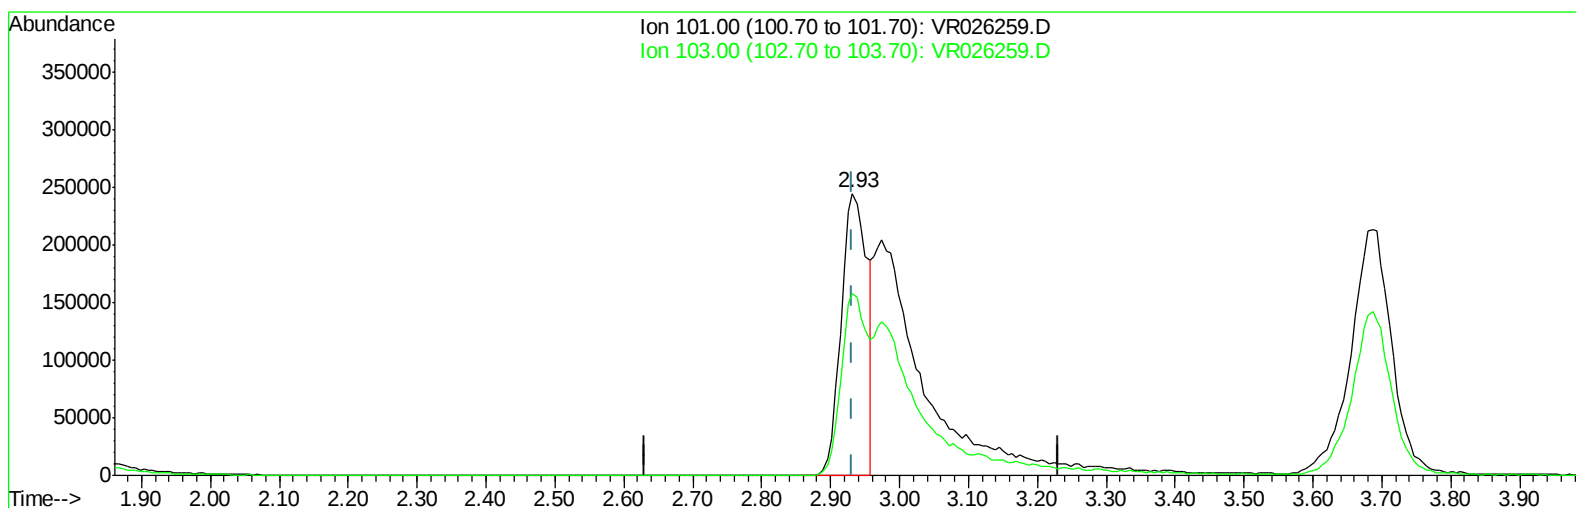

TIC: VR026259.D

(9) Trichlorofluoromethane (T)

2.932min (-0.000) 7.53ug/L

response 631526

Ion	Exp%	Act%
101.00	100	100
103.00	23.30	64.63#
0.00	0.00	0.00
0.00	0.00	0.00




Data File : VR026259.D
Acq On : 21 Nov 2018 13:50
Operator : SY/MD
Sample : VSTD02081
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
VSTD02081

Manual Integrations
APPROVED

MMDadoda
11/26/2018 9:21:24 AM

Quant Time: Nov 21 14:16:12 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR112118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Nov 21 13:44:11 2018
Response via : Initial Calibration

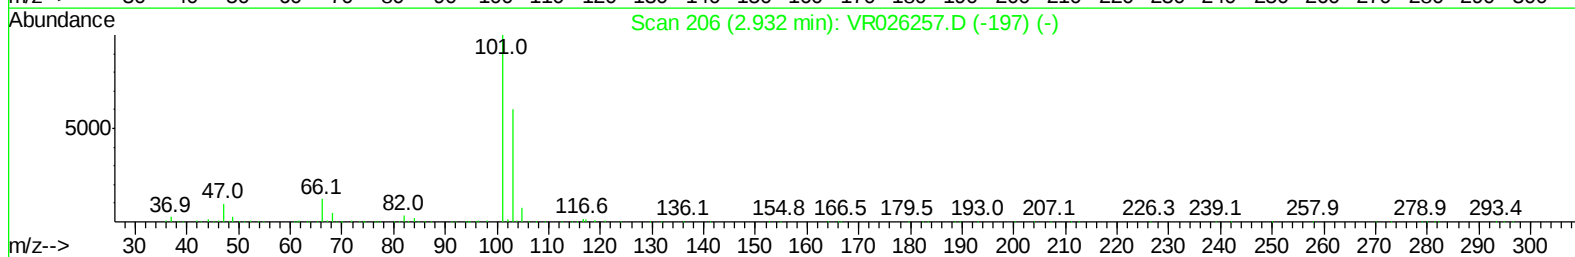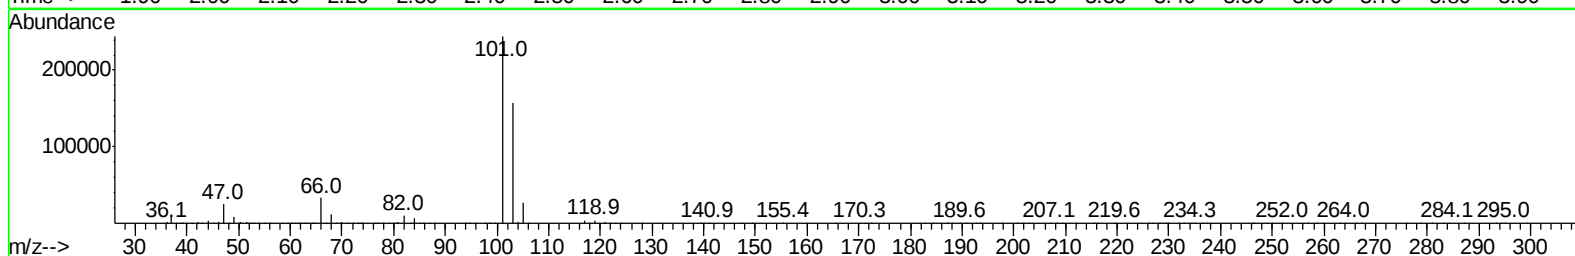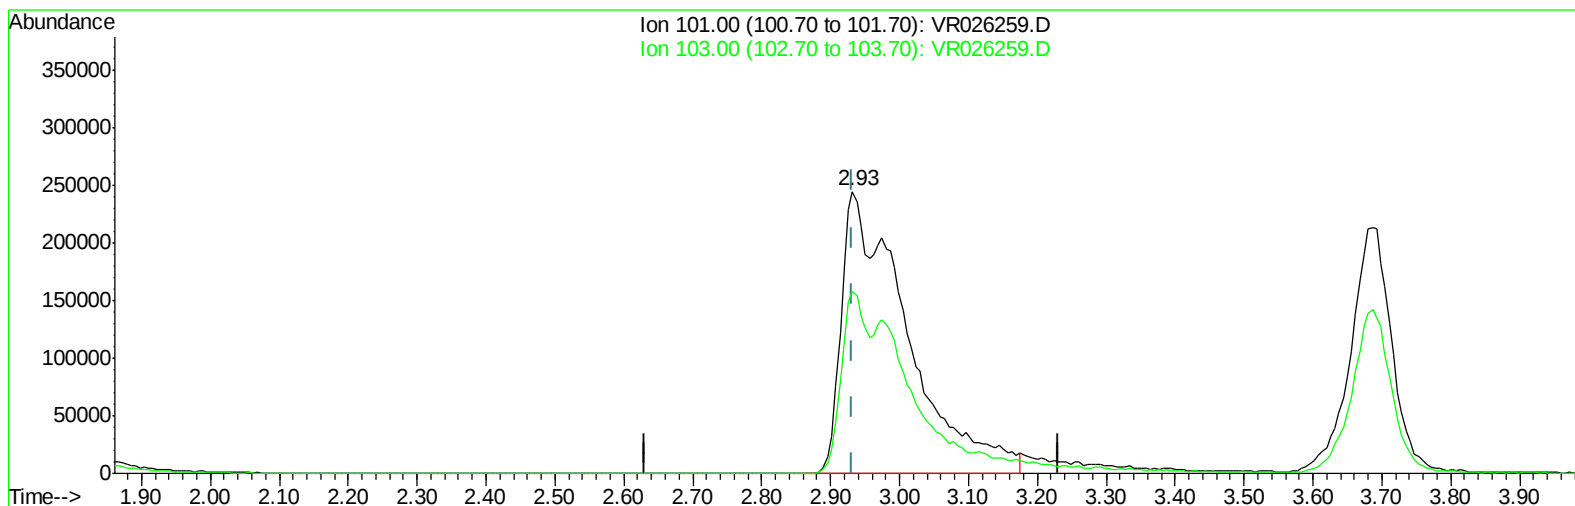

TIC: VR026259.D

(9) Trichlorofluoromethane (T)

2.932min (-0.000) 19.26ug/L m

response 1614956

Ion	Exp%	Act%
101.00	100	100
103.00	23.30	25.28
0.00	0.00	0.00
0.00	0.00	0.00

Data File : VR026259.D
Acq On : 21 Nov 2018 13:50
Operator : SY/MD
Sample : VSTD02081
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
VSTD02081

Manual Integrations
APPROVED

MMDadoda
11/26/2018 9:21:24 AM

Quant Time: Nov 21 14:17:33 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR112118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Nov 21 13:44:11 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	624583	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	547231	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.23	152	231368	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.17	65	955684	20.09	ug/L	0.00
7) Chloroethane-d5	2.63	69	798456	18.69	ug/L	0.00
11) 1,1-Dichloroethene-d2	3.61	63	2401039	19.87	ug/L	-0.02
20) 2-Butanone-d5	6.59	46	955488	216.65	ug/L	0.00
24) Chloroform-d	7.20	84	1879700	20.16	ug/L	0.00
26) 1,2-Dichloroethane-d4	7.90	65	729426	20.09	ug/L	0.00
32) Benzene-d6	7.85	84	3906329	20.55	ug/L	0.00
36) 1,2-Dichloropropane-d6	8.90	67	953657	19.95	ug/L	0.00
41) Toluene-d8	9.97	98	3805125	21.55	ug/L	0.00
43) trans-1,3-Dichloropropene-	10.24	79	283768	21.74	ug/L	0.00
46) 2-Hexanone-d5	10.59	63	727036	240.26	ug/L	0.00
57) 1,1,2,2-Tetrachloroethane-	12.36	84	382990	19.66	ug/L	0.00
64) 1,2-Dichlorobenzene-d4	13.52	152	834985	20.95	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	419.00%#

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.84	85	802373	18.349	ug/L	99
3) Chloromethane	2.02	50	1015293	18.073	ug/L	99
5) Vinyl chloride	2.17	62	1017038	18.412	ug/L	97
6) Bromomethane	2.53	94	646924	17.497	ug/L	98
8) Chloroethane	2.66	64	623185	18.036	ug/L	96
9) Trichlorofluoromethane	2.93	101	1614956m	19.255	ug/L	
10) 1,1,2-Trichloro-1,2,2-trif	3.69	101	880074	18.269	ug/L	98
12) 1,1-Dichloroethene	3.62	96	991220	18.914	ug/L	87
13) Acetone	3.70	43	719404	216.958	ug/L	99
14) Carbon disulfide	3.93	76	2694978	20.596	ug/L	99
15) Methyl Acetate	4.19	43	182727	18.991	ug/L	96
16) Methylene chloride	4.40	84	835704	17.832	ug/L	98
17) Methyl tert-butyl Ether	4.90	73	1145691	21.140	ug/L	97
18) trans-1,2-Dichloroethene	4.88	96	963205	20.006	ug/L	98
19) 1,1-Dichloroethane	5.69	63	1689097	19.549	ug/L	97
21) 2-Butanone	6.69	43	1027283	220.066	ug/L	100
22) cis-1,2-Dichloroethene	6.67	96	917586	21.148	ug/L #	99
23) Bromochloromethane	7.06	128	245642	18.806	ug/L	92
25) Chloroform	7.23	83	1673772	17.857	ug/L	99
27) 1,2-Dichloroethane	7.99	62	729015	19.099	ug/L	99
29) 1,1,1-Trichloroethane	7.43	97	1471153	19.013	ug/L	98
30) Cyclohexane	7.52	56	1465318	21.292	ug/L	99
31) Carbon tetrachloride	7.63	117	1326434	18.861	ug/L	100
33) Benzene	7.91	78	3985198	19.930	ug/L	100
34) Trichloroethene	8.71	95	1031093	19.469	ug/L	96
35) Methylcyclohexane	8.95	83	1528244	21.672	ug/L	97
37) 1,2-Dichloropropane	9.00	63	785424	18.979	ug/L	99
38) Bromodichloromethane	9.28	83	926751	19.186	ug/L	99
39) cis-1,3-Dichloropropene	9.72	75	1062210	22.361	ug/L	96

Data File : VR026259.D
Acq On : 21 Nov 2018 13:50
Operator : SY/MD
Sample : VSTD02081
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
VSTD02081

Manual Integrations
APPROVED

MMDadoda
11/26/2018 9:21:24 AM

Quant Time: Nov 21 14:17:33 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR112118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Nov 21 13:44:11 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
40) 4-Methyl-2-pentanone	9.87	43	2526746	219.699	ug/L	98
42) Toluene	10.04	91	4304039	18.016	ug/L	96
44) trans-1,3-Dichloropropene	10.26	75	727907	22.450	ug/L	97
45) 1,1,2-Trichloroethane	10.45	97	348986	19.596	ug/L	95
47) Tetrachloroethene	10.51	164	773538	19.888	ug/L	97
48) 2-Hexanone	10.63	43	1677233	217.125	ug/L	98
49) Dibromochloromethane	10.79	129	462511	21.370	ug/L	100
50) 1,2-Dibromoethane	10.89	107	309076	19.903	ug/L	97
51) Chlorobenzene	11.32	112	2346183	20.069	ug/L	98
52) Ethylbenzene	11.39	91	4887769	20.429	ug/L	94
53) m,p-Xylene	11.50	106	1921668	21.780	ug/L	99
54) o-Xylene	11.83	106	1869976	23.146	ug/L	86
55) Styrene	11.84	104	2851450	23.128	ug/L	99
56) Isopropylbenzene	12.13	105	4822694	21.792	ug/L	96
58) 1,1,2,2-Tetrachloroethane	12.39	83	332108	19.158	ug/L #	93
59) 1,2,3-Trichloropropane	12.43	75	242761	18.680	ug/L	98
61) Bromoform	12.01	173	187765	21.162	ug/L	97
62) 1,3-Dichlorobenzene	13.16	146	1545085	20.975	ug/L	98
63) 1,4-Dichlorobenzene	13.24	146	1514454	19.057	ug/L	99
65) 1,2-Dichlorobenzene	13.53	146	1204531	19.911	ug/L	96
66) 1,2-Dibromo-3-chloropropan	14.14	75	33866	16.745	ug/L	93
67) 1,3,5-Trichlorobenzene	14.30	180	967223	20.279	ug/L	98
68) 1,2,4-trichlorobenzene	14.79	180	581869	21.574	ug/L	99
69) Naphthalene	15.00	128	653730	24.883	ug/L	99
70) 1,2,3-Trichlorobenzene	15.18	180	392525	20.344	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VR026259.D
Acq On : 21 Nov 2018 13:50
Operator : SY/MD
Sample : VSTD02081
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_R
Client Sample Id :
VSTD02081

Manual Integrations
APPROVED

MMDadoda
11/26/2018 9:21:24 AM

Quant Time: Nov 21 14:17:33 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR112118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Nov 21 13:44:11 2018
Response via : Initial Calibration

