
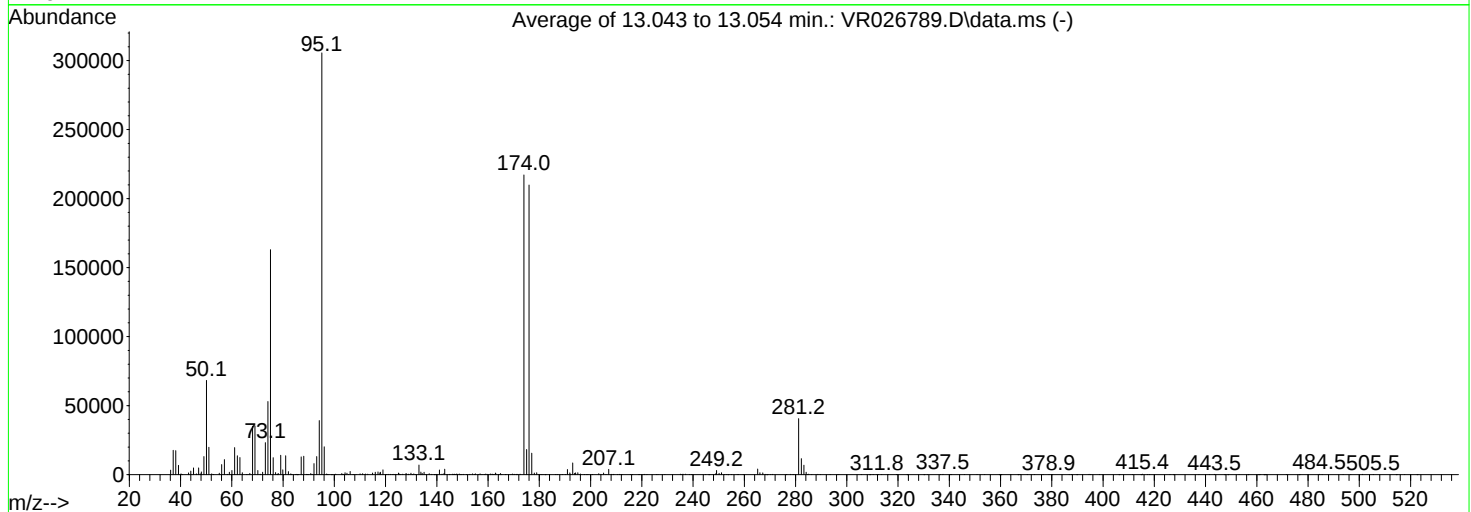


Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR120425\
Data File : VR026789.D
Acq On : 4 Dec 2025 9:17
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5mL/MSVOA_R/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_R\methods\82R120425S.M
Title : SW846 8260
Last Update : Fri Dec 05 04:05:32 2025

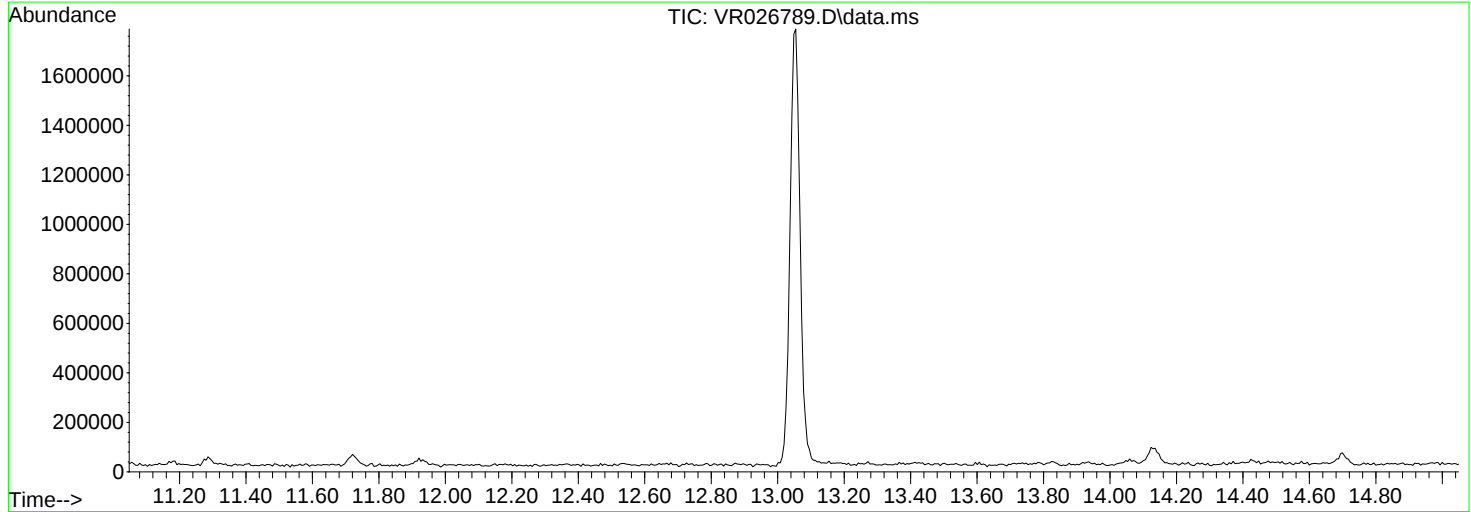

AutoFind: Scans 1900, 1901, 1902; Background Corrected with Scan 1891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	68280	PASS
75	95	30	60	53.3	162965	PASS
95	95	100	100	100.0	305600	PASS
96	95	5	9	6.6	20149	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	71.1	217152	PASS
175	174	5	9	8.4	18270	PASS
176	174	95	101	96.6	209877	PASS
177	176	5	9	7.4	15490	PASS