

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR121718\
 Data File : VR026273.D
 Acq On : 17 Dec 2018 20:52
 Operator : SY/MD
 Sample : J6418-14
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 BF037

Quant Time: Dec 18 00:49:31 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR121718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Dec 18 00:30:13 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	511487	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	419865	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.23	152	125741	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.14	65	181966	5.59	ug/L	-0.01
Spiked Amount	5.000	Range	40 - 130	Recovery	=	111.80%
7) Chloroethane-d5	2.62	69	179118	5.55	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	111.00%
11) 1,1-Dichloroethene-d2	3.61	63	357209	3.88	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.60%
20) 2-Butanone-d5	6.59	46	145874	50.47	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.94%
24) Chloroform-d	7.20	84	335836	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.60%
26) 1,2-Dichloroethane-d4	7.90	65	130720	5.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.40%
32) Benzene-d6	7.85	84	640257	4.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.80%
36) 1,2-Dichloropropane-d6	8.90	67	169352	4.93	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.60%
41) Toluene-d8	9.97	98	573428	4.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.80%
43) trans-1,3-Dichloropropene-	10.24	79	36389	4.03	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.60%
46) 2-Hexanone-d5	10.59	63	94268	50.22	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.44%
57) 1,1,2,2-Tetrachloroethane-	12.37	84	60565	4.76	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.20%
64) 1,2-Dichlorobenzene-d4	13.52	152	109735	5.48	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.60%


Target Compounds					Ovalue
13) Acetone	3.69	43	30638	10.405 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR121718\
Data File : VR026273.D
Acq On : 17 Dec 2018 20:52
Operator : SY/MD
Sample : J6418-14
Misc : 25mL/MSVOA R/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
BF037

Quant Time: Dec 18 00:49:31 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR121718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 18 00:30:13 2018
Response via : Initial Calibration

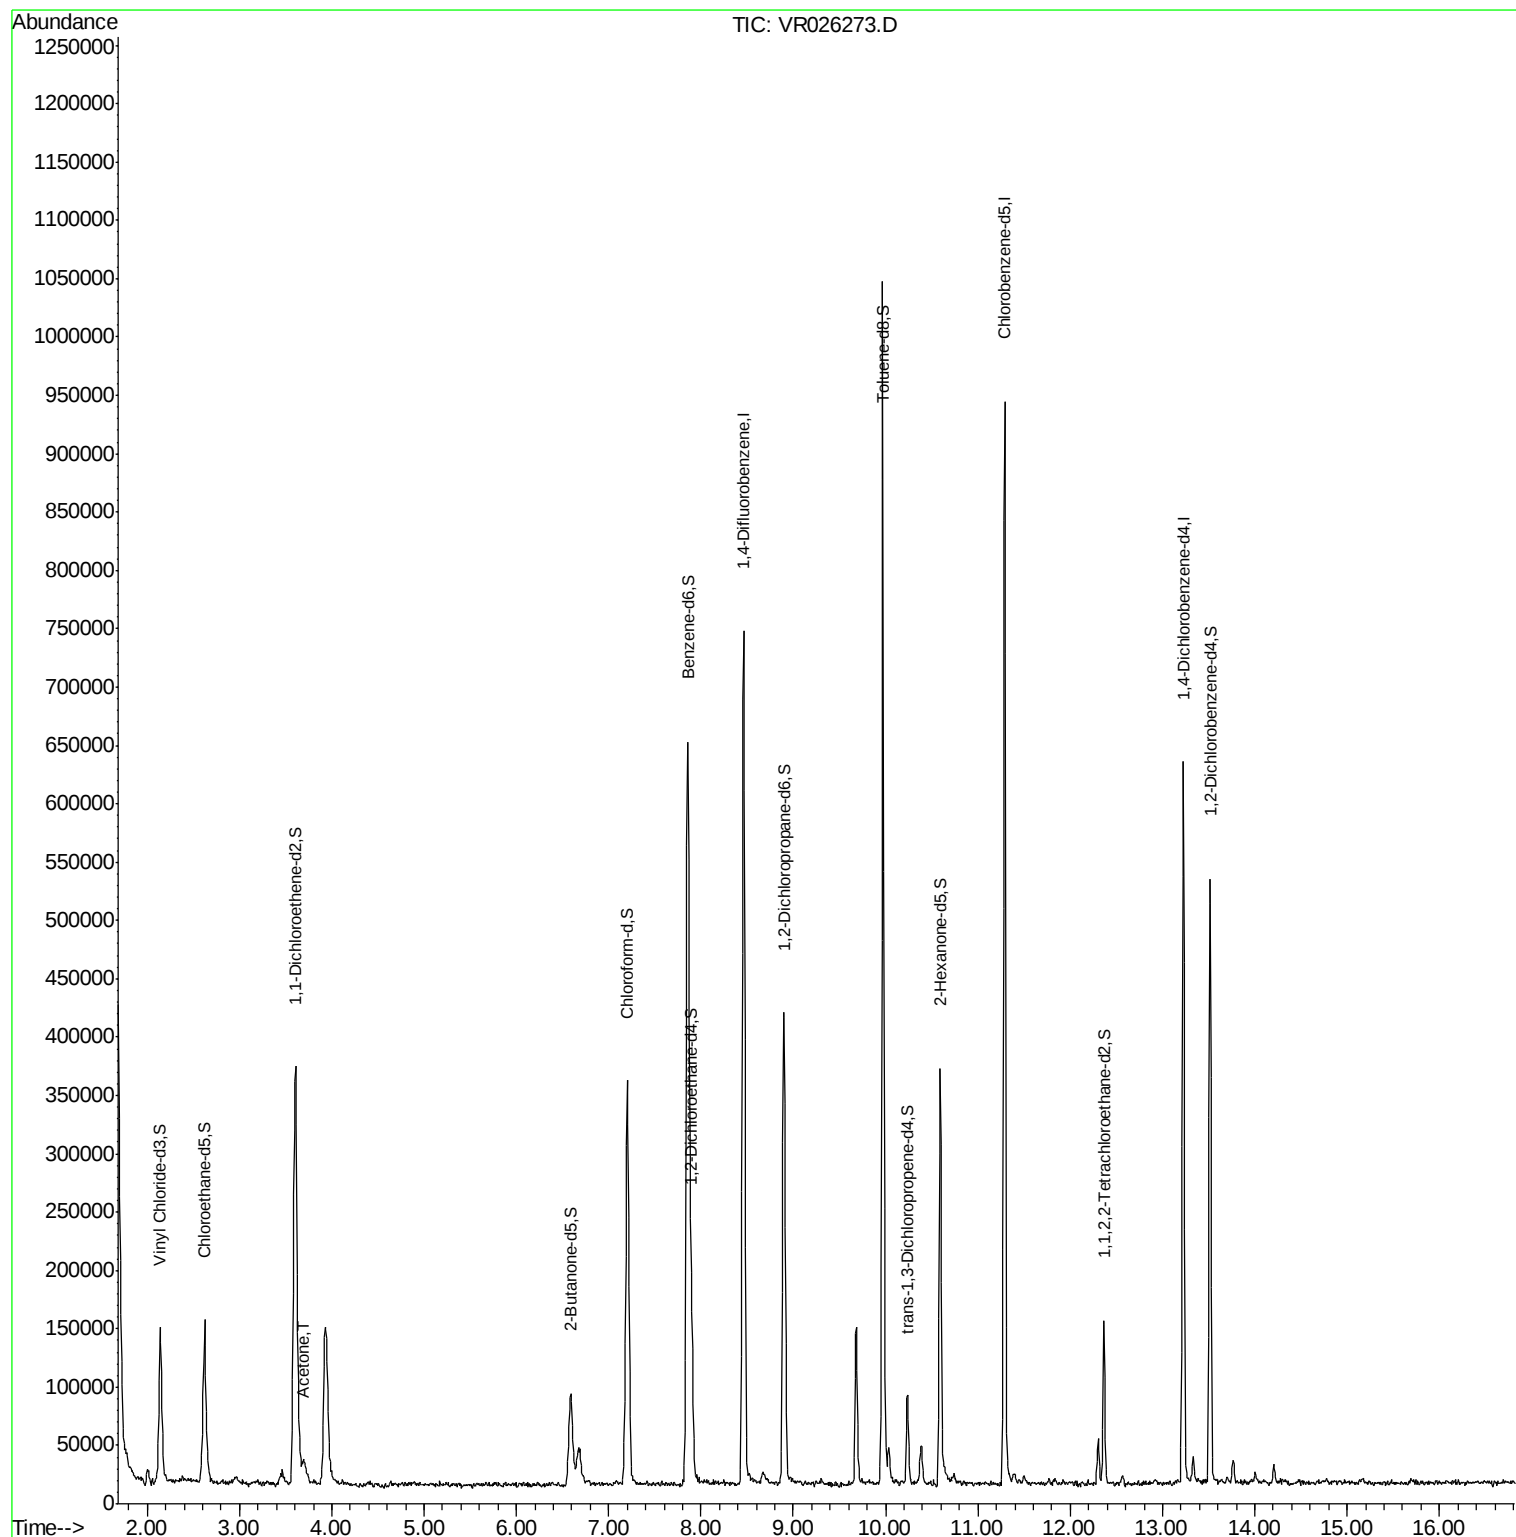

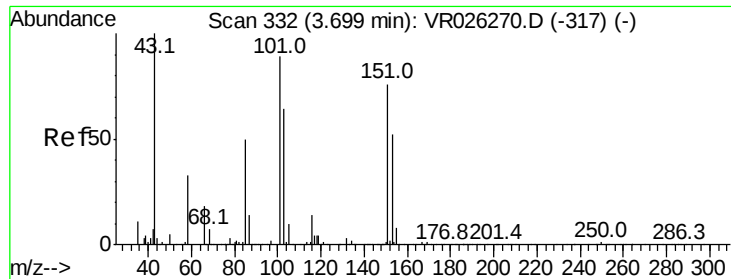

#13

Acetone

Concen: 10.405 ug/L

RT: 3.69 min Scan# 331

Delta R.T. -0.01 min

Lab File: VR026273.D

Acq: 17 Dec 2018 20:52

Instrument :
MSVOA_R
ClientSampleId :
BF037

Tot Ion: 43 Resp: 30638

Ion Ratio Lower Upper

43 100

58 27.7 0.0 60.8

