

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR121718\
 Data File : VR026276.D
 Acq On : 17 Dec 2018 22:31
 Operator : SY/MD
 Sample : J6419-18
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 BF028

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR121718WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.007	50	54	59	rBV	16084	29412	1.69%	0.228%
2	2.141	68	76	90	rBV	124197	289133	16.58%	2.237%
3	2.622	143	155	169	rBV	127520	344182	19.74%	2.663%
4	3.455	284	292	297	rBV6	15199	40316	2.31%	0.312%
5	3.607	305	317	328	rBV	343505	974111	55.85%	7.536%
6	3.693	329	331	338	rVB2	16274	34635	1.99%	0.268%
7	3.936	358	371	385	rBV	117999	389059	22.31%	3.010%
8	6.582	797	806	816	rBV2	72726	229665	13.17%	1.777%
9	7.203	897	908	921	rBV	316937	820963	47.07%	6.351%
10	7.860	1007	1016	1032	rBV2	640726	1744013	100.00%	13.492%
11	8.462	1106	1115	1126	rBV	708008	1296794	74.36%	10.032%
12	8.900	1179	1187	1198	rBV	389357	768833	44.08%	5.948%
13	9.679	1309	1315	1321	rBV	133426	226508	12.99%	1.752%
14	9.971	1356	1363	1370	rBV	1026389	1584128	90.83%	12.255%
15	10.032	1370	1373	1379	rVB2	42707	67056	3.84%	0.519%
16	10.239	1402	1407	1417	rVB	72491	122887	7.05%	0.951%
17	10.385	1423	1431	1438	rBV3	24047	56480	3.24%	0.437%
18	10.591	1459	1465	1474	rBV	359348	558927	32.05%	4.324%
19	11.291	1573	1580	1590	rBV	896773	1348574	77.33%	10.433%
20	12.307	1739	1747	1752	rBV2	36372	72346	4.15%	0.560%
21	12.362	1752	1756	1763	rVB	148315	216209	12.40%	1.673%
22	13.226	1892	1898	1908	rBV	601626	841000	48.22%	6.506%
23	13.329	1910	1915	1921	rBV3	24602	43793	2.51%	0.339%
24	13.518	1939	1946	1953	rVB	516459	752359	43.14%	5.820%
25	13.767	1981	1987	1993	rVB	22763	42839	2.46%	0.331%
26	14.211	2056	2060	2066	rVB5	23139	32016	1.84%	0.248%


Sum of corrected areas: 12926238

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA R\DATA\VR121718\
Data File : VR026276.D
Acq On : 17 Dec 2018 22:31
Operator : SY/MD
Sample : J6419-18
Misc : 25mL/MSVOA R/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
BF028

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR121718WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

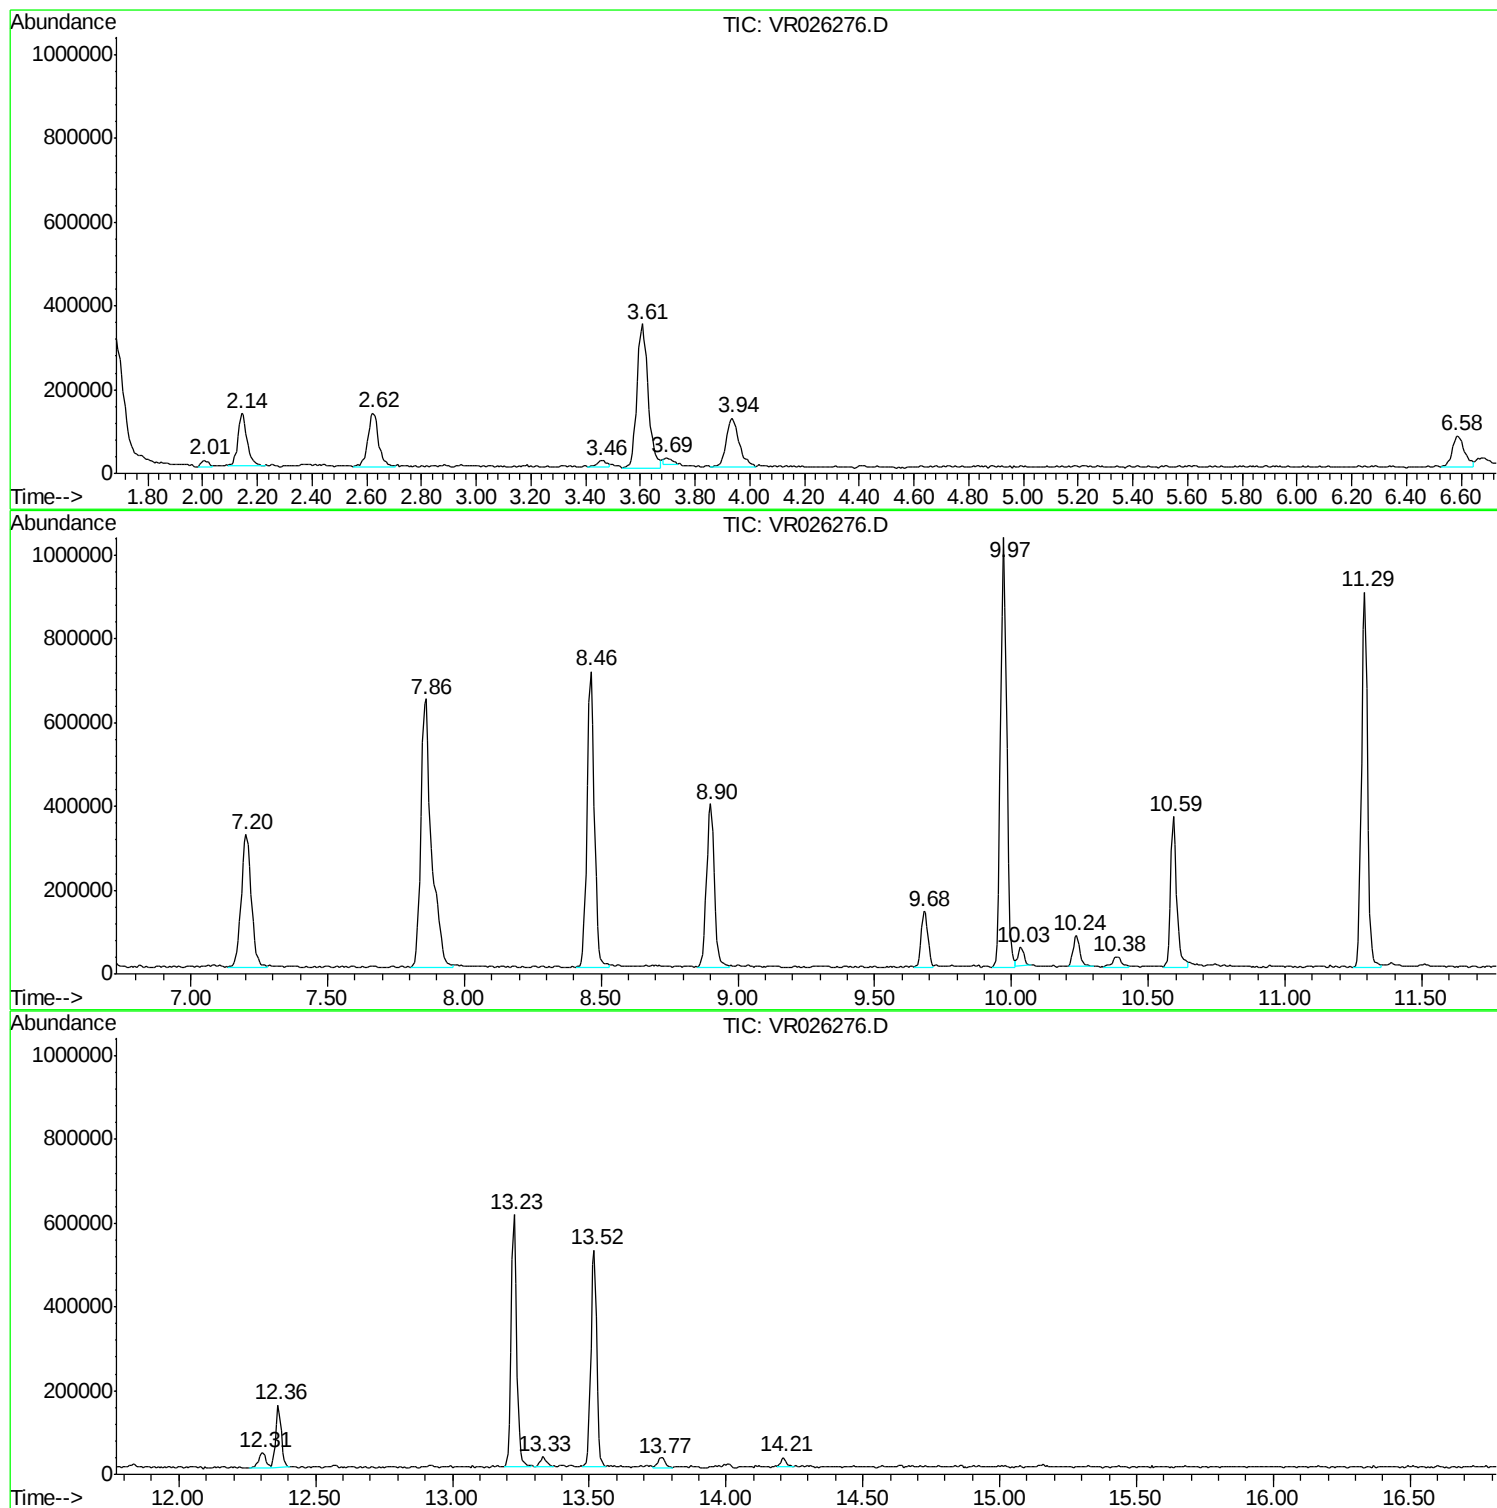

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR121718\
Data File : VR026276.D
Acq On : 17 Dec 2018 22:31
Operator : SY/MD
Sample : J6419-18
Misc : 25mL/MSVOA R/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
BF028










Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR121718WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.94	1.50 ug/L	389059	1,4-Difluorobenzene	8.46

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	72
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	64
3			Isopropyl Alcohol	60	C3H8O	000067-63-0	56
4			Propane, 2-ethoxy-	88	C5H12O	000625-54-7	40
5			Formic acid, 1-methylethyl ester	88	C4H8O2	000625-55-8	39

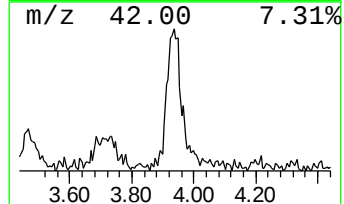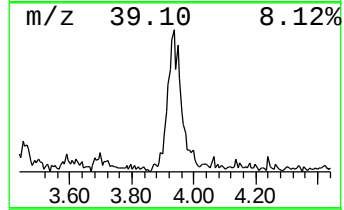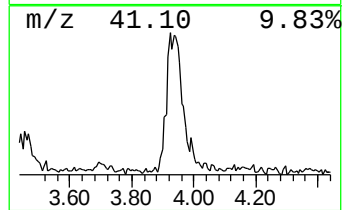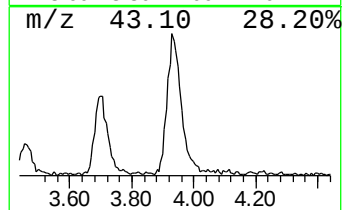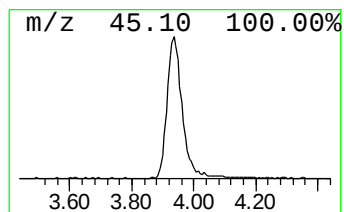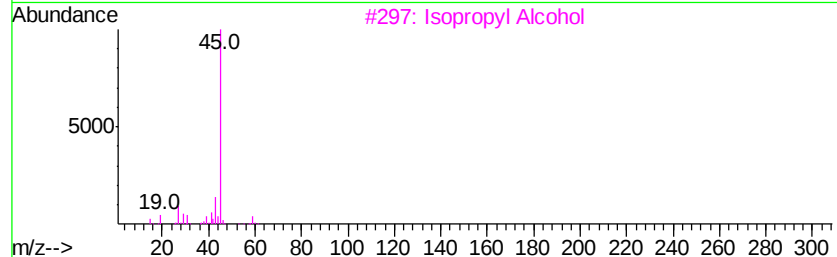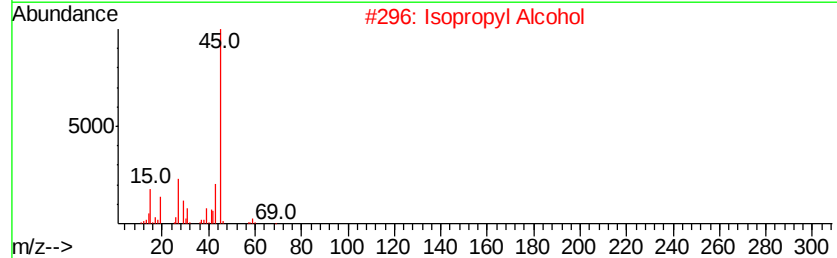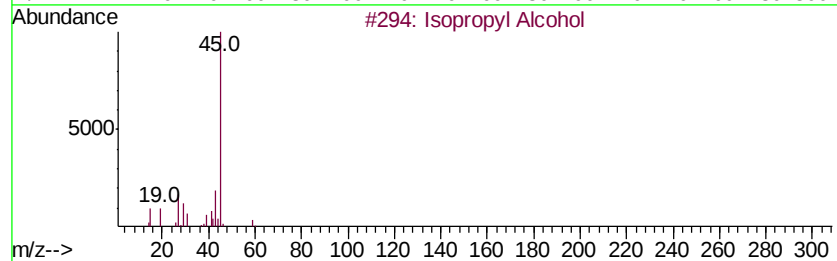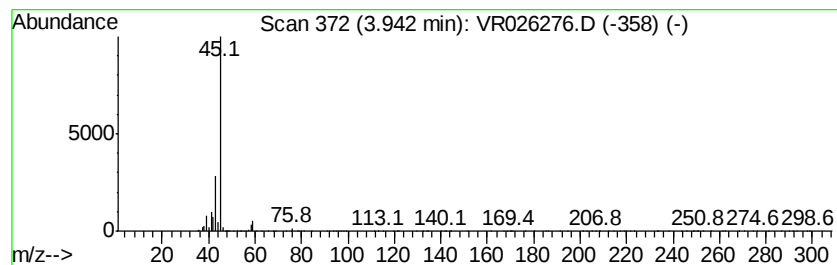

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR121718\
Data File : VR026276.D
Acq On : 17 Dec 2018 22:31
Operator : SY/MD
Sample : J6419-18
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
BF028

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR121718WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	3.94	1.5	ug/L	389059	1	8.46	1296790	5.0