

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR022819\
 Data File : VR026424.D
 Acq On : 28 Feb 2019 17:56
 Operator : SY/MD
 Sample : K1624-10
 Misc : 25mL/MSVOA_R/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 C0TT0

Quant Time: Mar 01 07:11:39 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR022219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Mar 01 06:30:52 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	491407	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	405063	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.23	152	134802	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.14	65	183776	3.82	ug/L	-0.01
Spiked Amount	5.000	Range	40 - 130	Recovery	=	76.40%
7) Chloroethane-d5	2.62	69	162291	4.12	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	82.40%
11) 1,1-Dichloroethene-d2	3.60	63	363033	3.22	ug/L	-0.02
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.40%
20) 2-Butanone-d5	6.58	46	182173	51.92	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.84%
24) Chloroform-d	7.20	84	332519	4.25	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.00%
26) 1,2-Dichloroethane-d4	7.89	65	139025	4.37	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.40%
32) Benzene-d6	7.85	84	599879	3.94	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	78.80%
36) 1,2-Dichloropropane-d6	8.89	67	162456	4.21	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	84.20%
41) Toluene-d8	9.96	98	534037	3.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.80%
43) trans-1,3-Dichloropropene-	10.24	79	37352	3.67	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	73.40%
46) 2-Hexanone-d5	10.59	63	139145	54.15	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	108.30%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	57705	3.94	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	78.80%
64) 1,2-Dichlorobenzene-d4	13.51	152	104591	4.49	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	89.80%


Target Compounds					Qvalue
13) Acetone	3.69	43	35715	11.315 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR022819\
Data File : VR026424.D
Acq On : 28 Feb 2019 17:56
Operator : SY/MD
Sample : K1624-10
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
C0TT0

Quant Time: Mar 01 07:11:39 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR022219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Mar 01 06:30:52 2019
Response via : Initial Calibration

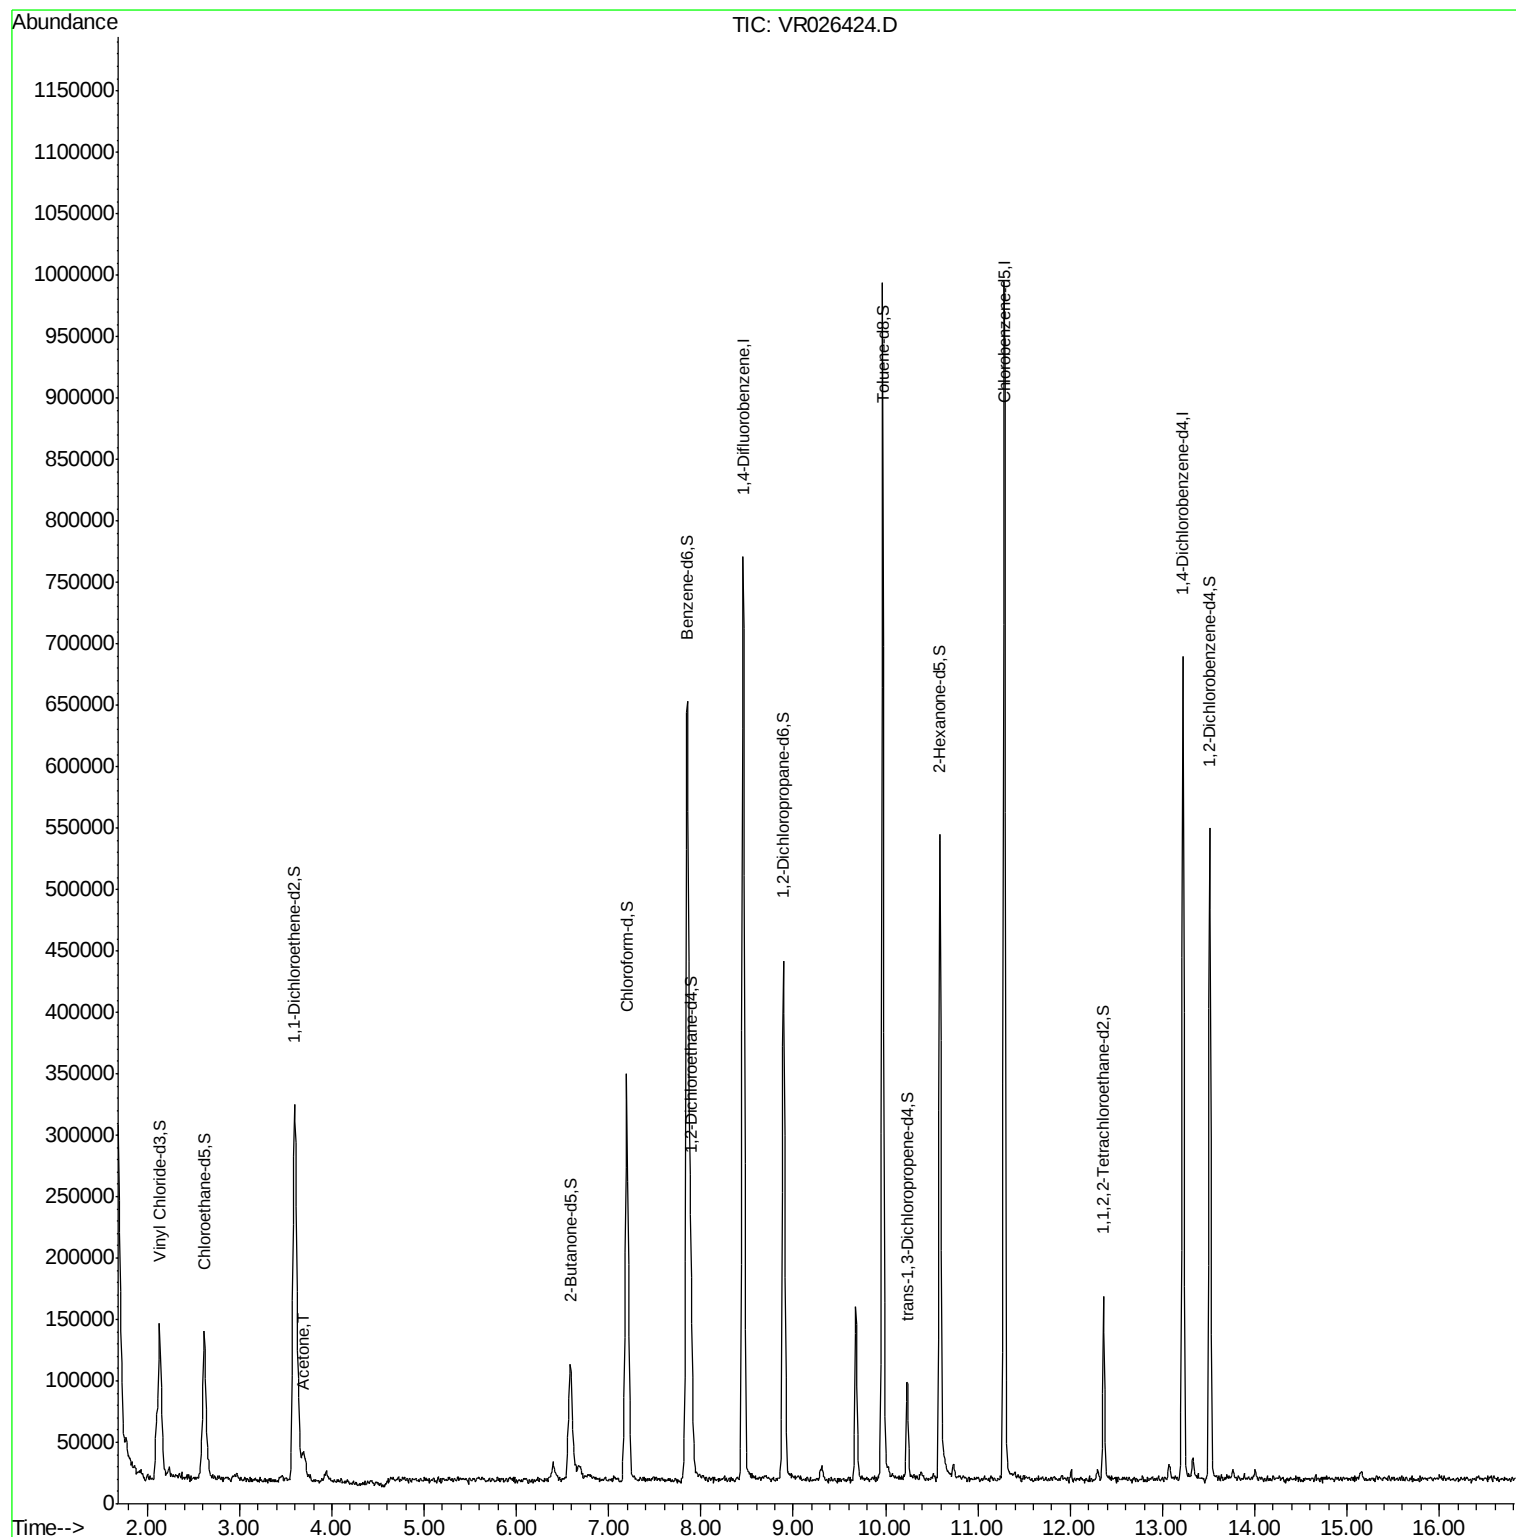

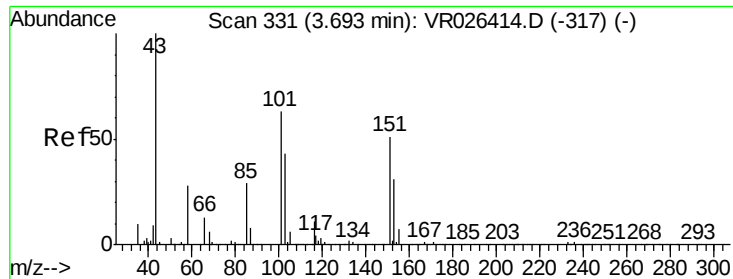

#13

Acetone

Concen: 11.315 ug/L

RT: 3.69 min Scan# 331

Delta R.T. 0.00 min

Lab File: VR026424.D

Acq: 28 Feb 2019 17:56

Instrument :
MSVOA_R
ClientSampleId :
C0TT0

Tgt Ion: 43 Resp: 35715

Ion Ratio Lower Upper

43 100

58 29.2 0.0 52.2

