

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR022819\
 Data File : VR026427.D
 Acq On : 28 Feb 2019 19:35
 Operator : SY/MD
 Sample : K1588-14DL 5X
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 C0AB2DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR022219WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.941	41	43	50	rVB4	13451	22579	1.23%	0.147%
2	2.141	68	76	89	rBV	133793	299208	16.34%	1.944%
3	2.622	146	155	166	rBV	129893	305925	16.70%	1.987%
4	3.607	307	317	331	rBV3	290196	957675	52.28%	6.221%
5	3.936	362	371	384	rBV	112653	335516	18.32%	2.179%
6	4.885	516	527	540	rVB3	49582	172768	9.43%	1.122%
7	6.588	798	807	815	rBV2	100064	306028	16.71%	1.988%
8	6.674	815	821	834	rVB4	91590	256989	14.03%	1.669%
9	7.203	897	908	918	rBV	335030	884359	48.28%	5.745%
10	7.854	1005	1015	1033	rBV2	664021	1831649	100.00%	11.898%
11	8.456	1106	1114	1125	rBV	670139	1236782	67.52%	8.034%
12	8.706	1147	1155	1163	rBV	860102	1647053	89.92%	10.699%
13	8.894	1177	1186	1198	rBV	418331	831791	45.41%	5.403%
14	9.679	1308	1315	1322	rBV	158910	261305	14.27%	1.697%
15	9.807	1331	1336	1343	rBV7	12037	29848	1.63%	0.194%
16	9.971	1354	1363	1369	rBV	990272	1560343	85.19%	10.135%
17	10.038	1369	1374	1379	rVB2	70195	123379	6.74%	0.801%
18	10.232	1401	1406	1413	rBV	83003	143131	7.81%	0.930%
19	10.385	1426	1431	1439	rBV5	13263	32490	1.77%	0.211%
20	10.591	1457	1465	1478	rBV	554578	911400	49.76%	5.920%
21	11.285	1570	1579	1587	rBV	932248	1353765	73.91%	8.794%
22	11.498	1609	1614	1617	rBV7	10514	19614	1.07%	0.127%
23	12.301	1740	1746	1751	rVB5	13226	24044	1.31%	0.156%
24	12.362	1751	1756	1762	rBV2	163434	237202	12.95%	1.541%
25	13.226	1890	1898	1903	rBV	574163	821266	44.84%	5.335%
26	13.512	1936	1945	1954	rBV	547933	788734	43.06%	5.123%


Sum of corrected areas: 15394843

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA R\DATA\VR022819\
Data File : VR026427.D
Acq On : 28 Feb 2019 19:35
Operator : SY/MD
Sample : K1588-14DL 5X
Misc : 25mL/MSVOA R/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampled :
C0AB2DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR022219WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

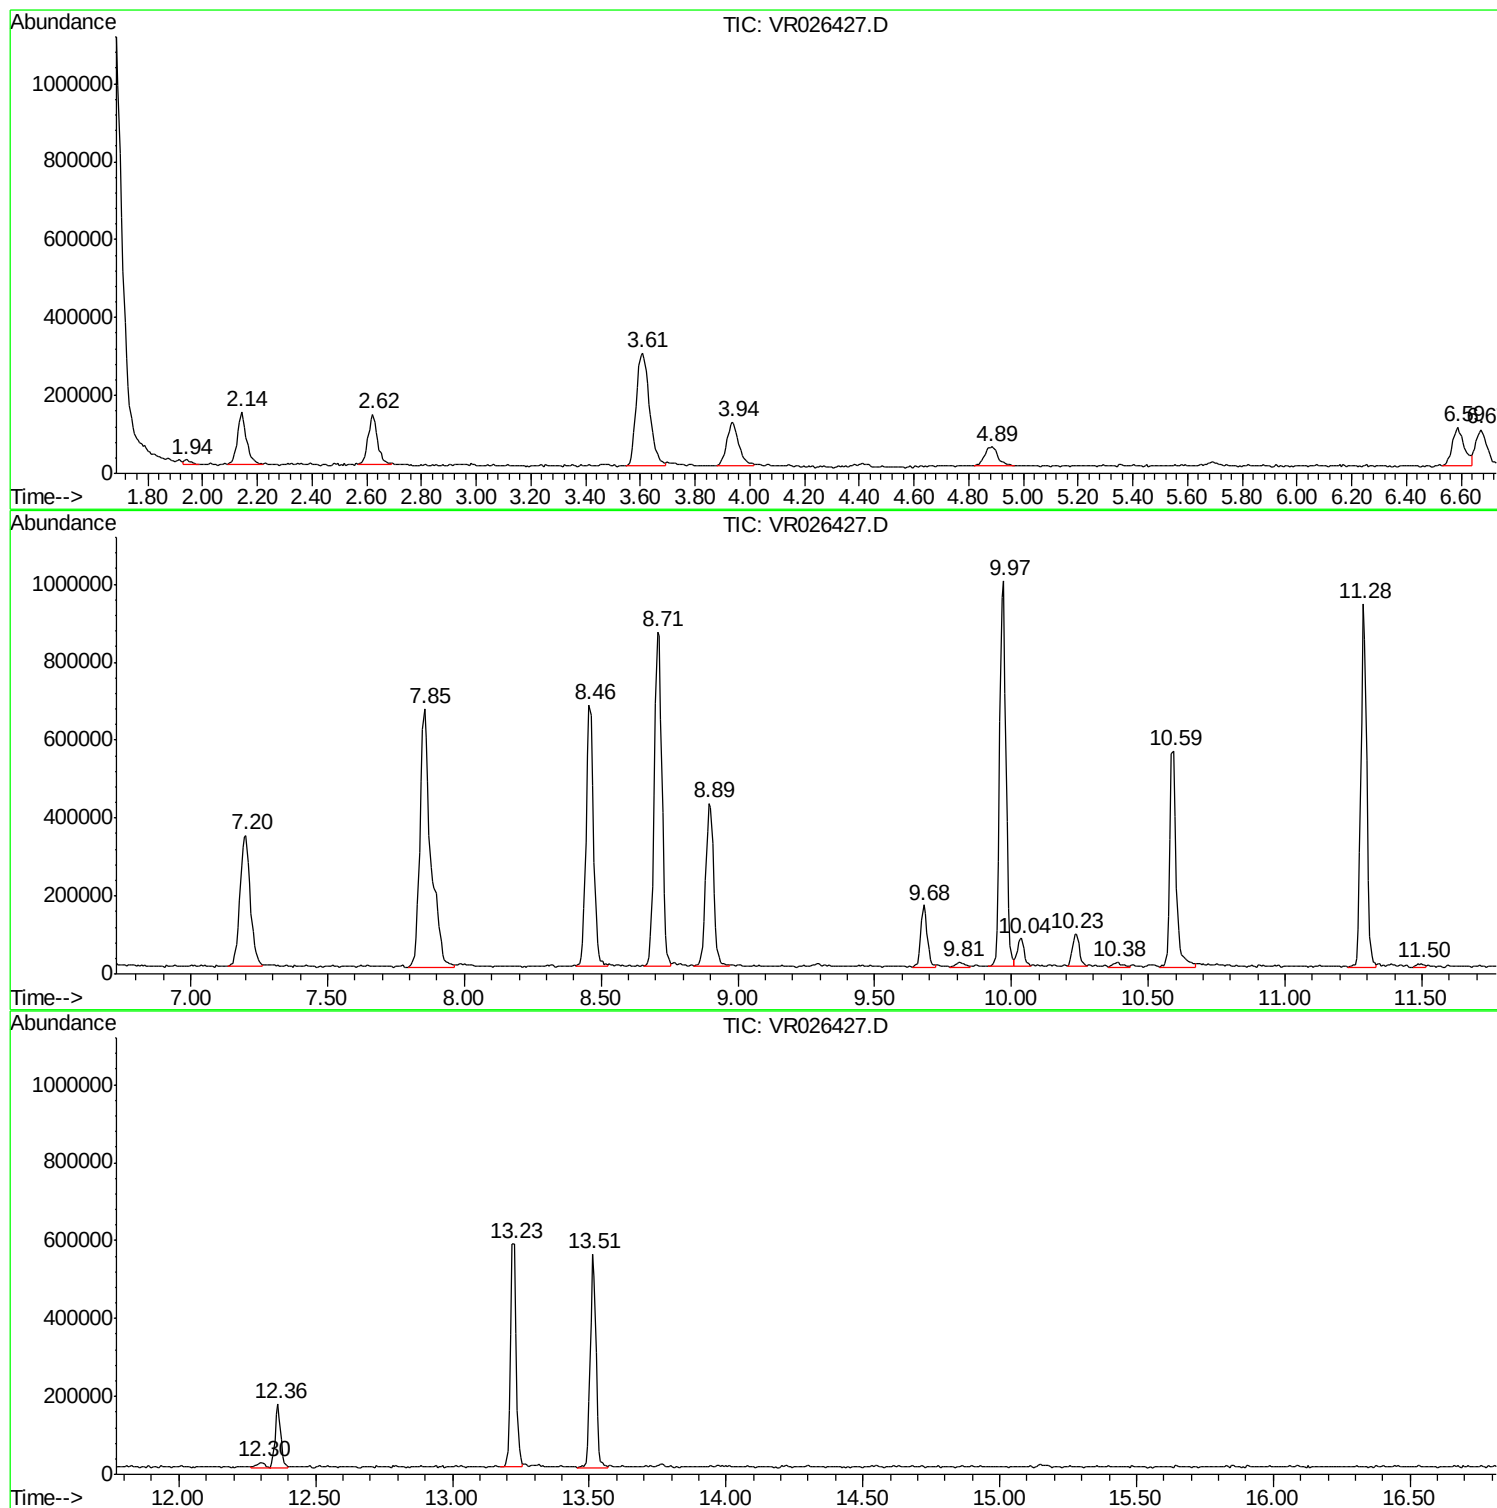

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA R\DATA\VR022819\
Data File : VR026427.D
Acq On : 28 Feb 2019 19:35
Operator : SY/MD
Sample : K1588-14DL 5X
Misc : 25mL/MSVOA R/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
C0AB2DL










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR022219WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.94	1.36 ug/L	335516	1,4-Difluorobenzene	8.46

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Isopropyl Alcohol	60	C3H8O	000067-63-0	64
2		Isopropyl Alcohol	60	C3H8O	000067-63-0	64
3		Isopropyl Alcohol	60	C3H8O	000067-63-0	50
4		2-Propanol, 1-bromo-	138	C3H7BrO	019686-73-8	38
5		2-Pentanol	88	C5H12O	006032-29-7	9

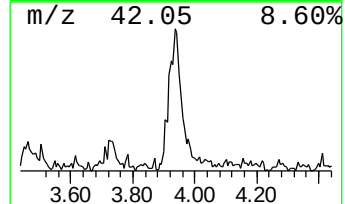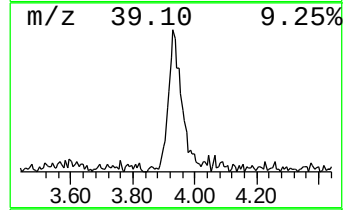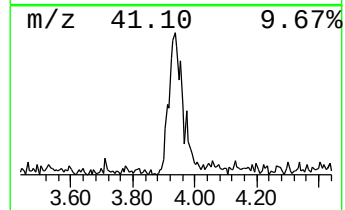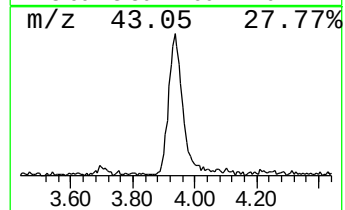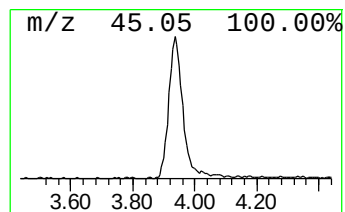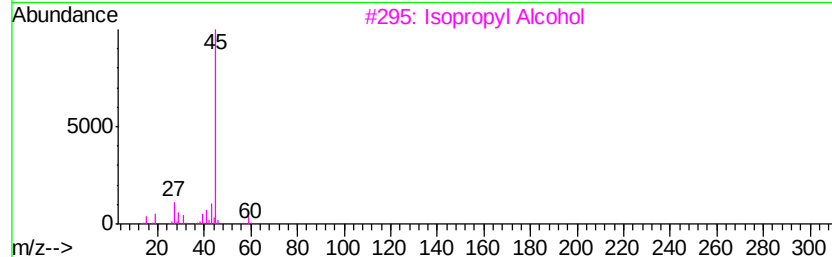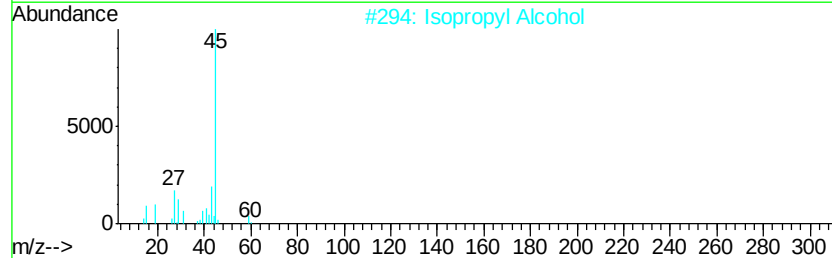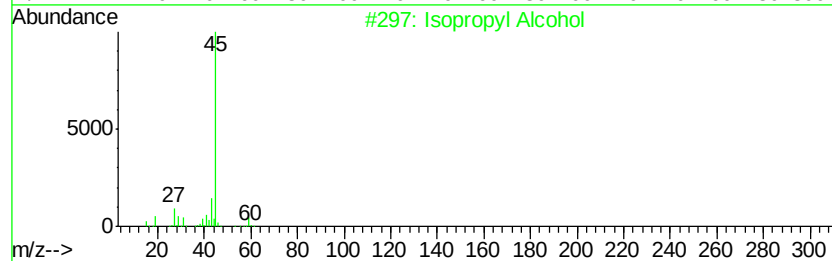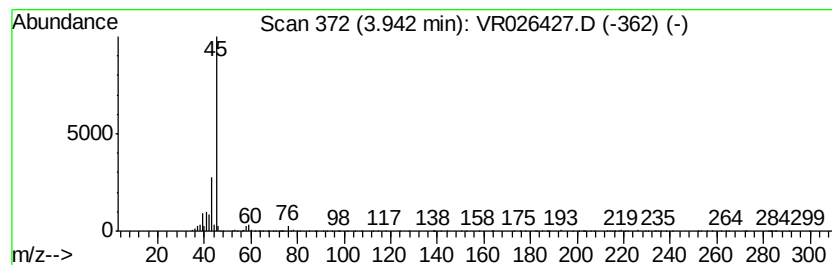

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_R\DATA\VR022819\
Data File : VR026427.D
Acq On : 28 Feb 2019 19:35
Operator : SY/MD
Sample : K1588-14DL 5X
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
C0AB2DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR022219WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	3.94	1.4	ug/L	335516	1	8.46	1236780	5.0