

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR062218\
 Data File : VR025412.D
 Acq On : 22 Jun 2018 13:54
 Operator : SY/MD
 Sample : J3674-11
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 DAZC3

Quant Time: Jun 22 22:58:25 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR061518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 22 22:38:28 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	572987	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	471471	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.22	152	160953	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.14	65	65189	3.34	ug/L	-0.01
Spiked Amount	5.000	Range	40 - 130	Recovery	=	66.80%
7) Chloroethane-d5	2.64	69	52266	3.64	ug/L	0.01
Spiked Amount	5.000	Range	65 - 130	Recovery	=	72.80%
11) 1,1-Dichloroethene-d2	3.65	63	133347	2.66	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	53.20%#
20) 2-Butanone-d5	6.60	46	281805	53.87	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.74%
24) Chloroform-d	7.20	84	325074	4.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.20%
26) 1,2-Dichloroethane-d4	7.89	65	136615	4.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.00%
32) Benzene-d6	7.86	84	653348	4.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.80%
36) 1,2-Dichloropropane-d6	8.90	67	204851	4.51	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.20%
41) Toluene-d8	9.97	98	545393	3.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.20%
43) trans-1,3-Dichloropropene-	10.24	79	43387	3.59	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	71.80%
46) 2-Hexanone-d5	10.59	63	228947	54.58	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	109.16%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	96082	5.44	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	108.80%
64) 1,2-Dichlorobenzene-d4	13.51	152	136887	5.01	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.20%


Target Compounds					Ovalue
13) Acetone	3.71	43	9760	4.13 ug/L	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA R\DATA\VR062218\
Data File : VR025412.D
Acq On : 22 Jun 2018 13:54
Operator : SY/MD
Sample : J3674-11
Misc : 25mL/MSVOA R/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
DAZC3

Quant Time: Jun 22 22:58:25 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR061518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 22 22:38:28 2018
Response via : Initial Calibration

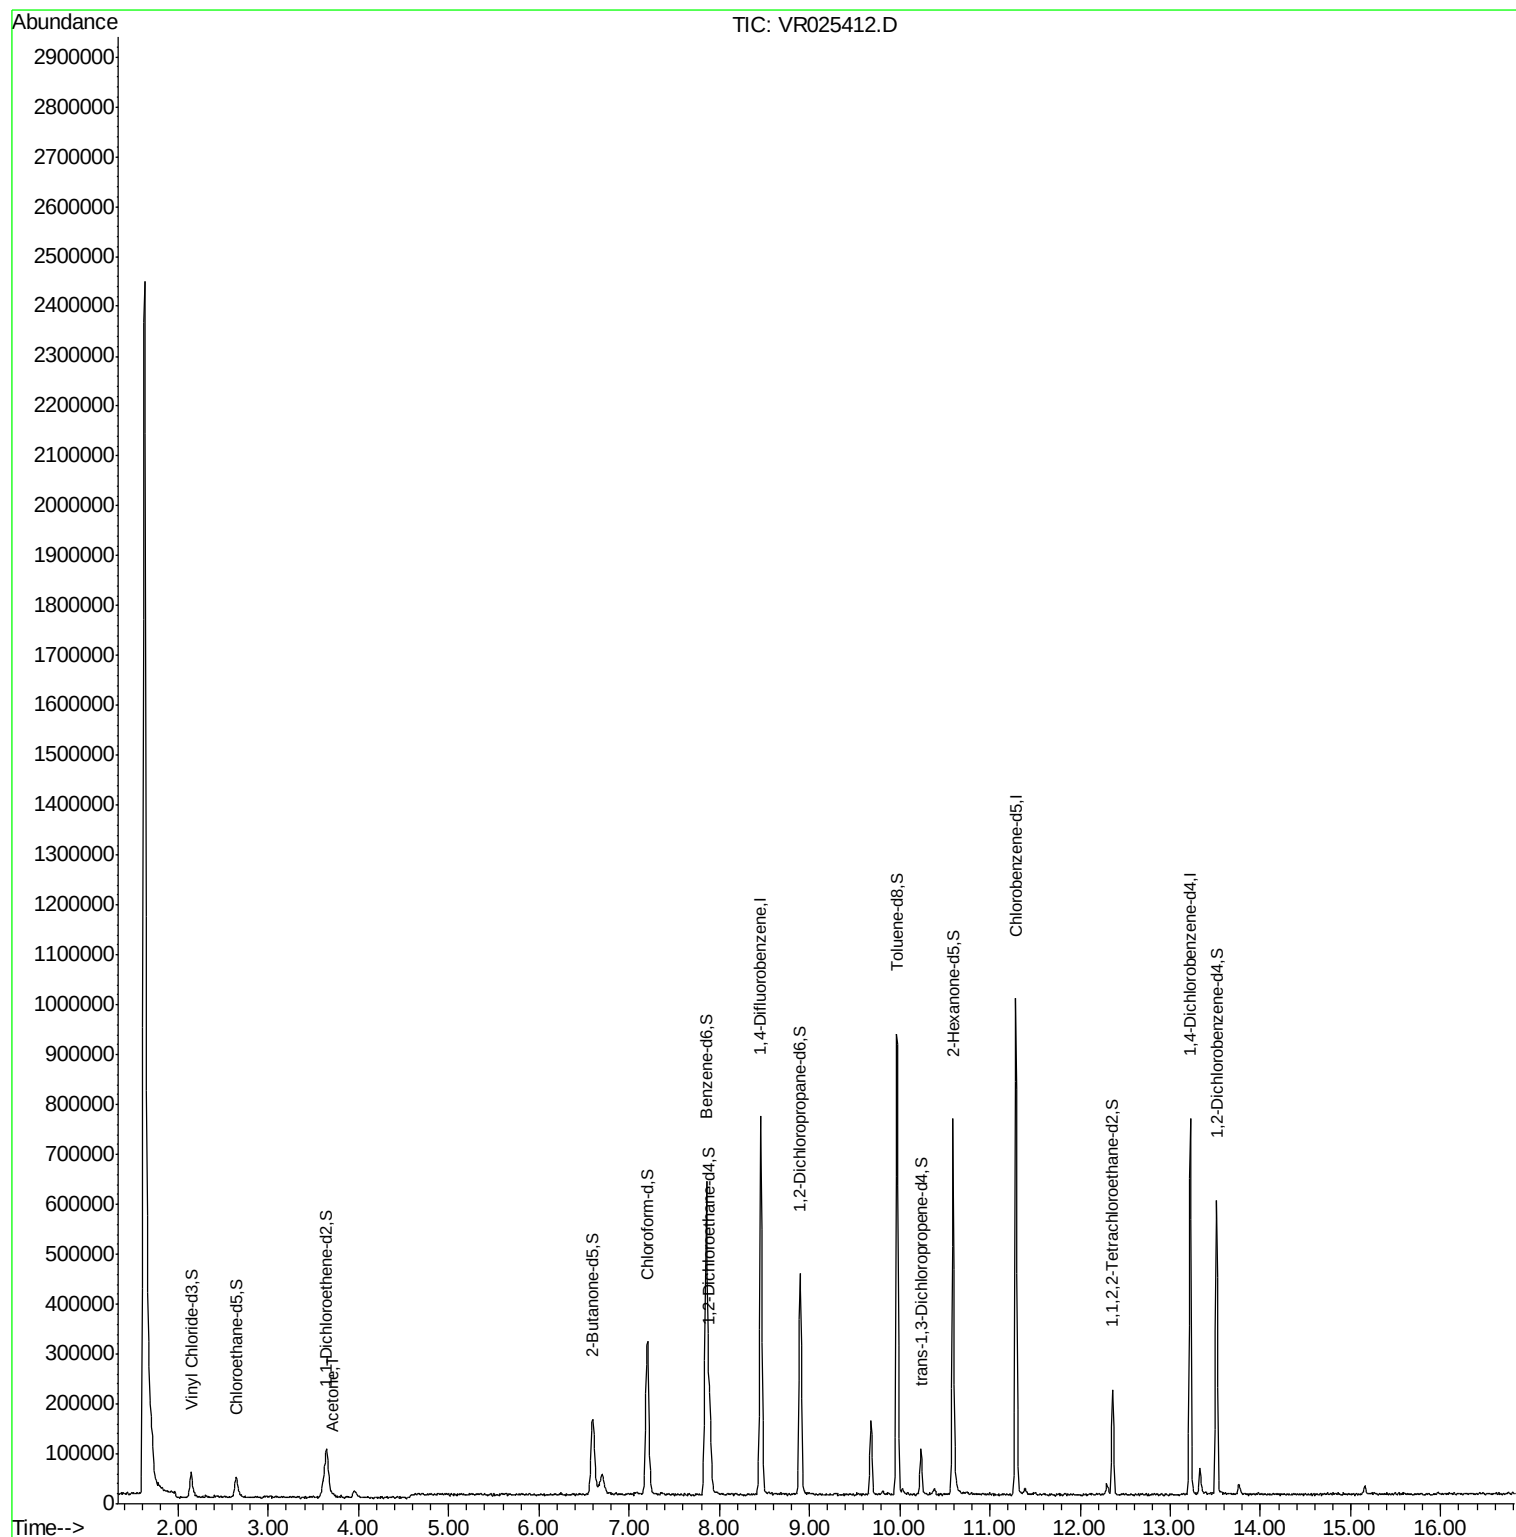

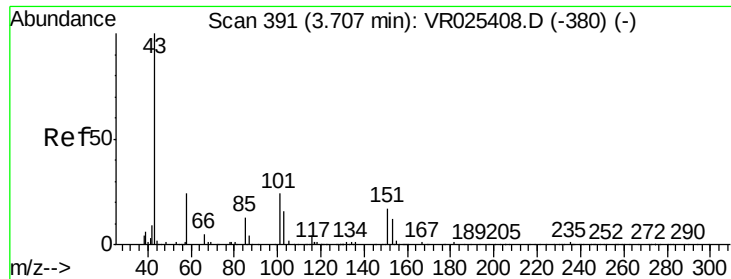

#13

Acetone

Concen: 4.13 ug/L

RT: 3.71 min Scan# 392

Delta R.T. 0.01 min

Lab File: VR025412.D

Acq: 22 Jun 2018 13:54

Instrument :
MSVOA_R
ClientSampleId :
DAZC3

Tot Ion: 43 Resp: 9760

Ion Ratio Lower Upper

43 100

58 7.4 0.0 41.6

