

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR071718\
 Data File : VR025497.D
 Acq On : 17 Jul 2018 17:47
 Operator : SY/MD
 Sample : J4002-05
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 C0AG3

Quant Time: Jul 18 02:30:37 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR070518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Jul 18 01:02:47 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	738109	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	590285	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.22	152	215043	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.15	65	97529	4.79	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.80%
7) Chloroethane-d5	2.64	69	75492	4.35	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.00%
11) 1,1-Dichloroethene-d2	3.63	63	200287	3.25	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.00%
20) 2-Butanone-d5	6.60	46	270321	42.77	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	85.54%
24) Chloroform-d	7.21	84	428441	4.26	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.20%
26) 1,2-Dichloroethane-d4	7.89	65	176916	4.59	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.80%
32) Benzene-d6	7.86	84	917402	4.65	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.00%
36) 1,2-Dichloropropane-d6	8.90	67	261192	4.56	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.20%
41) Toluene-d8	9.97	98	822010	4.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.80%
43) trans-1,3-Dichloropropene-	10.24	79	66274	4.36	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.20%
46) 2-Hexanone-d5	10.59	63	252621	51.48	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.96%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	111042	4.33	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.60%
64) 1,2-Dichlorobenzene-d4	13.51	152	180703	5.09	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.80%


Target Compounds					Ovalue
22) cis-1,2-Dichloroethene	6.68	96	122836	2.44 ug/L	99
34) Trichloroethene	8.71	95	649624	12.54 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA R\DATA\VR071718\
Data File : VR025497.D
Acq On : 17 Jul 2018 17:47
Operator : SY/MD
Sample : J4002-05
Misc : 25mL/MSVOA R/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
C0AG3

Quant Time: Jul 18 02:30:37 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR070518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jul 18 01:02:47 2018
Response via : Initial Calibration

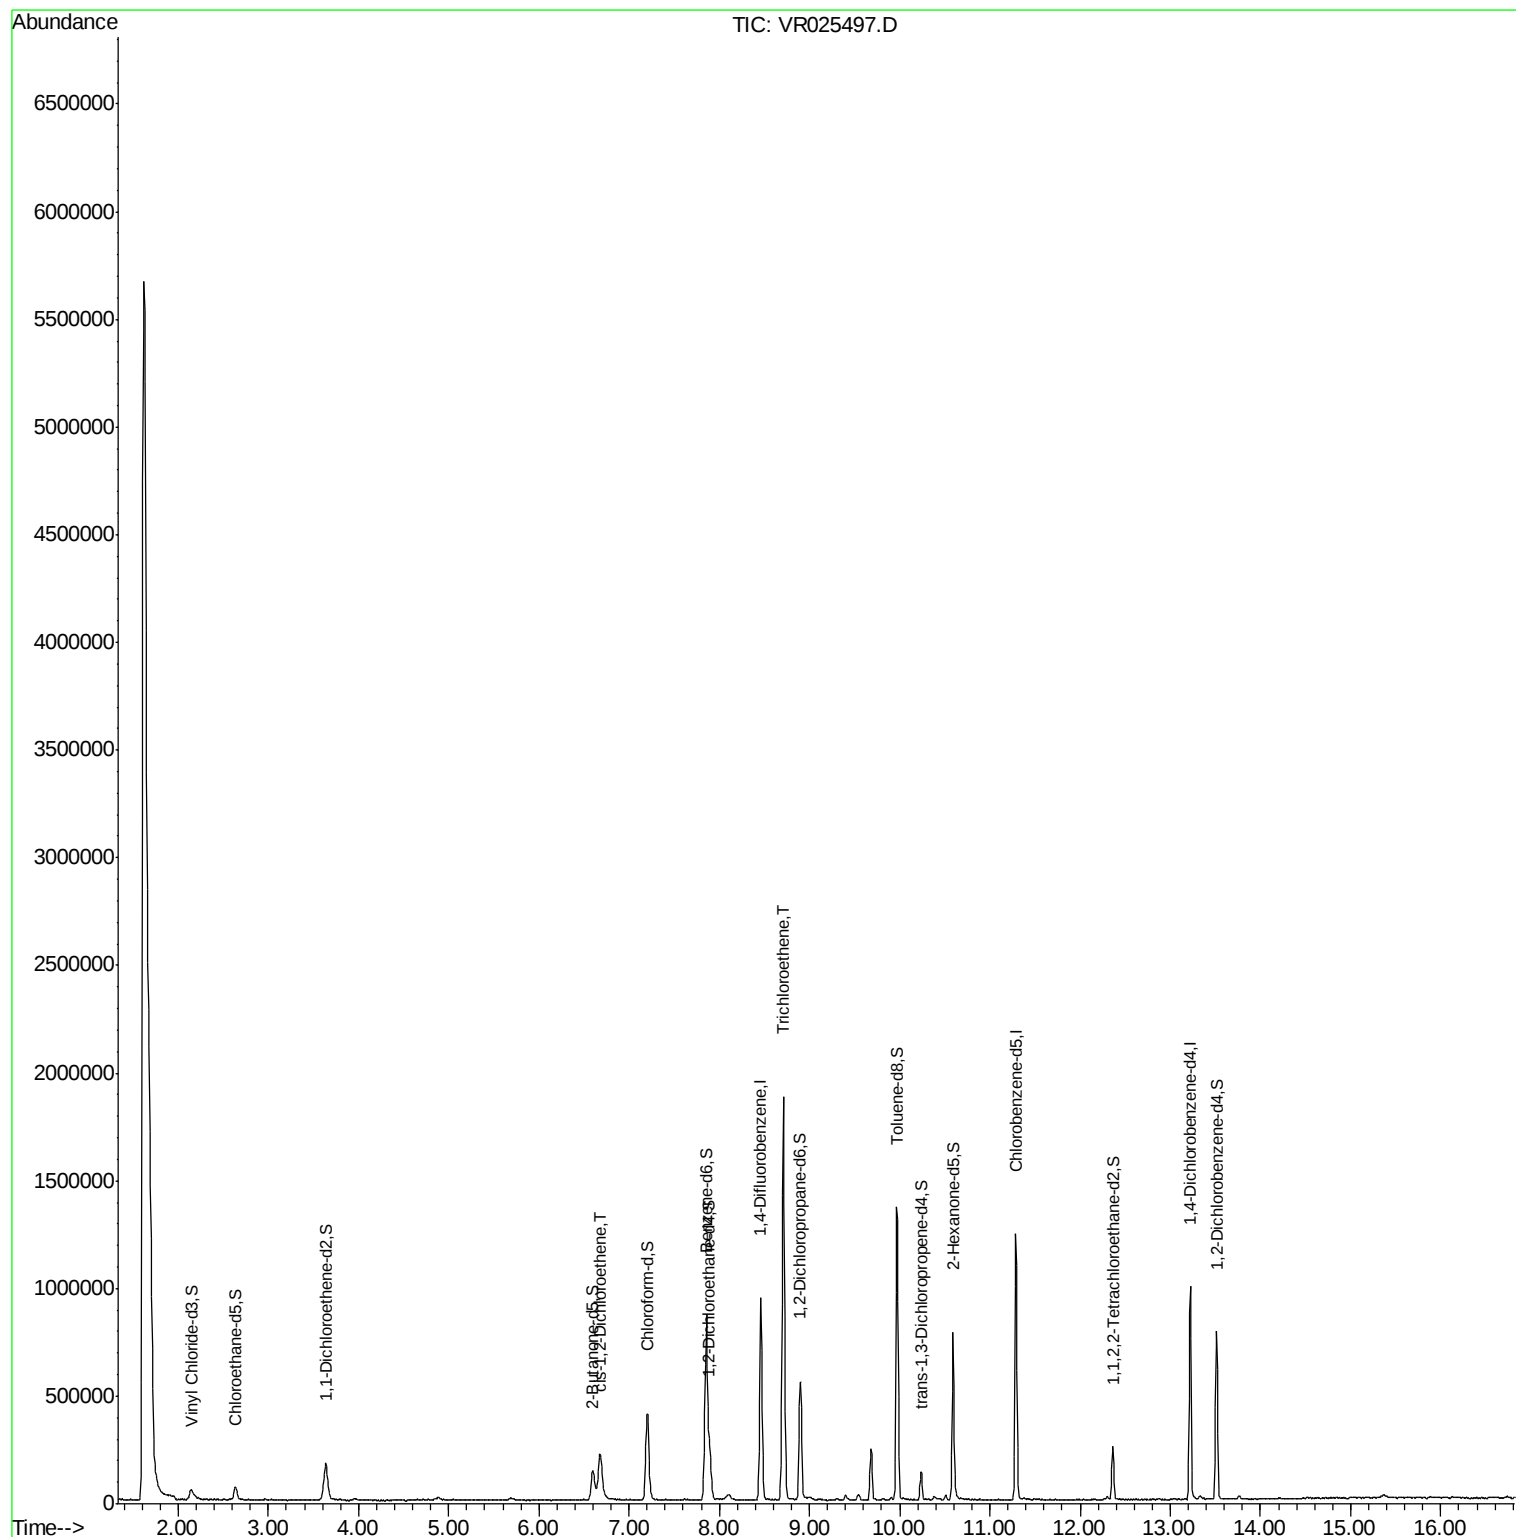

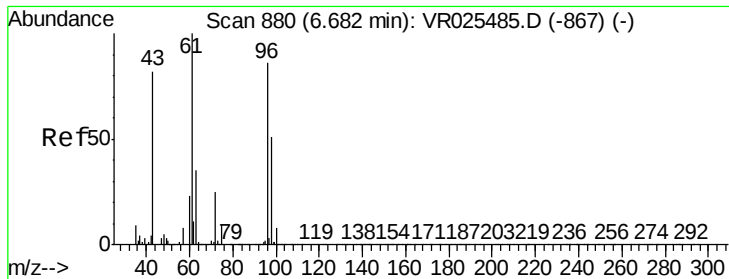

#22

cis-1,2-Dichloroethene

Concen: 2.44 ug/L

RT: 6.68 min Scan# 879

Delta R.T. -0.01 min

Lab File: VR025497.D

Acq: 17 Jul 2018 17:47

Instrument :

MSVOA_R

ClientSampleId :

C0AG3


Tot Ion: 96 Resp: 122836

Ion Ratio Lower Upper

96 100

61 131.0 91.0 169.0




68 0.0 0.0 0.0

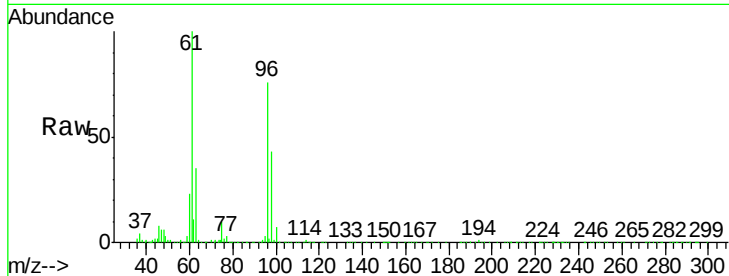

Abundance Ion 96.00 (95.70 to 96.70): VR0

Ion 61.05 (60.75 to 61.75): VR0

Ion 68.15 (67.85 to 68.85): VR0

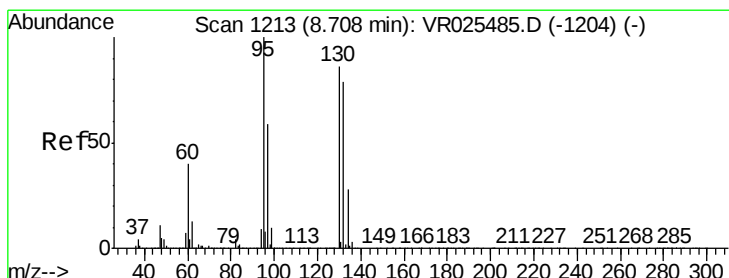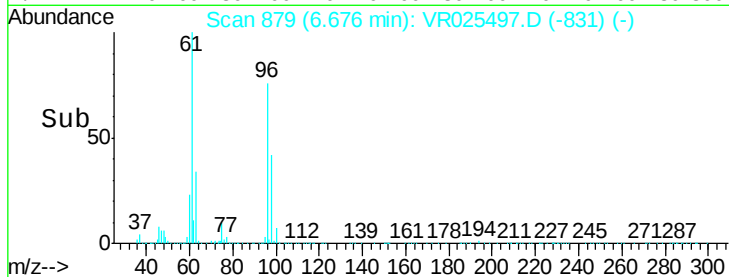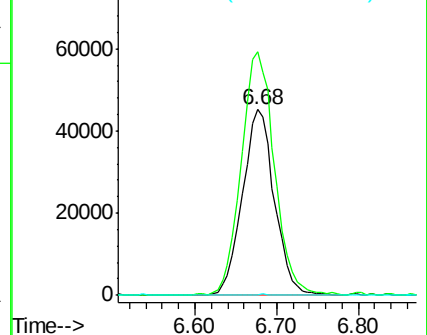

#34

Trichloroethene

Concen: 12.54 ug/L

RT: 8.71 min Scan# 1214

Delta R.T. 0.01 min

Lab File: VR025497.D

Acq: 17 Jul 2018 17:47

Tgt Ion: 95 Resp: 649624


Ion Ratio Lower Upper

95 100

97 64.5 45.6 84.6

132 88.6 60.9 113.1

130 90.5 62.0 115.2

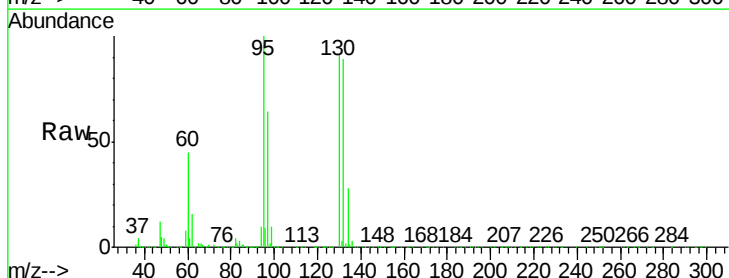

Abundance Ion 95.00 (94.70 to 95.70): VR0

Ion 96.95 (96.65 to 97.65): VR0

Ion 131.95 (131.65 to 132.65): V

Ion 129.95 (129.65 to 130.65): V

