

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR071818\
 Data File : VR025507.D
 Acq On : 18 Jul 2018 15:23
 Operator : SY/MD
 Sample : J4002-02
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 C0AF4

Quant Time: Jul 19 05:43:44 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR070518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jul 19 05:17:34 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	640534	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	525954	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.22	152	170022	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.14	65	74277	4.21	ug/L	-0.01
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.20%
7) Chloroethane-d5	2.63	69	61138	4.06	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	81.20%
11) 1,1-Dichloroethene-d2	3.64	63	170514	3.19	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.80%
20) 2-Butanone-d5	6.60	46	220436	40.19	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	80.38%
24) Chloroform-d	7.21	84	374116	4.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.60%
26) 1,2-Dichloroethane-d4	7.90	65	148599	4.44	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.80%
32) Benzene-d6	7.86	84	781357	4.44	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.80%
36) 1,2-Dichloropropane-d6	8.90	67	223443	4.38	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	87.60%
41) Toluene-d8	9.97	98	703279	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.00%
43) trans-1,3-Dichloropropene-	10.24	79	51824	3.83	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.60%
46) 2-Hexanone-d5	10.59	63	210551	48.16	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.32%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	97813	4.28	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	85.60%
64) 1,2-Dichlorobenzene-d4	13.51	152	154605	5.51	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.20%


Target Compounds					Ovalue
19) 1,1-Dichloroethane	5.69	63	50109	0.61 ug/L	# 85
22) cis-1,2-Dichloroethene	6.68	96	189228	4.33 ug/L	# 99
25) Chloroform	7.24	83	53587	0.68 ug/L	95
34) Trichloroethene	8.71	95	73253	1.59 ug/L	94
47) Tetrachloroethene	10.52	164	130417	4.33 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA R\DATA\VR071818\
Data File : VR025507.D
Acq On : 18 Jul 2018 15:23
Operator : SY/MD
Sample : J4002-02
Misc : 25mL/MSVOA R/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
C0AF4

Quant Time: Jul 19 05:43:44 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR070518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jul 19 05:17:34 2018
Response via : Initial Calibration

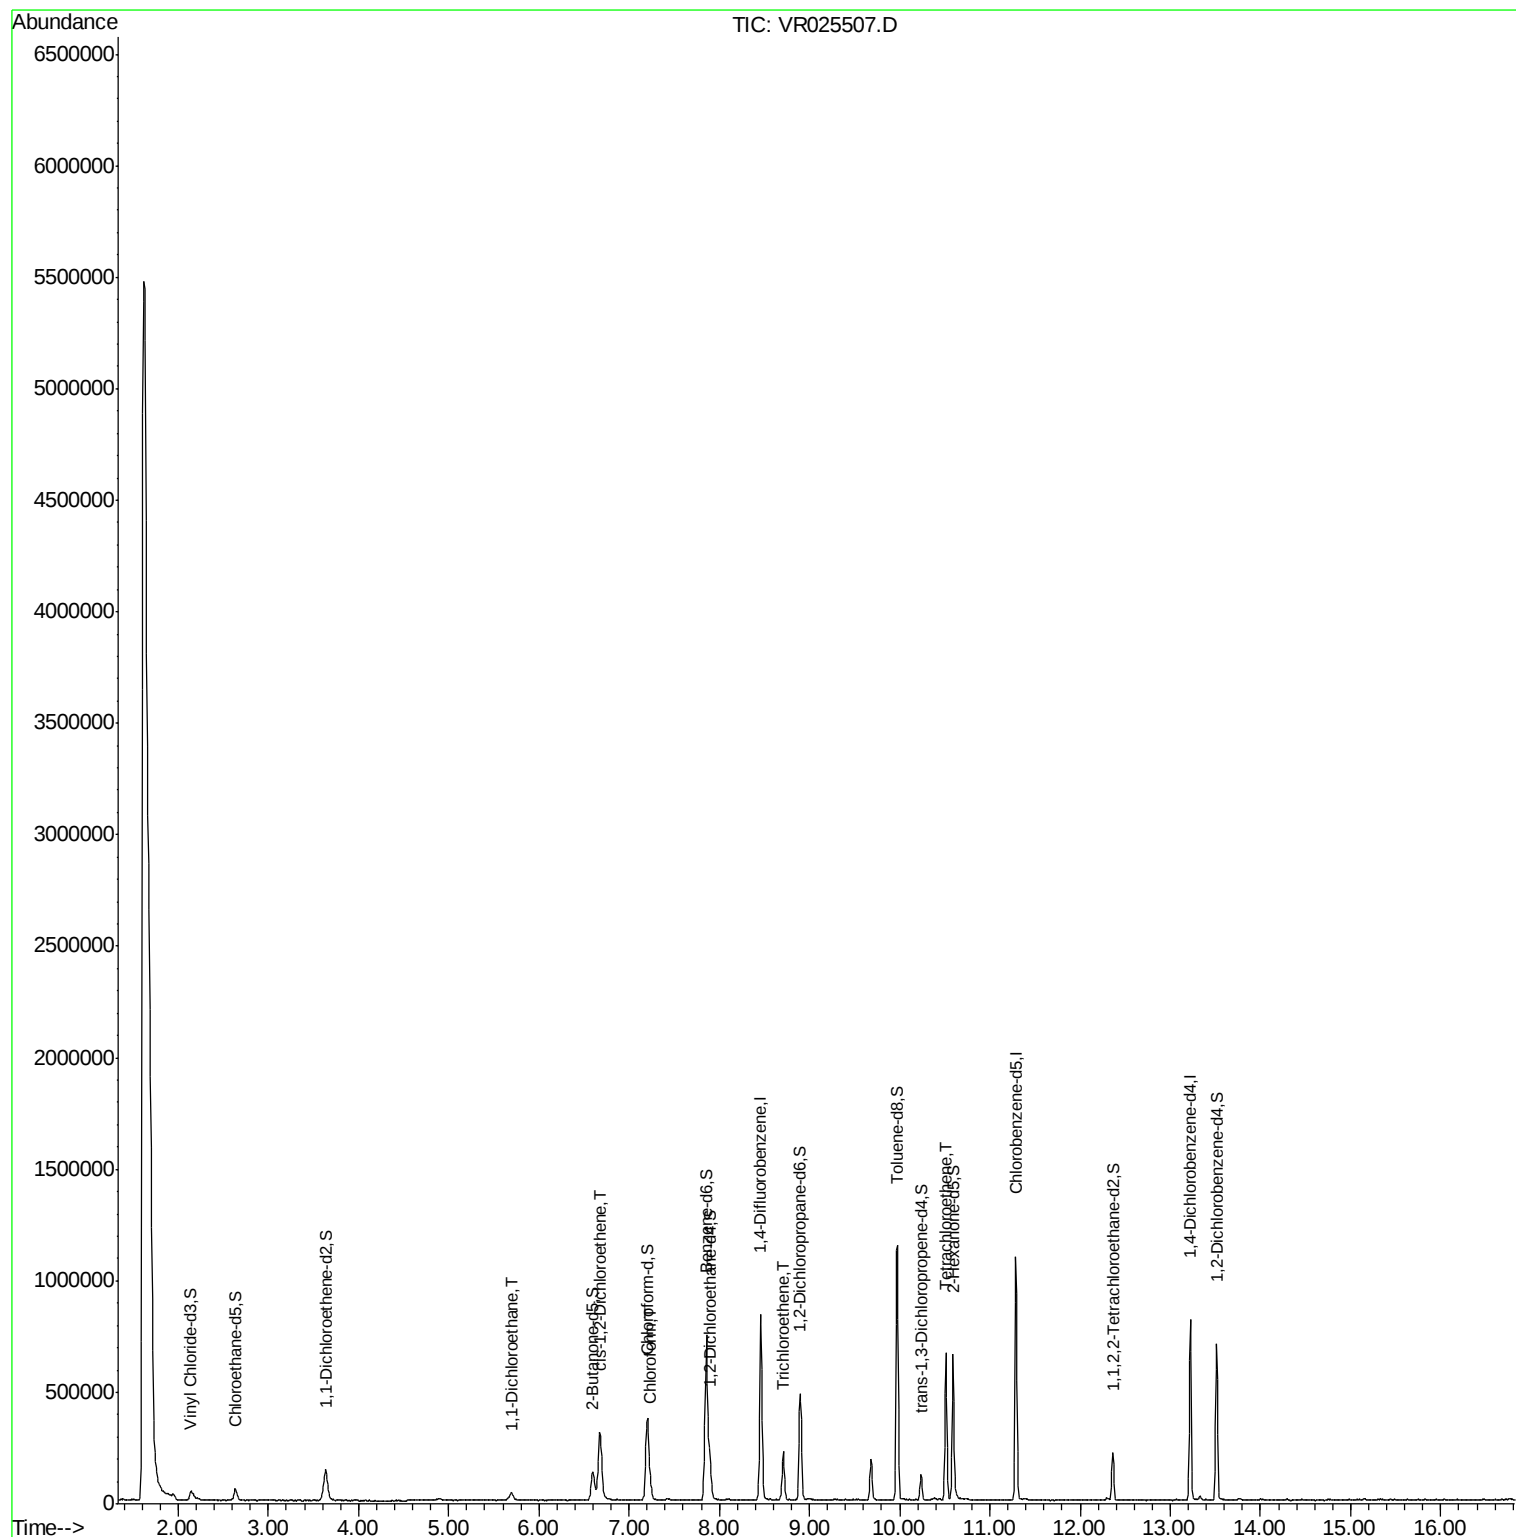

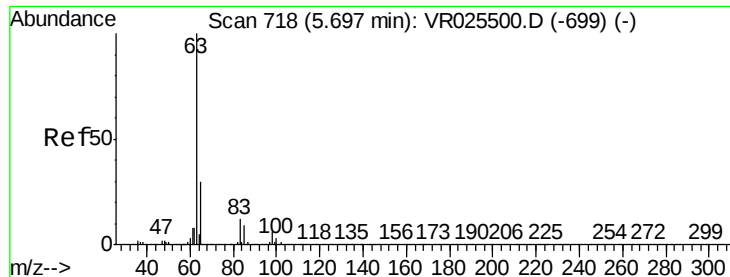

#19

1,1-Dichloroethane

Concen: 0.61 ug/L

RT: 5.69 min Scan# 717

Delta R.T. -0.01 min

Lab File: VR025507.D

Acq: 18 Jul 2018 15:23

Instrument :

MSVOA_R

ClientSampleId :

C0AF4


Tot Ion: 63 Resp: 50109

Ion Ratio Lower Upper

63 100

65 20.9 22.5 41.7#




83 12.2 9.5 17.7

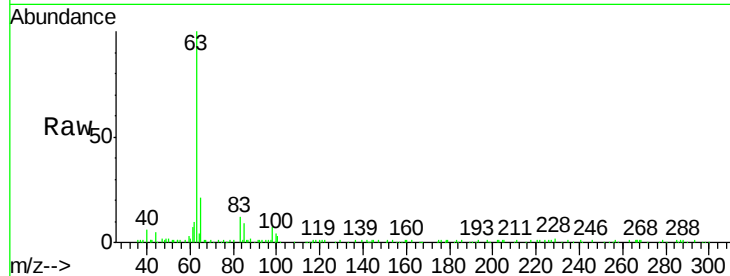

Abundance Ion 63.10 (62.80 to 63.80): VR0

Ion 65.10 (64.80 to 65.80): VR0

Ion 83.05 (82.75 to 83.75): VR0

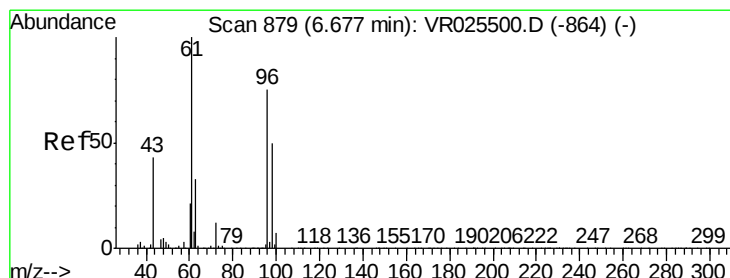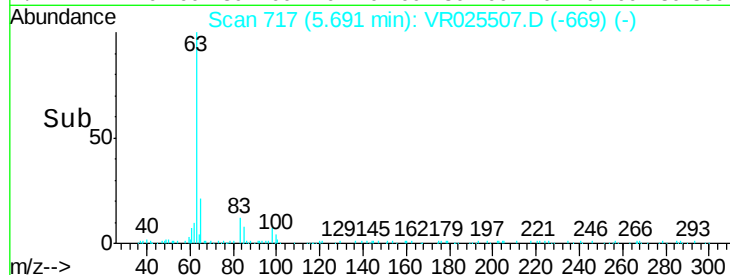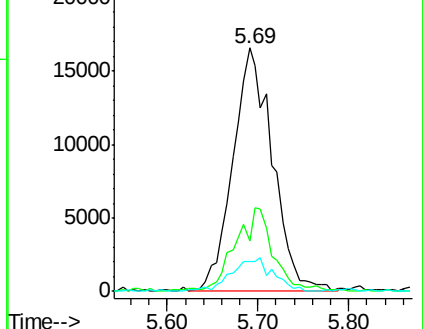

#22

cis-1,2-Dichloroethene

Concen: 4.33 ug/L

RT: 6.68 min Scan# 880

Delta R.T. 0.01 min

Lab File: VR025507.D

Acq: 18 Jul 2018 15:23


Tgt Ion: 96 Resp: 189228

Ion Ratio Lower Upper

96 100

61 130.7 91.0 169.0



68 0.1 0.0 0.0#

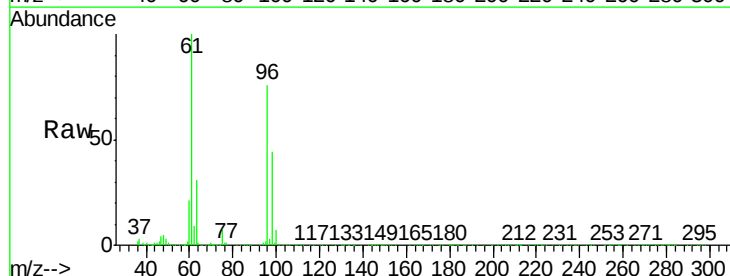


Abundance Ion 96.00 (95.70 to 96.70): VR0

Ion 61.05 (60.75 to 61.75): VR0

Ion 68.15 (67.85 to 68.85): VR0

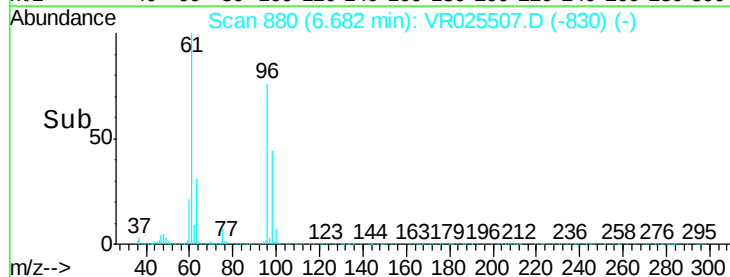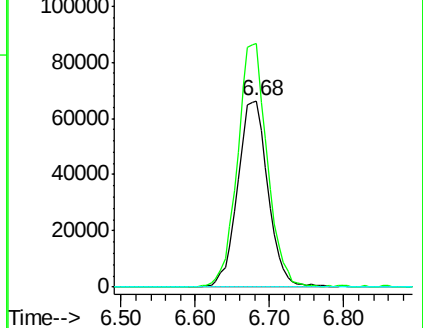

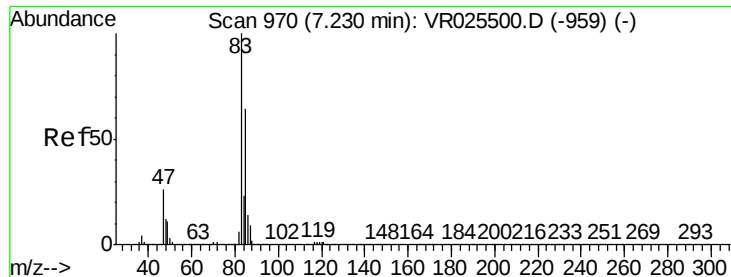

#25

Chloroform

Concen: 0.68 ug/L

RT: 7.24 min Scan# 971

Delta R.T. 0.01 min

Lab File: VR025507.D

Acq: 18 Jul 2018 15:23

Instrument :

MSVOA_R

ClientSampleId :





C0AF4

Tot Ion: 83 Resp: 53587

Ion Ratio Lower Upper

83 100

85 60.7 45.4 84.4

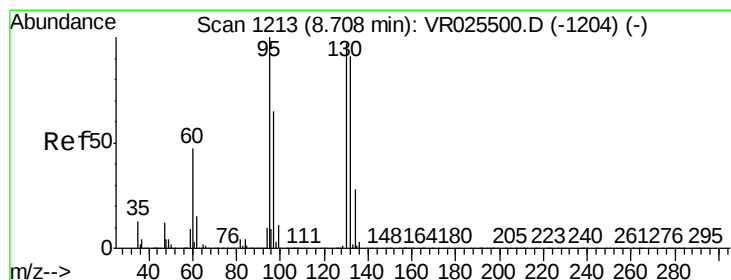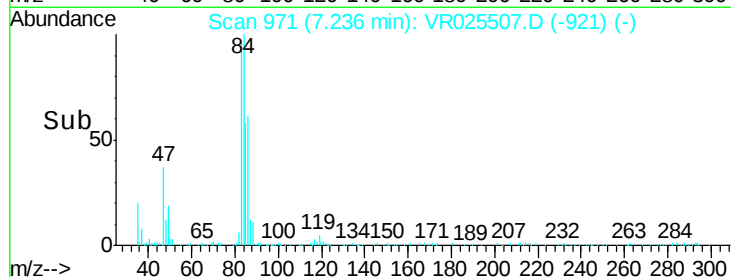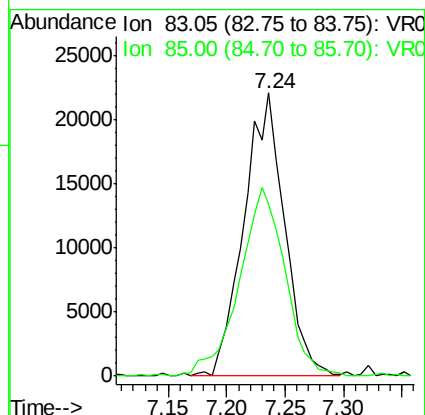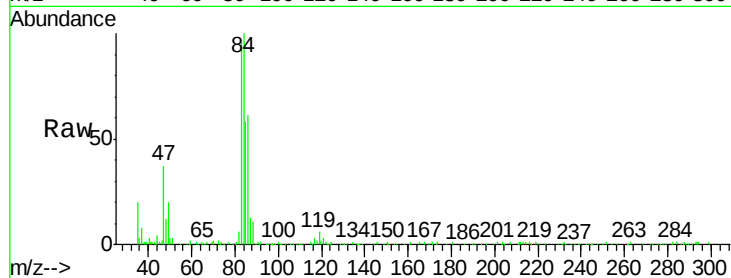

#34

Trichloroethene

Concen: 1.59 ug/L

RT: 8.71 min Scan# 1213

Delta R.T. -0.00 min

Lab File: VR025507.D

Acq: 18 Jul 2018 15:23

Tgt Ion: 95 Resp: 73253




Ion Ratio Lower Upper


95 100

97 67.3 45.6 84.6

132 92.0 60.9 113.1

130 97.1 62.0 115.2

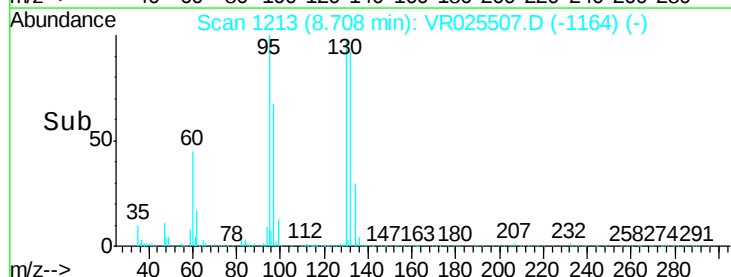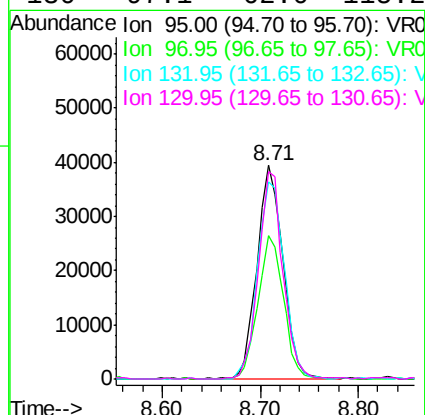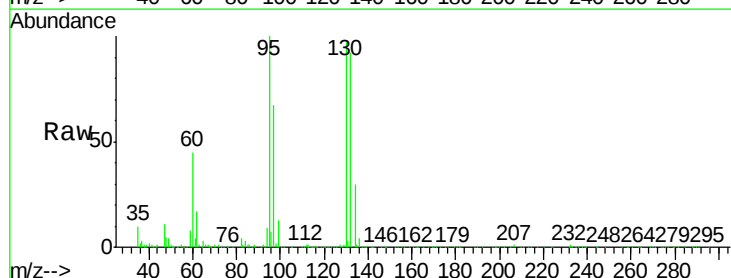

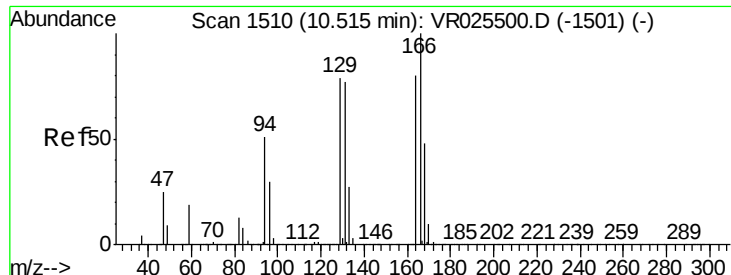

#47

Tetrachloroethene

Concen: 4.33 ug/L

RT: 10.52 min Scan# 1510

Delta R.T. -0.00 min

Lab File: VR025507.D


Acq: 18 Jul 2018 15:23

Instrument :

MSVOA_R

ClientSampleId :

C0AF4

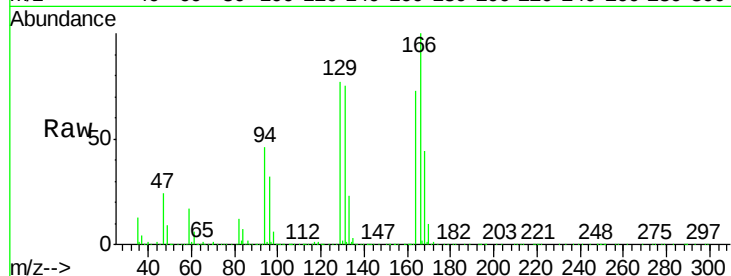

Tot Ion:164 Resp: 130417

Ion Ratio Lower Upper

164 100

129 104.8 68.1 126.5

131 101.8 68.5 127.1

166 136.2 89.9 166.9

Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

