

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR080618\
Data File : VR025566.D
Acq On : 6 Aug 2018 22:00
Operator : SY/MD
Sample : VSTCCC005EC
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_R
LabSampleId :
VSTD00591

Manual Integrations
APPROVED

MMDadoda
8/8/2018 1:10:39 PM

Quant Time: Aug 07 00:48:40 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR073018WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Aug 06 23:40:46 2018
Response via : Initial Calibration

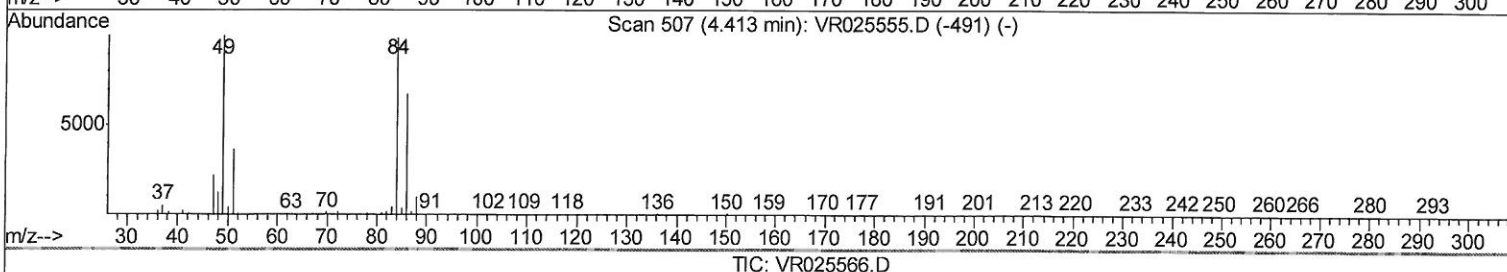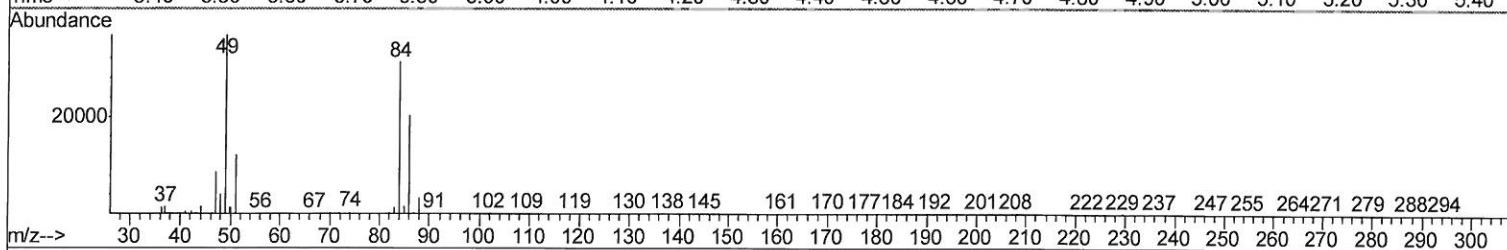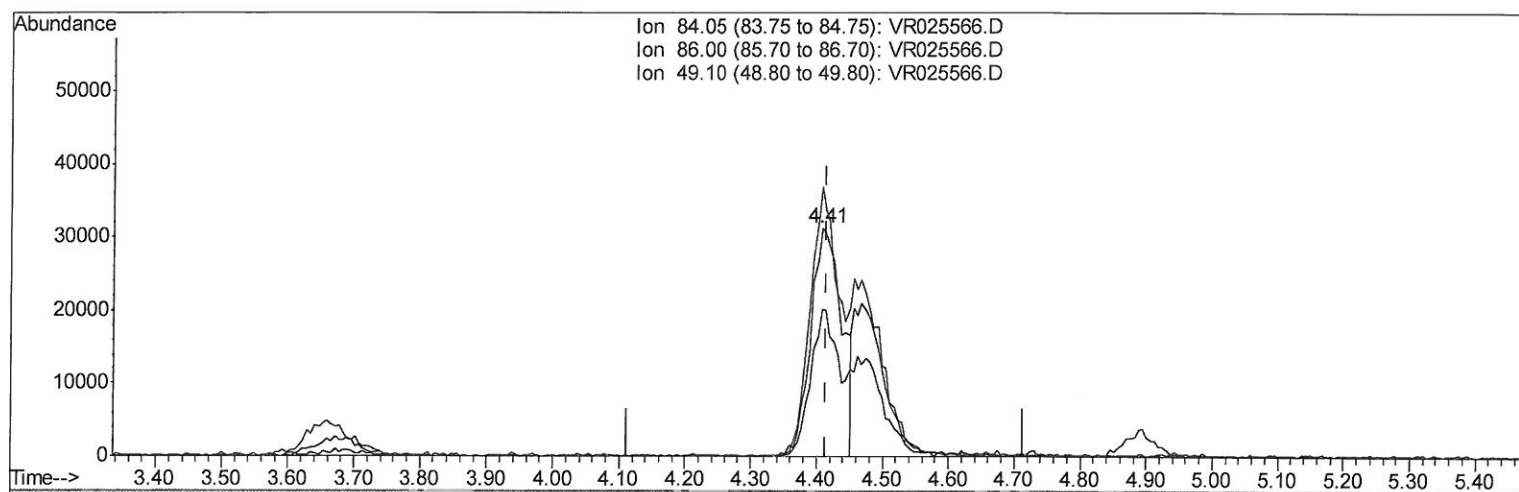

(16) Methylene chloride (T)

4.407min (-0.006) 2.95ug/L

response 101156

Ion	Exp%	Act%
84.05	100	100
86.00	57.70	64.52
49.10	108.80	118.07
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR080618\
 Data File : VR025566.D
 Acq On : 6 Aug 2018 22:00
 Operator : SY/MD
 Sample : VSTCCC005EC
 Misc : 25mL/MSVOA_R/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_R
 LabSampled :
 VSTD00591

Manual Integrations
 APPROVED

MMDadoda
 8/8/2018 1:10:39 PM

Quant Time: Aug 07 00:48:40 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR073018WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Aug 06 23:40:46 2018
 Response via : Initial Calibration

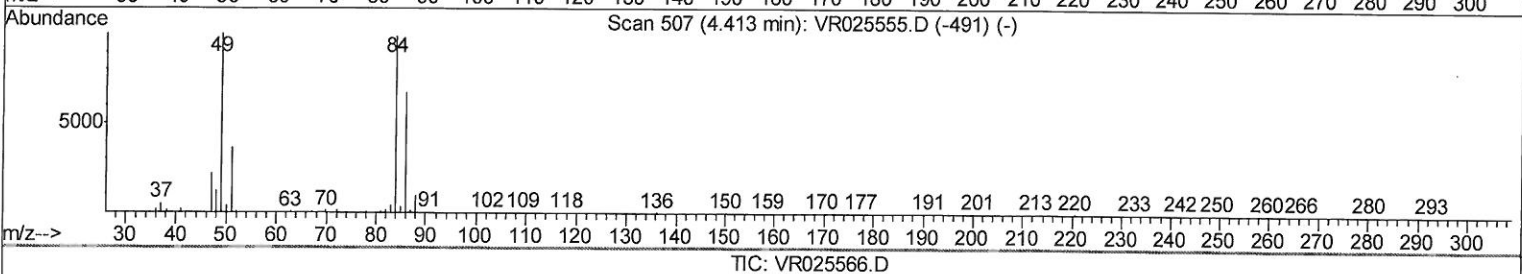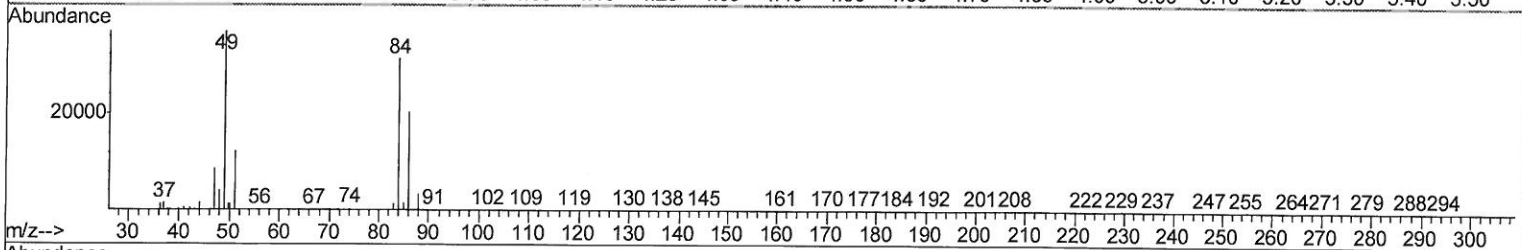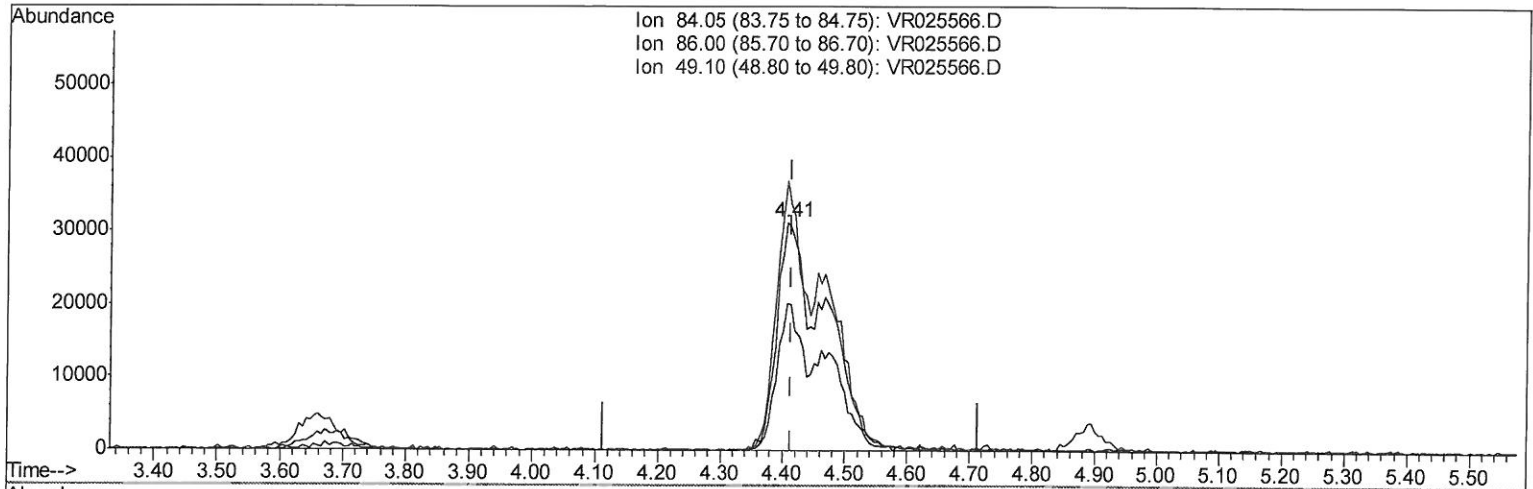

(16) Methylene chloride (T)

4.407min (-0.006) 4.90ug/L m

response 167889

Ion	Exp%	Act%
84.05	100	100
86.00	57.70	64.52
49.10	108.80	118.07
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR080618\
 Data File : VR025566.D
 Acq On : 6 Aug 2018 22:00
 Operator : SY/MD
 Sample : VSTCCC005EC
 Misc : 25mL/MSVOA_R/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_R
 LabSampleId :
 VSTD00591

Manual Integrations
 APPROVED

MMDadoda
 8/8/2018 1:10:39 PM

Quant Time: Aug 07 00:49:12 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR073018WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Aug 06 23:40:46 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.47	114	567777	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	502826	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.22	152	227785	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.14	65	148347	4.21	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	84.20%		
7) Chloroethane-d5	2.64	69	105358	3.80	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	76.00%		
11) 1,1-Dichloroethene-d2	3.65	63	370907	4.56	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	91.20%		
20) 2-Butanone-d5	6.60	46	153819	52.90	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	105.80%		
24) Chloroform-d	7.21	84	281883	4.82	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	96.40%		
26) 1,2-Dichloroethane-d4	7.90	65	101718	5.13	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	102.60%		
32) Benzene-d6	7.86	84	639330	4.74	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	94.80%		
36) 1,2-Dichloropropane-d6	8.90	67	171092	4.83	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	96.60%		
41) Toluene-d8	9.97	98	637079	4.80	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	96.00%		
43) trans-1,3-Dichloropropene-	10.24	79	40896	4.51	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	90.20%		
46) 2-Hexanone-d5	10.59	63	169004	58.41	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	116.82%		
57) 1,1,2,2-Tetrachloroethane-	12.36	84	89803	5.61	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	112.20%		
64) 1,2-Dichlorobenzene-d4	13.51	152	165746	4.76	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	95.20%		

Target Compounds

					Qvalue
2) Dichlorodifluoromethane	1.83	85	161631	4.973	ug/L 99
3) Chloromethane	2.02	50	216283	5.038	ug/L 99
5) Vinyl chloride	2.16	62	206568	4.815	ug/L 98
6) Bromomethane	2.53	94	90005	3.815	ug/L 90
8) Chloroethane	2.67	64	96933	4.068	ug/L 99
9) Trichlorofluoromethane	2.98	101	312063	5.325	ug/L # 28
10) 1,1,2-Trichloro-1,2,2-trif	3.68	101	179689	4.745	ug/L 97
12) 1,1-Dichloroethene	3.67	96	201880	4.978	ug/L 88
13) Acetone	3.71	43	122076	49.945	ug/L 99
14) Carbon disulfide	3.97	76	418784	4.458	ug/L 99
15) Methyl Acetate	4.21	43	36416	4.719	ug/L 97
16) Methylene chloride	4.41	84	167889m	4.902	ug/L 99
17) Methyl tert-butyl Ether	4.91	73	202252	4.968	ug/L 99
18) trans-1,2-Dichloroethene	4.89	96	195898	5.044	ug/L 96
19) 1,1-Dichloroethane	5.70	63	282624	4.973	ug/L 96
21) 2-Butanone	6.70	43	199993	58.895	ug/L 98
22) cis-1,2-Dichloroethene	6.68	96	187820	5.294	ug/L # 97

08/03/18 Sy

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR080618\
 Data File : VR025566.D
 Acq On : 6 Aug 2018 22:00
 Operator : SY/MD
 Sample : VSTCCC005EC
 Misc : 25mL/MSVOA_R/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_R
 LabSampleId :
 VSTD00591

Manual Integrations
 APPROVED

MMDadoda
 8/8/2018 1:10:39 PM

Quant Time: Aug 07 00:49:12 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR073018WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Aug 06 23:40:46 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
23) Bromochloromethane	7.05	128	63247	5.374	ug/L	91
25) Chloroform	7.24	83	289264	5.141	ug/L	99
27) 1,2-Dichloroethane	8.00	62	119486	5.329	ug/L #	88
29) 1,1,1-Trichloroethane	7.44	97	200128	4.494	ug/L	99
30) Cyclohexane	7.52	56	254253	4.956	ug/L	99
31) Carbon tetrachloride	7.64	117	210248	4.574	ug/L	100
33) Benzene	7.91	78	764902	4.924	ug/L	100
34) Trichloroethene	8.71	95	179825	4.655	ug/L	92
35) Methylcyclohexane	8.96	83	293425	5.051	ug/L	97
37) 1,2-Dichloropropane	8.99	63	164207	5.022	ug/L	98
38) Bromodichloromethane	9.28	83	166174	4.975	ug/L	94
39) cis-1,3-Dichloropropene	9.72	75	184233	5.103	ug/L	98
40) 4-Methyl-2-pentanone	9.87	43	570113	61.873	ug/L	99
42) Toluene	10.03	91	871407	5.268	ug/L	95
44) trans-1,3-Dichloropropene	10.27	75	130848	5.191	ug/L	100
45) 1,1,2-Trichloroethane	10.45	97	89000	5.465	ug/L	95
47) Tetrachloroethene	10.52	164	164358	4.972	ug/L	98
48) 2-Hexanone	10.64	43	391008	62.924	ug/L	98
49) Dibromochloromethane	10.78	129	106357	5.536	ug/L	96
50) 1,2-Dibromoethane	10.89	107	75393	5.549	ug/L	94
51) Chlorobenzene	11.31	112	519876	5.197	ug/L	99
52) Ethylbenzene	11.39	91	927344	5.156	ug/L	100
53) m,p-Xylene	11.51	106	375489	5.395	ug/L	99
54) o-Xylene	11.83	106	343765	5.380	ug/L	97
55) Styrene	11.85	104	574709	5.646	ug/L	100
56) Isopropylbenzene	12.13	105	877288	5.220	ug/L	100
58) 1,1,2,2-Tetrachloroethane	12.38	83	85440	5.536	ug/L	94
59) 1,2,3-Trichloropropane	12.44	75	58876	5.711	ug/L	97
61) Bromoform	12.01	173	44053	4.855	ug/L	99
62) 1,3-Dichlorobenzene	13.16	146	327273	4.969	ug/L	98
63) 1,4-Dichlorobenzene	13.24	146	358743	5.018	ug/L	97
65) 1,2-Dichlorobenzene	13.53	146	287594	5.082	ug/L	96
66) 1,2-Dibromo-3-chloropropan	14.15	75	7530	4.300	ug/L #	59
67) 1,3,5-Trichlorobenzene	14.29	180	212544	4.747	ug/L	97
68) 1,2,4-trichlorobenzene	14.79	180	145420	5.054	ug/L	100
69) Naphthalene	15.00	128	163740	4.982	ug/L	100
70) 1,2,3-Trichlorobenzene	15.18	180	125498	5.672	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR080618\
 Data File : VR025566.D
 Acq On : 6 Aug 2018 22:00
 Operator : SY/MD
 Sample : VSTCCC005EC
 Misc : 25mL/MSVOA_R/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_R
 LabSampleId :
 VSTD00591

Manual Integrations
 APPROVED

MMDadoda
 8/8/2018 1:10:39 PM

Quant Time: Aug 07 00:49:12 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR073018WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Aug 06 23:40:46 2018
 Response via : Initial Calibration

