

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR082918\
 Data File : VR025661.D
 Acq On : 29 Aug 2018 18:49
 Operator : SY/MD
 Sample : J4633-08
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 DB3K2

Quant Time: Aug 30 07:09:17 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR082118WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Aug 30 06:43:05 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	386597	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	339934	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.22	152	97886	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.14	65	103639	4.12	ug/L	-0.02
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.40%
7) Chloroethane-d5	2.63	69	88760	4.09	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	81.80%
11) 1,1-Dichloroethene-d2	3.63	63	175361	2.82	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	56.40%#
20) 2-Butanone-d5	6.60	46	128672	67.10	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	134.20%#
24) Chloroform-d	7.20	84	193823	4.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.80%
26) 1,2-Dichloroethane-d4	7.89	65	73251	4.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.20%
32) Benzene-d6	7.86	84	431743	3.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	77.60%
36) 1,2-Dichloropropane-d6	8.90	67	132845	4.69	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.80%
41) Toluene-d8	9.97	98	376238	3.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.80%
43) trans-1,3-Dichloropropene-	10.24	79	24807	3.71	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	74.20%
46) 2-Hexanone-d5	10.59	63	131775	60.24	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	120.48%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	59660	4.56	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.20%
64) 1,2-Dichlorobenzene-d4	13.51	152	88650	5.67	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	113.40%


Target Compounds					Ovalue
13) Acetone	3.71	43	10374	8.684 ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA R\DATA\VR082918\
Data File : VR025661.D
Acq On : 29 Aug 2018 18:49
Operator : SY/MD
Sample : J4633-08
Misc : 25mL/MSVOA R/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
DB3K2

Quant Time: Aug 30 07:09:17 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR082118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Aug 30 06:43:05 2018
Response via : Initial Calibration

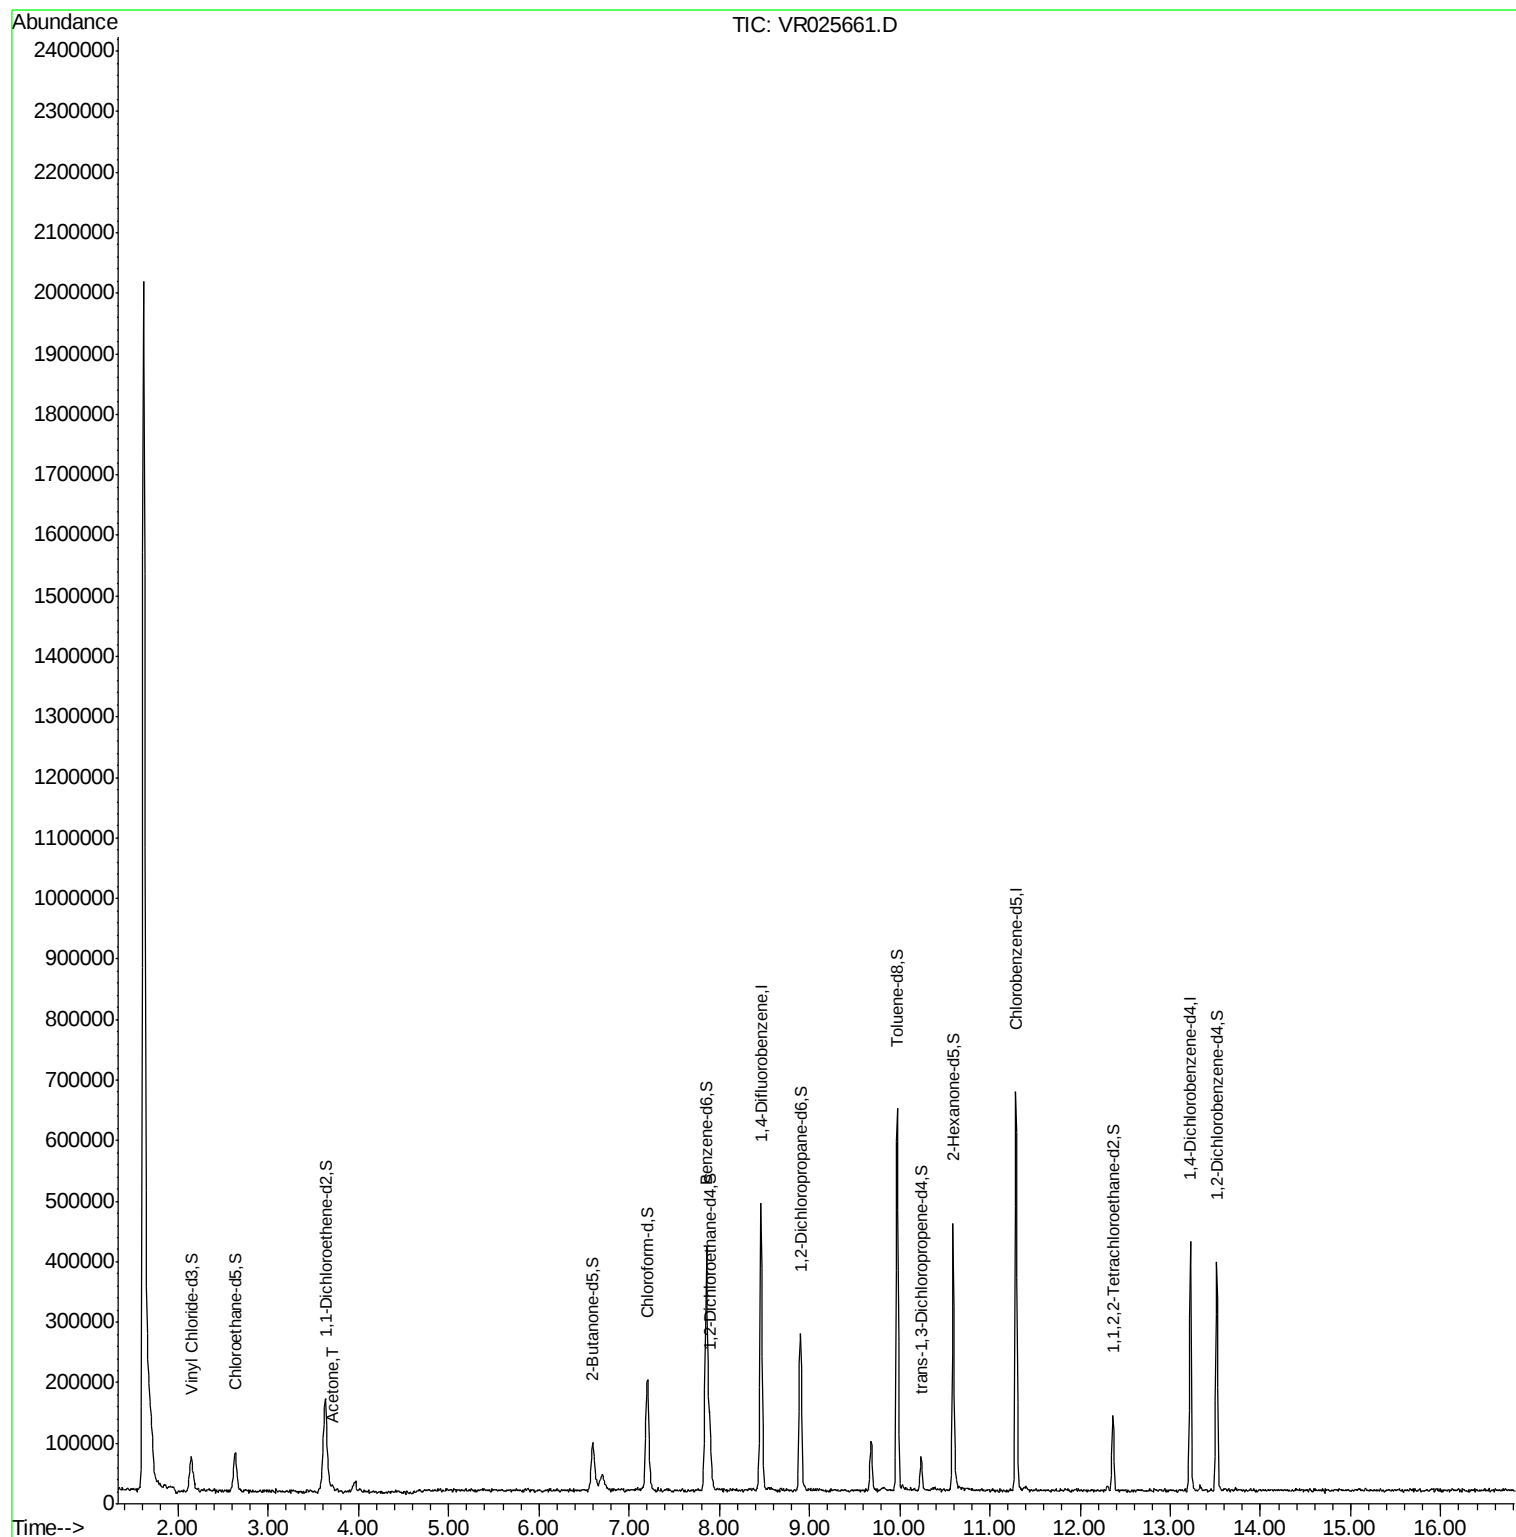

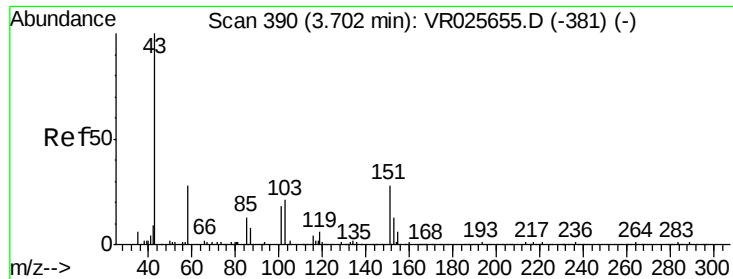

#13

Acetone

Concen: 8.684 ug/L

RT: 3.71 min Scan# 391

Delta R.T. 0.01 min

Lab File: VR025661.D

Acq: 29 Aug 2018 18:49

Instrument :
MSVOA_R
ClientSampleId :
DB3K2

Tot Ion: 43 Resp: 10374

Ion Ratio Lower Upper

43 100

58 22.4 0.0 63.4

