

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR091119\
 Data File : VR026618.D
 Acq On : 11 Sep 2019 13:10
 Operator : SY/MD
 Sample : MDL01
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :

Quant Time: Sep 12 08:53:49 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR091019WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Sep 12 08:46:28 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.48	114	448623	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.30	117	355339	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.24	152	157994	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.18	65	56439	4.07	ug/L	0.01
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.40%
7) Chloroethane-d5	2.64	69	52292	4.45	ug/L	0.01
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.00%
11) 1,1-Dichloroethene-d2	3.63	63	104145	3.18	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.60%
20) 2-Butanone-d5	6.62	46	118696	39.37	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	78.74%
24) Chloroform-d	7.23	84	210593	4.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.00%
26) 1,2-Dichloroethane-d4	7.91	65	68707	4.41	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.20%
32) Benzene-d6	7.88	84	427569	4.25	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.00%
36) 1,2-Dichloropropane-d6	8.92	67	110435	4.07	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	81.40%
41) Toluene-d8	9.99	98	319450	4.18	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.60%
43) trans-1,3-Dichloropropene-	10.25	79	23589	3.67	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	73.40%
46) 2-Hexanone-d5	10.61	63	78297	40.36	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	80.72%
57) 1,1,2,2-Tetrachloroethane-	12.38	84	52118	4.10	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	82.00%
64) 1,2-Dichlorobenzene-d4	13.53	152	90457	4.33	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	86.60%

Target Compounds

					Ovalue
2) Dichlorodifluoromethane	1.86	85	12998	0.286 ug/L	93
3) Chloromethane	2.07	50	7230	0.266 ug/L	90
5) Vinyl chloride	2.21	62	6793	0.264 ug/L	83
6) Bromomethane	2.53	94	1763	0.119 ug/L	77
8) Chloroethane	2.66	64	3956	0.272 ug/L	89
9) Trichlorofluoromethane	2.97	101	12109	0.313 ug/L #	57
10) 1,1,2-Trichloro-1,2,2-trif	3.69	101	3296	0.195 ug/L #	60
12) 1,1-Dichloroethene	3.65	96	5988	0.341 ug/L #	1
13) Acetone	3.72	43	4212	2.274 ug/L	86
14) Carbon disulfide	3.98	76	16686	0.238 ug/L #	92
15) Methyl Acetate	4.23	43	1798	0.218 ug/L	92
16) Methylene chloride	4.43	84	14467	0.392 ug/L	89
17) Methyl tert-butyl Ether	4.93	73	8960	0.203 ug/L #	71
18) trans-1,2-Dichloroethene	4.92	96	10331	0.273 ug/L	93
19) 1,1-Dichloroethane	5.72	63	20143	0.279 ug/L #	91
21) 2-Butanone	6.72	43	8484	2.217 ug/L	90
22) cis-1,2-Dichloroethene	6.71	96	9888	0.265 ug/L #	80

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR091119\
 Data File : VR026618.D
 Acq On : 11 Sep 2019 13:10
 Operator : SY/MD
 Sample : MDL01
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :

Quant Time: Sep 12 08:53:49 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR091019WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Sep 12 08:46:28 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)


23) Bromochloromethane	7.09	128	2863	0.286	ug/L #	67
25) Chloroform	7.26	83	24506	0.369	ug/L	93
27) 1,2-Dichloroethane	8.01	62	7184	0.296	ug/L	96
29) 1,1,1-Trichloroethane	7.46	97	14357	0.267	ug/L	95
30) Cyclohexane	7.54	56	15072	0.236	ug/L	98
31) Carbon tetrachloride	7.65	117	11227	0.252	ug/L	91
33) Benzene	7.92	78	41674	0.265	ug/L	100
34) Trichloroethene	8.74	95	9754	0.251	ug/L	87
35) Methylcyclohexane	8.98	83	15803	0.271	ug/L	97
37) 1,2-Dichloropropane	9.01	63	8183	0.261	ug/L #	91
38) Bromodichloromethane	9.30	83	8091	0.250	ug/L	95
39) cis-1,3-Dichloropropene	9.73	75	10334	0.303	ug/L	99
40) 4-Methyl-2-pentanone	9.88	43	16954	1.890	ug/L #	91
42) Toluene	10.05	91	37701	0.268	ug/L	99
45) 1,1,2-Trichloroethane	10.46	97	3737	0.285	ug/L	82
47) Tetrachloroethene	10.53	164	5790	0.265	ug/L	78
48) 2-Hexanone	10.65	43	13671	2.563	ug/L	96
49) Dibromochloromethane	10.80	129	3153	0.231	ug/L	81
50) 1,2-Dibromoethane	10.90	107	2963	0.270	ug/L #	84
51) Chlorobenzene	11.33	112	20218	0.267	ug/L	91
52) Ethylbenzene	11.41	91	36940	0.240	ug/L	97
53) m,p-Xylene	11.52	106	13859	0.246	ug/L	97
54) o-Xylene	11.84	106	12825	0.234	ug/L	87
55) Styrene	11.86	104	16015	0.212	ug/L	85
56) Isopropylbenzene	12.14	105	34252	0.224	ug/L	97
58) 1,1,2,2-Tetrachloroethane	12.40	83	4217	0.283	ug/L #	94
61) Bromoform	12.03	173	1337	0.230	ug/L #	66
62) 1,3-Dichlorobenzene	13.18	146	13050	0.243	ug/L	90
63) 1,4-Dichlorobenzene	13.26	146	14455	0.279	ug/L	96
65) 1,2-Dichlorobenzene	13.55	146	12740	0.284	ug/L	97
66) 1,2-Dibromo-3-chloropropan	14.16	75	1330	0.583	ug/L #	33
67) 1,3,5-Trichlorobenzene	14.30	180	11058	0.255	ug/L #	86
68) 1,2,4-trichlorobenzene	14.80	180	8322	0.262	ug/L	92
69) Naphthalene	15.02	128	9669	0.216	ug/L #	92
70) 1,2,3-Trichlorobenzene	15.20	180	7201	0.270	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR091119\
Data File : VR026618.D
Acq On : 11 Sep 2019 13:10
Operator : SY/MD
Sample : MDL01
Misc : 25mL/MSVOA R/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :

Quant Time: Sep 12 08:53:49 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR091019WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 12 08:46:28 2019
Response via : Initial Calibration

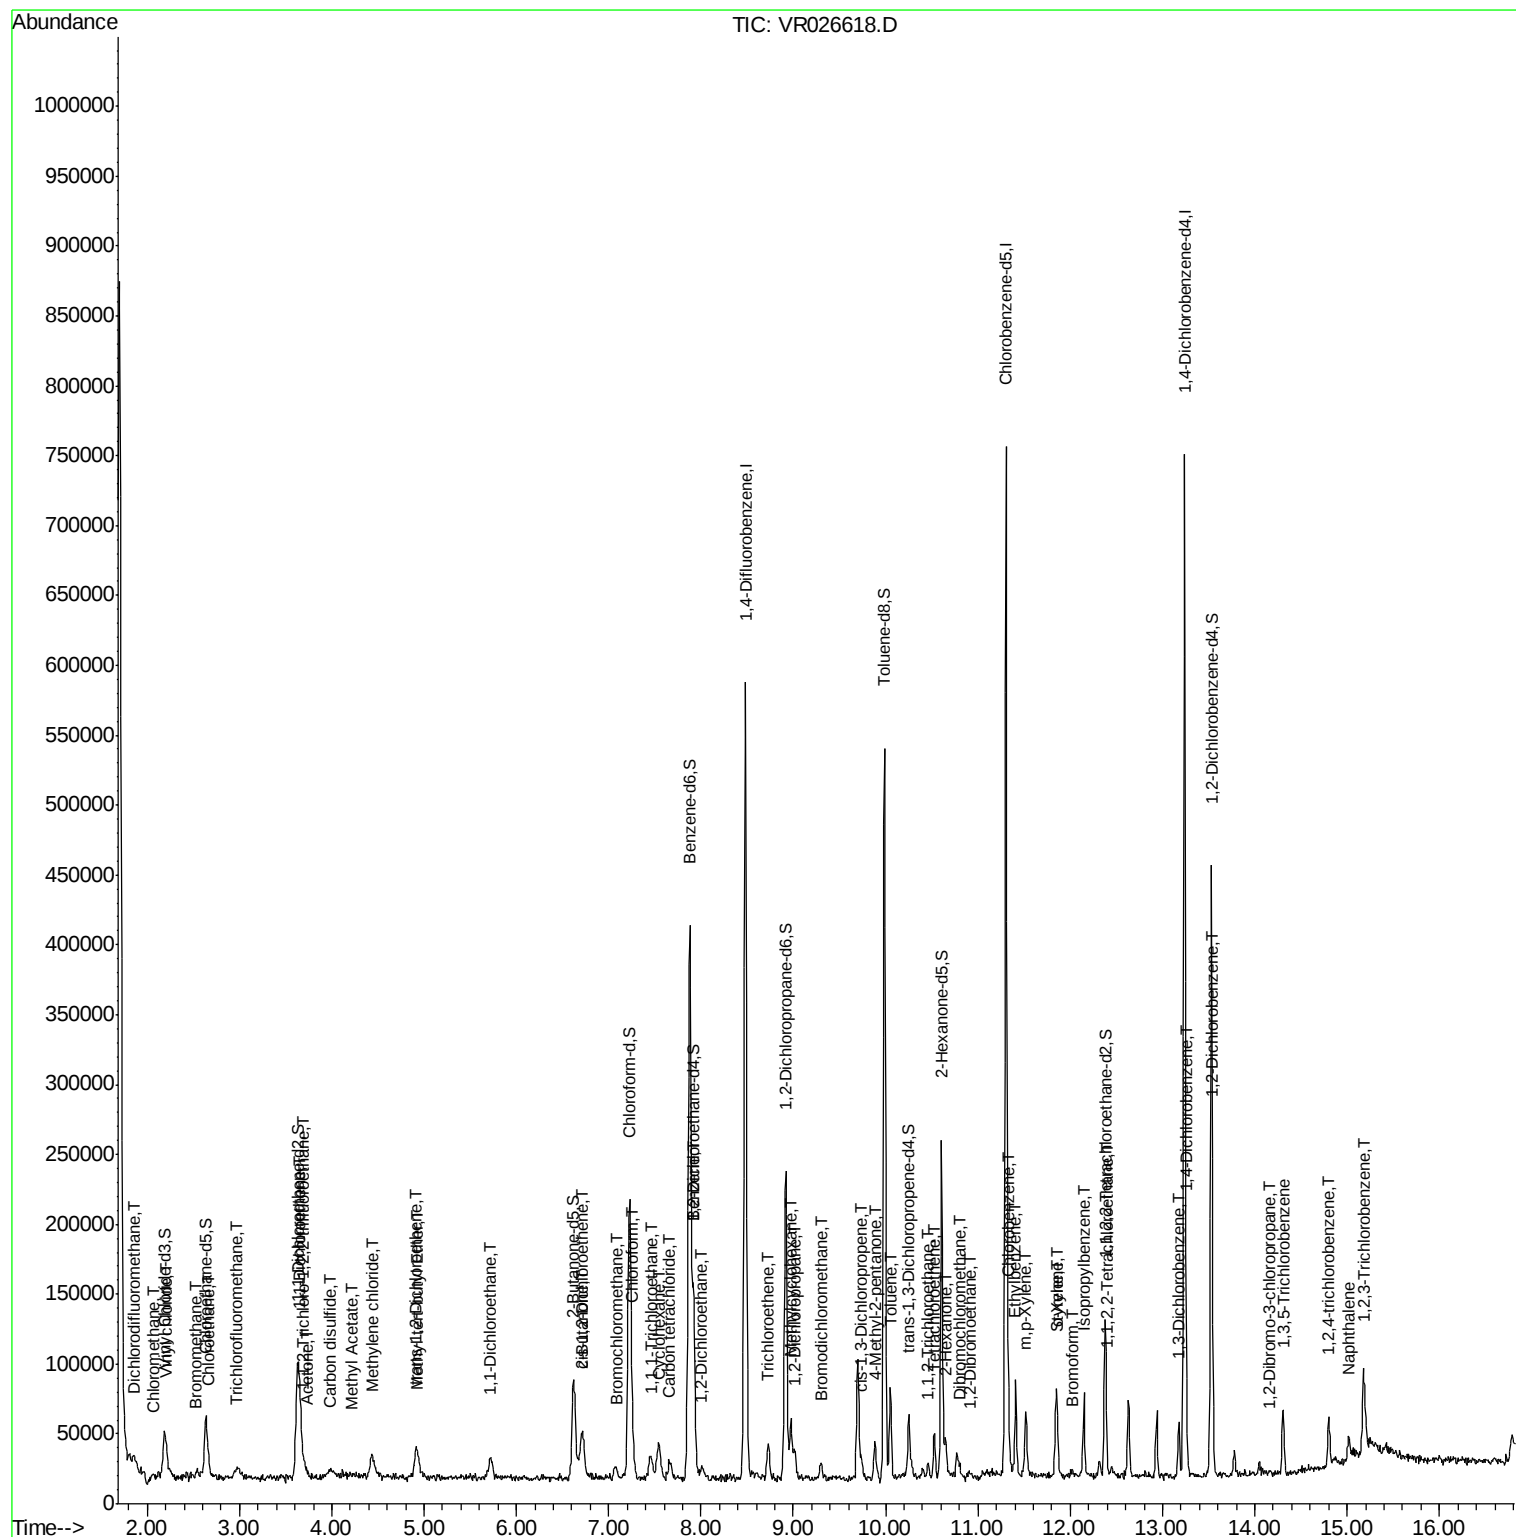

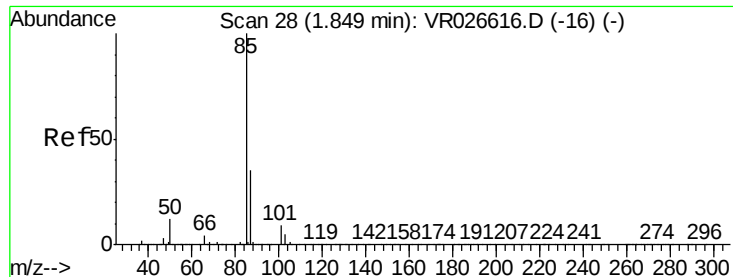

#2

Dichlorodifluoromethane

Concen: 0.286 ug/L

RT: 1.86 min Scan# 30

Delta R.T. 0.01 min

Lab File: VR026618.D

Acq: 11 Sep 2019 13:10


Instrument :
MSVOA_R
ClientSampled :

Tot Ion: 85 Resp: 12998




Ion Ratio Lower Upper

85 100

87 28.1 25.4 38.2

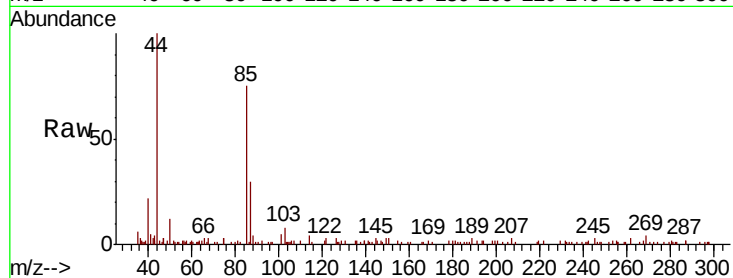

Abundance Ion 85.00 (84.70 to 85.70): VR0
Ion 87.00 (86.70 to 87.70): VR0

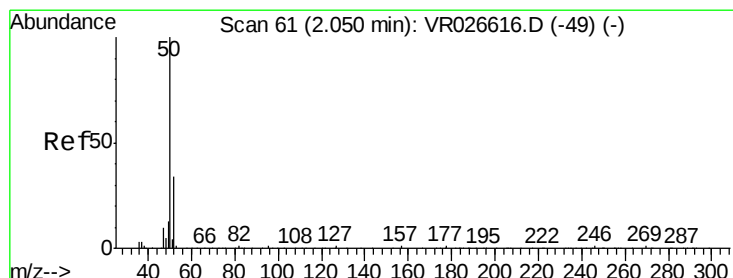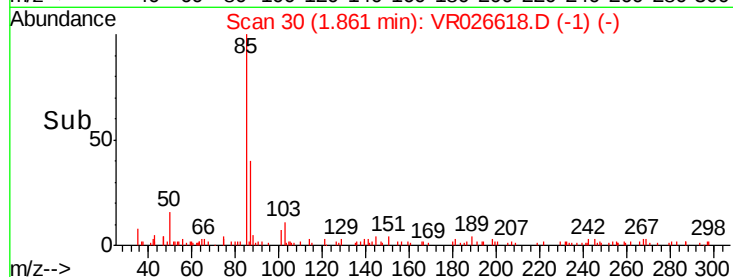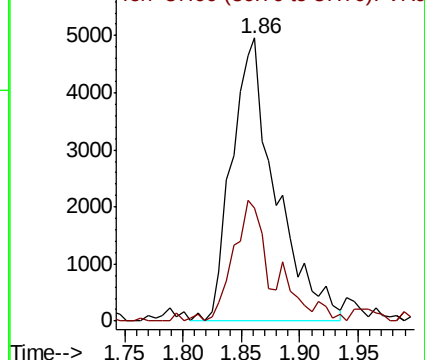

#3

Chloromethane

Concen: 0.266 ug/L

RT: 2.07 min Scan# 64

Delta R.T. 0.02 min

Lab File: VR026618.D


Acq: 11 Sep 2019 13:10

Tgt Ion: 50 Resp: 7230



Ion Ratio Lower Upper


50 100

52 26.4 22.2 41.2

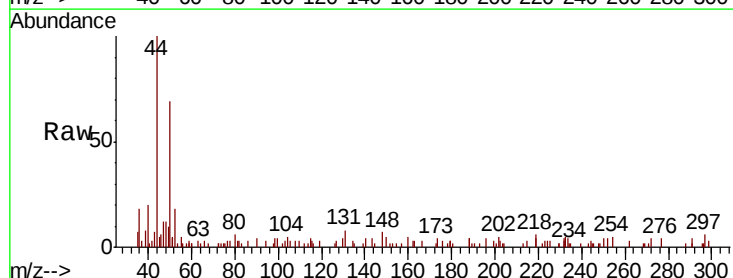

Abundance Ion 50.05 (49.75 to 50.75): VR0
Ion 52.05 (51.75 to 52.75): VR0

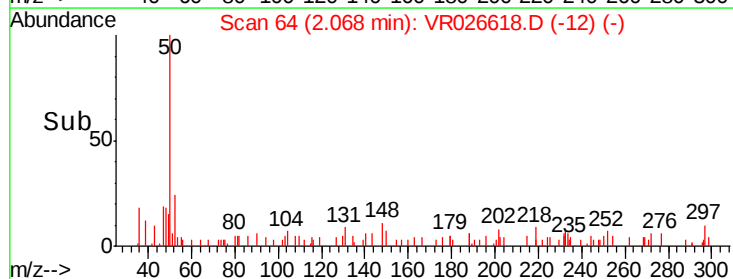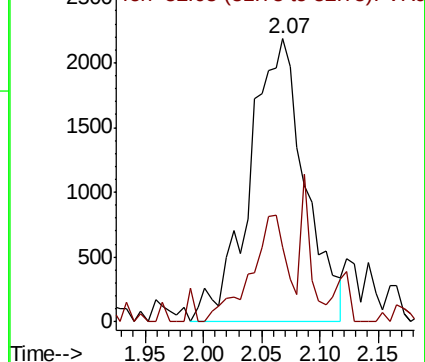

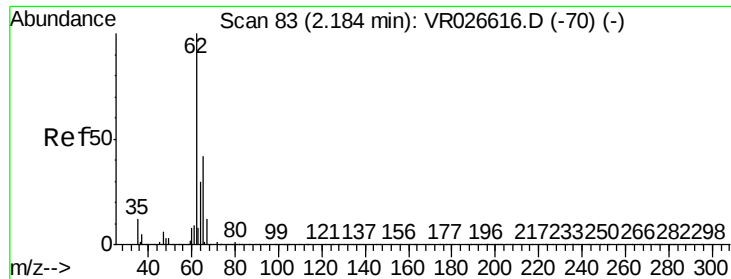

#5

Vinyl chloride

Concen: 0.264 ug/L

RT: 2.21 min Scan# 87

Delta R.T. 0.02 min

Lab File: VR026618.D

Acq: 11 Sep 2019 13:10

Instrument :

MSVOA_R





ClientSampleId :

Tot Ion: 62 Resp: 6793

Ion Ratio Lower Upper

62 100

64 26.5 25.4 47.2

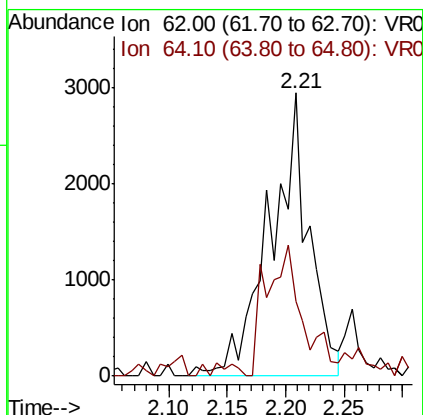

#6

Bromomethane

Concen: 0.119 ug/L

RT: 2.53 min Scan# 140

Delta R.T. 0.00 min

Lab File: VR026618.D




Acq: 11 Sep 2019 13:10


Tgt Ion: 94 Resp: 1763

Ion Ratio Lower Upper

94 100

96 72.0 65.7 122.1

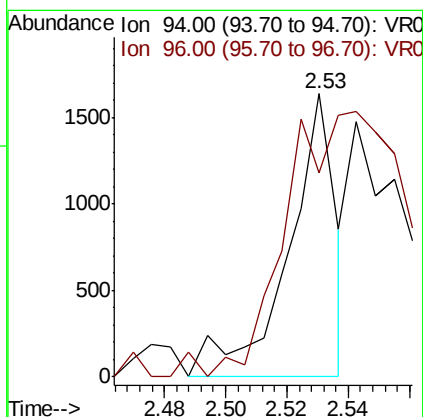

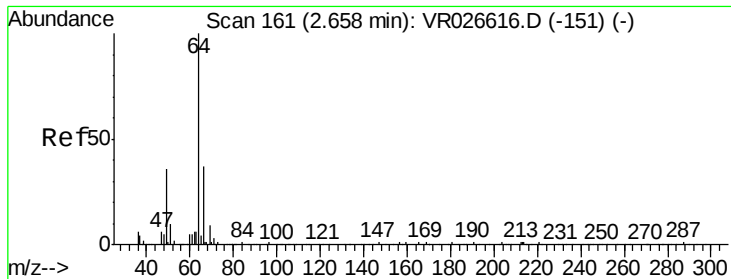

#8

Chloroethane

Concen: 0.272 ug/L

RT: 2.66 min Scan# 162

Delta R.T. 0.01 min

Lab File: VR026618.D

Acq: 11 Sep 2019 13:10

Instrument :

MSVOA_R


ClientSampleId :

Tot Ion: 64 Resp: 3956

Ion Ratio Lower Upper

64 100

66 29.3 25.1 46.5



Abundance Ion 64.10 (63.80 to 64.80): VR0

Ion 66.05 (65.75 to 66.75): VR0

2000

1500



1000

500

0

2.60 2.65 2.70

Time-->

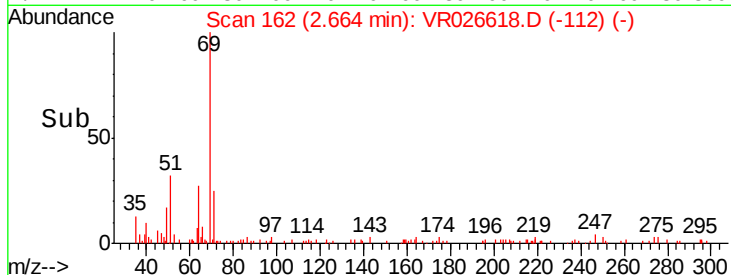

#9

Trichlorofluoromethane

Concen: 0.313 ug/L

RT: 2.97 min Scan# 213

Delta R.T. 0.01 min

Lab File: VR026618.D


Acq: 11 Sep 2019 13:10

Tgt Ion: 101 Resp: 12109

Ion Ratio Lower Upper

101 100

103 30.3 51.1 76.7#



Abundance Ion 101.00 (100.70 to 101.70): V

Ion 103.00 (102.70 to 103.70): V

3000


2000


1000

0

2.90 3.00 3.10

Time-->





#10

1,1,2-Trichloro-1,2,2-trifluoroethane

Concen: 0.195 ug/L

RT: 3.69 min Scan# 331

Delta R.T. 0.01 min

Lab File: VR026618.D





Acq: 11 Sep 2019 13:10

Instrument :

MSVOA_R

ClientSampled :

Tot Ion:	101	Resp:	3296
Ion	Ratio	Lower	Upper
101	100		
85	74.2	40.6	61.0#
151	111.1	58.6	87.8#

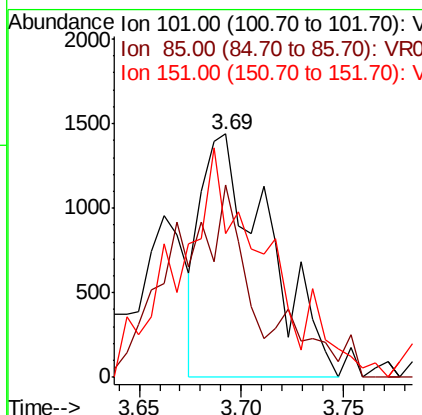

#12

1,1-Dichloroethene

Concen: 0.341 ug/L




RT: 3.65 min Scan# 324


Delta R.T. 0.01 min

Lab File: VR026618.D

Acq: 11 Sep 2019 13:10

Tgt Ion:	96	Resp:	5988
Ion	Ratio	Lower	Upper
96	100		
61	366.6	137.8	255.8#
63	1451.9	108.6	201.8#

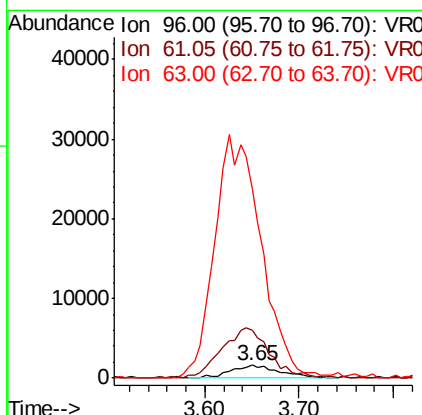

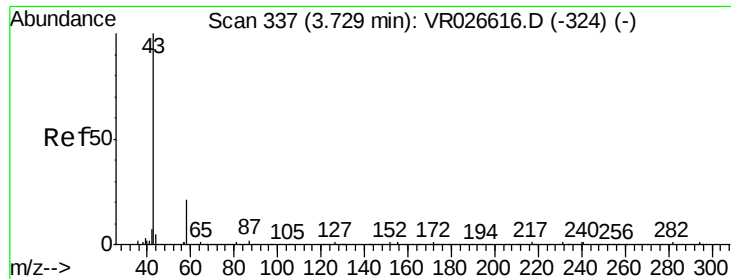

#13

Acetone

Concen: 2.274 ug/L

RT: 3.72 min Scan# 336

Delta R.T. -0.01 min

Lab File: VR026618.D

Acq: 11 Sep 2019 13:10

Instrument :

MSVOA_R





ClientSampleId :

Tot Ion: 43 Resp: 4212

Ion Ratio Lower Upper

43 100

58 29.9 0.0 46.2

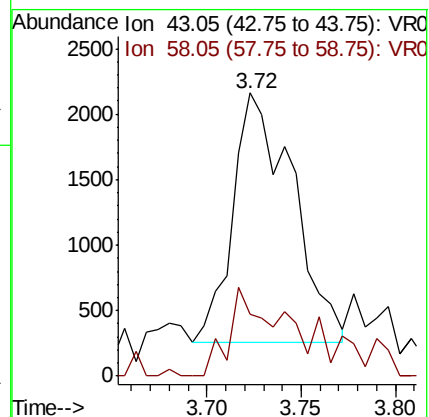

#14

Carbon disulfide

Concen: 0.238 ug/L

RT: 3.98 min Scan# 378

Delta R.T. 0.02 min

Lab File: VR026618.D




Acq: 11 Sep 2019 13:10


Tgt Ion: 76 Resp: 16686

Ion Ratio Lower Upper

76 100

78 6.3 7.3 10.9#



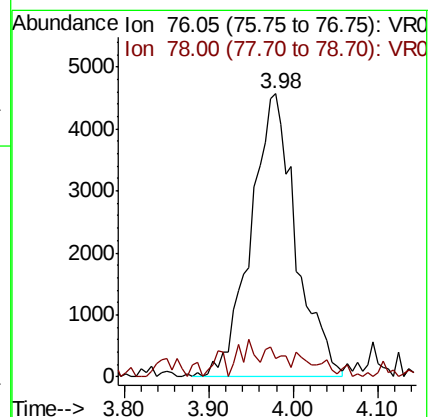





#15
Methyl Acetate
Concen: 0.218 ug/L
RT: 4.23 min Scan# 419
Delta R.T. 0.01 min
Lab File: VR026618.D
Acq: 11 Sep 2019 13:10




Instrument :
MSVOA_R
ClientSampled :


Tot Ion: 43 Resp: 1798
Ion Ratio Lower Upper
43 100
74 28.2 19.4 29.2

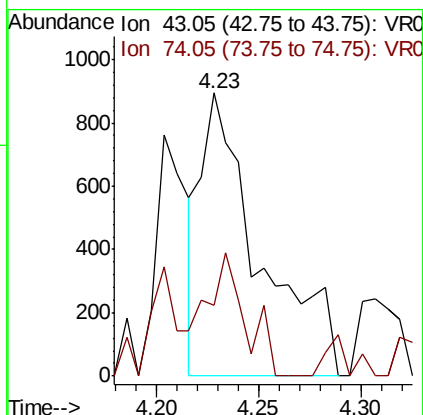

#16
Methylene chloride
Concen: 0.392 ug/L
RT: 4.43 min Scan# 453
Delta R.T. 0.01 min
Lab File: VR026618.D
Acq: 11 Sep 2019 13:10

Tgt Ion: 84 Resp: 14467
Ion Ratio Lower Upper
84 100
86 54.4 43.6 81.0
49 109.6 85.9 159.5


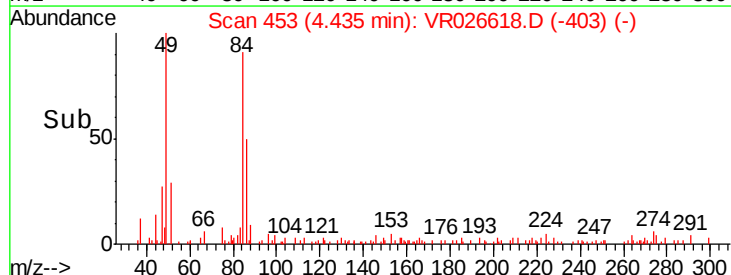
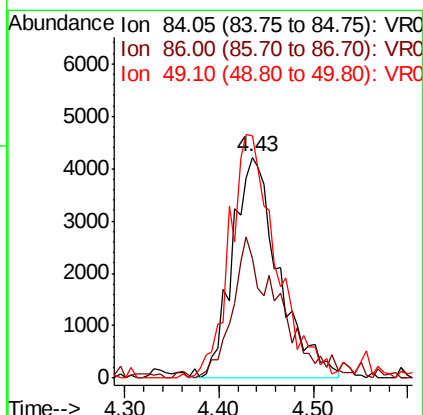





#17
Methvl tert-butvl Ether
Concen: 0.203 ug/L
RT: 4.93 min Scan# 535
Delta R.T. 0.01 min
Lab File: VR026618.D
Acq: 11 Sep 2019 13:10




Instrument :
MSVOA_R
ClientSampled :


Tot Ion: 73 Resp: 8960
Ion Ratio Lower Upper
73 100
43 8.8 15.4 23.2#
57 7.5 19.0 28.4#

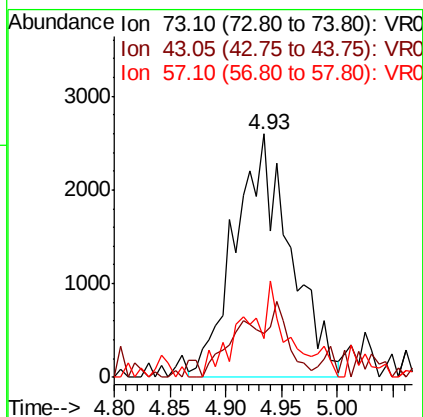

#18
trans-1,2-Dichloroethene
Concen: 0.273 ug/L
RT: 4.92 min Scan# 532
Delta R.T. 0.01 min
Lab File: VR026618.D
Acq: 11 Sep 2019 13:10

Tgt Ion: 96 Resp: 10331
Ion Ratio Lower Upper
96 100
61 158.8 106.7 198.1
98 56.0 45.4 84.4

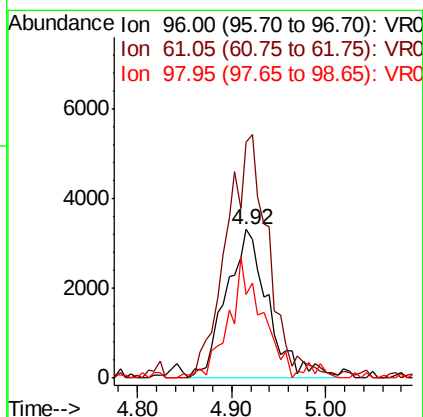

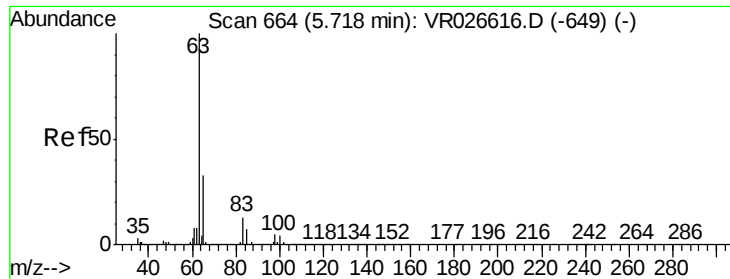

#19

1,1-Dichloroethane

Concen: 0.279 ug/L

RT: 5.72 min Scan# 665

Delta R.T. 0.01 min

Lab File: VR026618.D

Acq: 11 Sep 2019 13:10

Instrument :

MSVOA_R

ClientSampleId :


Tot Ion: 63 Resp: 20143

Ion Ratio Lower Upper

63 100

65 28.8 23.2 43.0




83 8.4 9.5 17.7#



Abundance Ion 63.10 (62.80 to 63.80): VR0

Ion 65.10 (64.80 to 65.80): VR0

Ion 83.05 (82.75 to 83.75): VR0

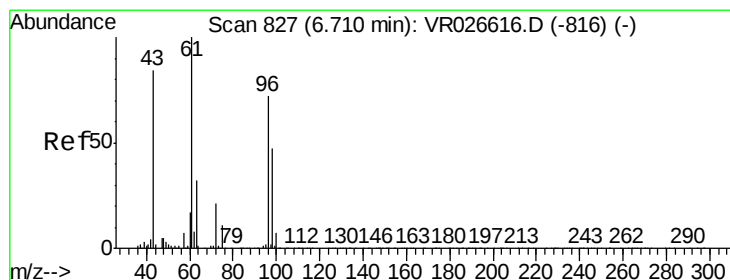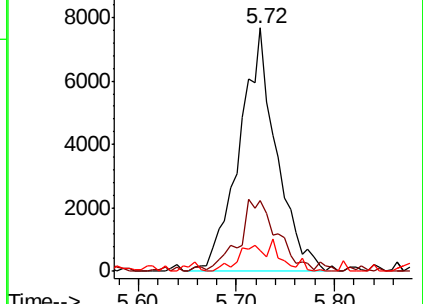

#21

2-Butanone

Concen: 2.217 ug/L

RT: 6.72 min Scan# 828

Delta R.T. 0.01 min

Lab File: VR026618.D


Acq: 11 Sep 2019 13:10

Tgt Ion: 43 Resp: 8484

Ion Ratio Lower Upper



43 100


72 33.5 14.2 42.6



Abundance Ion 43.05 (42.75 to 43.75): VR0

Ion 72.10 (71.80 to 72.80): VR0

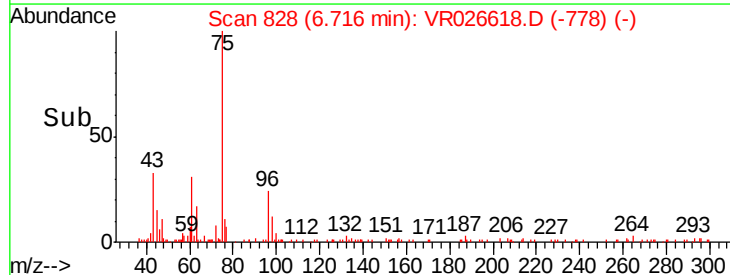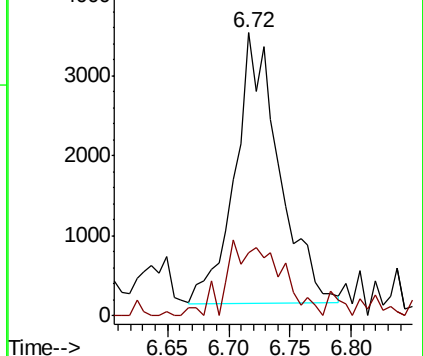







#22

cis-1,2-Dichloroethene
Concen: 0.265 ug/L
RT: 6.71 min Scan# 827
Delta R.T. 0.01 min
Lab File: VR026618.D
Acq: 11 Sep 2019 13:10

Instrument :
MSVOA_R
ClientSampleId :




Tot Ion	Ratio	Lower	Upper
96	100		
61	110.4	94.0	174.6
68	0.0	0.1	0.1#

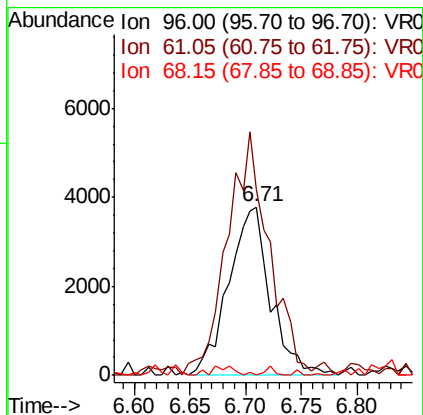


#23

Bromochloromethane
Concen: 0.286 ug/L
RT: 7.09 min Scan# 889
Delta R.T. 0.01 min
Lab File: VR026618.D
Acq: 11 Sep 2019 13:10

Tgt Ion	Ratio	Lower	Upper
128	100		
49	122.7	113.2	210.2
130	72.7	84.1	156.1#
51	43.1	51.1	76.7#


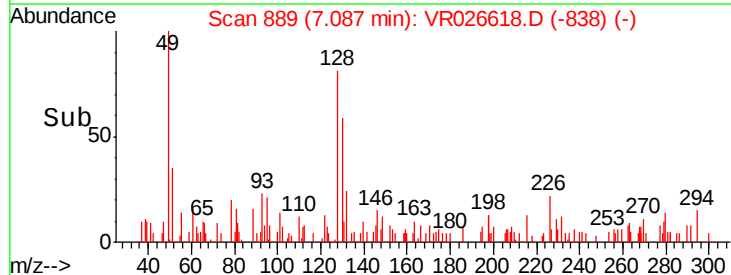
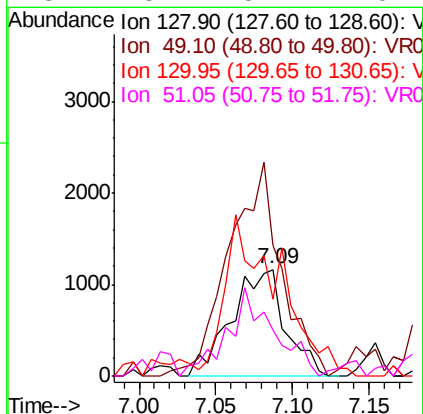





#25
Chloroform
Concen: 0.369 ug/L
RT: 7.26 min Scan# 917
Delta R.T. 0.01 min
Lab File: VR026618.D
Acq: 11 Sep 2019 13:10




Instrument :
MSVOA_R
ClientSampled :


Tot Ion: 83 Resp: 24506
Ion Ratio Lower Upper
83 100
85 58.5 44.5 82.7

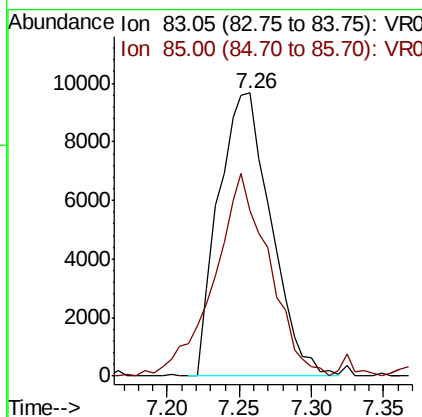

#27
1,2-Dichloroethane
Concen: 0.296 ug/L
RT: 8.01 min Scan# 1041
Delta R.T. 0.00 min
Lab File: VR026618.D
Acq: 11 Sep 2019 13:10

Tgt Ion: 62 Resp: 7184
Ion Ratio Lower Upper
62 100
98 11.3 7.8 11.8



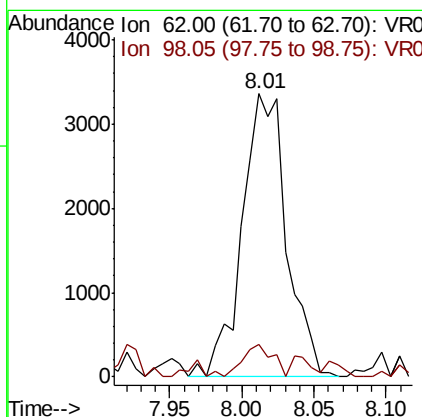





#29
 1,1,1-Trichloroethane
 Concen: 0.267 ug/L
 RT: 7.46 min Scan# 951
 Delta R.T. 0.01 min
 Lab File: VR026618.D
 Acq: 11 Sep 2019 13:10




Instrument :
 MSVOA_R
 ClientSampleId :


Tot Ion:	97	Resp:	14357
Ion	Ratio	Lower	Upper
97	100		
99	56.6	50.8	76.2
61	48.8	39.2	58.8

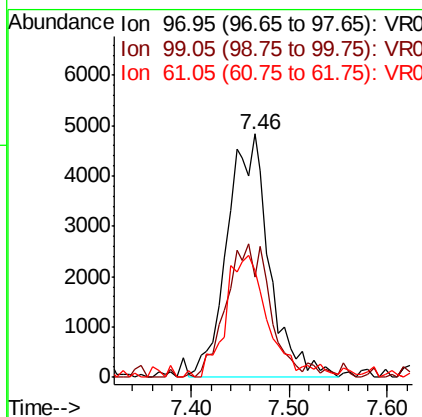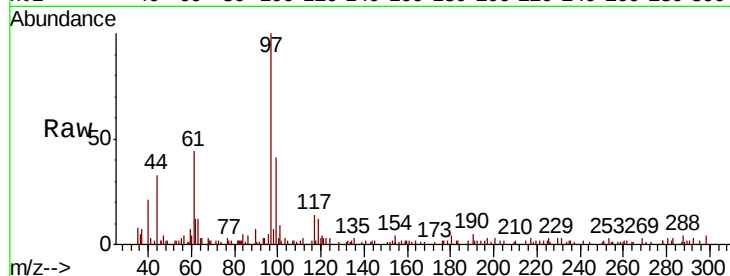

#30
 Cyclohexane
 Concen: 0.236 ug/L
 RT: 7.54 min Scan# 964
 Delta R.T. 0.01 min
 Lab File: VR026618.D
 Acq: 11 Sep 2019 13:10

Tgt Ion:	56	Resp:	15072
Ion	Ratio	Lower	Upper
56	100		
69	34.4	25.0	37.4
84	79.4	63.6	95.4

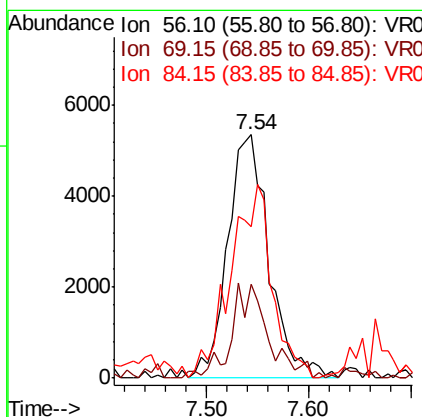



#31

Carbon tetrachloride

Concen: 0.252 ug/L

RT: 7.65 min Scan# 982

Delta R.T. -0.01 min

Lab File: VR026618.D

Acq: 11 Sep 2019 13:10

Instrument :

MSVOA_R


ClientSampleId :

Tot Ion:117 Resp: 11227

Ion Ratio Lower Upper




117 100

119 87.0 76.7 115.1



Abundance Ion 116.90 (116.60 to 117.60): V

Ion 118.90 (118.60 to 119.60): V

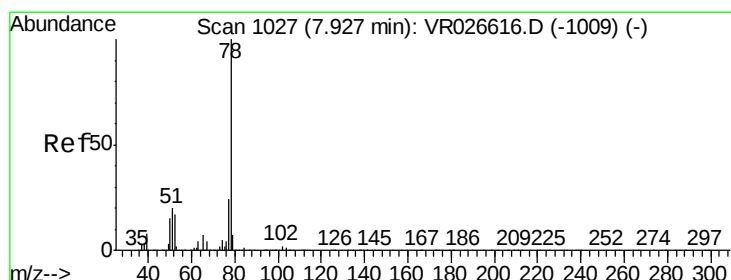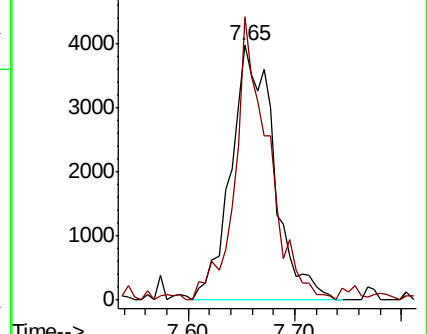

#33

Benzene

Concen: 0.265 ug/L


RT: 7.92 min Scan# 1026

Delta R.T. -0.01 min



Lab File: VR026618.D


Acq: 11 Sep 2019 13:10

Tgt Ion: 78 Resp: 41674



Abundance Ion 78.10 (77.80 to 78.80): VR0

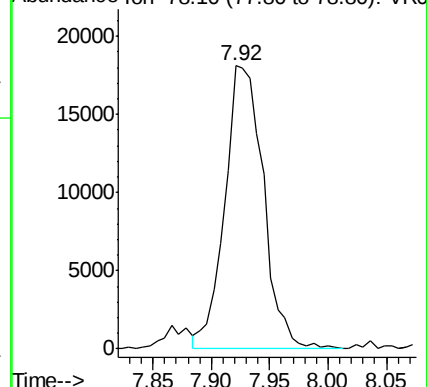



#34

Trichloroethene

Concen: 0.251 ug/L

RT: 8.74 min Scan# 1160

Delta R.T. 0.01 min

Lab File: VR026618.D

Acq: 11 Sep 2019 13:10

Instrument :

MSVOA_R

ClientSampleId :

Tot Ion: 95 Resp: 9754


Ion Ratio Lower Upper

95 100

97 50.4 42.8 79.4

132 74.4 61.5 114.1

130 103.4 64.5 119.7






Abundance Ion 95.00 (94.70 to 95.70): VR0

Ion 96.95 (96.65 to 97.65): VR0

Ion 131.95 (131.65 to 132.65): V

Ion 129.95 (129.65 to 130.65): V

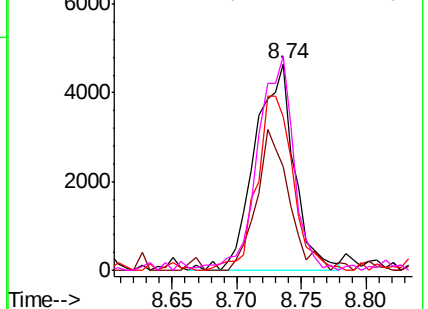

#35

Methylcyclohexane

Concen: 0.271 ug/L

RT: 8.98 min Scan# 1200

Delta R.T. 0.01 min

Lab File: VR026618.D

Acq: 11 Sep 2019 13:10


Tgt Ion: 83 Resp: 15803

Ion Ratio Lower Upper

83 100

55 82.4 65.0 97.6



98 41.2 35.8 53.8




Abundance Ion 83.15 (82.85 to 83.85): VR0

Ion 55.10 (54.80 to 55.80): VR0

Ion 98.15 (97.85 to 98.85): VR0




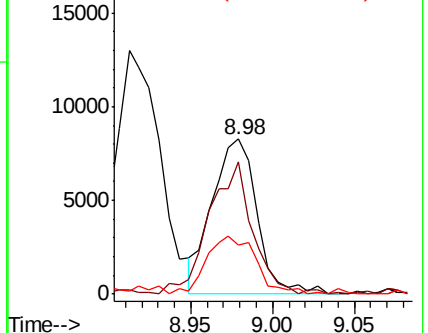




#37
 1,2-Dichloropropane
 Concen: 0.261 ug/L
 RT: 9.01 min Scan# 1205
 Delta R.T. -0.01 min
 Lab File: VR026618.D
 Acq: 11 Sep 2019 13:10




Instrument :
 MSVOA_R
 ClientSampled :


Tot Ion: 63 Resp: 8183
 Ion Ratio Lower Upper
 63 100
 112 6.5 2.9 4.3#

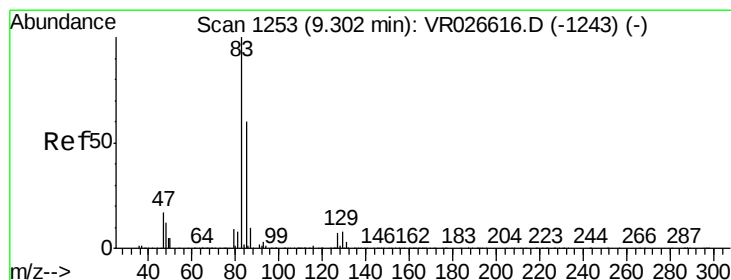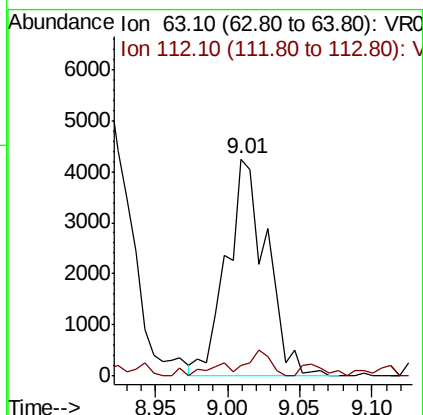

#38
 Bromodichloromethane
 Concen: 0.250 ug/L
 RT: 9.30 min Scan# 1253
 Delta R.T. 0.00 min
 Lab File: VR026618.D
 Acq: 11 Sep 2019 13:10

Tgt Ion: 83 Resp: 8091
 Ion Ratio Lower Upper
 83 100
 85 58.1 44.0 81.6
 127 8.2 6.9 10.3


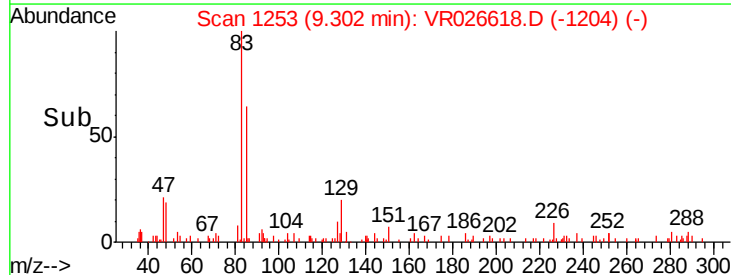
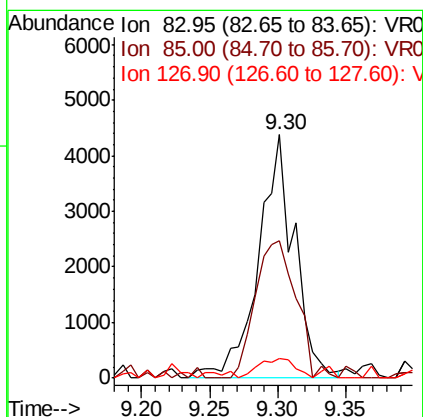



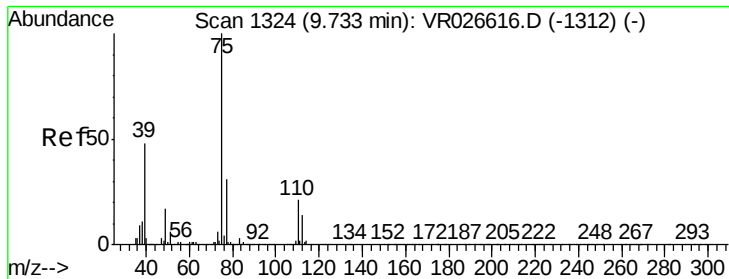

#39
 cis-1,3-Dichloropropene
 Concen: 0.303 ug/L
 RT: 9.73 min Scan# 1324
 Delta R.T. 0.00 min
 Lab File: VR026618.D
 Acq: 11 Sep 2019 13:10




Instrument :
 MSVOA_R
 ClientSampleId :


Tot Ion: 75 Resp: 10334
 Ion Ratio Lower Upper
 75 100
 77 29.2 21.0 39.0

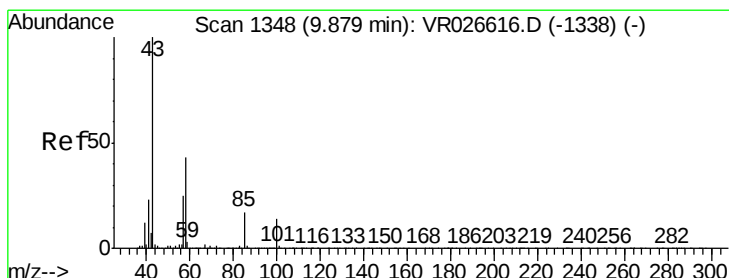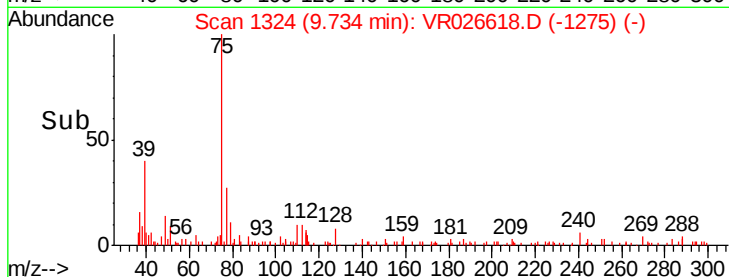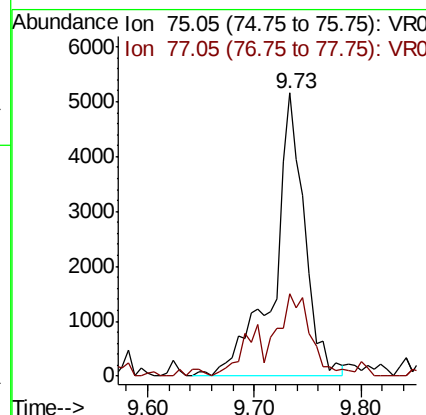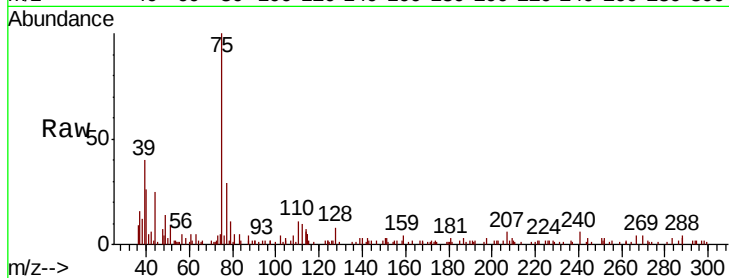

#40
 4-Methyl-2-pentanone
 Concen: 1.890 ug/L
 RT: 9.88 min Scan# 1348
 Delta R.T. 0.00 min
 Lab File: VR026618.D
 Acq: 11 Sep 2019 13:10

Tgt Ion: 43 Resp: 16954
 Ion Ratio Lower Upper
 43 100
 58 39.5 31.6 47.4
 100 0.0 11.4 17.0#

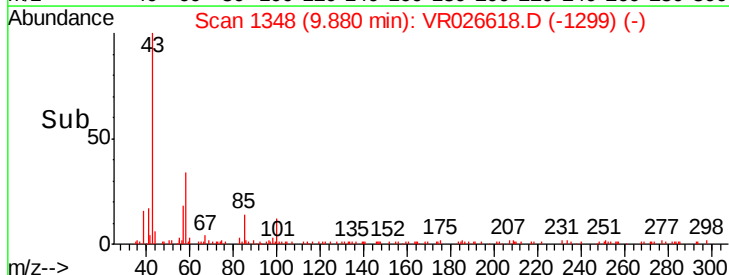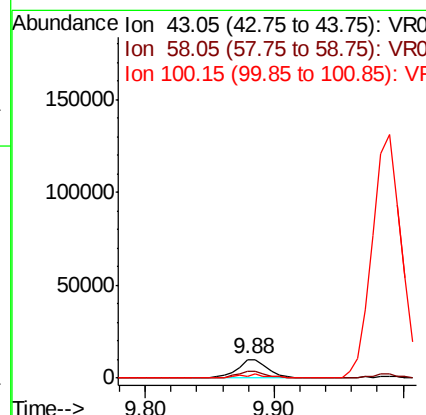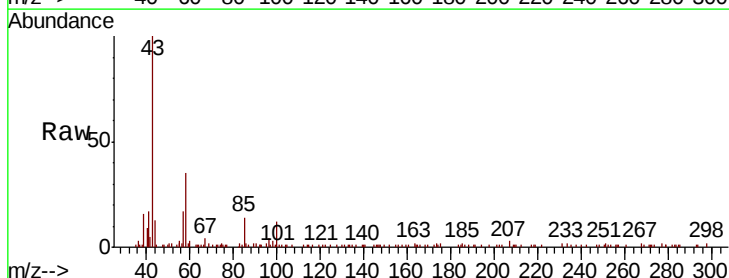



#42

Toluene

Concen: 0.268 ug/L

RT: 10.05 min Scan# 1376

Delta R.T. 0.00 min

Lab File: VR026618.D

Acq: 11 Sep 2019 13:10

Instrument :

MSVOA_R





ClientSampleId :

Tot Ion: 91 Resp: 37701

Ion Ratio Lower Upper

91 100

92 57.9 40.2 74.6

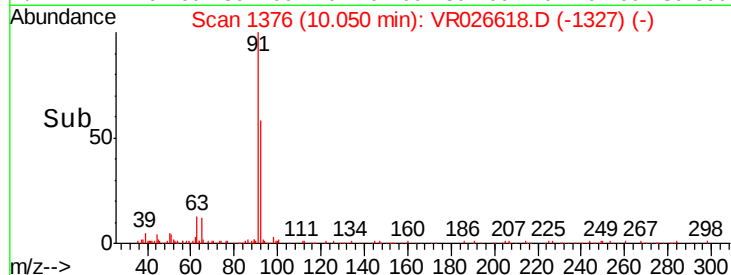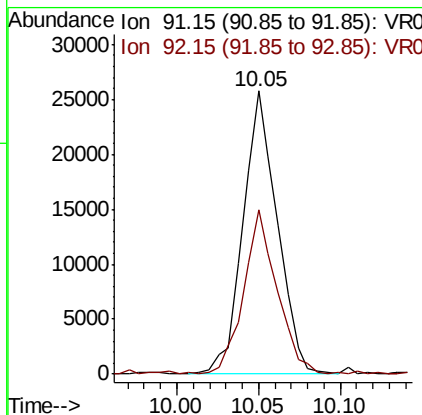

#45

1,1,2-Trichloroethane

Concen: 0.285 ug/L

RT: 10.46 min Scan# 1444

Delta R.T. 0.01 min

Lab File: VR026618.D

Acq: 11 Sep 2019 13:10

Tgt Ion: 97 Resp: 3737




Ion Ratio Lower Upper


97 100

99 42.4 40.4 75.0

83 74.0 61.2 113.8

85 39.5 37.5 69.7

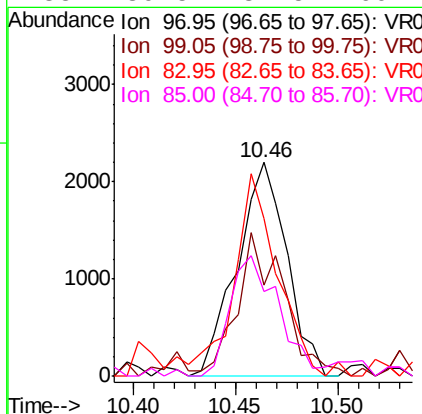



#47

Tetrachloroethene

Concen: 0.265 ug/L

RT: 10.53 min Scan# 1455

Delta R.T. 0.00 min

Lab File: VR026618.D

Acq: 11 Sep 2019 13:10

Instrument :

MSVOA_R

ClientSampleId :

Tot Ion:164 Resp: 5790


Ion Ratio Lower Upper

164 100

129 76.0 69.4 128.8

131 110.9 63.6 118.0

166 92.5 80.4 149.2






Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

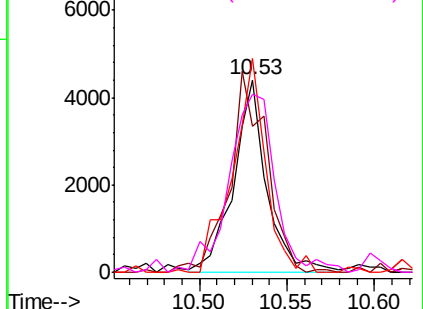

#48

2-Hexanone

Concen: 2.563 ug/L

RT: 10.65 min Scan# 1474

Delta R.T. 0.00 min

Lab File: VR026618.D

Acq: 11 Sep 2019 13:10

Tgt Ion: 43 Resp: 13671


Ion Ratio Lower Upper

43 100

58 60.3 46.0 69.0

57 18.5 16.1 24.1

100 10.1 8.9 13.3






Abundance Ion 43.05 (42.75 to 43.75): VR0

Ion 58.05 (57.75 to 58.75): VR0

Ion 57.20 (56.90 to 57.90): VR0

Ion 100.15 (99.85 to 100.85): VR0

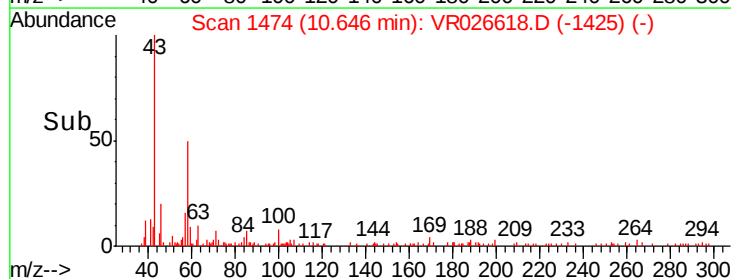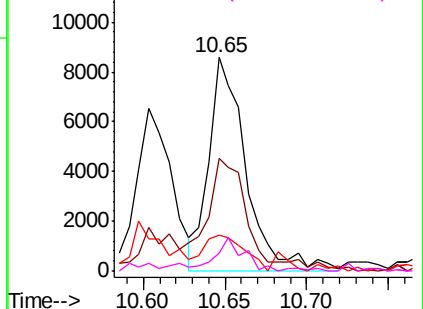



#49

Dibromochloromethane

Concen: 0.231 ug/L

RT: 10.80 min Scan# 1500

Delta R.T. 0.01 min

Lab File: VR026618.D

Acq: 11 Sep 2019 13:10

Instrument :

MSVOA_R


ClientSampleId :

Tot Ion:129 Resp: 3153

Ion Ratio Lower Upper




129 100

127 103.3 59.9 111.3



Abundance Ion 128.95 (128.65 to 129.65): V

Ion 126.90 (126.60 to 127.60): V

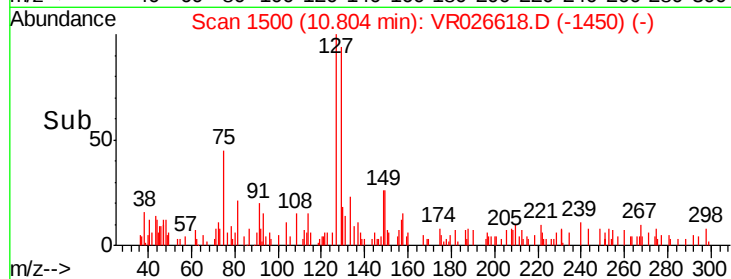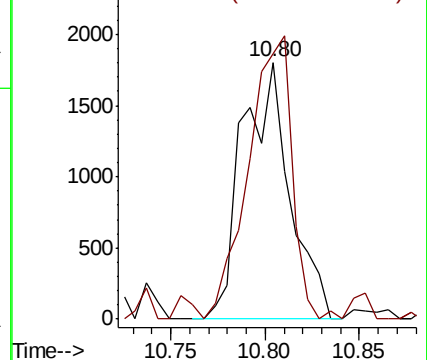

#50

1,2-Dibromoethane

Concen: 0.270 ug/L

RT: 10.90 min Scan# 1516

Delta R.T. 0.00 min

Lab File: VR026618.D

Acq: 11 Sep 2019 13:10


Tgt Ion:107 Resp: 2963

Ion Ratio Lower Upper

107 100

109 79.9 66.8 124.2



188 0.0 1.9 2.9#




Abundance Ion 106.95 (106.65 to 107.65): V

Ion 109.00 (108.70 to 109.70): V

Ion 187.90 (187.60 to 188.60): V

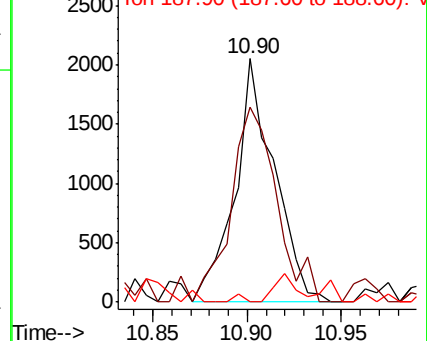



#51

Chlorobenzene

Concen: 0.267 ug/L

RT: 11.33 min Scan# 1587

Delta R.T. 0.01 min

Lab File: VR026618.D

Acq: 11 Sep 2019 13:10

Instrument :

MSVOA_R

ClientSampleId :





Tot Ion: 112 Resp: 20218

Ion Ratio Lower Upper

112 100

114 29.3 22.7 42.3

77 76.7 54.3 81.5

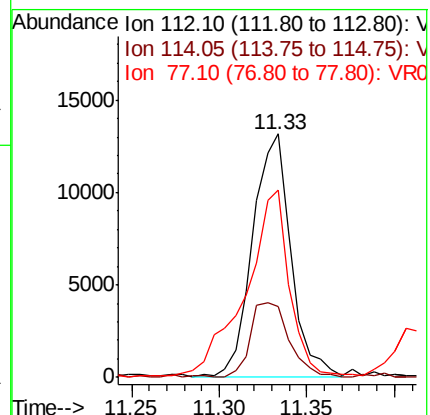

#52

Ethylbenzene

Concen: 0.240 ug/L

RT: 11.41 min Scan# 1599

Delta R.T. 0.00 min

Lab File: VR026618.D




Acq: 11 Sep 2019 13:10


Tgt Ion: 91 Resp: 36940

Ion Ratio Lower Upper

91 100

106 30.8 20.6 38.2

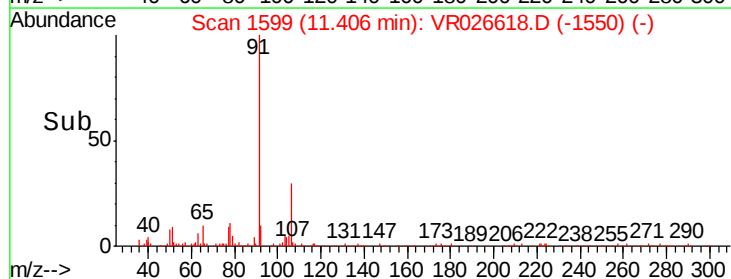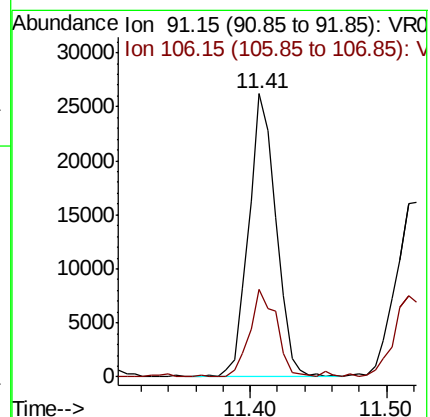



#53

m,p-Xylene

Concen: 0.246 ug/L

RT: 11.52 min Scan# 1617

Delta R.T. -0.01 min

Lab File: VR026618.D

Acq: 11 Sep 2019 13:10

Instrument :

MSVOA_R


ClientSampled :

Tot Ion:106 Resp: 13859

Ion Ratio Lower Upper




106 100

91 211.7 151.8 282.0



Abundance Ion 106.15 (105.85 to 106.85): V

Ion 91.15 (90.85 to 91.85): VR0

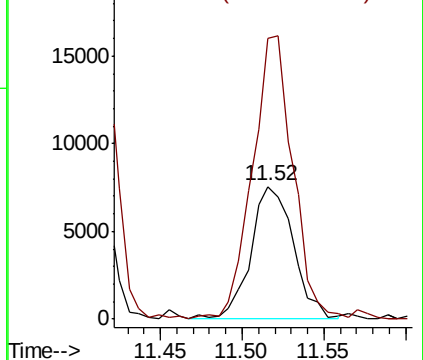

#54

o-Xylene

Concen: 0.234 ug/L

RT: 11.84 min Scan# 1671

Delta R.T. 0.00 min

Lab File: VR026618.D


Acq: 11 Sep 2019 13:10

Tgt Ion:106 Resp: 12825

Ion Ratio Lower Upper



106 100


91 209.3 161.3 299.5



Abundance Ion 106.15 (105.85 to 106.85): V

Ion 91.15 (90.85 to 91.85): VR0

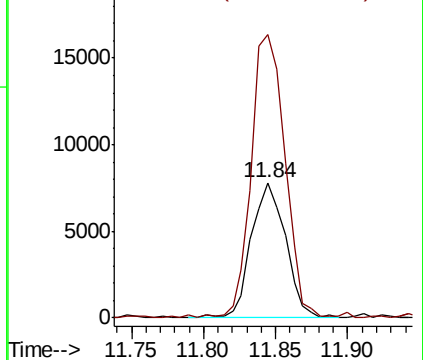



#55

Stvrene

Concen: 0.212 ug/L

RT: 11.86 min Scan# 1674

Delta R.T. 0.00 min

Lab File: VR026618.D

Acq: 11 Sep 2019 13:10

Instrument :

MSVOA_R


ClientSampleId :

Tot Ion:104 Resp: 16015

Ion Ratio Lower Upper




104 100

78 59.6 34.3 63.7



Abundance Ion 104.10 (103.80 to 104.80): V

Ion 78.10 (77.80 to 78.80): VR0

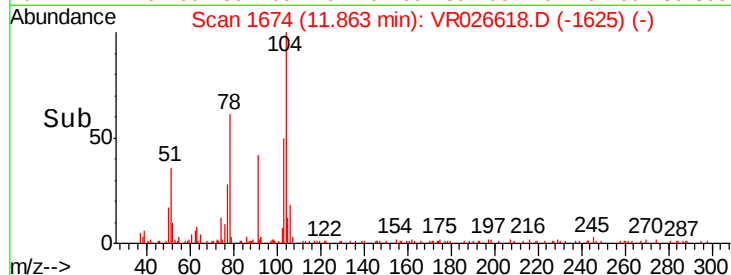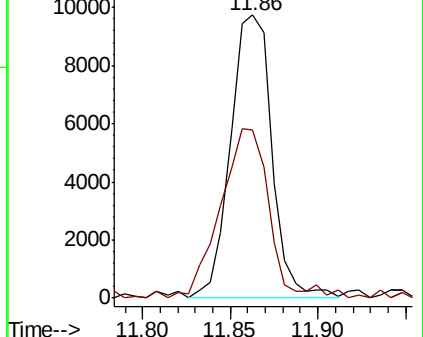

#56

Isopropylbenzene

Concen: 0.224 ug/L

RT: 12.14 min Scan# 1720

Delta R.T. -0.01 min

Lab File: VR026618.D

Acq: 11 Sep 2019 13:10


Tgt Ion:105 Resp: 34252

Ion Ratio Lower Upper

105 100

120 24.3 20.7 31.1



77 18.0 13.1 19.7




Abundance Ion 105.05 (104.75 to 105.75): V

Ion 120.10 (119.80 to 120.80): V

Ion 77.10 (76.80 to 77.80): VR0

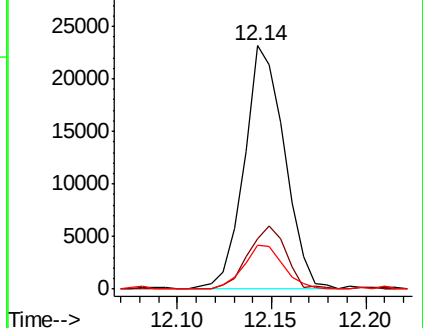



#58

1,1,2,2-Tetrachloroethane

Concen: 0.283 ug/L

RT: 12.40 min Scan# 1762

Delta R.T. 0.00 min

Lab File: VR026618.D

Acq: 11 Sep 2019 13:10

Instrument :

MSVOA_R

ClientSampleId :





Tot Ion: 83 Resp: 4217

Ion Ratio Lower Upper

83 100

85 61.4 45.7 84.9

131 15.2 7.9 11.9#

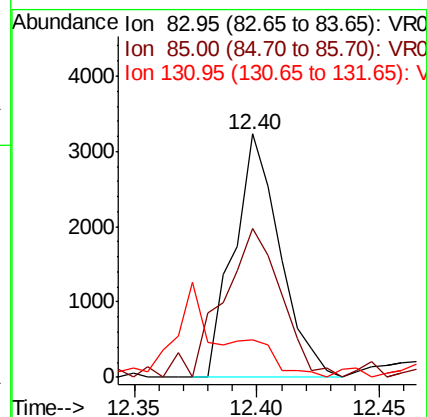

#61

Bromoform

Concen: 0.230 ug/L

RT: 12.03 min Scan# 1701

Delta R.T. 0.01 min

Lab File: VR026618.D

Acq: 11 Sep 2019 13:10




Tgt Ion: 173 Resp: 1337


Ion Ratio Lower Upper

173 100

175 71.0 38.8 58.2#

254 27.5 10.0 15.0#

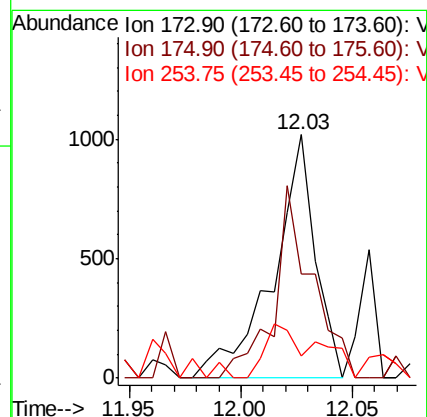

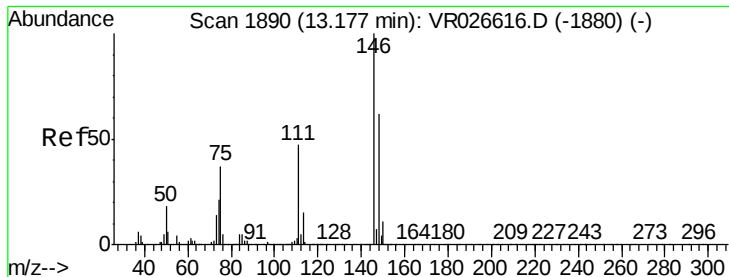

#62

1,3-Dichlorobenzene

Concen: 0.243 ug/L

RT: 13.18 min Scan# 1890

Delta R.T. 0.00 min

Lab File: VR026618.D





Acq: 11 Sep 2019 13:10

Instrument :

MSVOA_R

ClientSampled :

Tot Ion:146	Resp:	13050
Ion	Ratio	Lower Upper
146	100	
111	36.0	32.2 59.8
148	70.6	45.6 84.8

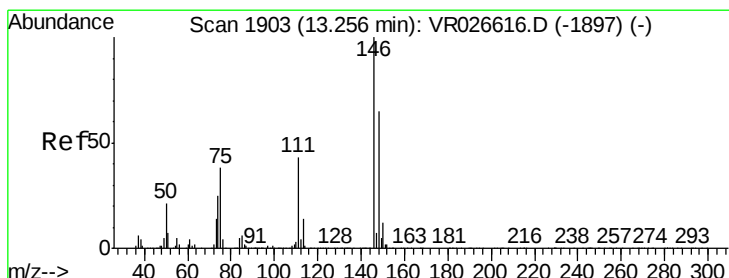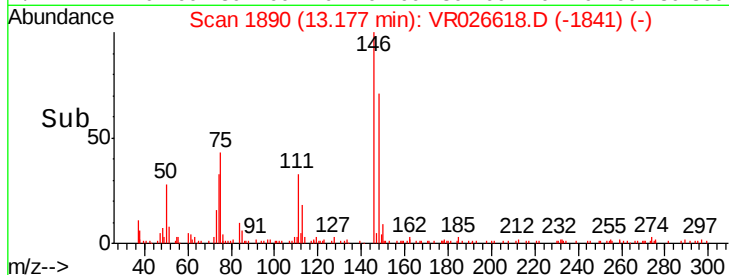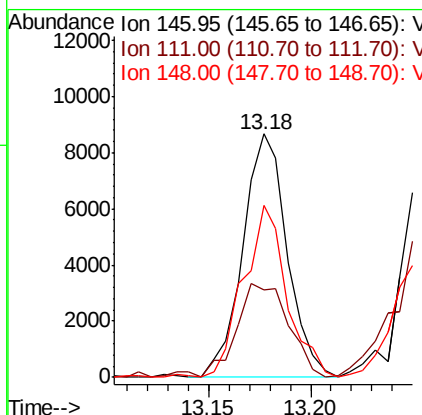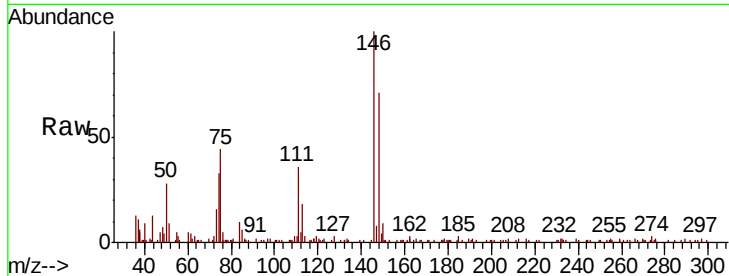

#63

1,4-Dichlorobenzene

Concen: 0.279 ug/L




RT: 13.26 min Scan# 1904


Delta R.T. 0.01 min

Lab File: VR026618.D

Acq: 11 Sep 2019 13:10

Tgt Ion:146	Resp:	14455
Ion	Ratio	Lower Upper
146	100	
111	45.7	33.2 61.7
148	56.4	42.4 78.6


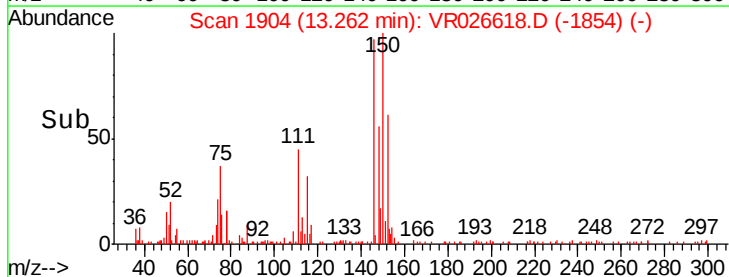
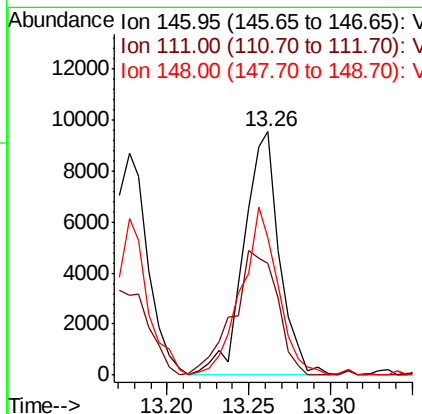
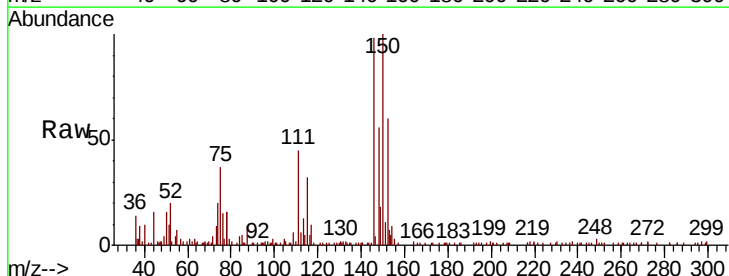




#65
 1,2-Dichlorobenzene
 Concen: 0.284 ug/L
 RT: 13.55 min Scan# 1951
 Delta R.T. 0.00 min
 Lab File: VR026618.D
 Acq: 11 Sep 2019 13:10




Instrument :
 MSVOA_R
 ClientSampled :


Tot Ion	Ratio	Lower	Upper
146	100		
111	51.6	39.3	58.9
148	59.8	49.3	73.9

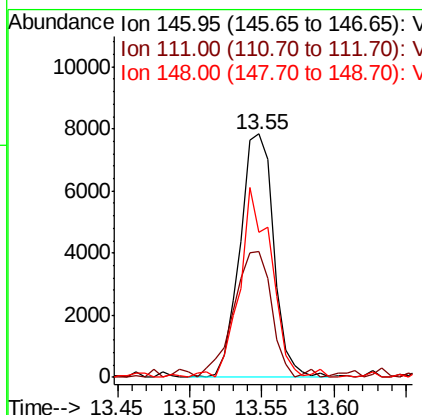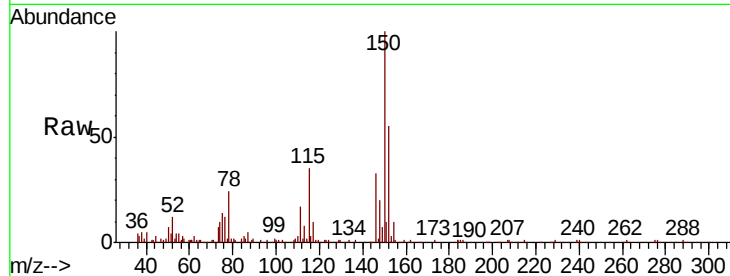

#66
 1,2-Dibromo-3-chloropropane
 Concen: 0.583 ug/L
 RT: 14.16 min Scan# 2052
 Delta R.T. 0.00 min
 Lab File: VR026618.D
 Acq: 11 Sep 2019 13:10

Tgt Ion	Ratio	Lower	Upper
75	100		
155	28.4	50.2	75.4#
157	14.2	74.5	111.7#

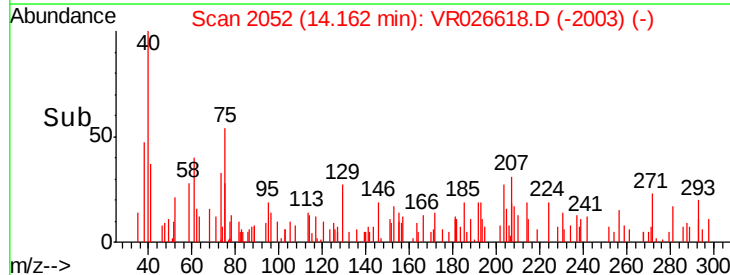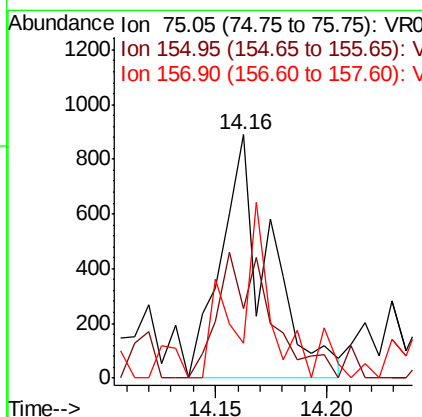




#67
 1,3,5-Trichlorobenzene
 Concen: 0.255 ug/L
 RT: 14.30 min Scan# 2075
 Delta R.T. -0.01 min
 Lab File: VR026618.D
 Acq: 11 Sep 2019 13:10

Instrument :
 MSVOA_R
 ClientSampled :

Tot Ion	Ratio	Lower	Upper
180	100		
182	111.8	75.1	112.7
184	36.4	23.5	35.3
145	33.5	25.8	38.8






Abundance

Ion 180.00 (179.70 to 180.70): V

Ion 182.00 (181.70 to 182.70): V


Ion 184.00 (183.70 to 184.70): V

Ion 145.00 (144.70 to 145.70): V

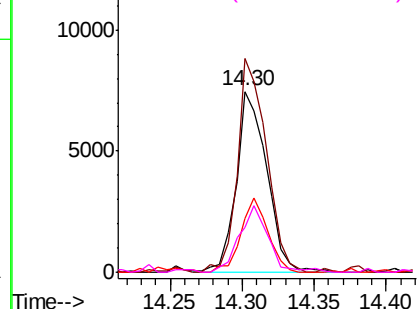

#68
 1,2,4-trichlorobenzene
 Concen: 0.262 ug/L
 RT: 14.80 min Scan# 2157
 Delta R.T. 0.00 min
 Lab File: VR026618.D
 Acq: 11 Sep 2019 13:10

Tgt Ion	Ratio	Lower	Upper
180	100		
182	106.9	77.7	116.5
145	32.8	26.0	39.0






Abundance

Ion 179.90 (179.60 to 180.60): V

Ion 182.00 (181.70 to 182.70): V

Ion 144.95 (144.65 to 145.65): V

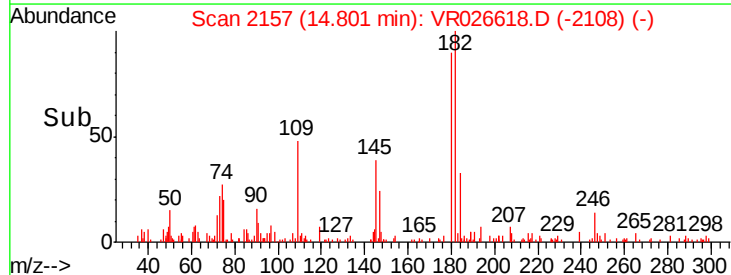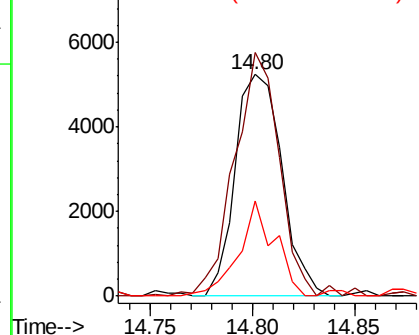



#69

Naphthalene

Concen: 0.216 ug/L

RT: 15.02 min Scan# 2193

Delta R.T. 0.00 min

Lab File: VR026618.D

Acq: 11 Sep 2019 13:10

Instrument :

MSVOA_R

ClientSampled :


Tot Ion:128 Resp: 9669

Ion Ratio Lower Upper

128 100

127 16.4 11.4 17.2




129 15.4 9.0 13.4#



Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

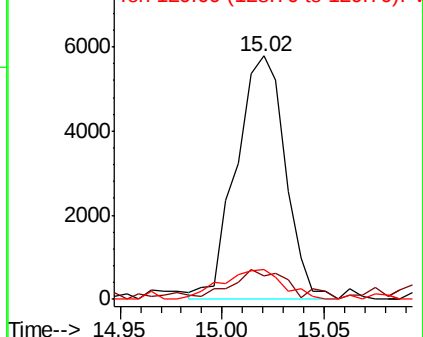

#70

1,2,3-Trichlorobenzene

Concen: 0.270 ug/L

RT: 15.20 min Scan# 2222

Delta R.T. 0.00 min

Lab File: VR026618.D

Acq: 11 Sep 2019 13:10


Tgt Ion:180 Resp: 7201

Ion Ratio Lower Upper

180 100

182 95.8 76.1 114.1

145 37.0 27.4 41.2



Abundance Ion 179.90 (179.60 to 180.60): V

Ion 181.90 (181.60 to 182.60): V

Ion 144.95 (144.65 to 145.65): V

