

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR092718\
Quantitation Report (Qedit)

Data File : VR025872.D
Acq On : 27 Sep 2018 12:29
Operator : SY/MD
Sample : VSTD0.588
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 3 Sample Multiplier: 1




Instrument :
MSVOA_R
ClientSampleId :
VSTD0.588

Manual Integrations
APPROVED

MMDadoda
10/1/2018 11:53:50 AM

10/1/2018 11:53:50 AM

Quant Time: Sep 27 15:06:35 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 27 15:06:01 2018
Response via : Initial Calibration

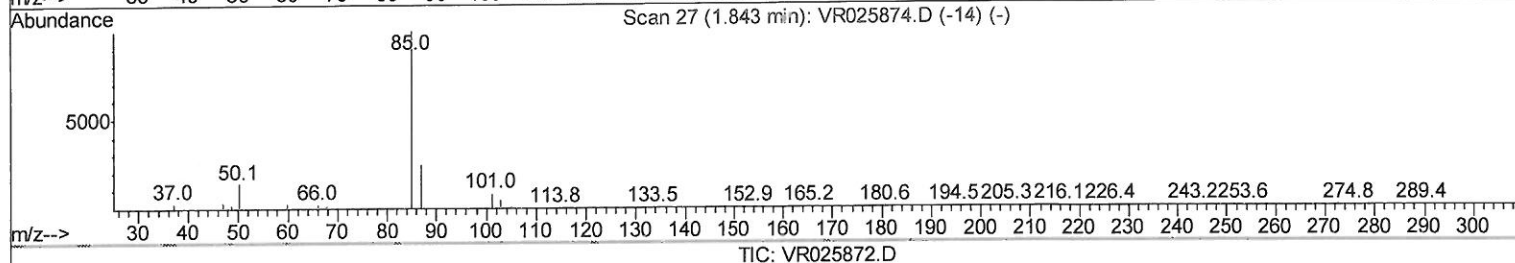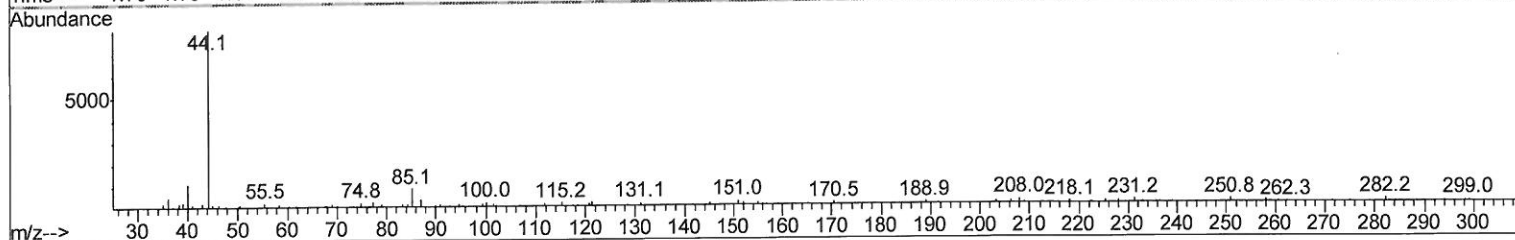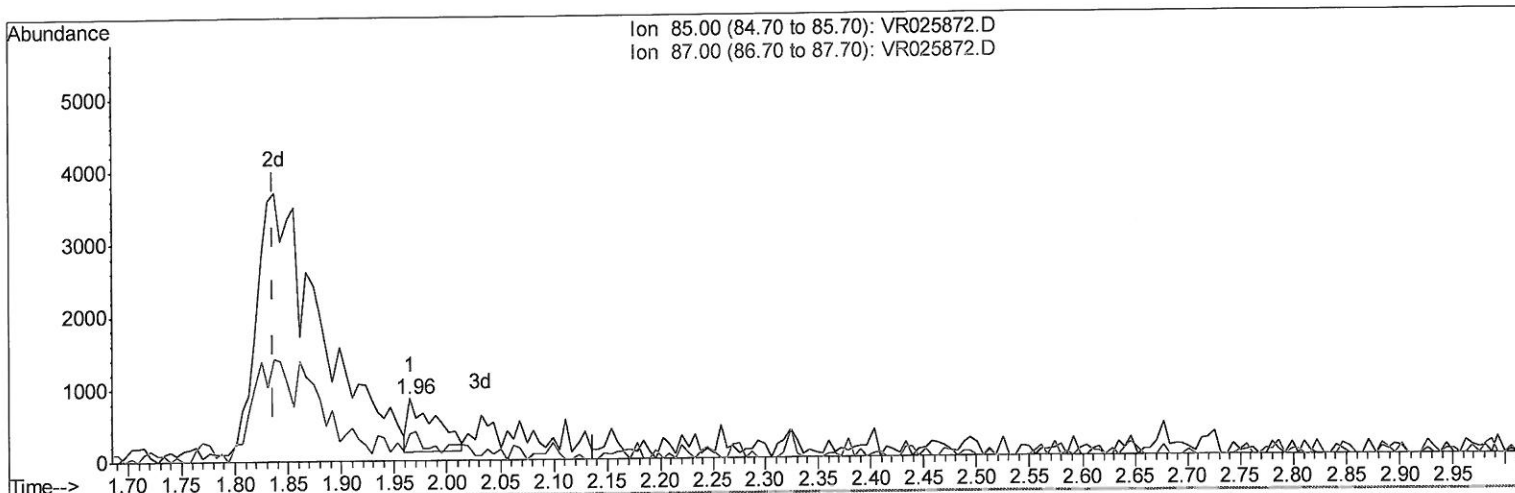

(2) Dichlorodifluoromethane (T)

1.965min (+0.128) 0.03ug/L

response 1338

Ion	Exp%	Act%
85.00	100	100
87.00	31.40	30.27
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR092718\
Quantitation Report (Qedit)

Data File : VR025872.D
Acq On : 27 Sep 2018 12:29
Operator : SY/MD
Sample : VSTD0.588
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 3 Sample Multiplier: 1




Instrument :
MSVOA_R
ClientSampleId :
VSTD0.588

Manual Integrations
APPROVED

MMDadoda
10/1/2018 11:53:50 AM

10/1/2018 11:53:50 AM

Quant Time: Sep 27 15:06:35 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 27 15:06:01 2018
Response via : Initial Calibration

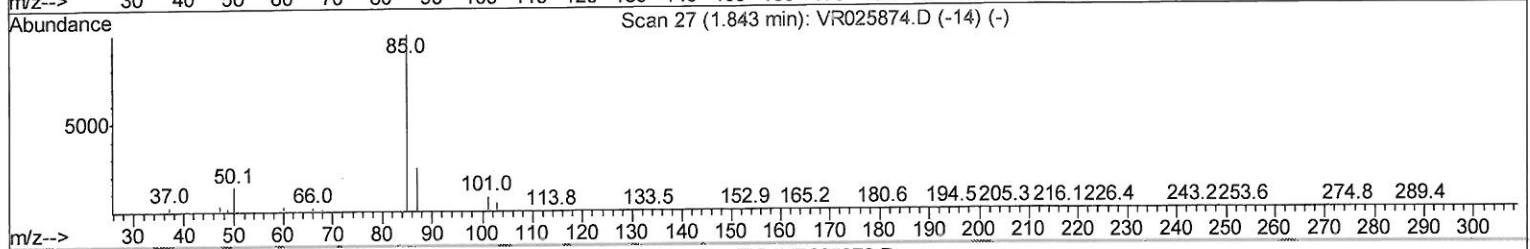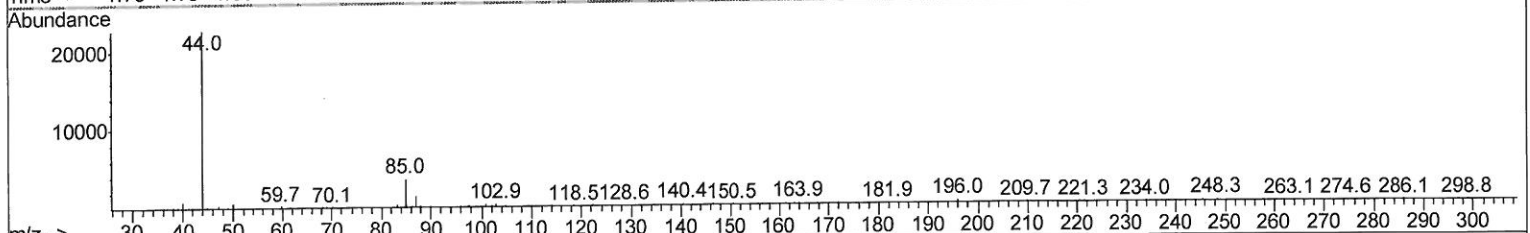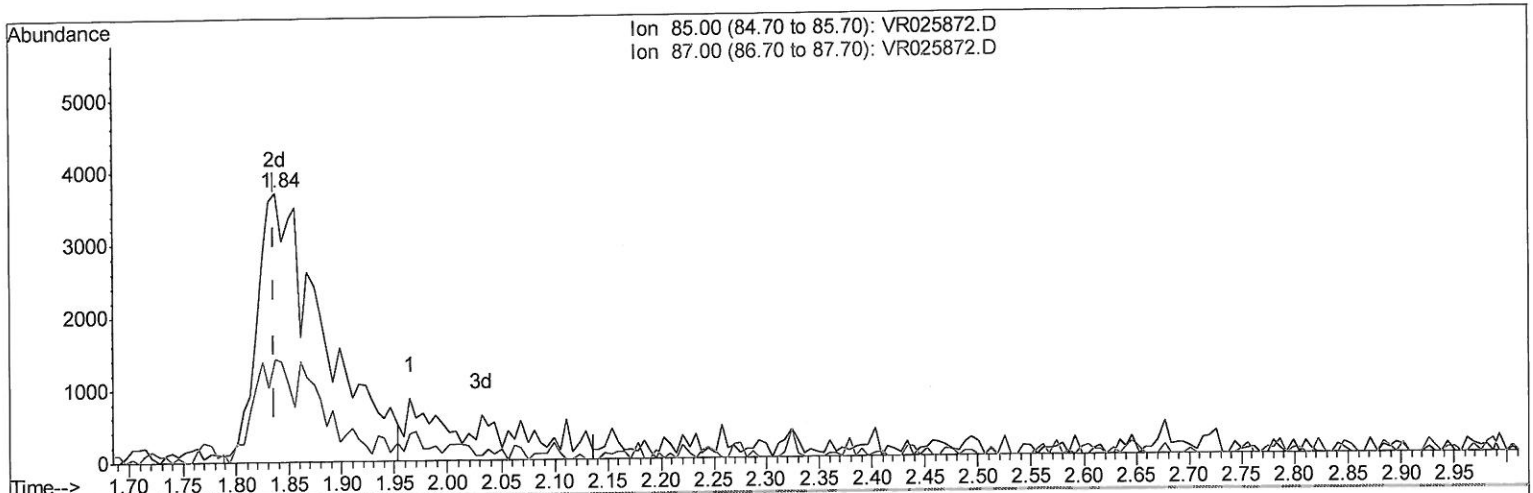

TIC: VR025872.D

(2) Dichlorodifluoromethane (T)

1.837min (+0.000) 0.31ug/L m³ 10/01/18 SY

response 16171

Ion	Exp%	Act%
85.00	100	100
87.00	31.40	2.50#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR092718\
Quantitation Report (Qedit)

Data File : VR025872.D
Acq On : 27 Sep 2018 12:29
Operator : SY/MD
Sample : VSTD0.588
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 3 Sample Multiplier: 1




Instrument :
MSVOA_R
ClientSampleId :
VSTD0.588

Manual Integrations
APPROVED

MMDadoda
10/1/2018 11:53:50 AM

10/1/2018 11:53:50 AM

Quant Time: Sep 27 15:06:35 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 27 15:06:01 2018
Response via : Initial Calibration

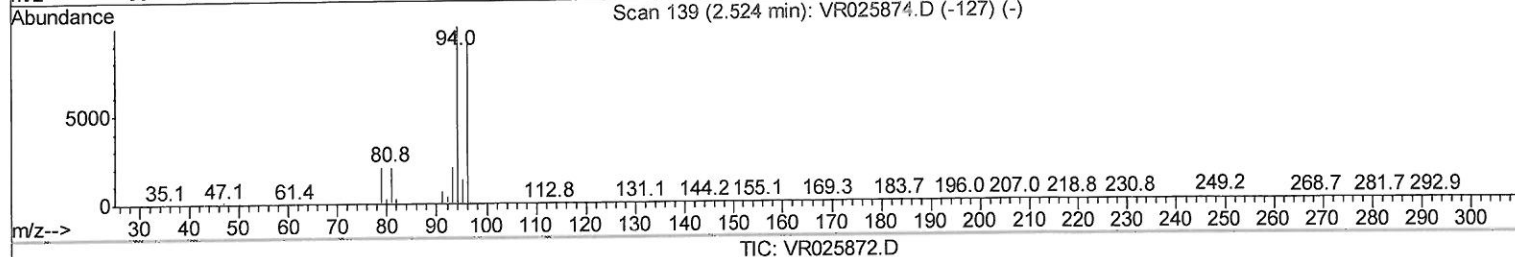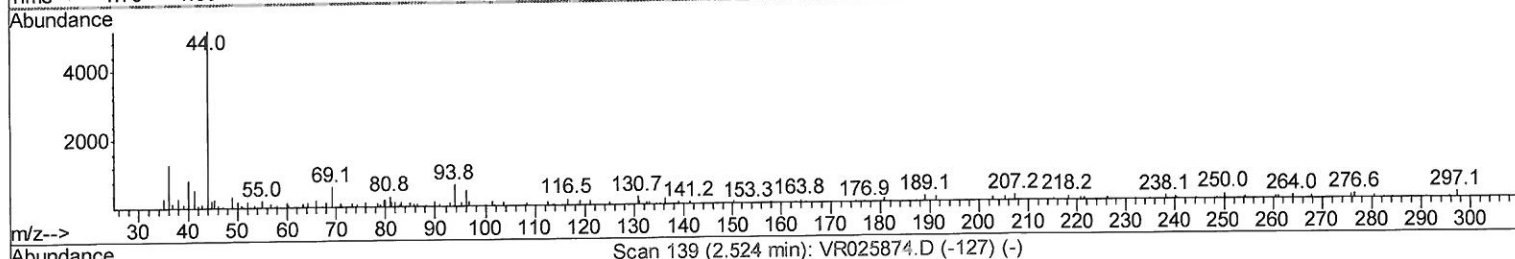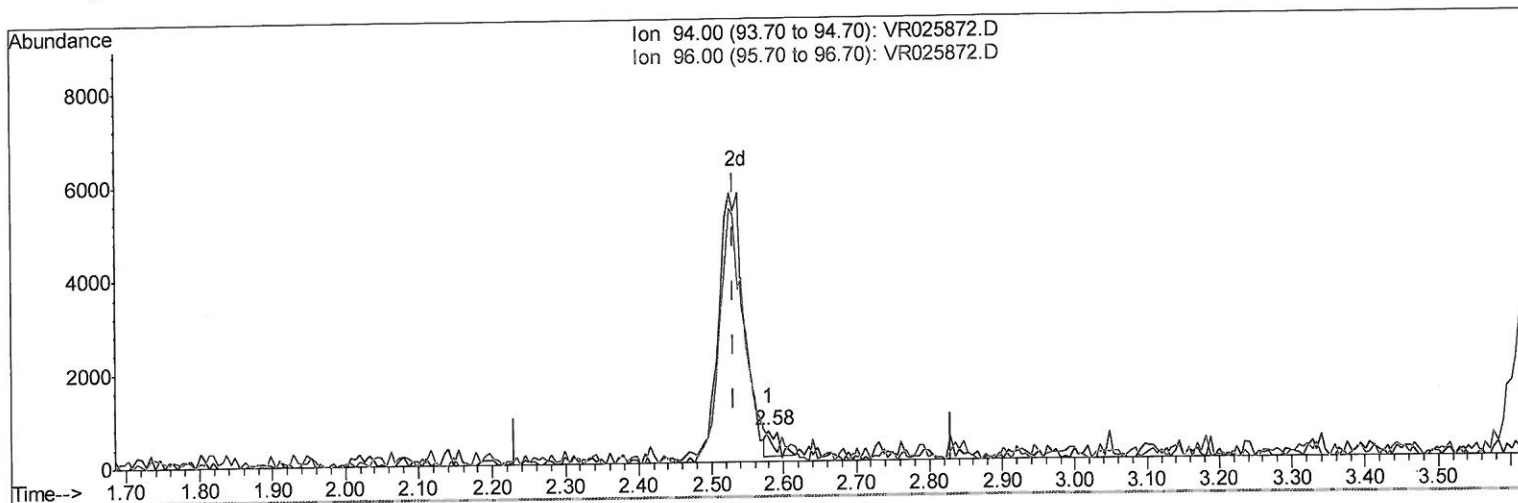

(6) Bromomethane (T)

2.579min (+0.049) 0.02ug/L

response 630

Ion	Exp%	Act%
94.00	100	100
96.00	94.50	107.06
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR092718\
Quantitation Report (Qedit)

Data File : VR025872.D
Acq On : 27 Sep 2018 12:29
Operator : SY/MD
Sample : VSTD0.588
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 3 Sample Multiplier: 1




Instrument :
MSVOA_R
ClientSampleId :
VSTD0.588

Manual Integrations
APPROVED

MMDadoda
10/1/2018 11:53:50 AM

10/1/2018 11:53:50 AM

Quant Time: Sep 27 15:06:35 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 27 15:06:01 2018
Response via : Initial Calibration

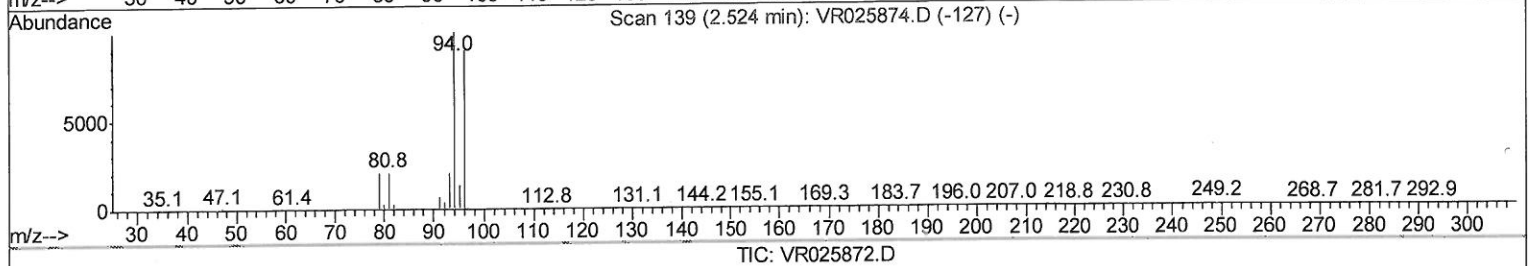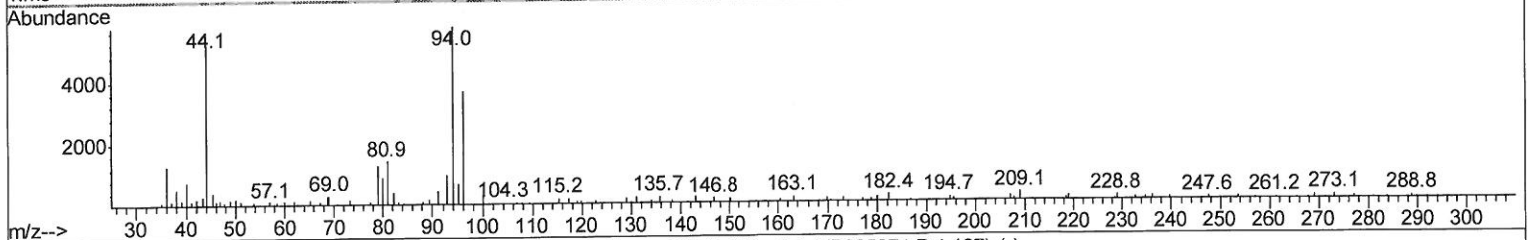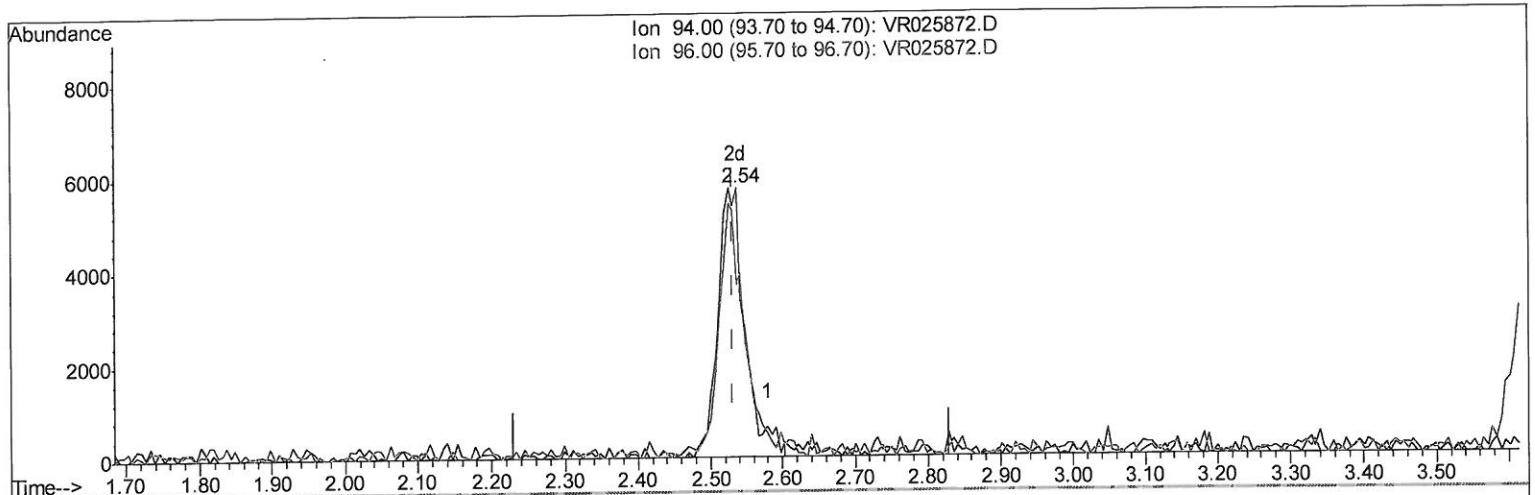

(6) Bromomethane (T)

2.537min (+0.006) 0.50ug/L m) 10/1/18 Jy

response 15412

Ion	Exp%	Act%
94.00	100	100
96.00	94.50	63.99#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR092718\
Quantitation Report (Qedit)

Data File : VR025872.D
Acq On : 27 Sep 2018 12:29
Operator : SY/MD
Sample : VSTD0.588
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 3 Sample Multiplier: 1




Instrument :
MSVOA_R
ClientSampleId :
VSTD0.588

Manual Integrations
APPROVED

MMDadoda
10/1/2018 11:53:50 AM

10/1/2018 11:53:50 AM

Quant Time: Sep 27 15:06:35 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 27 15:06:01 2018
Response via : Initial Calibration

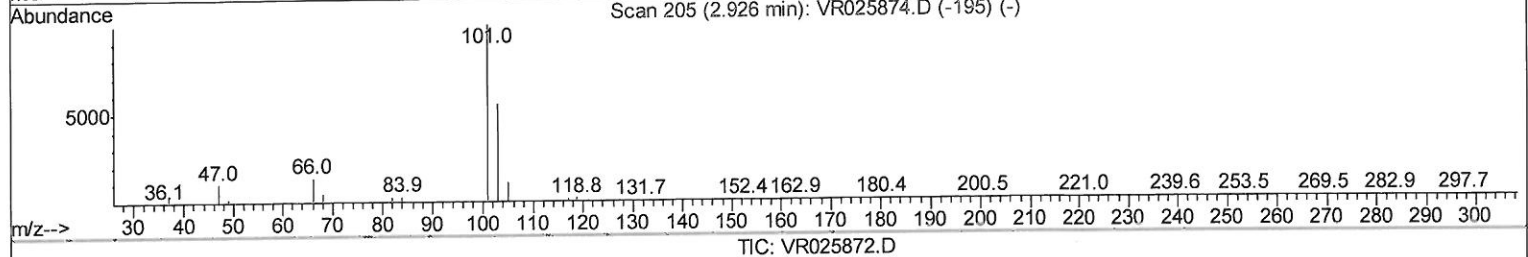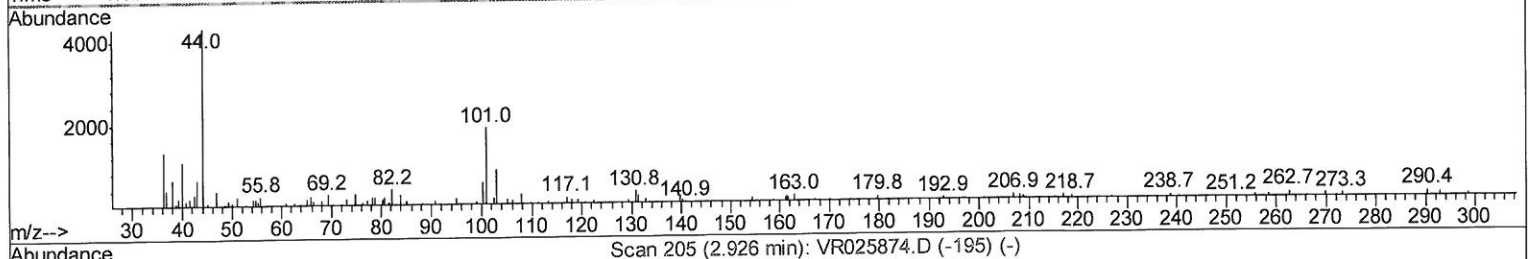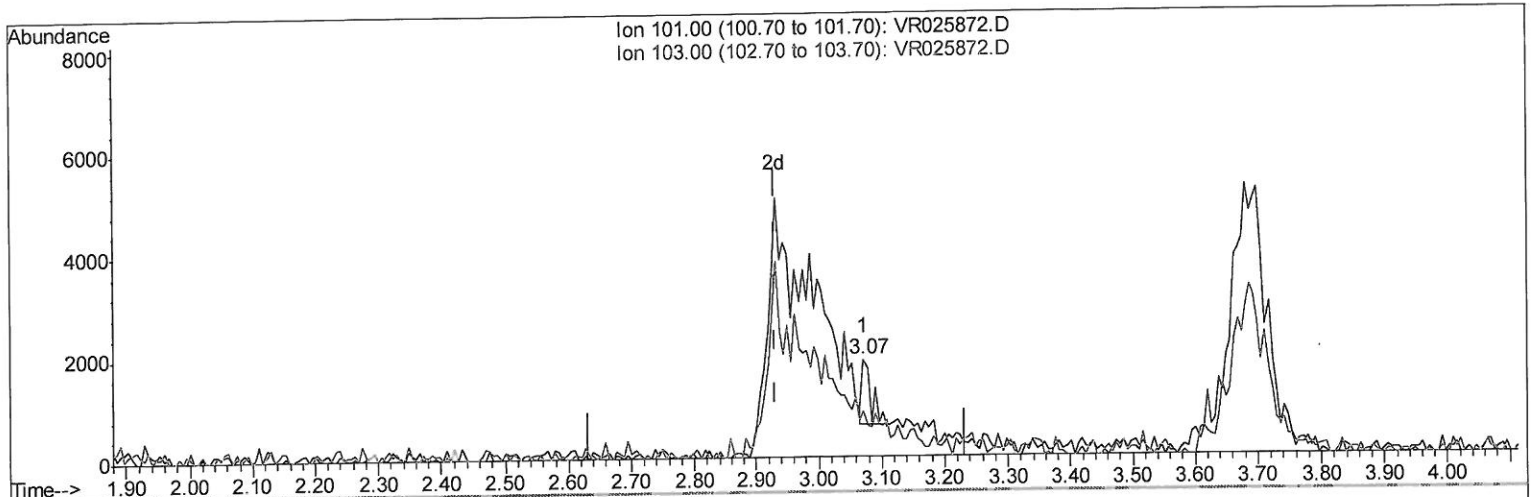

(9) Trichlorofluoromethane (T)

3.072min (+0.140) 0.02ug/L

response 1260

Ion	Exp%	Act%
101.00	100	100
103.00	27.60	29.76
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR092718\
Quantitation Report (Qedit)

Data File : VR025872.D
Acq On : 27 Sep 2018 12:29
Operator : SY/MD
Sample : VSTD0.588
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 3 Sample Multiplier: 1




Instrument :
MSVOA_R
ClientSampleId :
VSTD0.588

Manual Integrations
APPROVED

MMDadoda
10/1/2018 11:53:50 AM

10/1/2018 11:53:50 AM

Quant Time: Sep 27 15:06:35 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 27 15:06:01 2018
Response via : Initial Calibration

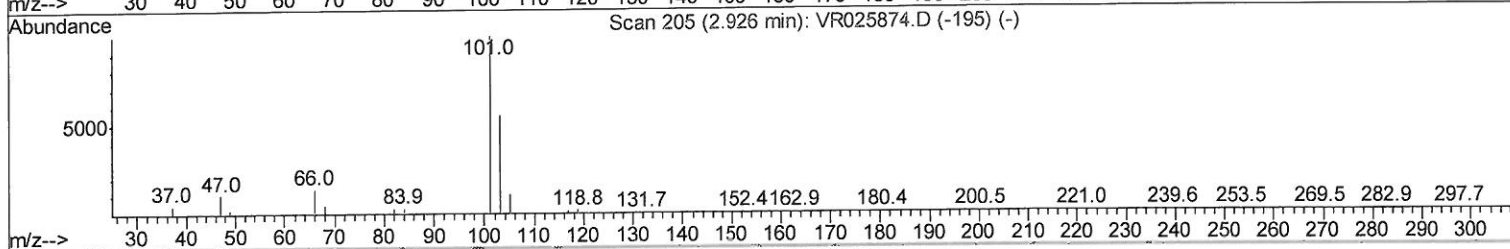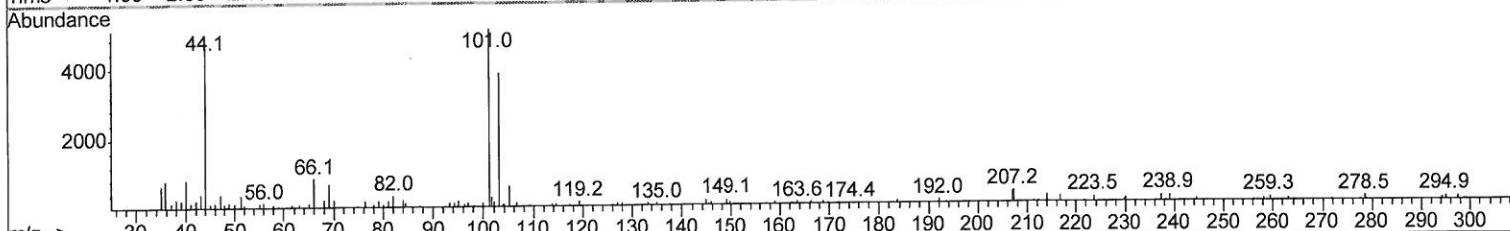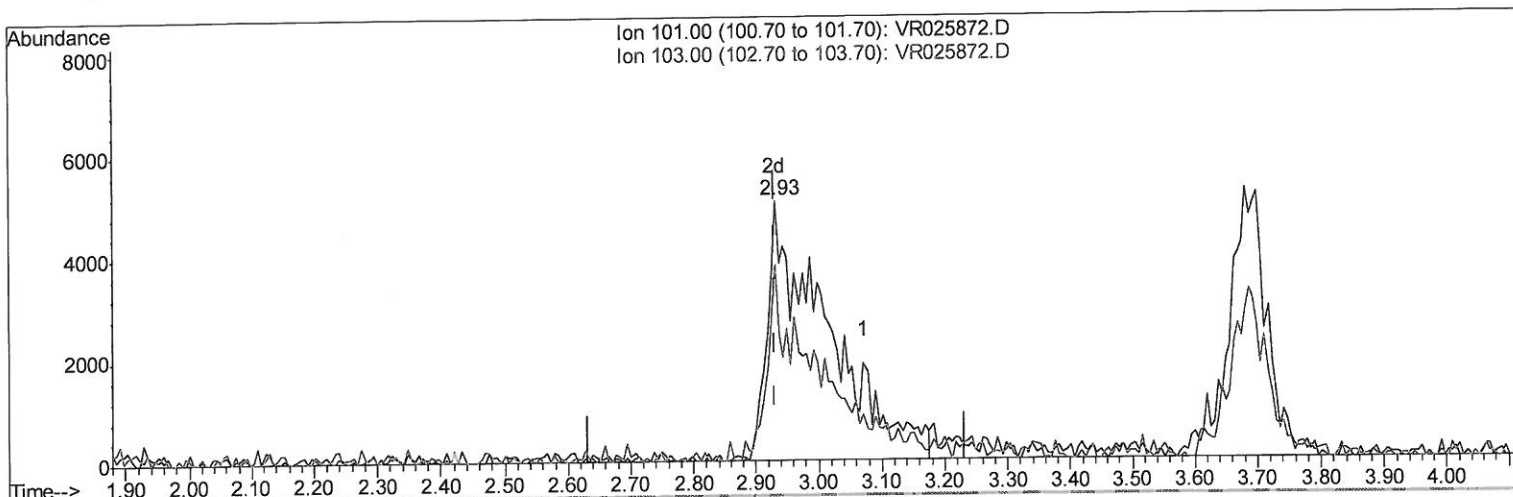

TIC: VR025872.D

(9) Trichlorofluoromethane (T)

2.932min (+0.000) 0.49ug/L m) 10/01/18 SY

response 33293

Ion	Exp%	Act%
101.00	100	100
103.00	27.60	1.13#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR092718\
Quantitation Report (Qedit)

Data File : VR025872.D
Acq On : 27 Sep 2018 12:29
Operator : SY/MD
Sample : VSTD0.588
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 3 Sample Multiplier: 1




Instrument :
MSVOA_R
ClientSampleId :
VSTD0.588

Manual Integrations
APPROVED

MMDadoda
10/1/2018 11:53:50 AM

10/1/2018 11:53:50 AM

Quant Time: Sep 27 15:06:35 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 27 15:06:01 2018
Response via : Initial Calibration

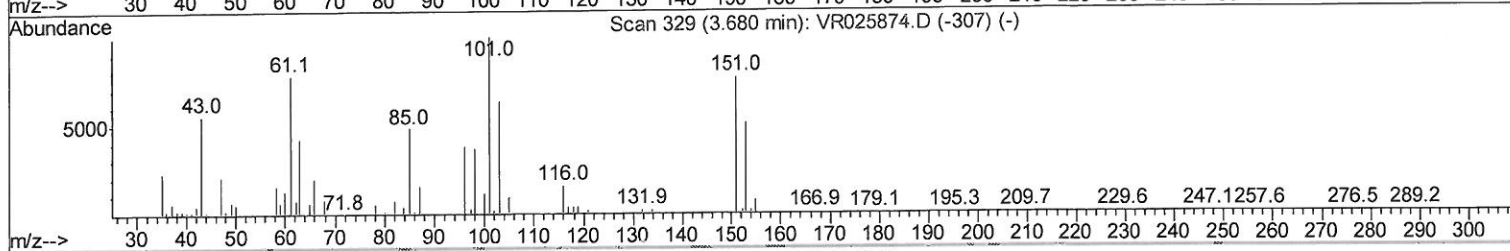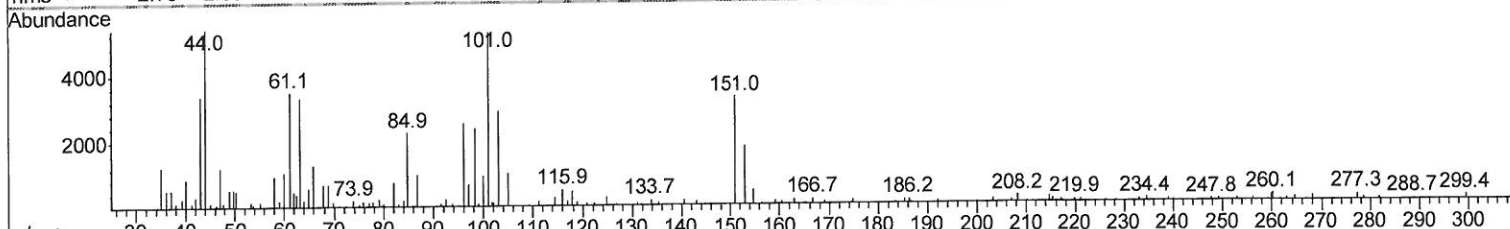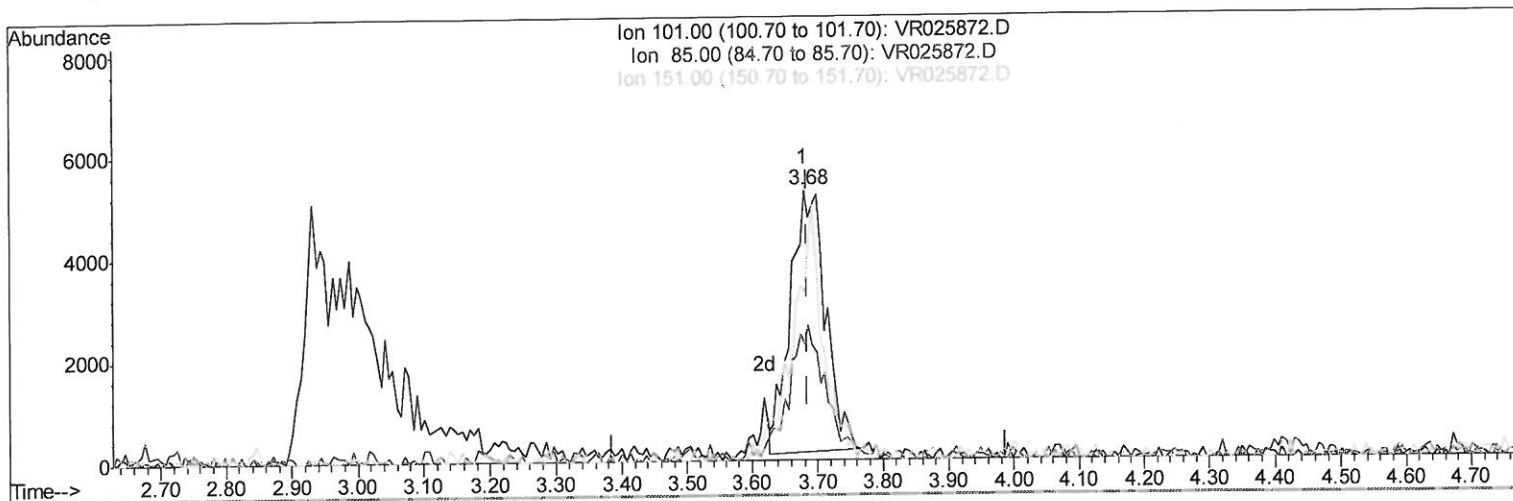

(10) 1,1,2-Trichloro-1,2,2-trifluoroethane (T)

3.680min (-0.006) 0.46ug/L

response 18942

Ion	Exp%	Act%
101.00	100	100
85.00	47.80	55.11
151.00	73.00	83.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR092718\
Quantitation Report (Qedit)

Data File : VR025872.D
Acq On : 27 Sep 2018 12:29
Operator : SY/MD
Sample : VSTD0.588
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 3 Sample Multiplier: 1




Instrument :
MSVOA_R
ClientSampleId :
VSTD0.588

Manual Integrations
APPROVED

MMDadoda
10/1/2018 11:53:50 AM

10/1/2018 11:53:50 AM

Quant Time: Sep 27 15:06:35 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 27 15:06:01 2018
Response via : Initial Calibration

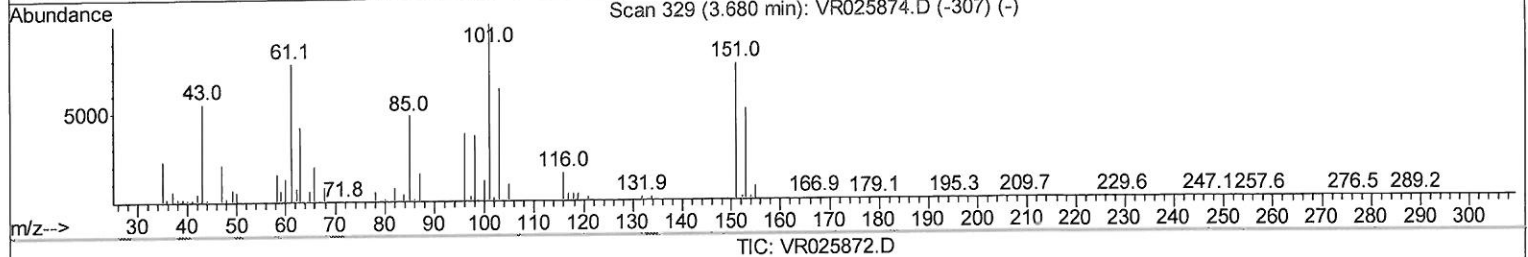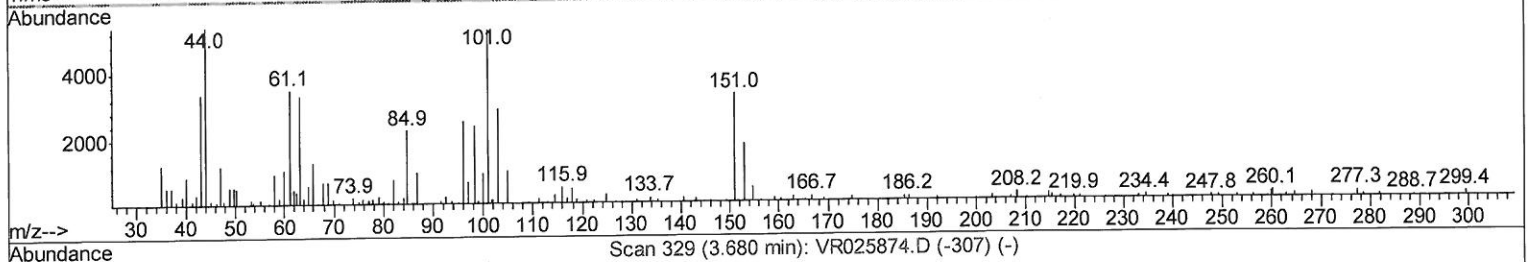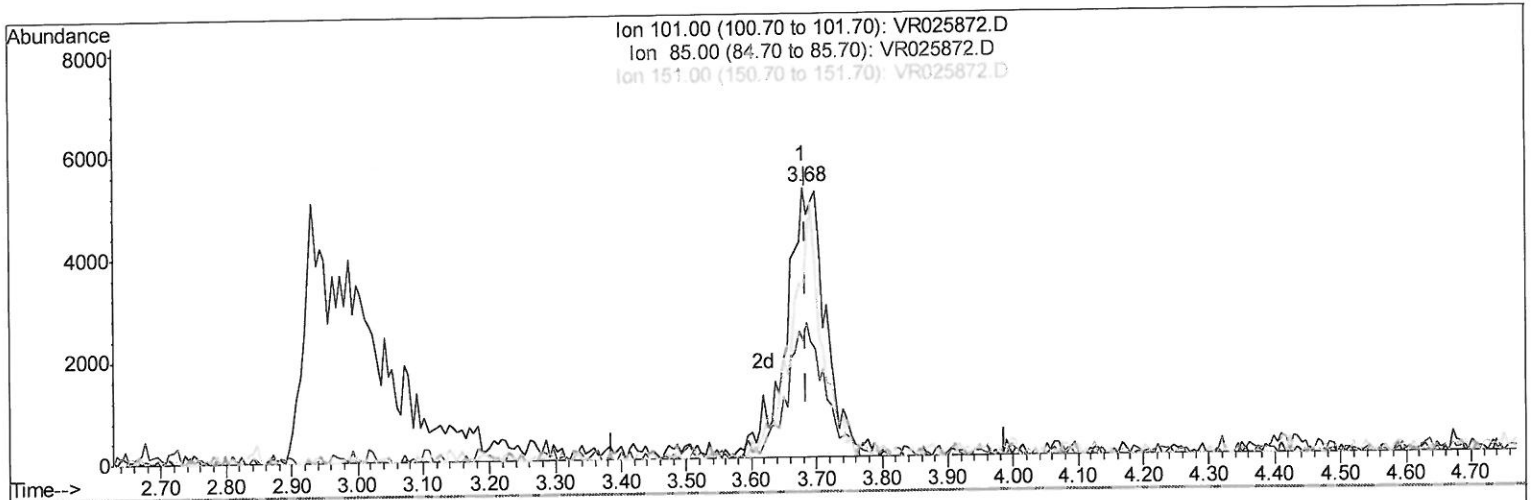

(10) 1,1,2-Trichloro-1,2,2-trifluoroethane (T)

3.680min (-0.006) 0.52ug/L m

> 10/01/18 Sy

response 21630

Ion	Exp%	Act%
101.00	100	100
85.00	47.80	48.26
151.00	73.00	72.68
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR092718\
Quantitation Report (Qedit)




Data File : VR025872.D
Acq On : 27 Sep 2018 12:29
Operator : SY/MD
Sample : VSTD0.588
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
VSTD0.588

Manual Integrations
APPROVED

MMDadoda
10/1/2018 11:53:50 AM

Quant Time: Sep 27 15:06:35 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 27 15:06:01 2018
Response via : Initial Calibration

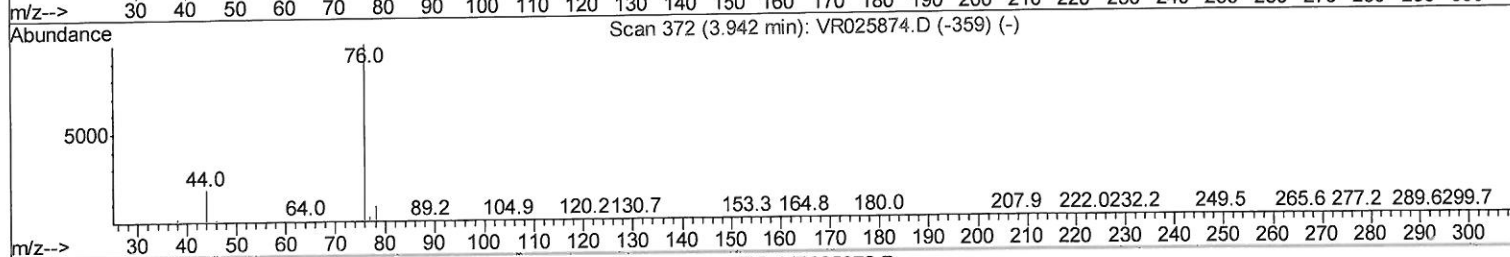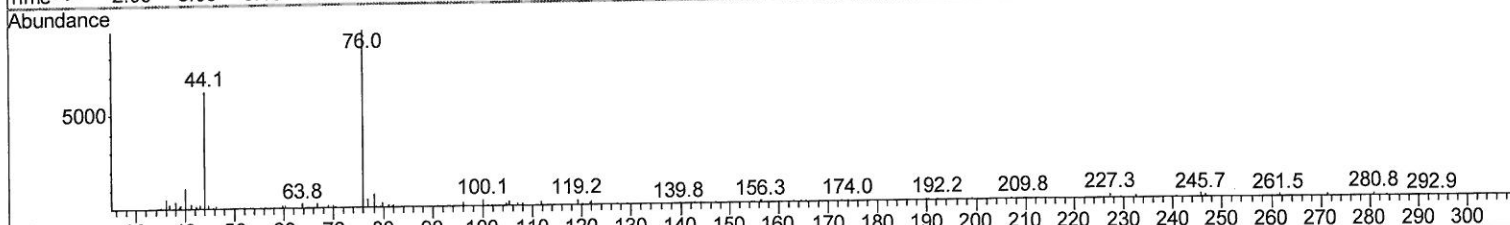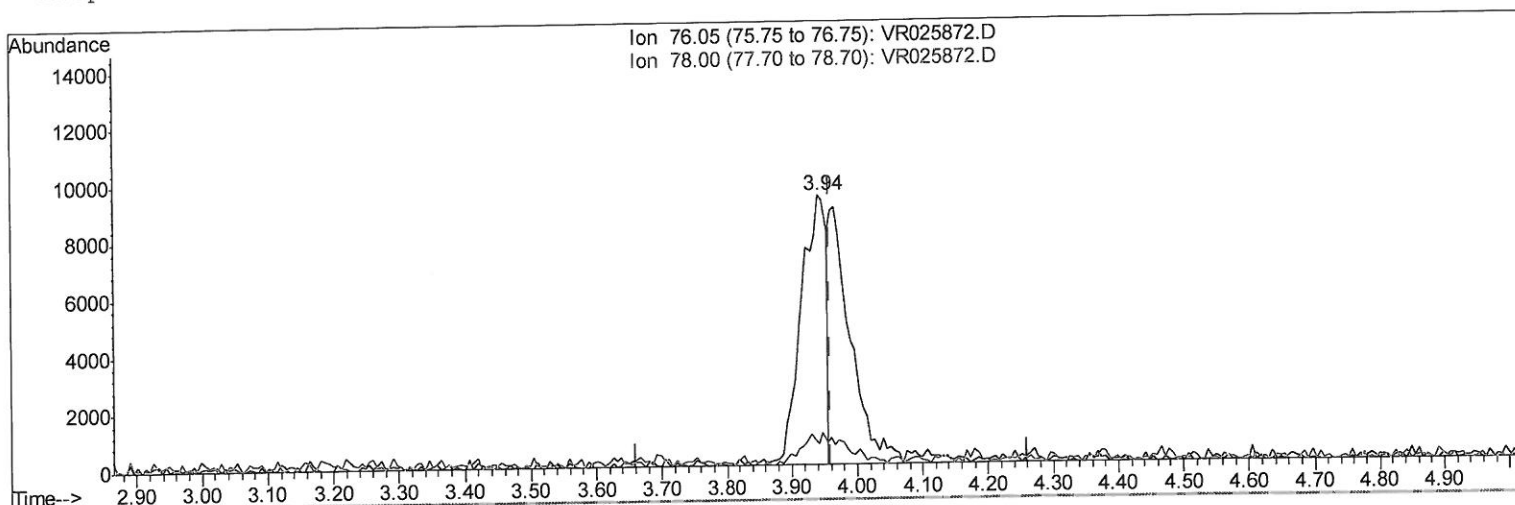

TIC: VR025872.D

(14) Carbon disulfide (T)

3.942min (-0.018) 0.20ug/L

response 24812

Ion	Exp%	Act%
76.05	100	100
78.00	8.80	8.96
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR092718\
Quantitation Report (Qedit)

Data File : VR025872.D
Acq On : 27 Sep 2018 12:29
Operator : SY/MD
Sample : VSTD0.588
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 3 Sample Multiplier: 1




Instrument :
MSVOA_R
ClientSampleId :
VSTD0.588

Manual Integrations
APPROVED

MMDadoda
10/1/2018 11:53:50 AM

10/1/2018 11:53:50 AM

Quant Time: Sep 27 15:06:35 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 27 15:06:01 2018
Response via : Initial Calibration

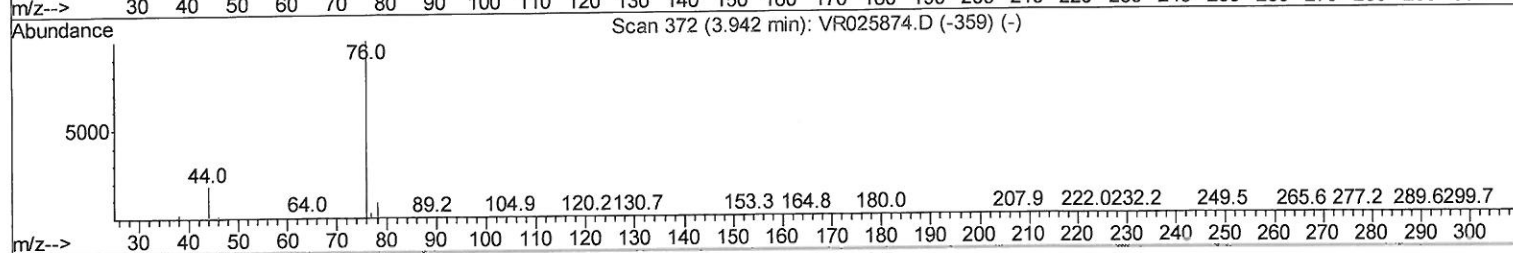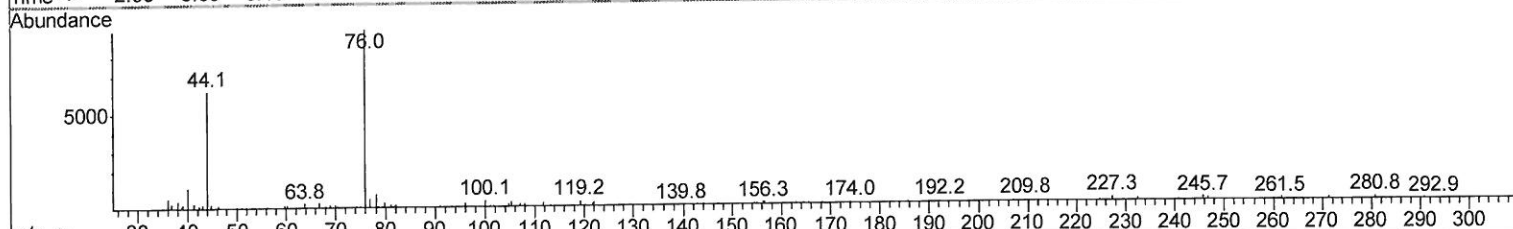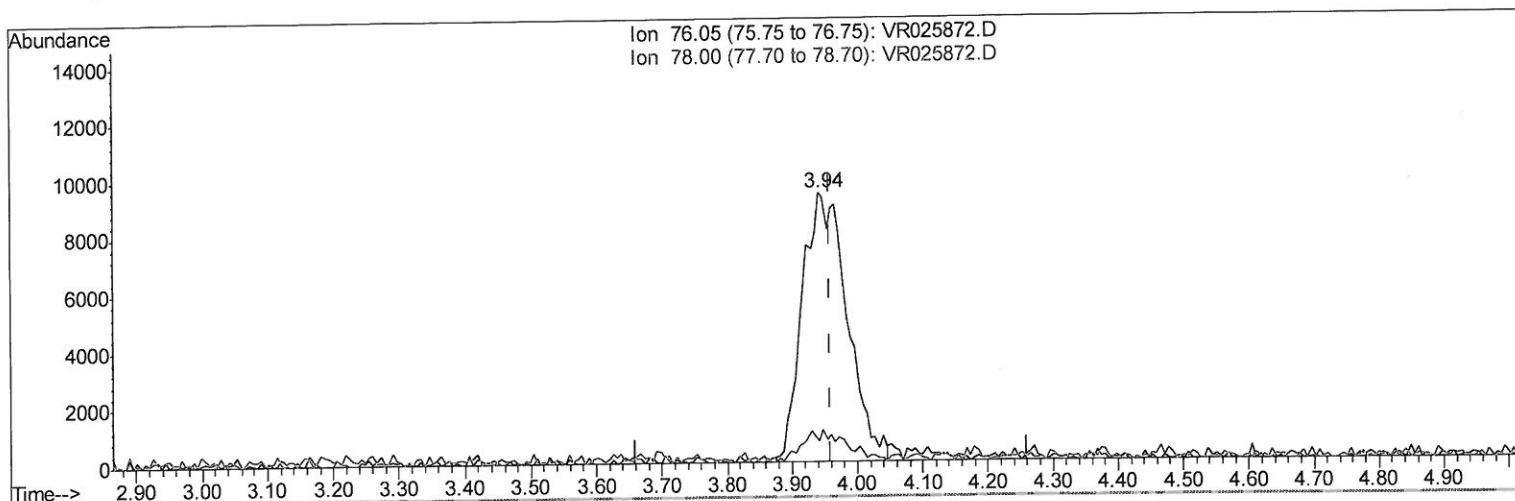

TIC: VR025872.D

(14) Carbon disulfide (T)

3.942min (-0.018) 0.36ug/L m

>10/01/18 SY

response 44810

Ion	Exp%	Act%
76.05	100	100
78.00	8.80	7.92
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR092718\
Quantitation Report (Qedit)

Data File : VR025872.D
Acq On : 27 Sep 2018 12:29
Operator : SY/MD
Sample : VSTD0.588
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 3 Sample Multiplier: 1




Instrument :
MSVOA_R
ClientSampleId :
VSTD0.588

Manual Integrations
APPROVED

MMDadoda
10/1/2018 11:53:50 AM

10/1/2018 11:53:50 AM

Quant Time: Sep 27 15:06:35 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 27 15:06:01 2018
Response via : Initial Calibration

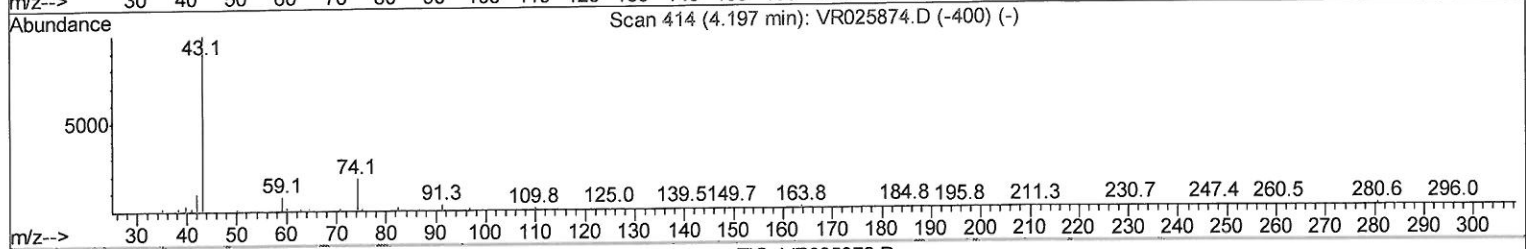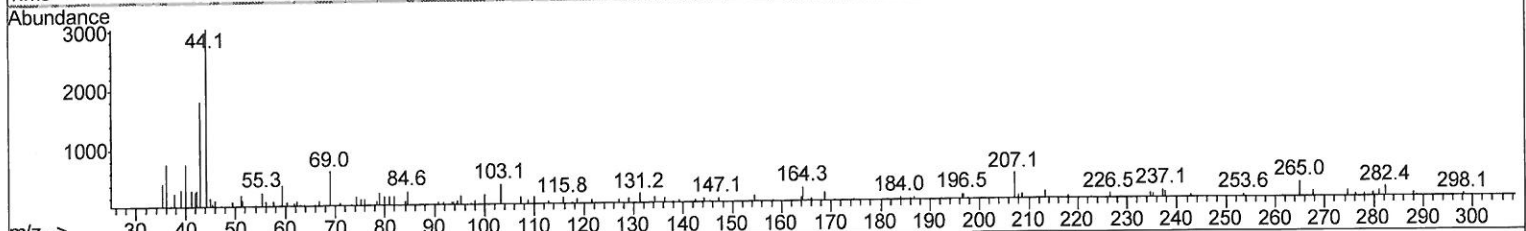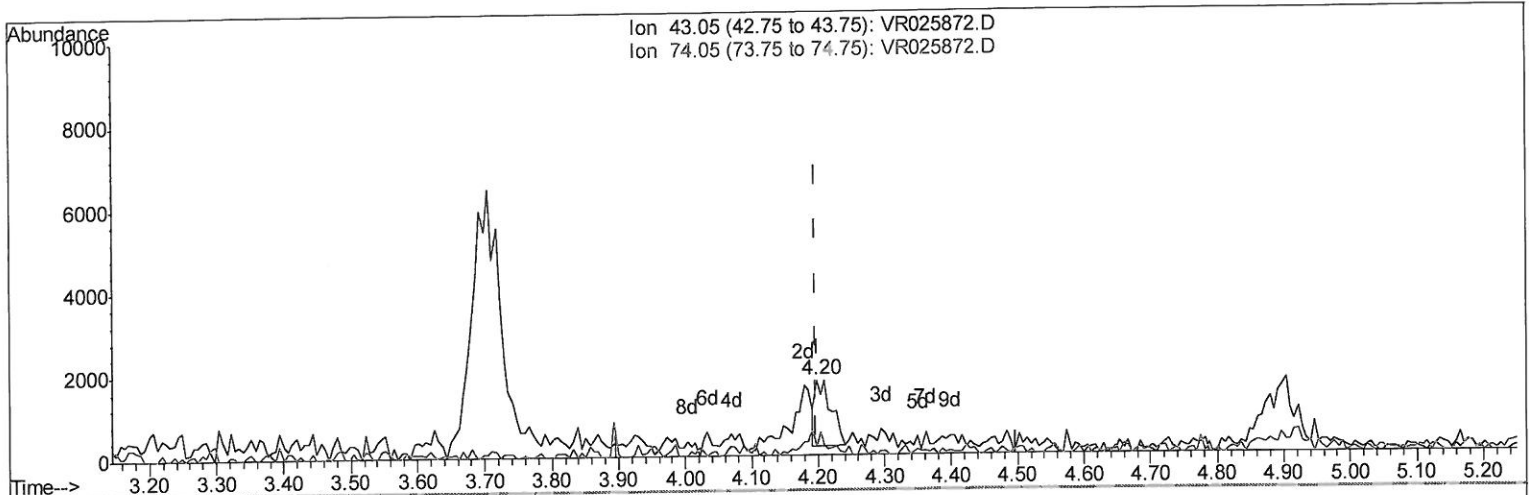

(15) Methyl Acetate (T)
4.198min (+0.000) 0.25ug/L
response 2607

Ion	Exp%	Act%
43.05	100	100
74.05	23.70	50.40#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR092718\
Quantitation Report (Qedit)

Data File : VR025872.D
Acq On : 27 Sep 2018 12:29
Operator : SY/MD
Sample : VSTD0.588
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 3 Sample Multiplier: 1




Instrument :
MSVOA_R
ClientSampleId :
VSTD0.588

Manual Integrations
APPROVED

MMDadoda
10/1/2018 11:53:50 AM

10/1/2018 11:53:50 AM

Quant Time: Sep 27 15:06:35 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 27 15:06:01 2018
Response via : Initial Calibration

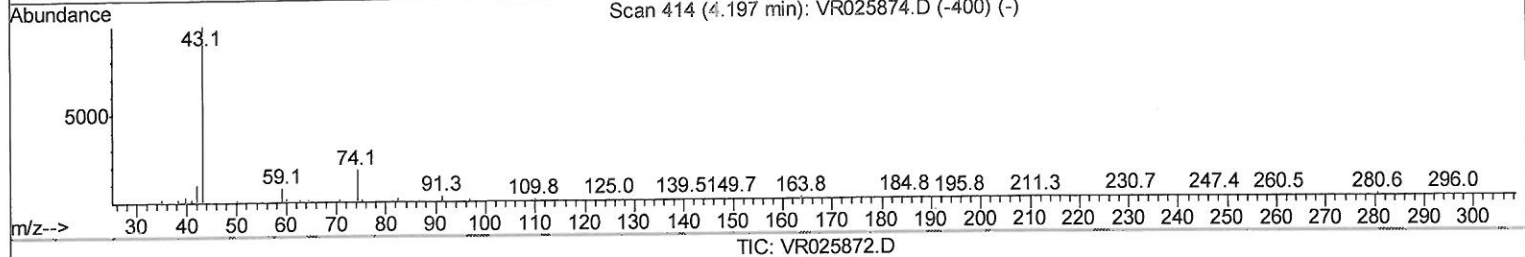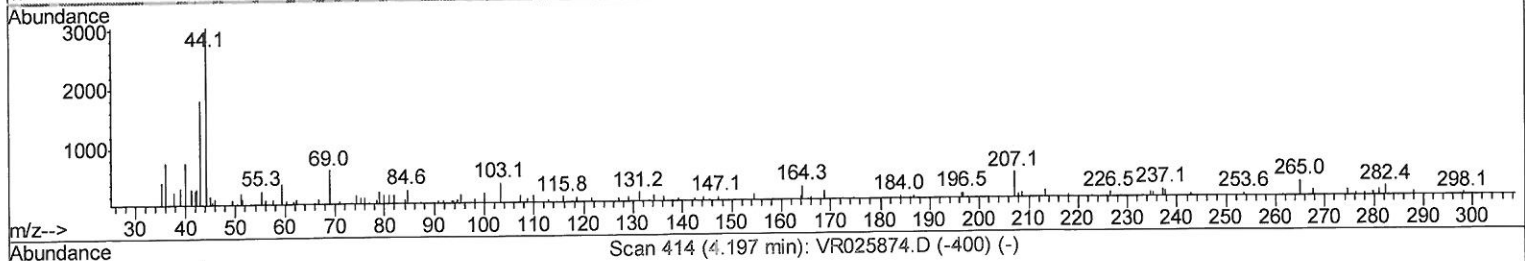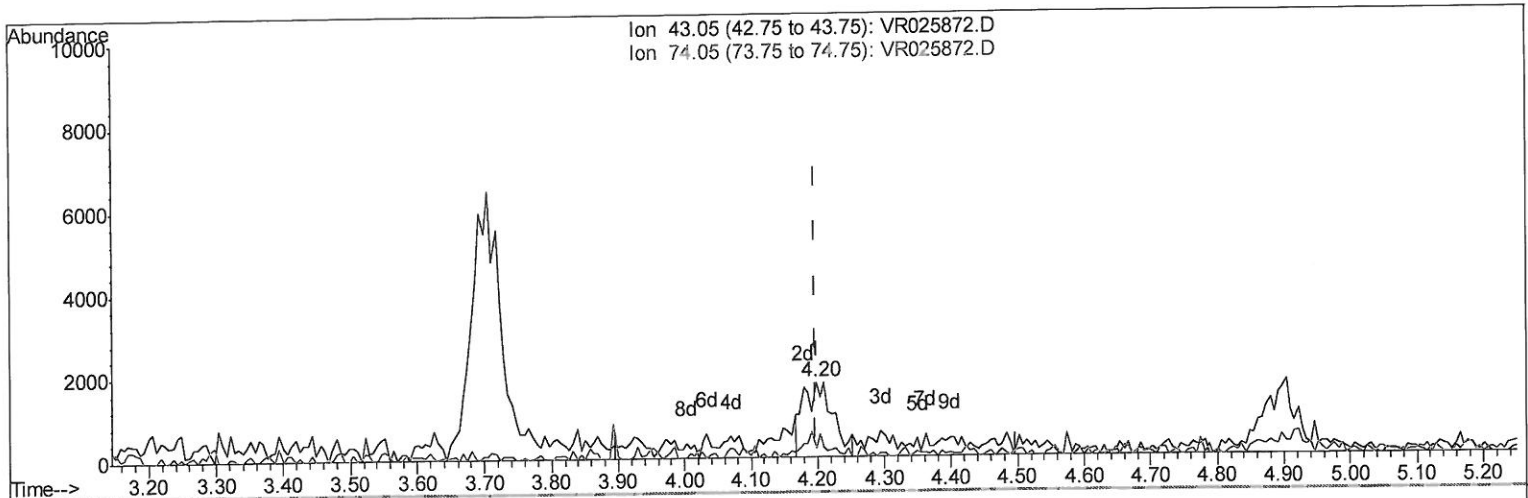

(15) Methyl Acetate (T)

4.198min (+0.000) 0.54ug/L m

2010/01/18 Jy

response 5552

Ion	Exp%	Act%
43.05	100	100
74.05	23.70	23.67
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR092718\
Quantitation Report (Qedit)




Data File : VR025872.D
Acq On : 27 Sep 2018 12:29
Operator : SY/MD
Sample : VSTD0.588
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
VSTD0.588

Manual Integrations
APPROVED

MMDadoda
10/1/2018 11:53:50 AM

Quant Time: Sep 27 15:06:35 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 27 15:06:01 2018
Response via : Initial Calibration

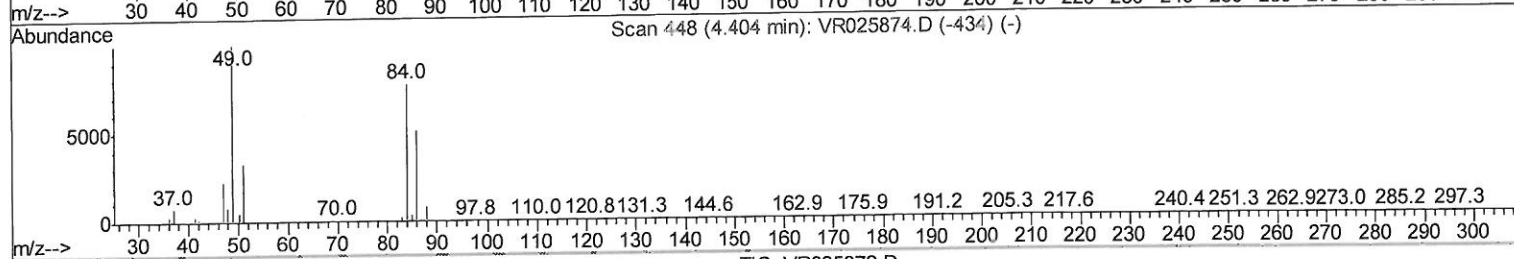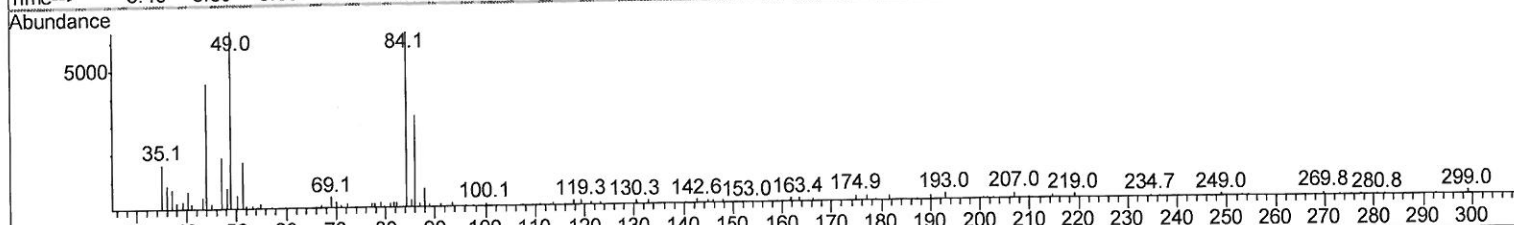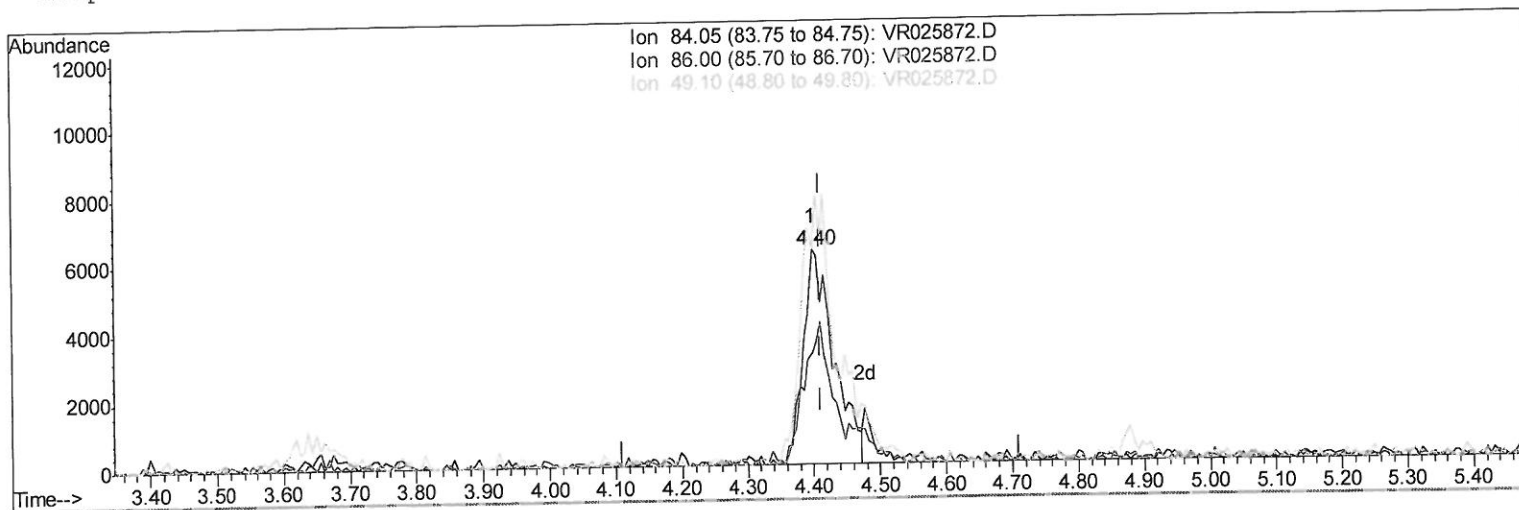

(16) Methylene chloride (T)

4.398min (-0.012) 0.51ug/L

response 20265

Ion	Exp%	Act%
84.05	100	100
86.00	61.60	52.21
49.10	136.40	101.35
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR092718\
Quantitation Report (Qedit)

Data File : VR025872.D
Acq On : 27 Sep 2018 12:29
Operator : SY/MD
Sample : VSTD0.588
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 3 Sample Multiplier: 1




Instrument :
MSVOA_R
ClientSampleId :
VSTD0.588

Manual Integrations
APPROVED

MMDadoda
10/1/2018 11:53:50 AM

10/1/2018 11:53:50 AM

Quant Time: Sep 27 15:06:35 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 27 15:06:01 2018
Response via : Initial Calibration

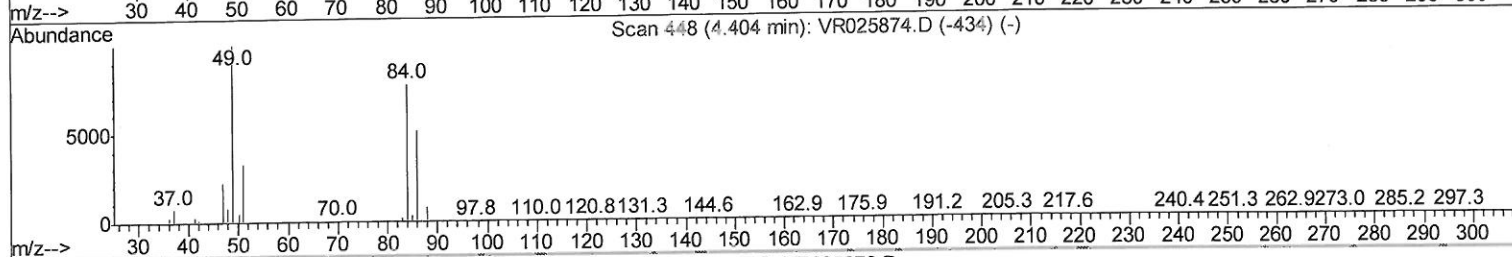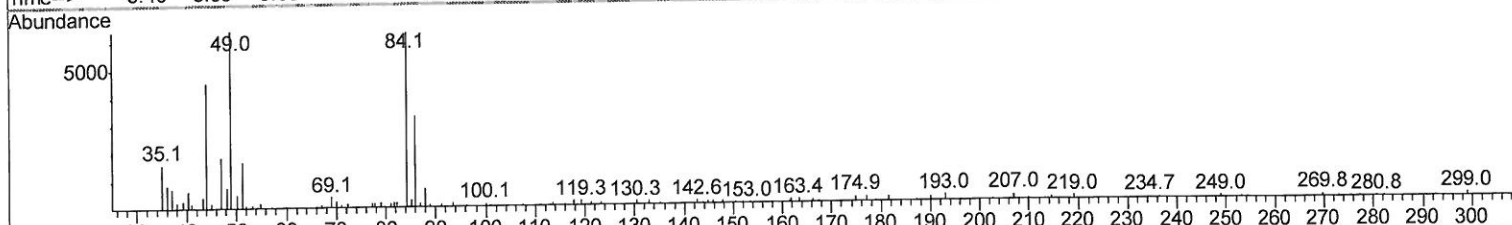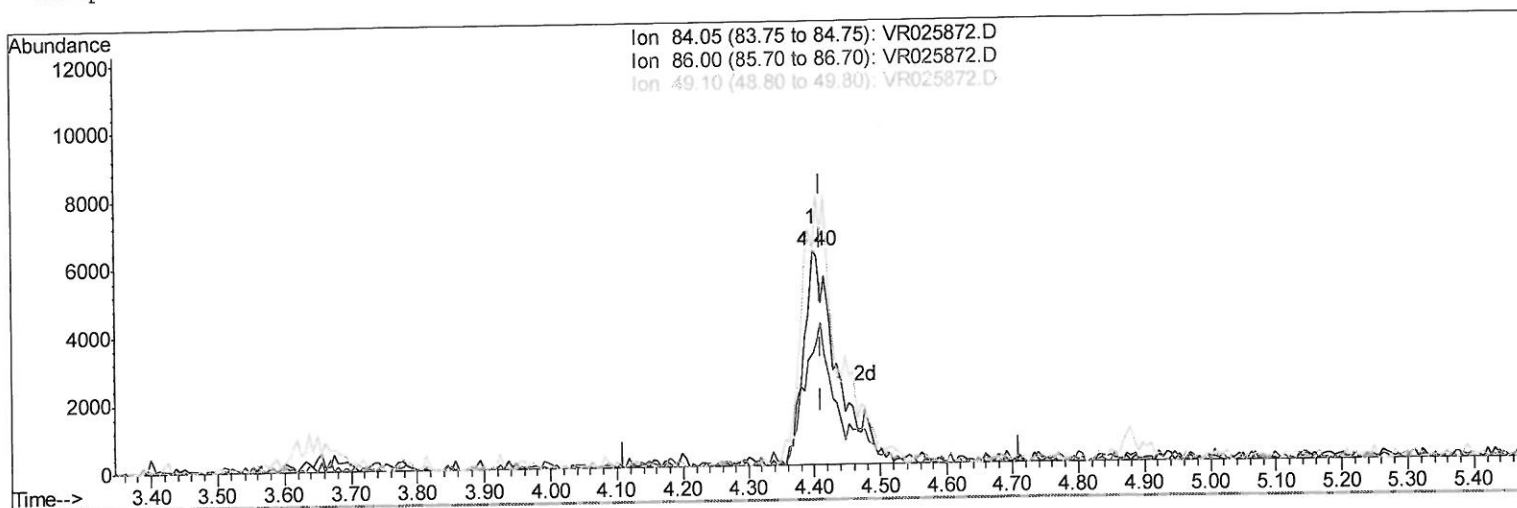

(16) Methylene chloride (T)

4.398min (-0.012) 0.56ug/L m

10/01/18 34

response 21963

Ion	Exp%	Act%
84.05	100	100
86.00	61.60	52.21
49.10	136.40	101.35
0.00	0.00	0.00

Data File : VR025872.D
Acq On : 27 Sep 2018 12:29
Operator : SY/MD
Sample : VSTD0.588
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
VSTD0.588

Manual Integrations
APPROVED

MMDadoda
10/1/2018 11:53:50 AM

10/1/2018 11:53:50 AM

Quant Time: Sep 27 15:29:52 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 27 15:06:01 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	508498	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	412156	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.22	152	138119	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.15	65	22695	0.62	ug/L	0.00
7) Chloroethane-d5	2.63	69	19515	0.68	ug/L	0.00
11) 1,1-Dichloroethene-d2	3.64	63	56223	0.64	ug/L	0.00
20) 2-Butanone-d5	6.59	46	22296	4.59	ug/L	0.00
24) Chloroform-d	7.20	84	37302	0.49	ug/L	0.00
26) 1,2-Dichloroethane-d4	7.90	65	15924	0.48	ug/L	0.00
32) Benzene-d6	7.85	84	76576	0.50	ug/L	0.00
36) 1,2-Dichloropropane-d6	8.89	67	20709	0.50	ug/L	0.00
41) Toluene-d8	9.97	98	69287	0.50	ug/L	0.00
43) trans-1,3-Dichloropropene-	10.24	79	3794	0.33	ug/L	0.00
46) 2-Hexanone-d5	10.59	63	13584	3.52	ug/L	0.00
57) 1,1,2,2-Tetrachloroethane-	12.36	84	8663	0.55	ug/L	0.00
64) 1,2-Dichlorobenzene-d4	13.51	152	11576	0.49	ug/L	0.00

Target Compounds

					Qvalue
2) Dichlorodifluoromethane	1.84	85	16171m	0.305 ug/L	
3) Chloromethane	2.01	50	25761	0.447 ug/L	88
5) Vinyl chloride	2.16	62	24386	0.447 ug/L	90
6) Bromomethane	2.54	94	15412m	0.496 ug/L	
8) Chloroethane	2.66	64	13890	0.448 ug/L	97
9) Trichlorofluoromethane	2.93	101	33293m	0.492 ug/L	
10) 1,1,2-Trichloro-1,2,2-trif	3.68	101	21630m	0.524 ug/L	
12) 1,1-Dichloroethene	3.65	96	22603	0.515 ug/L	77
13) Acetone	3.70	43	19925	6.221 ug/L	97
14) Carbon disulfide	3.94	76	44810m	0.363 ug/L	
15) Methyl Acetate	4.20	43	5552m	0.540 ug/L	
16) Methylene chloride	4.40	84	21963m	0.557 ug/L	
17) Methyl tert-butyl Ether	4.89	73	19689	0.257 ug/L	95
18) trans-1,2-Dichloroethene	4.89	96	14787	0.298 ug/L	86
19) 1,1-Dichloroethane	5.69	63	32479	0.320 ug/L #	94
21) 2-Butanone	6.69	43	22371	3.351 ug/L	96
22) cis-1,2-Dichloroethene	6.67	96	16736	0.335 ug/L #	99
23) Bromochloromethane	7.04	128	4593	0.349 ug/L #	56
25) Chloroform	7.23	83	31513	0.338 ug/L	96
27) 1,2-Dichloroethane	8.00	62	15922	0.330 ug/L #	94
29) 1,1,1-Trichloroethane	7.43	97	23375	0.281 ug/L	94
30) Cyclohexane	7.52	56	32303	0.326 ug/L	95
31) Carbon tetrachloride	7.64	117	20091	0.293 ug/L	95
33) Benzene	7.91	78	73036	0.338 ug/L	100
34) Trichloroethene	8.71	95	20322	0.354 ug/L	91
35) Methylcyclohexane	8.95	83	28820	0.306 ug/L	94
37) 1,2-Dichloropropane	8.99	63	15102	0.313 ug/L #	98
38) Bromodichloromethane	9.28	83	16249	0.305 ug/L	97
39) cis-1,3-Dichloropropene	9.72	75	13509	0.229 ug/L	92
40) 4-Methyl-2-pentanone	9.87	43	47973	2.856 ug/L	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR092718\
Quantitation Report (QT Reviewed)

Data File : VR025872.D
Acq On : 27 Sep 2018 12:29
Operator : SY/MD
Sample : VSTD0.588
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
VSTD0.588

Manual Integrations
APPROVED

MMDadoda
10/1/2018 11:53:50 AM

10/1/2018 11:53:50 AM

Quant Time: Sep 27 15:29:52 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 27 15:06:01 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
42) Toluene	10.04	91	73518	0.333	ug/L	99
44) trans-1,3-Dichloropropene	10.27	75	8713	0.213	ug/L	99
45) 1,1,2-Trichloroethane	10.45	97	6827	0.338	ug/L #	87
47) Tetrachloroethene	10.51	164	11156	0.340	ug/L	84
48) 2-Hexanone	10.63	43	31487	2.851	ug/L #	94
49) Dibromochloromethane	10.79	129	6419	0.305	ug/L	83
50) 1,2-Dibromoethane	10.89	107	5093	0.286	ug/L #	84
51) Chlorobenzene	11.32	112	39934	0.345	ug/L	92
52) Ethylbenzene	11.39	91	83255	0.328	ug/L	96
53) m,p-Xylene	11.50	106	29439	0.322	ug/L	90
54) o-Xylene	11.83	106	26167	0.312	ug/L	100
55) Styrene	11.84	104	37133	0.286	ug/L	94
56) Isopropylbenzene	12.13	105	70942	0.303	ug/L	98
58) 1,1,2,2-Tetrachloroethane	12.39	83	6140	0.309	ug/L #	64
59) 1,2,3-Trichloropropane	12.43	75	5142	0.326	ug/L	98
61) Bromoform	12.01	173	2034	0.316	ug/L #	90
62) 1,3-Dichlorobenzene	13.16	146	20232	0.317	ug/L	89
63) 1,4-Dichlorobenzene	13.24	146	22550	0.366	ug/L	90
65) 1,2-Dichlorobenzene	13.53	146	17236	0.354	ug/L	86
66) 1,2-Dibromo-3-chloropropan	14.15	75	950	0.427	ug/L #	77
67) 1,3,5-Trichlorobenzene	14.29	180	11868	0.329	ug/L #	97
68) 1,2,4-trichlorobenzene	14.78	180	8219	0.358	ug/L	96
69) Naphthalene	15.00	128	8671	0.260	ug/L #	95
70) 1,2,3-Trichlorobenzene	15.18	180	5143	0.316	ug/L #	80

(#) = qualifier out of range (m) = manual integration (+) = signals summed

