

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR100518\
 Data File : VR025956.D
 Acq On : 5 Oct 2018 14:21
 Operator : SY/MD
 Sample : J5276-03
 Misc : 25mL/MSVOA_R/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 BEYAO

Quant Time: Oct 06 05:06:55 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Oct 06 04:21:51 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	427822	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	349277	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.23	152	116869	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.15	65	119802	3.55	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	71.00%
7) Chloroethane-d5	2.64	69	114799	4.16	ug/L	0.01
Spiked Amount	5.000	Range	65 - 130	Recovery	=	83.20%
11) 1,1-Dichloroethene-d2	3.63	63	220947	2.79	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	55.80%#
20) 2-Butanone-d5	6.59	46	196071	52.13	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.26%
24) Chloroform-d	7.20	84	243769	4.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.00%
26) 1,2-Dichloroethane-d4	7.90	65	109796	4.35	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.00%
32) Benzene-d6	7.85	84	444724	3.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	76.60%
36) 1,2-Dichloropropane-d6	8.90	67	129768	4.14	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	82.80%
41) Toluene-d8	9.97	98	378579	3.47	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	69.40%#
43) trans-1,3-Dichloropropene-	10.24	79	28564	4.02	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.40%
46) 2-Hexanone-d5	10.59	63	140469	51.80	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.60%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	54609	4.30	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.00%
64) 1,2-Dichlorobenzene-d4	13.52	152	77514	4.14	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	82.80%


Target Compounds					Qvalue
13) Acetone	3.70	43	8656	3.175 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_R\DATA\VR100518\
Data File : VR025956.D
Acq On : 5 Oct 2018 14:21
Operator : SY/MD
Sample : J5276-03
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
BEYA0

Quant Time: Oct 06 05:06:55 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Oct 06 04:21:51 2018
Response via : Initial Calibration

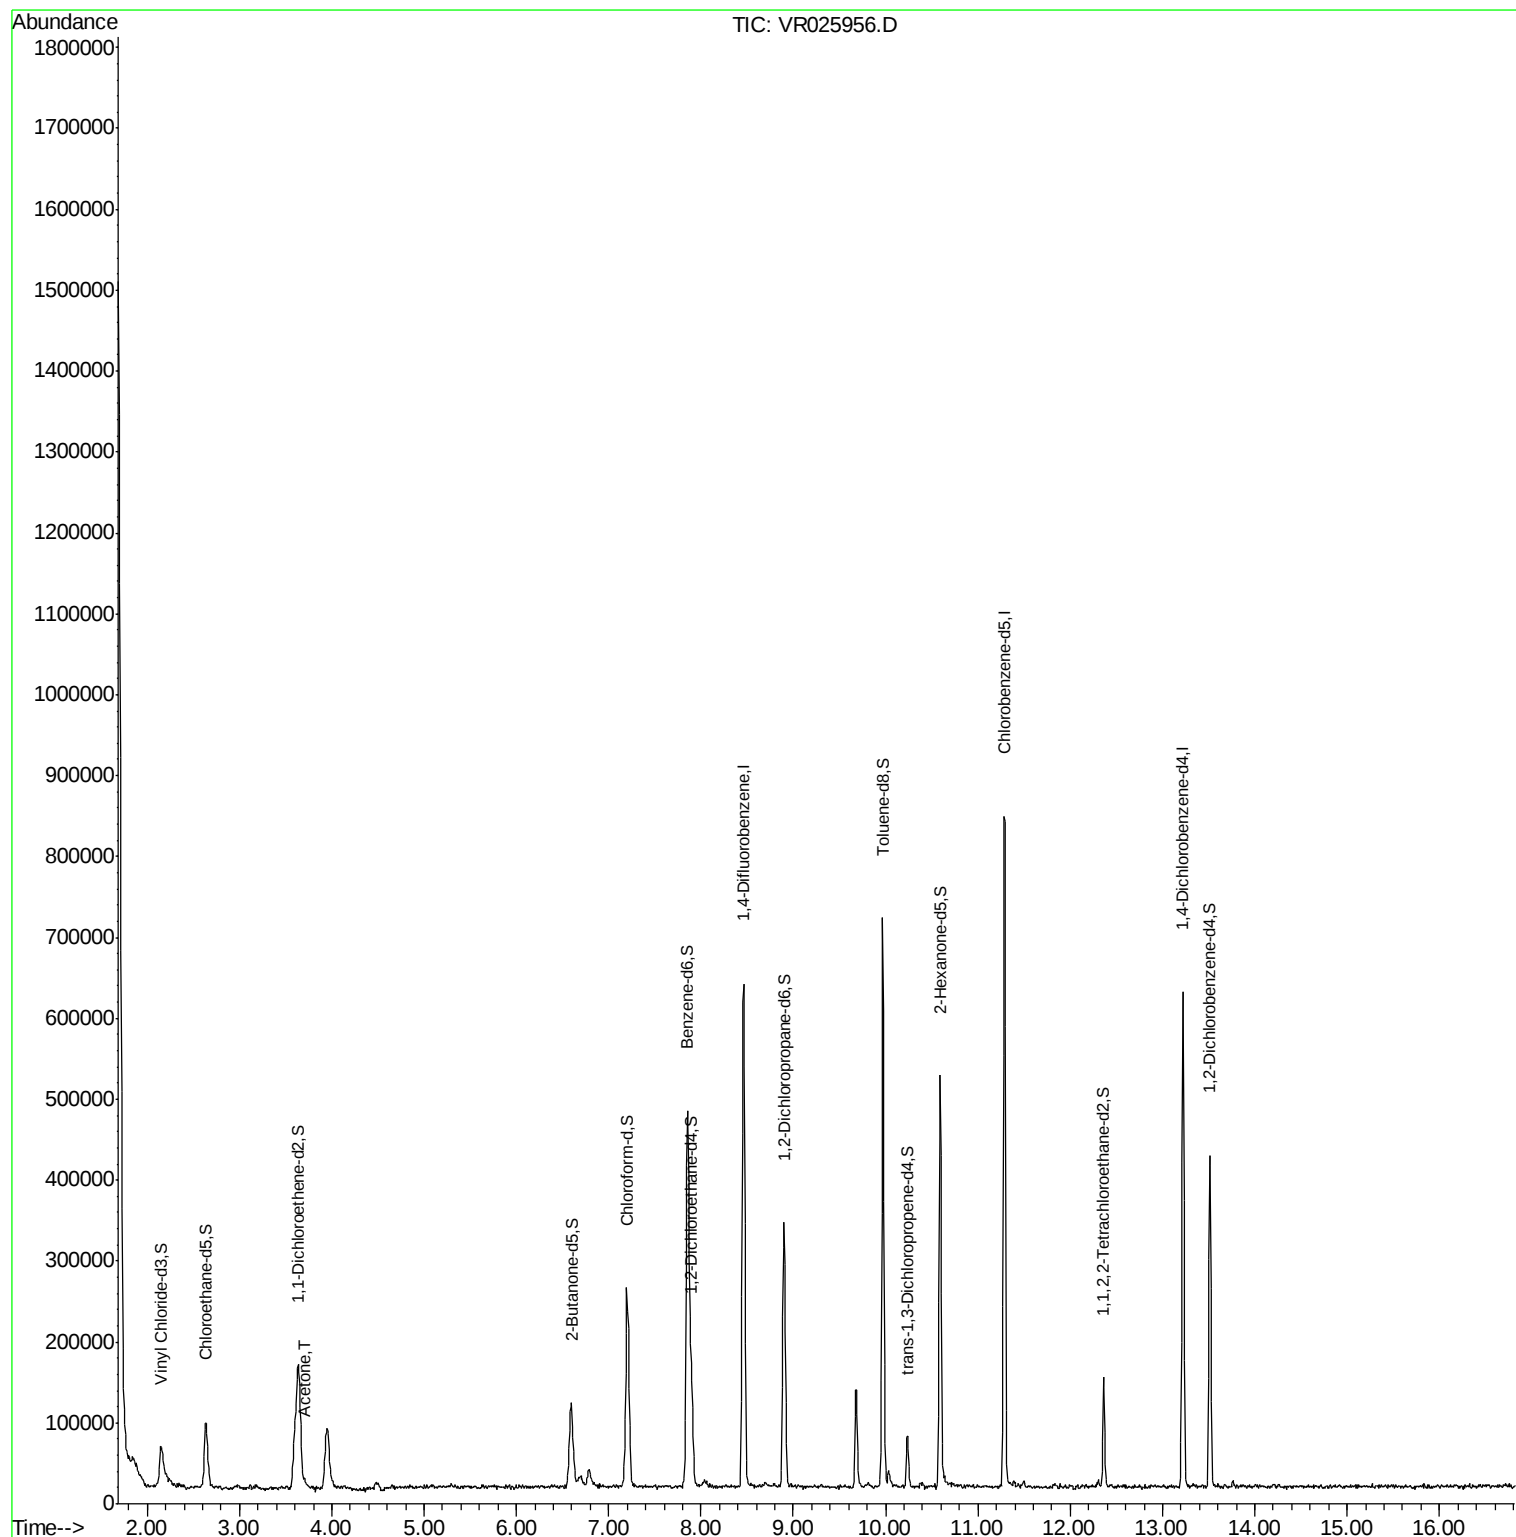

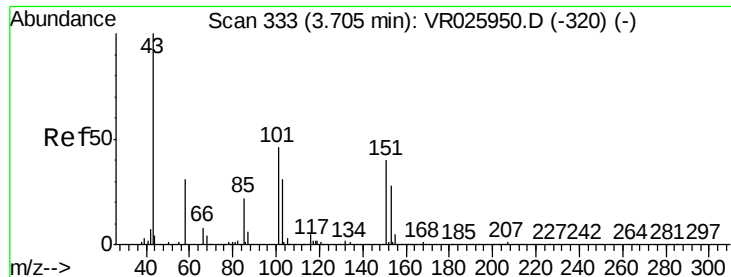

#13

Acetone

Concen: 3.175 ug/L

RT: 3.70 min Scan# 332

Delta R.T. -0.01 min

Lab File: VR025956.D

Acq: 5 Oct 2018 14:21

Instrument :
MSVOA_R
ClientSampleId :
BEYA0

Tgt Ion: 43 Resp: 8656

Ion Ratio Lower Upper

43 100

58 25.2 0.0 51.4

