

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR100518\
 Data File : VR025967.D
 Acq On : 5 Oct 2018 22:36
 Operator : SY/MD
 Sample : J5276-12
 Misc : 25mL/MSVOA_R/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 BEYA9

Quant Time: Oct 06 05:48:18 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Oct 06 05:30:02 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	394215	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	336577	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.22	152	111831	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.15	65	101646	3.27	ug/L	-0.01
Spiked Amount	5.000	Range	40 - 130	Recovery	=	65.40%
7) Chloroethane-d5	2.63	69	111792	4.40	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.00%
11) 1,1-Dichloroethene-d2	3.63	63	196486	2.69	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	53.80%#
20) 2-Butanone-d5	6.59	46	180791	52.17	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.34%
24) Chloroform-d	7.20	84	215024	3.97	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	79.40%
26) 1,2-Dichloroethane-d4	7.90	65	101654	4.37	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.40%
32) Benzene-d6	7.86	84	396925	3.54	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	70.80%
36) 1,2-Dichloropropane-d6	8.90	67	119894	3.97	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	79.40%
41) Toluene-d8	9.97	98	337814	3.21	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	64.20%#
43) trans-1,3-Dichloropropene-	10.24	79	23488	3.43	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	68.60%
46) 2-Hexanone-d5	10.59	63	137576	52.65	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.30%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	54487	4.45	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.00%
64) 1,2-Dichlorobenzene-d4	13.51	152	74956	4.19	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	83.80%


Target Compounds					Qvalue
13) Acetone	3.72	43	9276	3.693 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_R\DATA\VR100518\
Data File : VR025967.D
Acq On : 5 Oct 2018 22:36
Operator : SY/MD
Sample : J5276-12
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
BEYA9

Quant Time: Oct 06 05:48:18 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Oct 06 05:30:02 2018
Response via : Initial Calibration

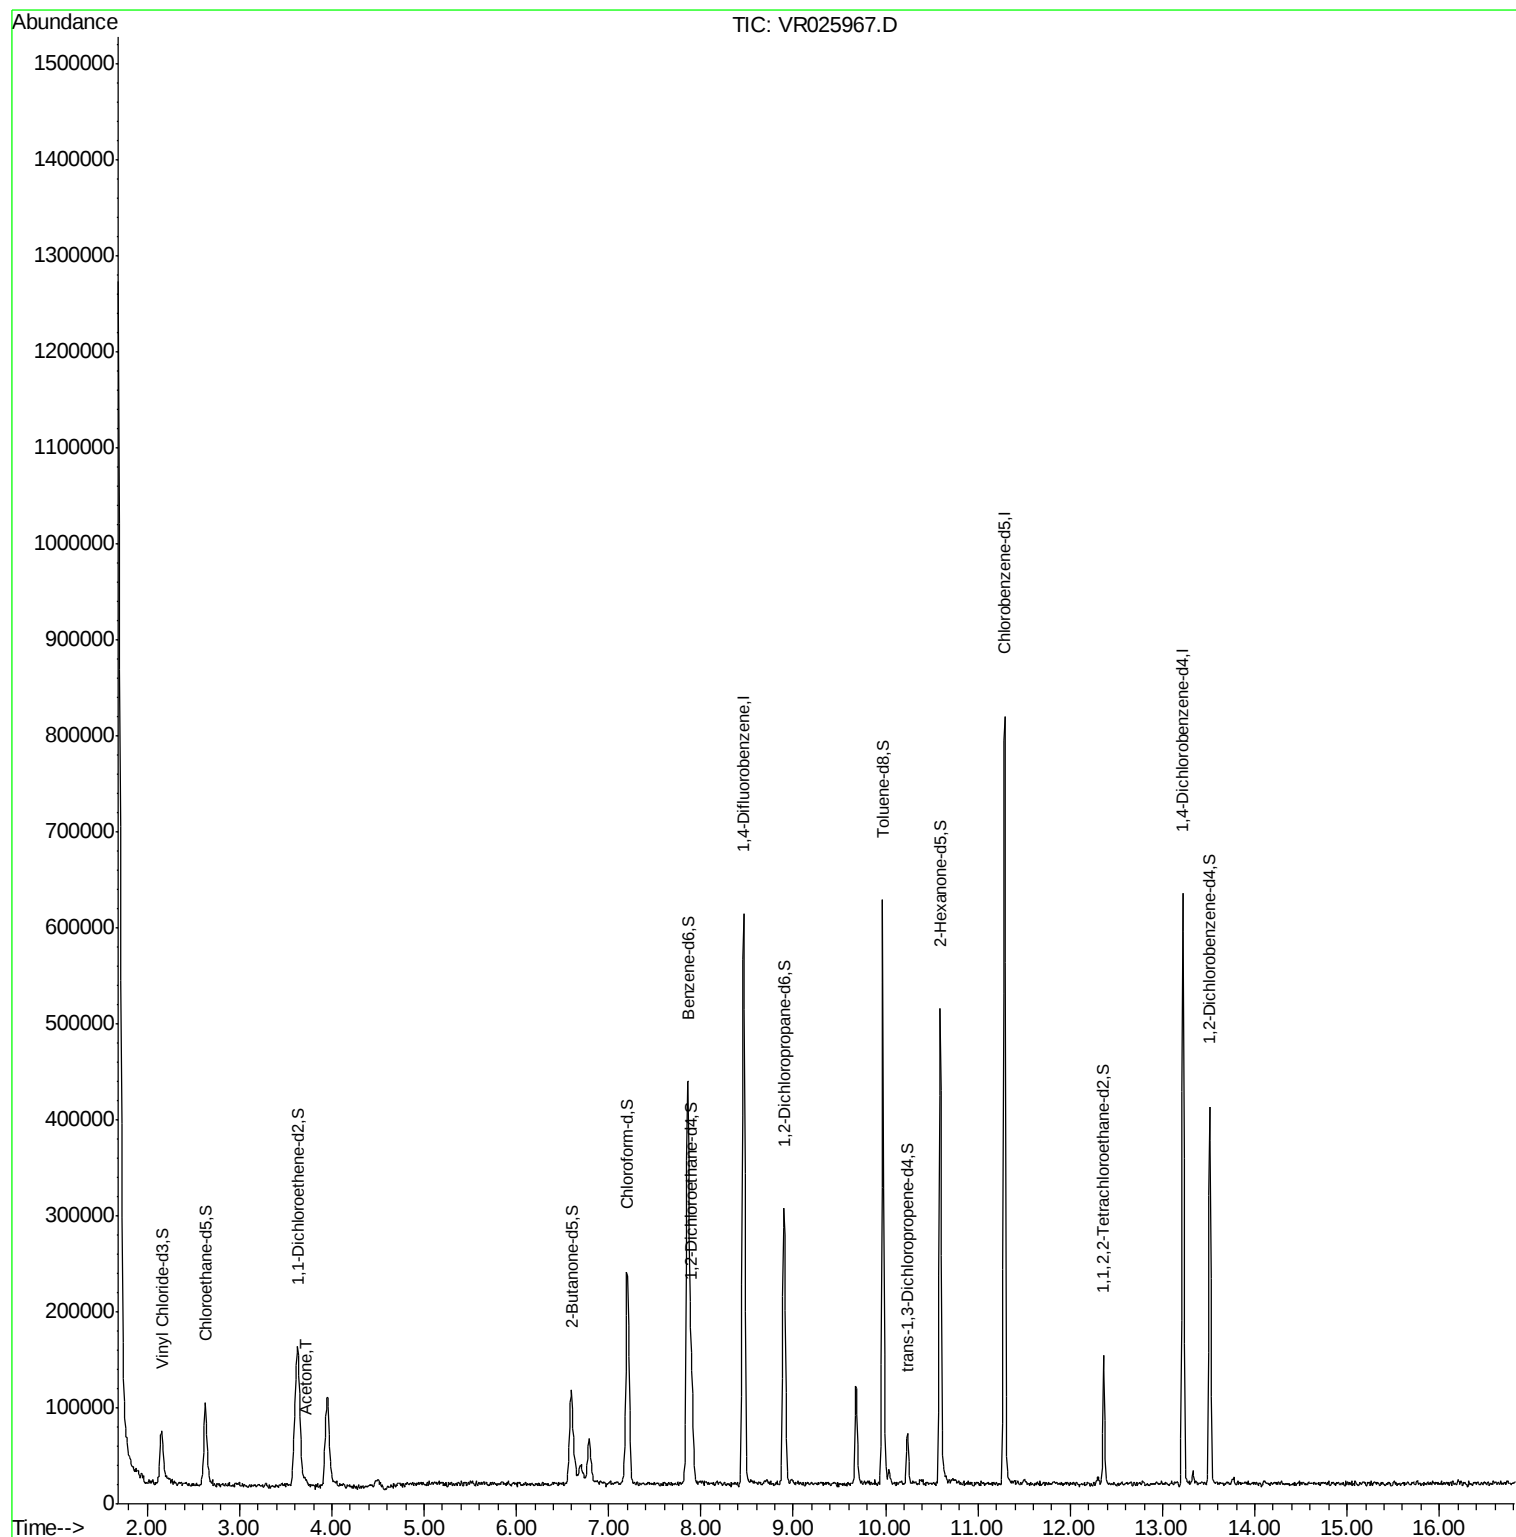

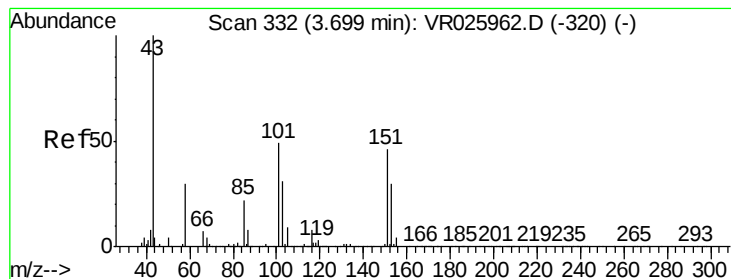

#13
 Acetone
 Concen: 3.693 ug/L
 RT: 3.72 min Scan# 335
 Delta R.T. 0.02 min
 Lab File: VR025967.D
 Acq: 5 Oct 2018 22:36

Instrument :
 MSVOA_R
 ClientSampleId :
 BEYA9

Tgt Ion: 43 Resp: 9276
 Ion Ratio Lower Upper
 43 100
 58 26.6 0.0 51.4

