

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR100518\
 Data File : VR025973.D
 Acq On : 6 Oct 2018 1:54
 Operator : SY/MD
 Sample : J5276-18
 Misc : 25mL/MSVOA_R/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 BEYB5

Quant Time: Oct 06 06:29:47 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Oct 06 05:30:02 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	413805	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	354353	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.23	152	122643	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.15	65	104537	3.20	ug/L	-0.02
Spiked Amount	5.000	Range	40 - 130	Recovery	=	64.00%
7) Chloroethane-d5	2.63	69	107064	4.01	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	80.20%
11) 1,1-Dichloroethene-d2	3.62	63	187795	2.45	ug/L	-0.01
Spiked Amount	5.000	Range	60 - 125	Recovery	=	49.00%#
20) 2-Butanone-d5	6.58	46	190162	52.27	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.54%
24) Chloroform-d	7.20	84	213880	3.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	75.40%
26) 1,2-Dichloroethane-d4	7.90	65	102988	4.22	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.40%
32) Benzene-d6	7.85	84	374998	3.18	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	63.60%#
36) 1,2-Dichloropropane-d6	8.90	67	118910	3.74	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	74.80%
41) Toluene-d8	9.97	98	319782	2.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	57.80%#
43) trans-1,3-Dichloropropene-	10.23	79	22297	3.09	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	61.80%
46) 2-Hexanone-d5	10.59	63	136023	49.44	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.88%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	53765	4.17	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	83.40%
64) 1,2-Dichlorobenzene-d4	13.51	152	73251	3.73	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	74.60%#


Target Compounds					Qvalue
13) Acetone	3.69	43	11082	4.203 ug/L	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_R\DATA\VR100518\
Data File : VR025973.D
Acq On : 6 Oct 2018 1:54
Operator : SY/MD
Sample : J5276-18
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
BEYB5

Quant Time: Oct 06 06:29:47 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Oct 06 05:30:02 2018
Response via : Initial Calibration

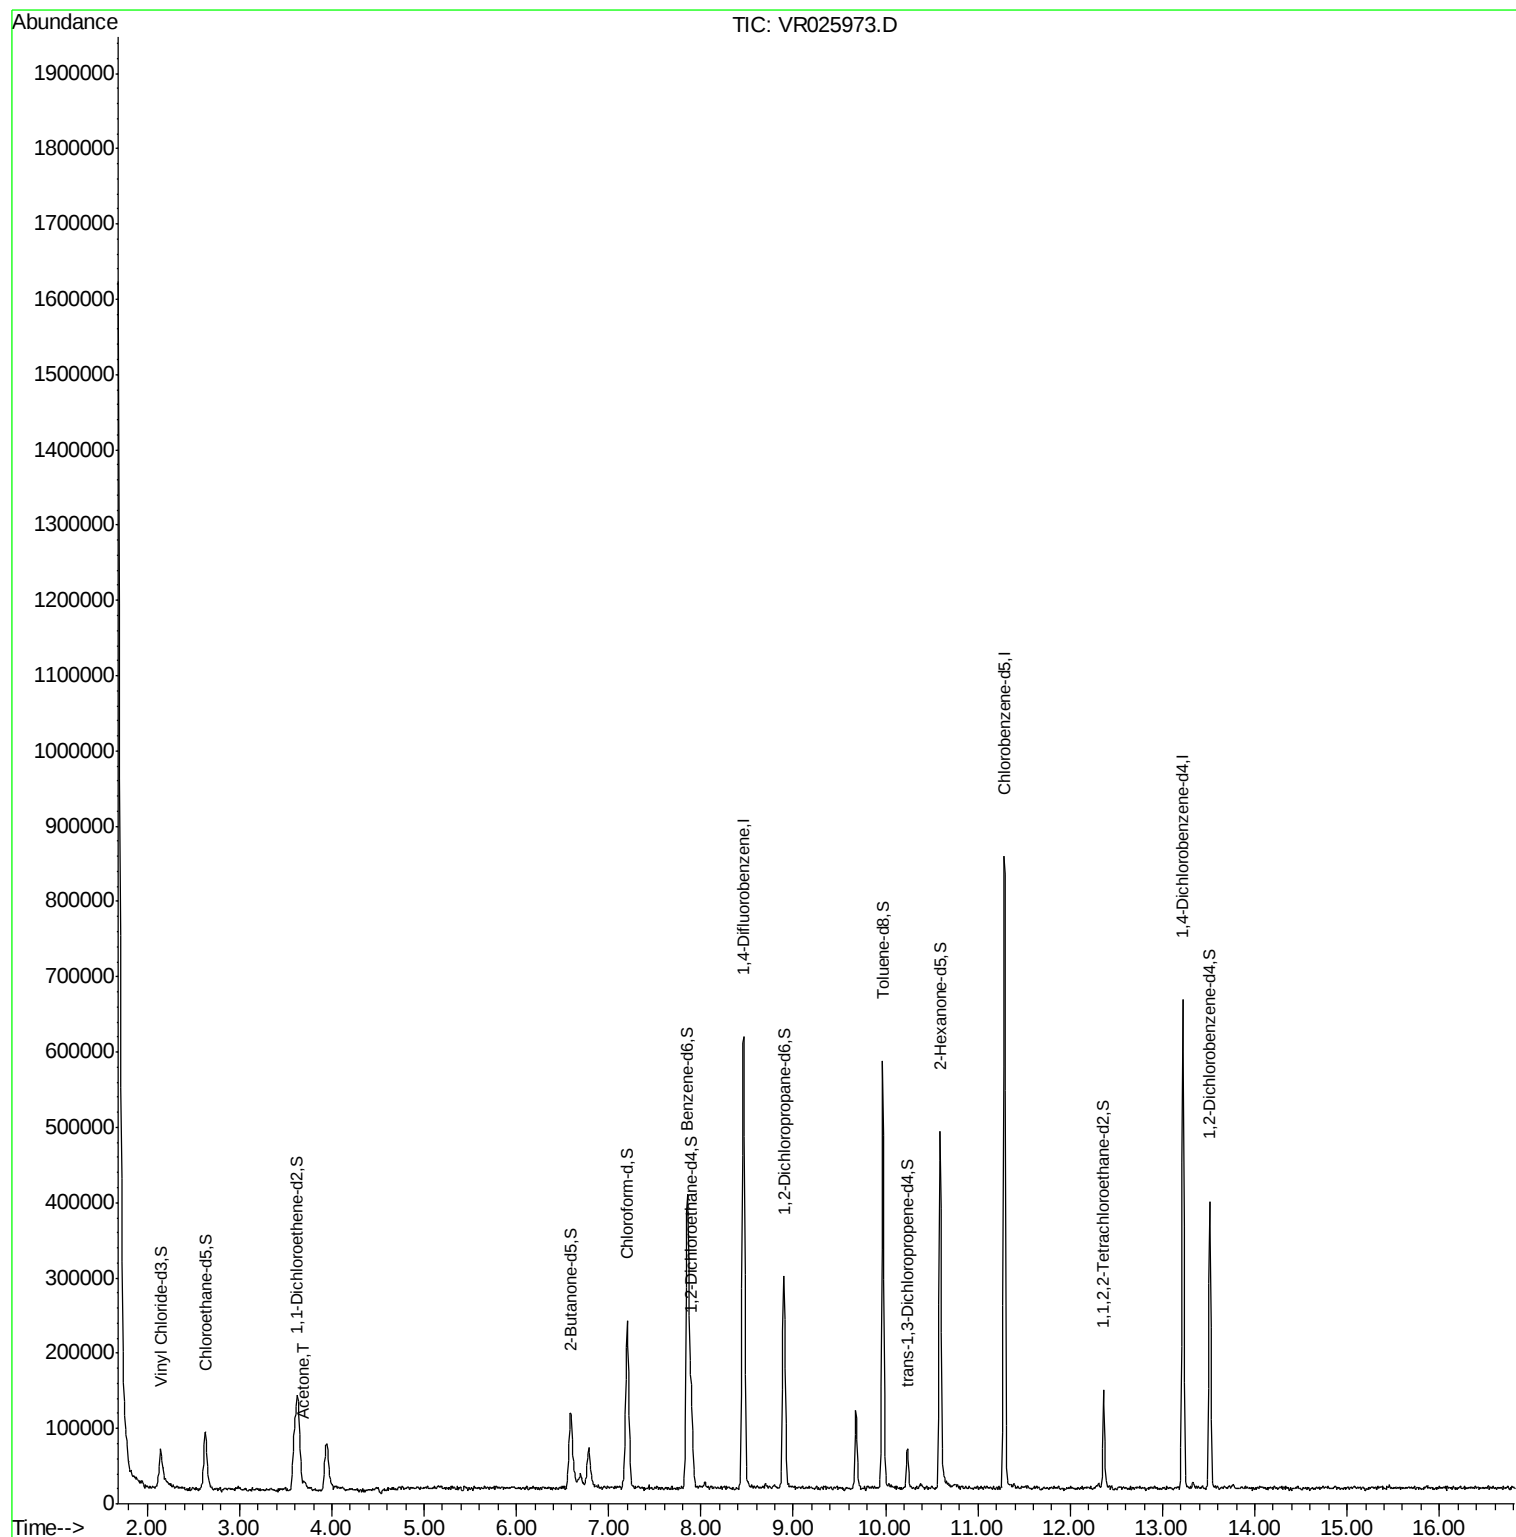

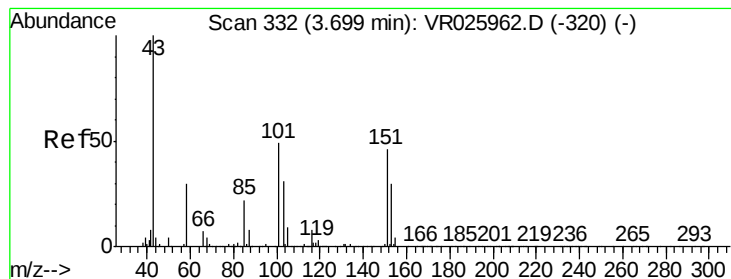

#13

Acetone

Concen: 4.203 ug/L

RT: 3.69 min Scan# 331

Delta R.T. -0.01 min

Lab File: VR025973.D

Acq: 6 Oct 2018 1:54

Instrument :
MSVOA_R
ClientSampleId :
BEYB5

Tgt Ion: 43 Resp: 11082

Ion Ratio Lower Upper

43 100

58 15.4 0.0 51.4

