

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR100518\
 Data File : VR025958.D
 Acq On : 5 Oct 2018 15:27
 Operator : SY/MD
 Sample : J5276-05
 Misc : 25mL/MSVOA_R/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 BEYA2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.147	69	77	90	rBV	61926	186022	14.66%	1.795%
2	2.622	147	155	167	rBV2	92530	244747	19.29%	2.362%
3	3.632	306	321	339	rBV3	158390	609465	48.03%	5.882%
4	3.948	365	373	383	rBV2	53777	168640	13.29%	1.627%
5	4.477	453	460	461	rBV7	10428	16041	1.26%	0.155%
6	6.588	798	807	819	rBV	105520	318764	25.12%	3.076%
7	6.795	833	841	846	rVB2	22670	56665	4.47%	0.547%
8	7.203	898	908	918	rBV2	234383	586788	46.24%	5.663%
9	7.854	1006	1015	1030	rBV2	452890	1268887	100.00%	12.246%
10	8.462	1107	1115	1123	rBV	600425	1129754	89.04%	10.903%
11	8.900	1179	1187	1195	rBV	319947	615233	48.49%	5.937%
12	9.679	1307	1315	1323	rBV	118346	205431	16.19%	1.983%
13	9.971	1353	1363	1371	rBV	690157	1072706	84.54%	10.352%
14	10.038	1371	1374	1379	rVB6	10066	15002	1.18%	0.145%
15	10.239	1401	1407	1411	rBV2	61217	99884	7.87%	0.964%
16	10.591	1459	1465	1477	rBV	506970	782990	61.71%	7.556%
17	11.291	1573	1580	1589	rBV	824840	1237976	97.56%	11.947%
18	12.362	1751	1756	1762	rBV	136132	207906	16.38%	2.006%
19	13.220	1890	1897	1904	rBV	635464	901710	71.06%	8.702%
20	13.329	1911	1915	1921	rBV9	10253	17978	1.42%	0.173%
21	13.512	1938	1945	1954	rBV	427479	619422	48.82%	5.978%


Sum of corrected areas: 10362011

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_R\DATA\VR100518\
Data File : VR025958.D
Acq On : 5 Oct 2018 15:27
Operator : SY/MD
Sample : J5276-05
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
BEYA2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

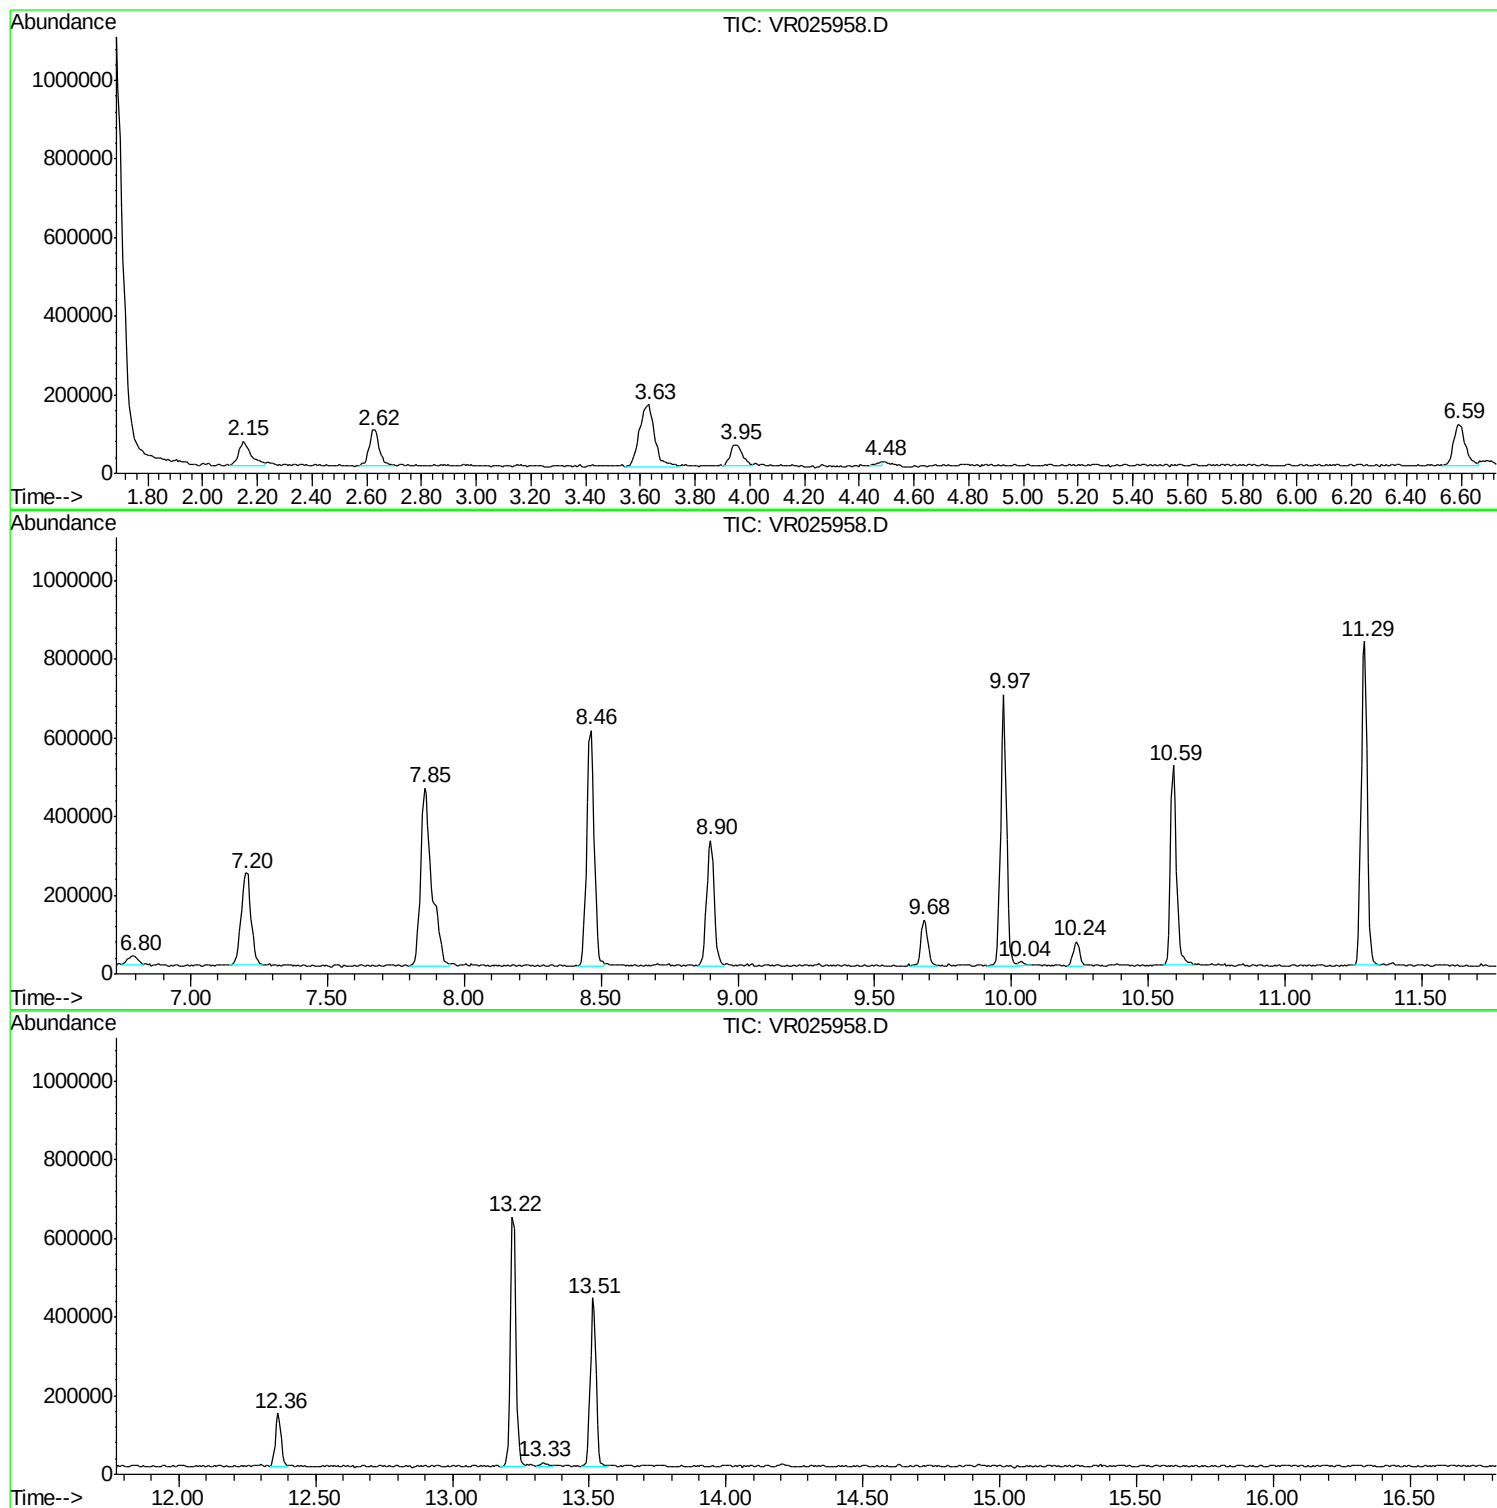

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_R\DATA\VR100518\
Data File : VR025958.D
Acq On : 5 Oct 2018 15:27
Operator : SY/MD
Sample : J5276-05
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 10 Sample Multiplier: 1










Instrument :
MSVOA_R
ClientSampleId :
BEYA2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.	
3.95	0.75 ug/L	168640	1,4-Difluorobenzene	8.46	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Isopropyl Alcohol	60	C3H8O	000067-63-0	64
2	Isopropyl Alcohol	60	C3H8O	000067-63-0	64
3	Isopropyl Alcohol	60	C3H8O	000067-63-0	50
4	Isopropyl Alcohol	60	C3H8O	000067-63-0	50
5	2-Propanol, 1-bromo-	138	C3H7BrO	019686-73-8	39

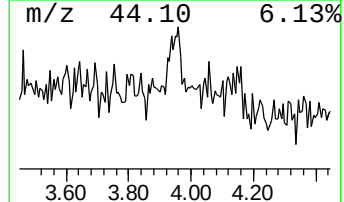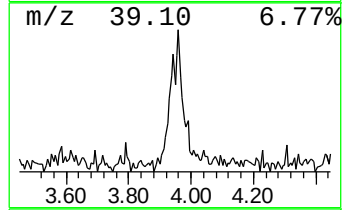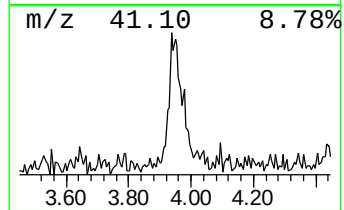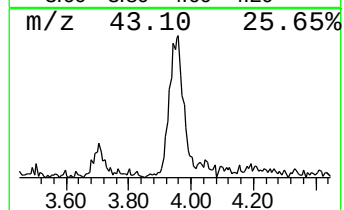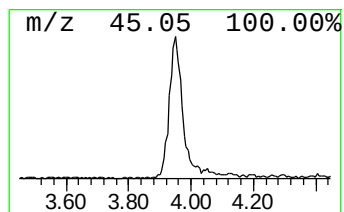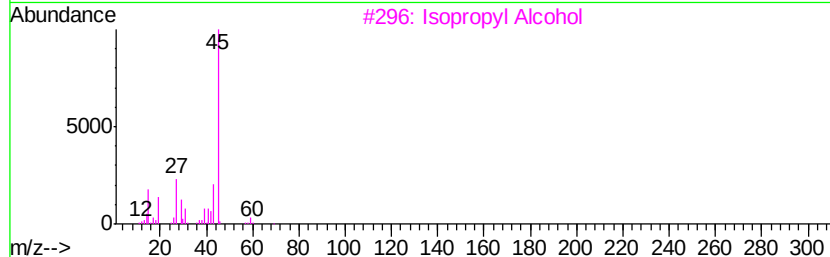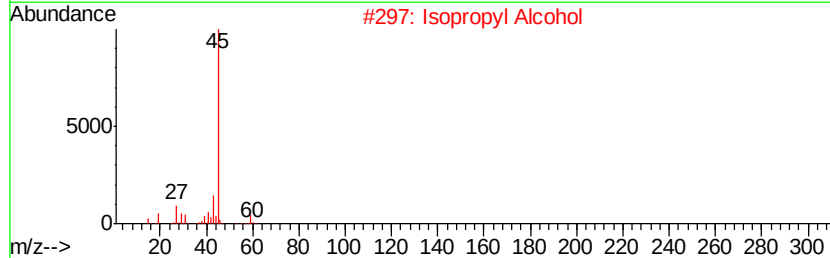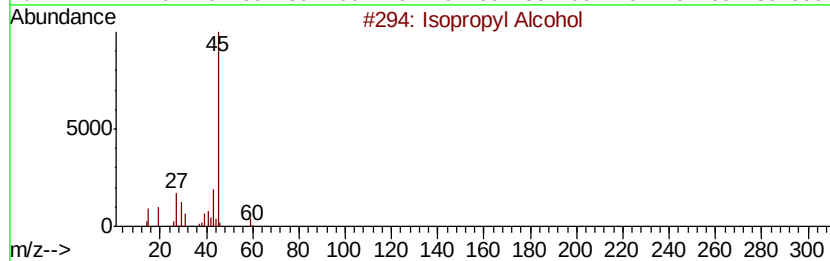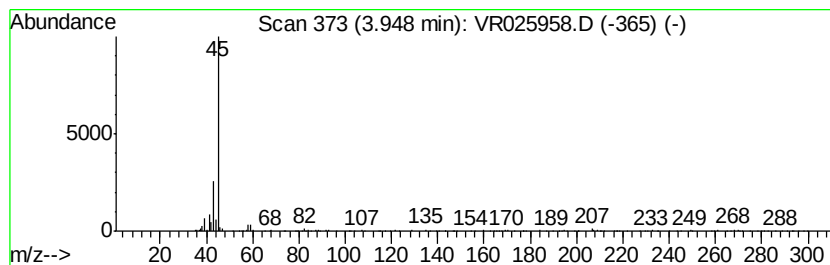

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR100518\
Data File : VR025958.D
Acq On : 5 Oct 2018 15:27
Operator : SY/MD
Sample : J5276-05
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
BEYA2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	3.95	0.8	ug/L	168640	1	8.46	1129750	5.0