

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR100818\
 Data File : VR026003.D
 Acq On : 9 Oct 2018 2:36
 Operator : SY/MD
 Sample : J5279-15
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 BEYH2

Quant Time: Oct 09 06:52:38 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 09 06:51:21 2018
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 10/9/2018 1:47:18 PM

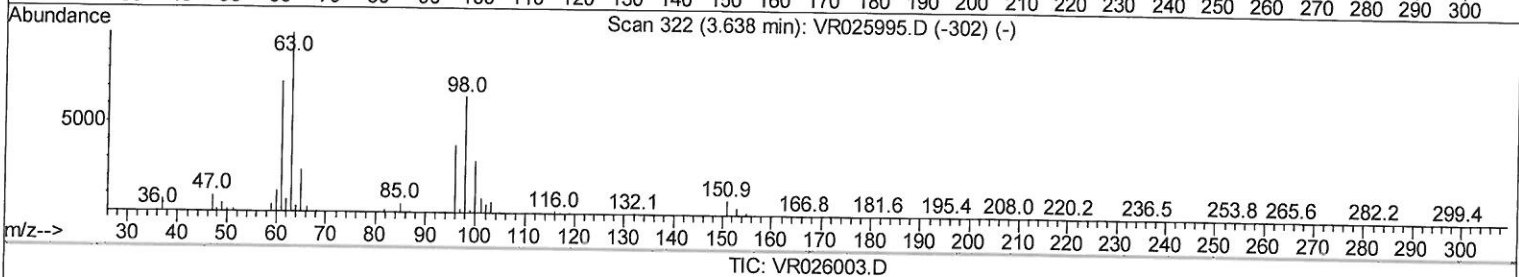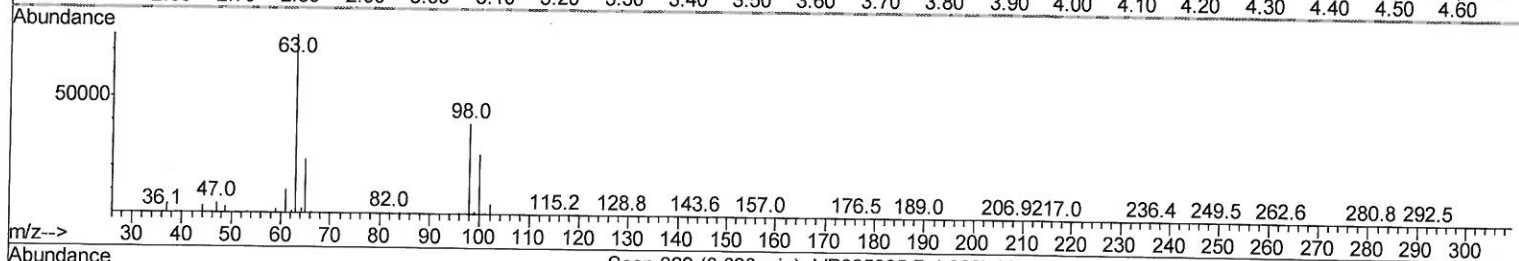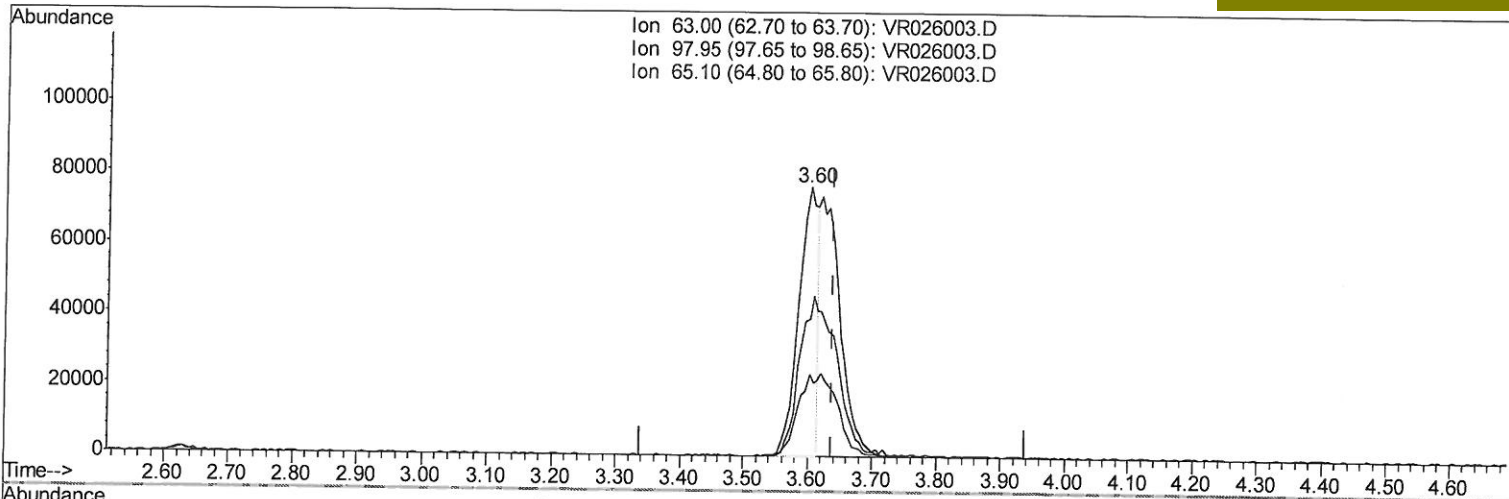

TIC: VR026003.D

(11) 1,1-Dichloroethene-d2 (S)

3.601min (-0.036) 2.12ug/L

response 160666

Ion	Exp%	Act%
63.00	100	100
97.95	68.20	113.70#
65.10	22.40	62.04#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR100818\
 Data File : VR026003.D
 Acq On : 9 Oct 2018 2:36
 Operator : SY/MD
 Sample : J5279-15
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 BEYH2

Quant Time: Oct 09 06:52:38 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 09 06:51:21 2018
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 10/9/2018 1:47:18 PM

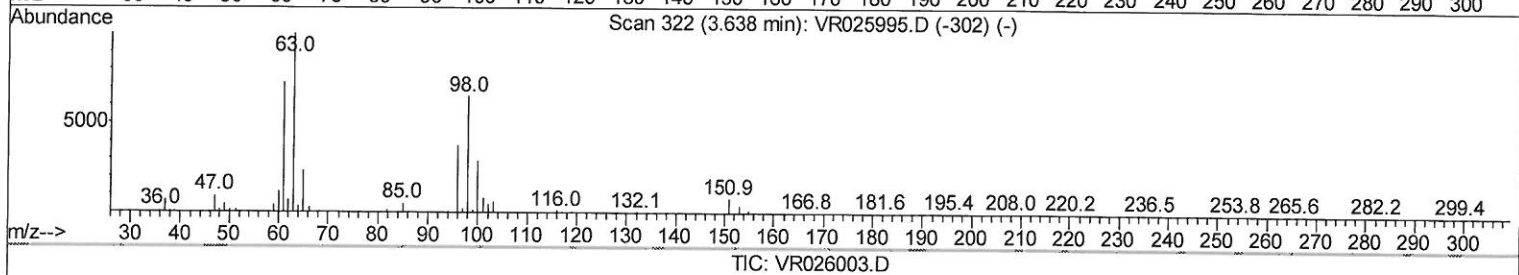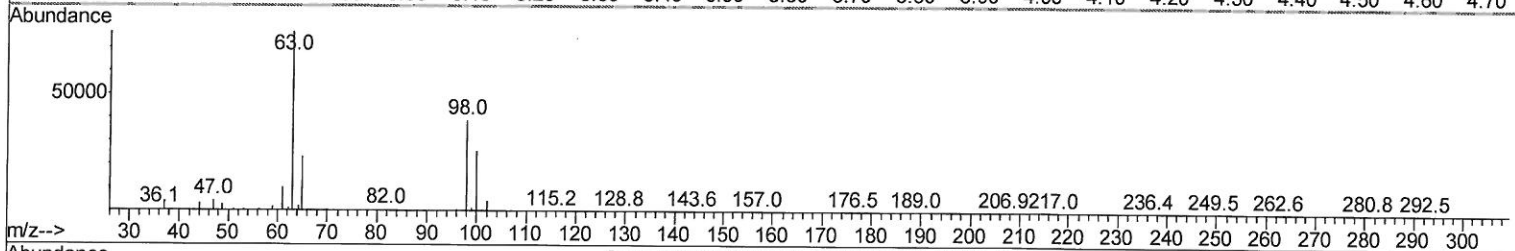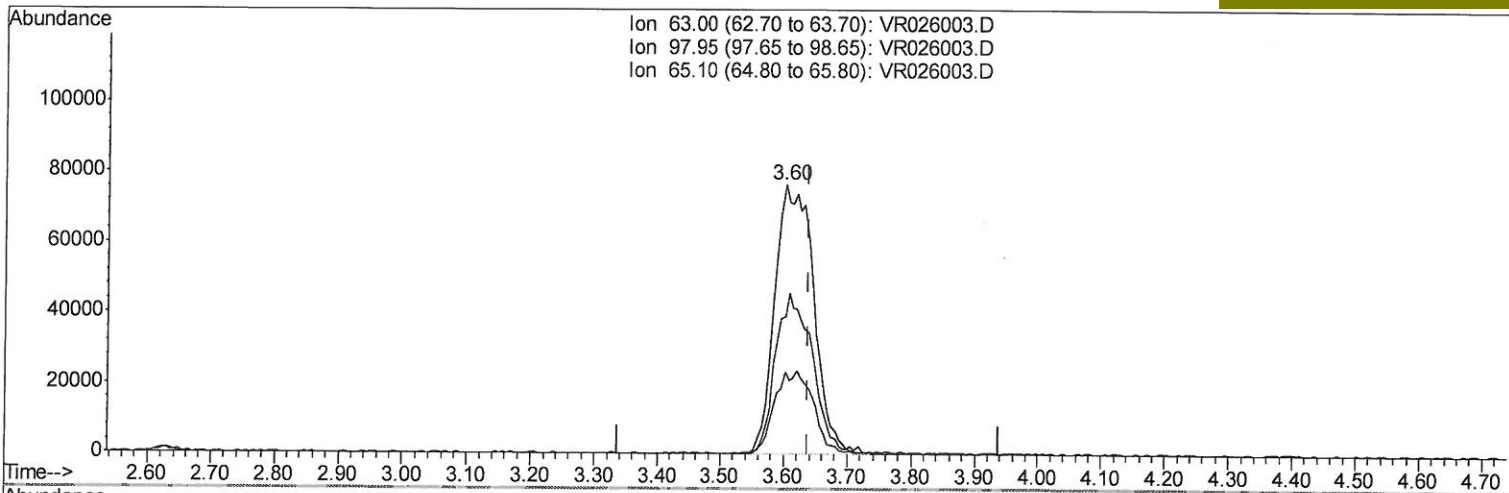

TIC: VR026003.D

(11) 1,1-Dichloroethene-d2 (S)

3.601min (-0.036) 4.25ug/L m > 10/11/18 dy

response 322192

Ion	Exp%	Act%
63.00	100	100
97.95	68.20	56.70
65.10	22.40	30.94#
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR100818\
 Data File : VR026003.D
 Acq On : 9 Oct 2018 2:36
 Operator : SY/MD
 Sample : J5279-15
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_R
 Client Sampled :
 BEYH2

Quant Time: Oct 09 07:16:03 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 09 06:51:21 2018
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 10/9/2018 1:47:18 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	408862	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	348496	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.22	152	113698	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.15	65	175620	5.45	ug/L	-0.01
Spiked Amount 5.000	Range 40 - 130		Recovery =	109.00%		
7) Chloroethane-d5	2.63	69	158488	6.01	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	120.20%		
11) 1,1-Dichloroethene-d2	3.60	63	322192m	4.25	ug/L	-0.04
Spiked Amount 5.000	Range 60 - 125		Recovery =	85.00%		
20) 2-Butanone-d5	6.59	46	192281	53.49	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	106.98%		
24) Chloroform-d	7.20	84	273956	4.88	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	97.60%		
26) 1,2-Dichloroethane-d4	7.90	65	126239	5.23	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	104.60%		
32) Benzene-d6	7.85	84	541520	4.67	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	93.40%		
36) 1,2-Dichloropropane-d6	8.90	67	153092	4.90	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	98.00%		
41) Toluene-d8	9.97	98	497684	4.57	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	91.40%		
43) trans-1,3-Dichloropropene-	10.24	79	31696	4.47	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	89.40%		
46) 2-Hexanone-d5	10.59	63	142530	52.68	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	105.36%		
57) 1,1,2,2-Tetrachloroethane-	12.36	84	59990	4.73	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	94.60%		
64) 1,2-Dichlorobenzene-d4	13.51	152	94946	5.21	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	104.20%		

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
34) Trichloroethene	8.71	95	184818	6.001	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR100818\
Data File : VR026003.D
Acq On : 9 Oct 2018 2:36
Operator : SY/MD
Sample : J5279-15
Misc : 25mL/MSVOA R/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_R
Client Sampled :
BEYH2

Quant Time: Oct 09 07:16:03 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Oct 09 06:51:21 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
10/9/2018 1:47:18 PM

