

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR101018\
 Data File : VR026027.D
 Acq On : 10 Oct 2018 13:42
 Operator : SY/MD
 Sample : J5380-05
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 C0T21

Quant Time: Oct 11 04:46:41 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Oct 11 04:11:41 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	456292	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	384026	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.23	152	124555	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.14	65	156246	4.34	ug/L	-0.01
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.80%
7) Chloroethane-d5	2.62	69	148537	5.05	ug/L	-0.01
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.00%
11) 1,1-Dichloroethene-d2	3.60	63	282310	3.34	ug/L	-0.03
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.80%
20) 2-Butanone-d5	6.58	46	192382	47.96	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.92%
24) Chloroform-d	7.20	84	260714	4.16	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.20%
26) 1,2-Dichloroethane-d4	7.90	65	122646	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.00%
32) Benzene-d6	7.85	84	483933	3.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	75.80%
36) 1,2-Dichloropropane-d6	8.90	67	142741	4.14	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	82.80%
41) Toluene-d8	9.97	98	436712	3.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	72.80%
43) trans-1,3-Dichloropropene-	10.23	79	31730	4.06	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.20%
46) 2-Hexanone-d5	10.59	63	146577	49.16	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.32%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	63096	4.51	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.20%
64) 1,2-Dichlorobenzene-d4	13.51	152	90254	4.52	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	90.40%


Target Compounds					Ovalue
13) Acetone	3.70	43	22897	7.875 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA R\DATA\VR101018\
Data File : VR026027.D
Acq On : 10 Oct 2018 13:42
Operator : SY/MD
Sample : J5380-05
Misc : 25mL/MSVOA R/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
C0T21

Quant Time: Oct 11 04:46:41 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Oct 11 04:11:41 2018
Response via : Initial Calibration

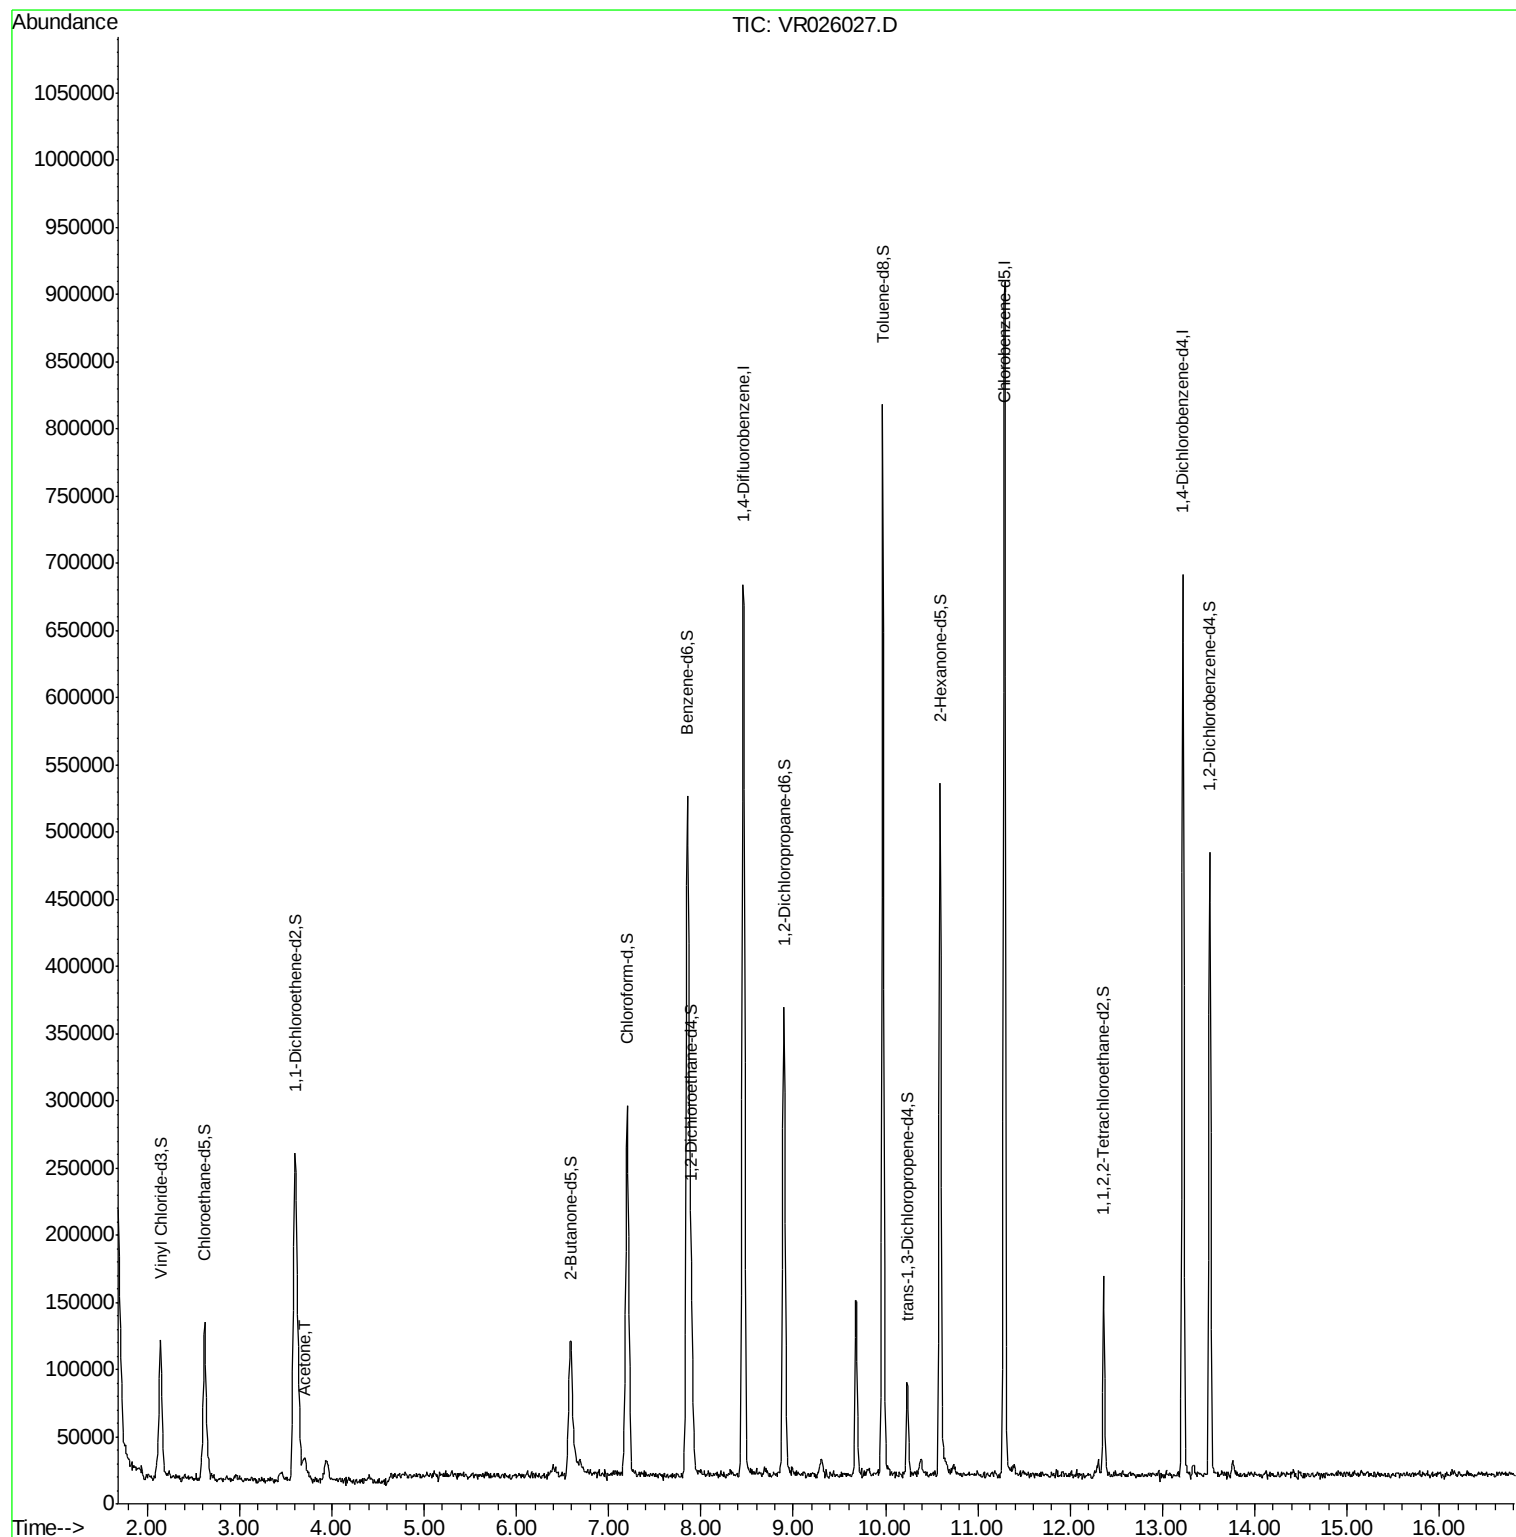

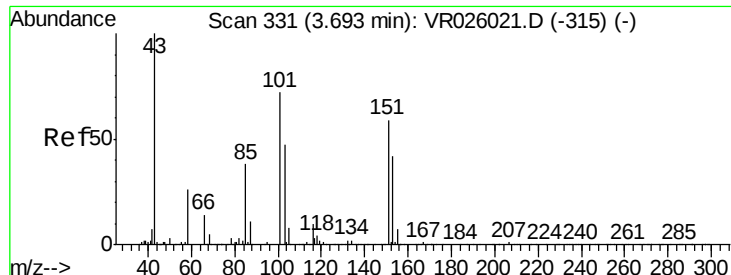

#13

Acetone

Concen: 7.875 ug/L

RT: 3.70 min Scan# 333

Delta R.T. 0.01 min

Lab File: VR026027.D

Acq: 10 Oct 2018 13:42

Instrument :
MSVOA_R
ClientSampleId :
C0T21

Tot Ion: 43 Resp: 22897

Ion Ratio Lower Upper

43 100

58 23.2 0.0 51.4

