

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR110518\
 Data File : VR026176.D
 Acq On : 5 Nov 2018 13:03
 Operator : SY/MD
 Sample : J5802-10
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 C0BD6

Quant Time: Nov 06 03:34:34 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR101518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Nov 06 03:06:52 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	559153	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.28	117	462053	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.23	152	138966	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.15	65	229756	4.69	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.80%
7) Chloroethane-d5	2.62	69	209756	4.99	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.80%
11) 1,1-Dichloroethene-d2	3.61	63	452425	3.76	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.20%
20) 2-Butanone-d5	6.58	46	203663	50.69	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.38%
24) Chloroform-d	7.20	84	385602	4.96	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.20%
26) 1,2-Dichloroethane-d4	7.90	65	163971	5.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.40%
32) Benzene-d6	7.85	84	789865	5.32	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.40%
36) 1,2-Dichloropropane-d6	8.89	67	209989	5.48	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	109.60%
41) Toluene-d8	9.97	98	754941	5.38	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.60%
43) trans-1,3-Dichloropropene-	10.23	79	50031	4.98	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	99.60%
46) 2-Hexanone-d5	10.59	63	162153	55.85	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	111.70%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	75058	4.99	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.80%
64) 1,2-Dichlorobenzene-d4	13.51	152	134455	6.12	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	122.40%#


Target Compounds				Ovalue
3) Chloromethane	2.01	50	7954	0.133 ug/L 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR110518\
Data File : VR026176.D
Acq On : 5 Nov 2018 13:03
Operator : SY/MD
Sample : J5802-10
Misc : 25mL/MSVOA R/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
C0BD6

Quant Time: Nov 06 03:34:34 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR101518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Nov 06 03:06:52 2018
Response via : Initial Calibration

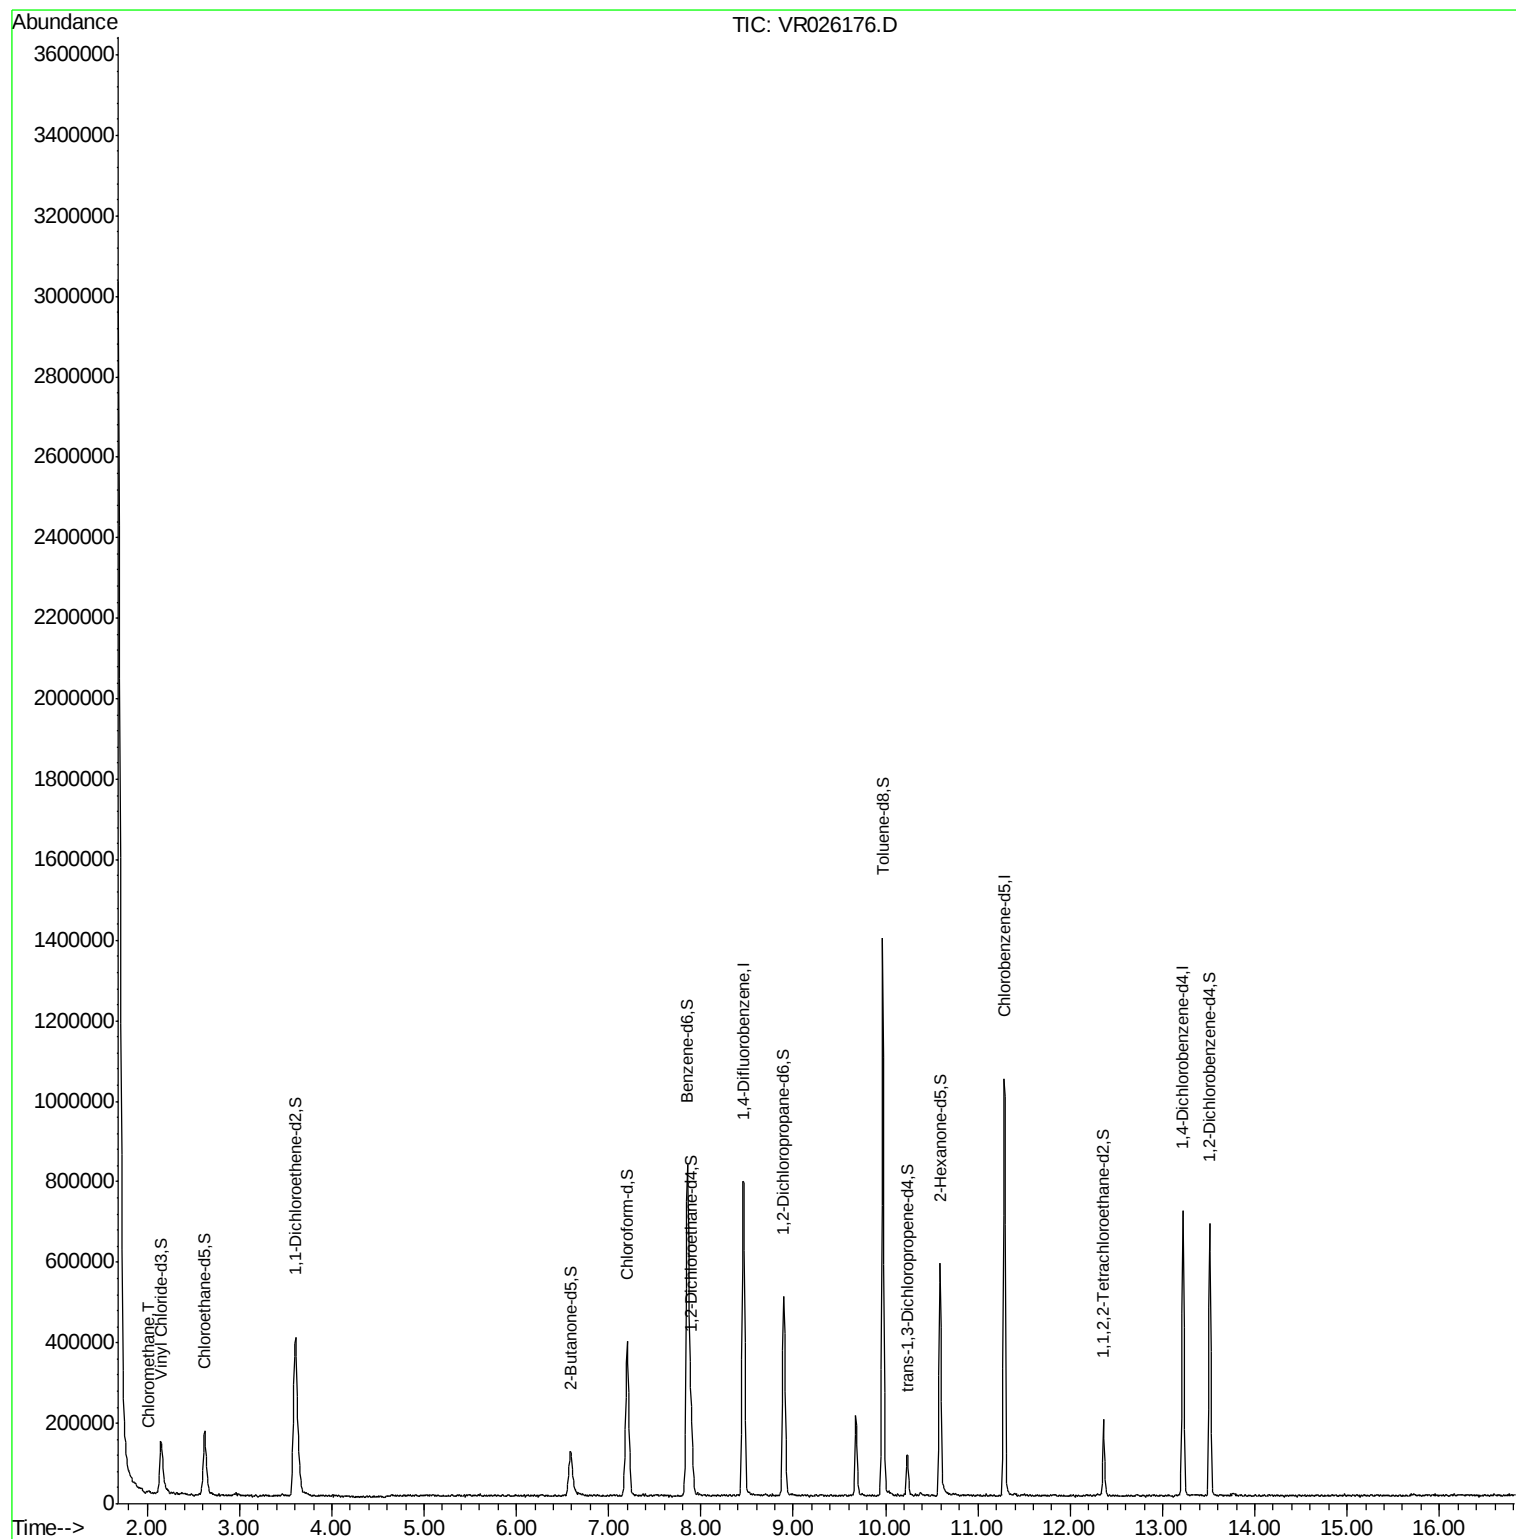

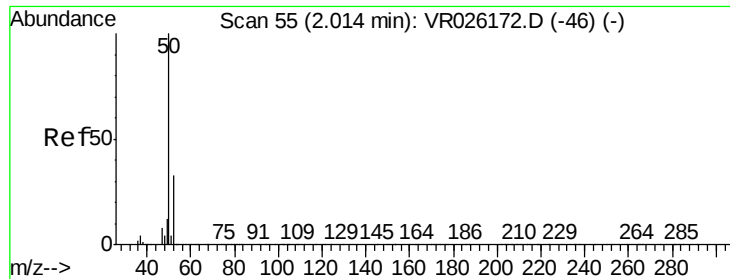

#3
 Chloromethane
 Concen: 0.133 ug/L
 RT: 2.01 min Scan# 54
 Delta R.T. -0.01 min
 Lab File: VR026176.D
 Acq: 5 Nov 2018 13:03

Instrument :
 MSVOA_R
 ClientSampleId :
 C0BD6

Tot Ion: 50 Resp: 7954
 Ion Ratio Lower Upper
 50 100
 52 30.9 22.0 40.8

