

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR122118\
 Data File : VR026292.D
 Acq On : 21 Dec 2018 21:11
 Operator : SY/MD
 Sample : J6536-02
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :

Quant Time: Dec 21 22:28:28 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR121718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Dec 21 22:24:46 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	490286	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	455689	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.23	152	209660	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.15	65	145619	4.67	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.40%
7) Chloroethane-d5	2.63	69	160358	5.18	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	103.60%
11) 1,1-Dichloroethene-d2	3.61	63	314193	3.56	ug/L	-0.01
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.20%
20) 2-Butanone-d5	6.59	46	119788	43.23	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	86.46%
24) Chloroform-d	7.20	84	325478	4.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.80%
26) 1,2-Dichloroethane-d4	7.90	65	131597	5.38	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.60%
32) Benzene-d6	7.85	84	643221	4.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.80%
36) 1,2-Dichloropropane-d6	8.90	67	157438	4.23	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	84.60%
41) Toluene-d8	9.97	98	575786	4.29	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.80%
43) trans-1,3-Dichloropropene-	10.24	79	41229	4.21	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.20%
46) 2-Hexanone-d5	10.59	63	129666	63.65	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	127.30%
57) 1,1,2,2-Tetrachloroethane-	12.37	84	79683	5.77	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	115.40%
64) 1,2-Dichlorobenzene-d4	13.52	152	171792	5.14	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.80%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
8) Chloroethane	2.66	64	23355	0.767	ug/L	98
13) Acetone	3.69	43	5840	2.069	ug/L	70
19) 1,1-Dichloroethane	5.69	63	86264	1.213	ug/L	96
30) Cyclohexane	7.52	56	103963	1.572	ug/L	99
33) Benzene	7.91	78	1164138	6.490	ug/L	100
35) Methylcyclohexane	8.96	83	42578	0.621	ug/L	89
37) 1,2-Dichloropropane	8.89	63	22770	0.620	ug/L #	96
42) Toluene	10.04	91	25268	0.138	ug/L	95
44) trans-1,3-Dichloropropene	10.24	75	3143	0.109	ug/L #	72
45) 1,1,2-Trichloroethane	10.42	97	42170	2.766	ug/L #	20
48) 2-Hexanone	10.59	43	29566	5.189	ug/L #	60
51) Chlorobenzene	11.32	112	29788	0.290	ug/L	98
52) Ethylbenzene	11.39	91	67308	0.325	ug/L	95
56) Isopropylbenzene	12.13	105	10237523	53.382	ug/L #	81
58) 1,1,2,2-Tetrachloroethane	12.35	83	21264	1.579	ug/L #	34
59) 1,2,3-Trichloropropane	12.48	75	115526	11.069	ug/L #	1
65) 1,2-Dichlorobenzene	13.53	146	21488	0.387	ug/L #	86

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR122118\
Data File : VR026292.D
Acq On : 21 Dec 2018 21:11
Operator : SY/MD
Sample : J6536-02
Misc : 25mL/MSVOA R/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :

Quant Time: Dec 21 22:28:28 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR121718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 21 22:24:46 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
66) 1,2-Dibromo-3-chloropropan	14.17	75	738	0.375	ug/L #	28
69) Naphthalene	15.00	128	5911	0.278	ug/L #	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA R\DATA\VR122118\
Data File : VR026292.D
Acq On : 21 Dec 2018 21:11
Operator : SY/MD
Sample : J6536-02
Misc : 25mL/MSVOA R/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :

Quant Time: Dec 21 22:28:28 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR121718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 21 22:24:46 2018
Response via : Initial Calibration




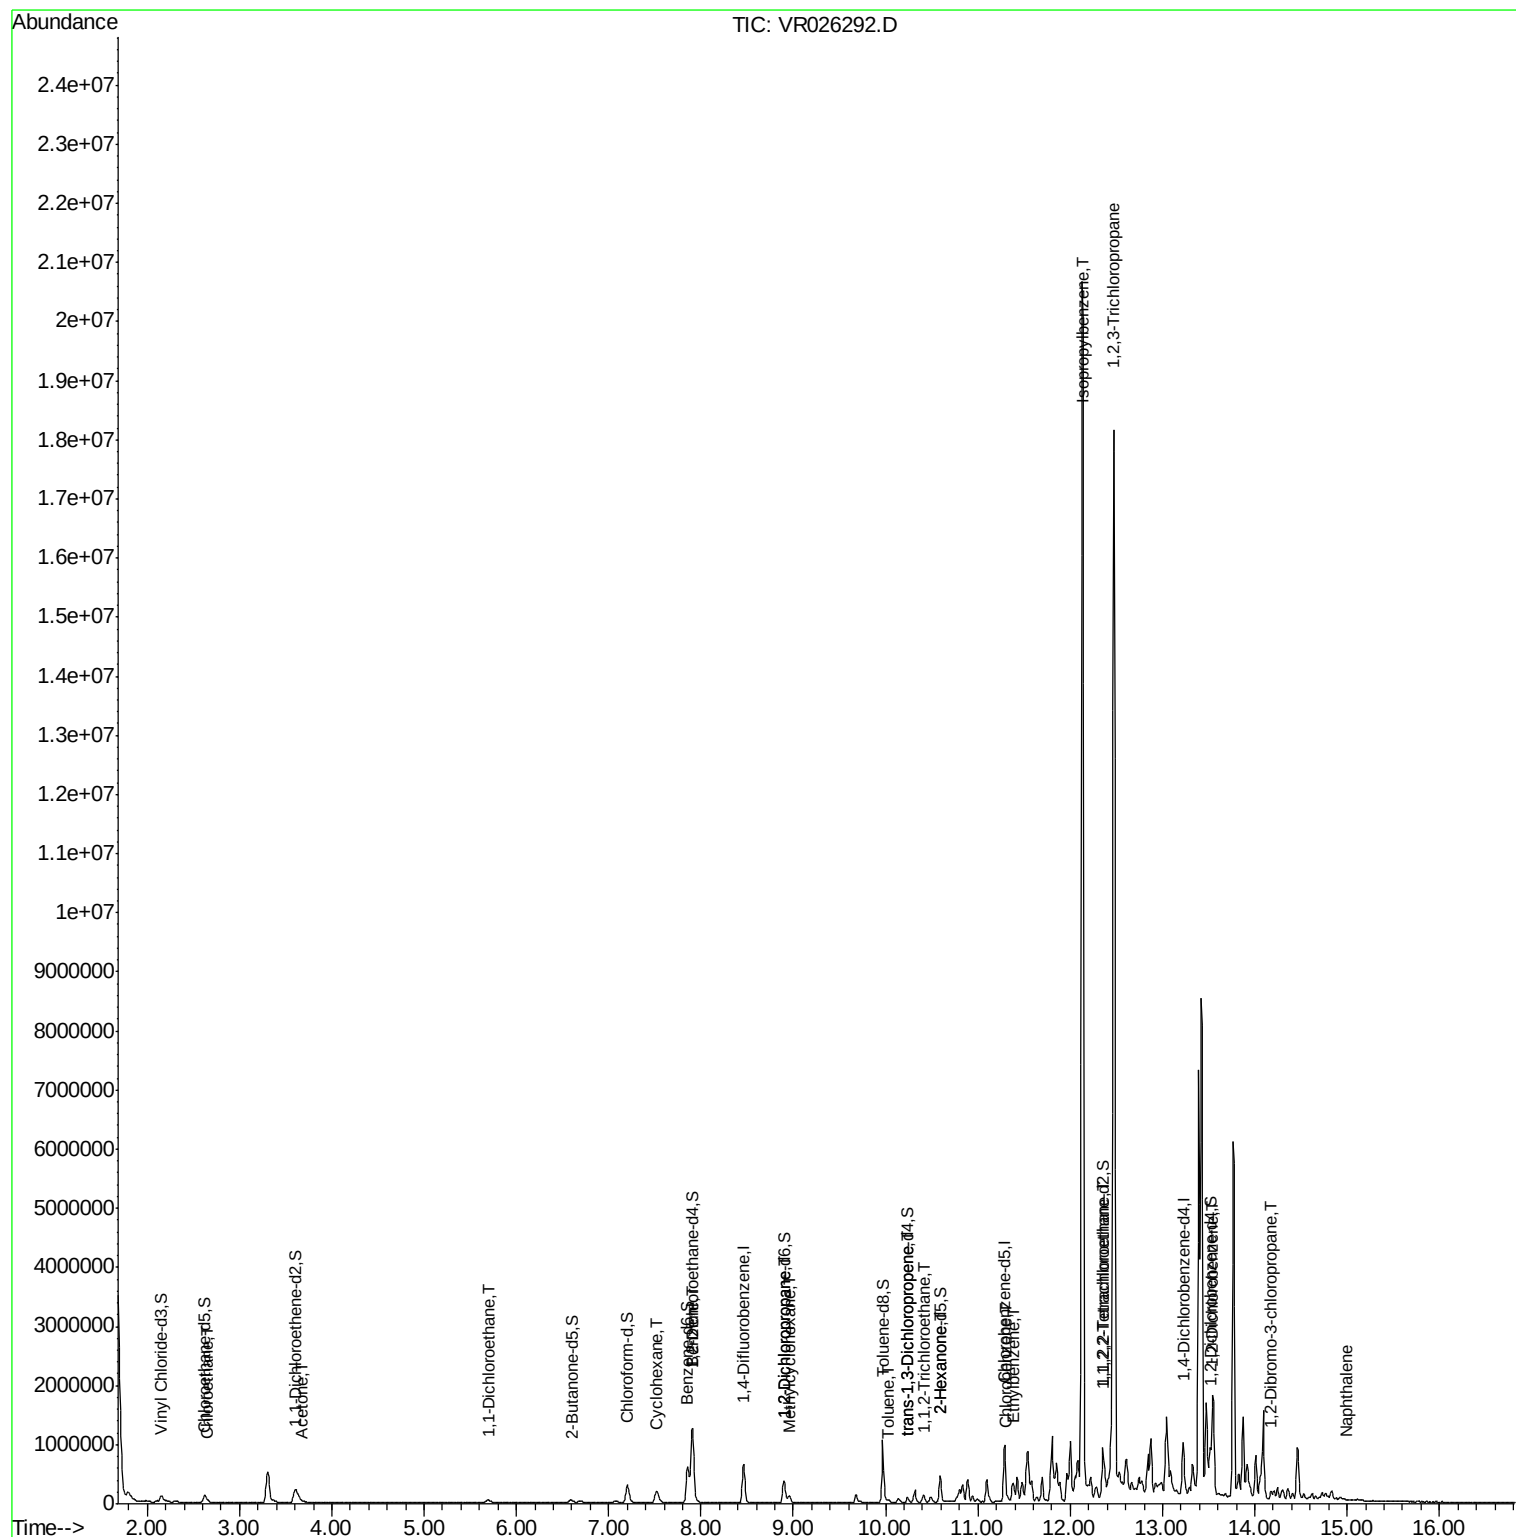


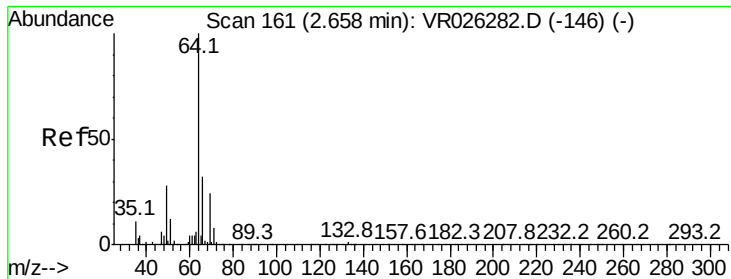

#8
Chloroethane
Concen: 0.767 ug/L
RT: 2.66 min Scan# 161
Delta R.T. 0.00 min
Lab File: VR026292.D
Acq: 21 Dec 2018 21:11




Instrument :
MSVOA_R
ClientSampled :


Tot Ion: 64 Resp: 23355
Ion Ratio Lower Upper
64 100
66 32.8 22.2 41.2

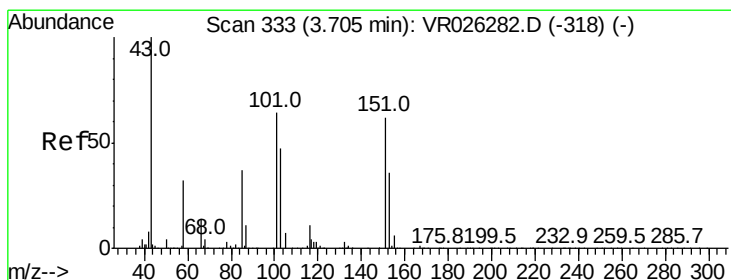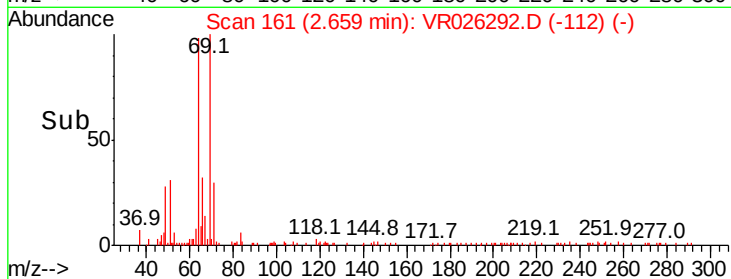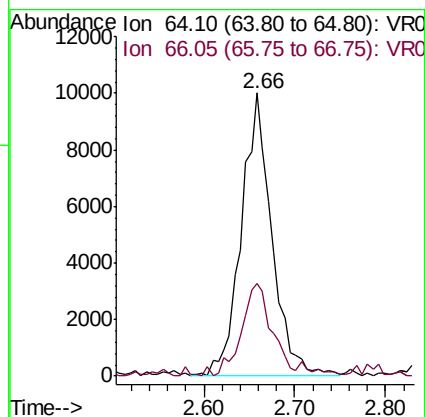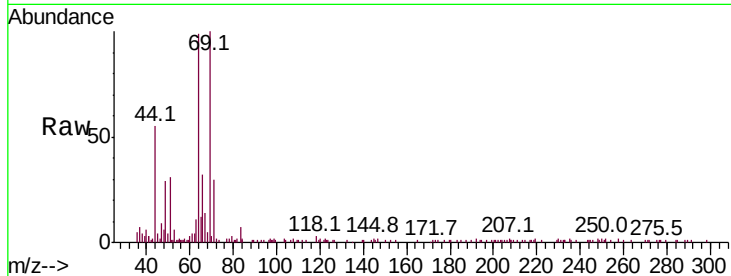

#13
Acetone
Concen: 2.069 ug/L
RT: 3.69 min Scan# 330
Delta R.T. -0.02 min
Lab File: VR026292.D
Acq: 21 Dec 2018 21:11

Tgt Ion: 43 Resp: 5840
Ion Ratio Lower Upper
43 100
58 14.3 0.0 60.8


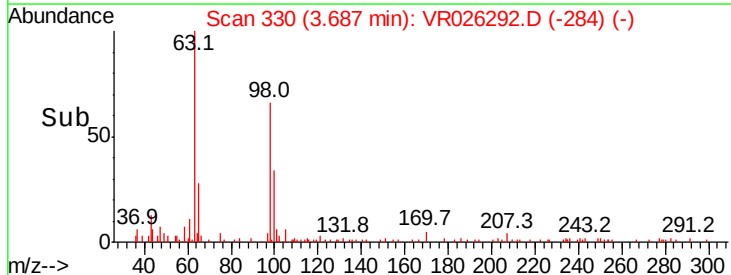
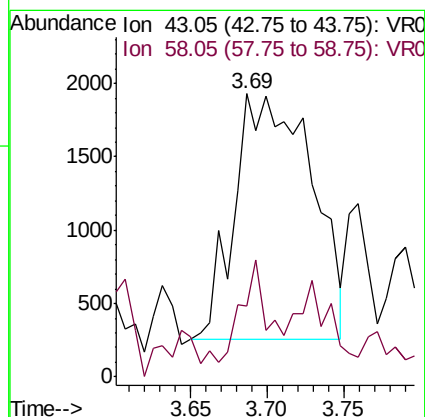
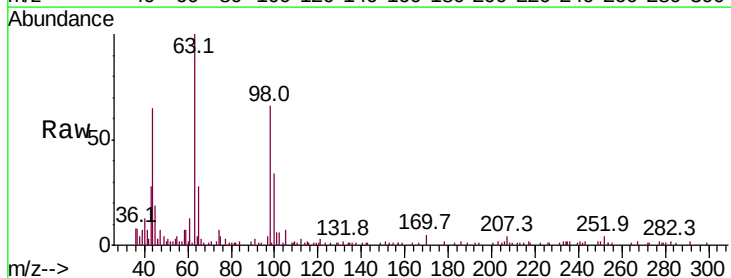


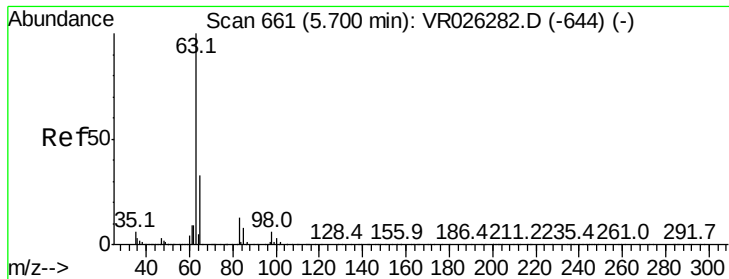

#19
 1,1-Dichloroethane
 Concen: 1.213 ug/L
 RT: 5.69 min Scan# 660
 Delta R.T. -0.01 min
 Lab File: VR026292.D
 Acq: 21 Dec 2018 21:11




Instrument :
 MSVOA_R
 ClientSampleId :


Tot Ion:	63	Resp:	86264
Ion	Ratio	Lower	Upper
63	100		
65	33.1	21.6	40.0
83	11.8	9.0	16.8

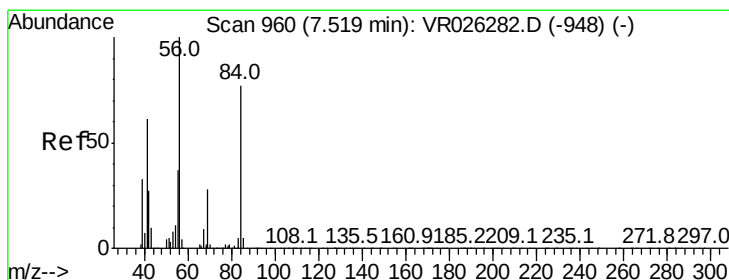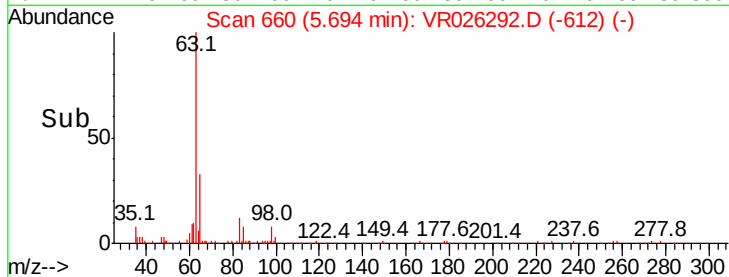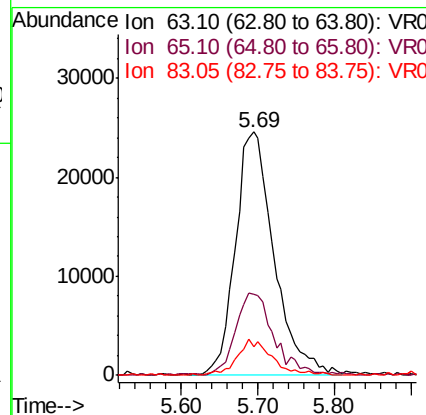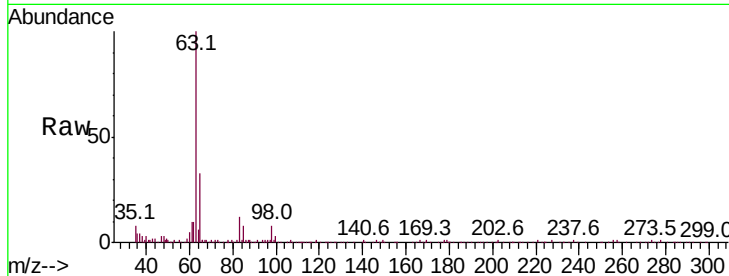

#30
 Cyclohexane
 Concen: 1.572 ug/L
 RT: 7.52 min Scan# 960
 Delta R.T. 0.00 min
 Lab File: VR026292.D
 Acq: 21 Dec 2018 21:11

Tgt Ion:	56	Resp:	103963
Ion	Ratio	Lower	Upper
56	100		
69	29.8	24.0	36.0
84	81.5	64.5	96.7

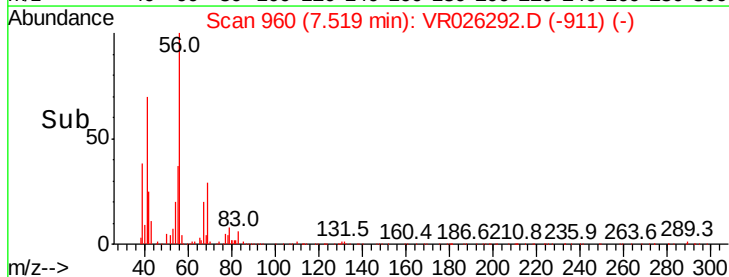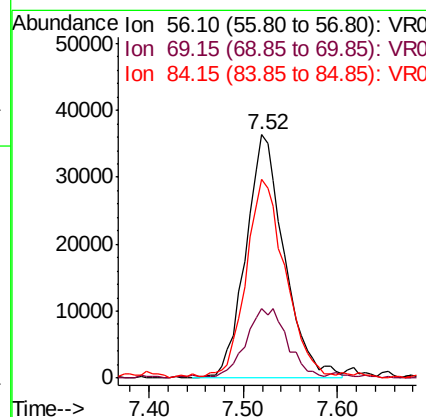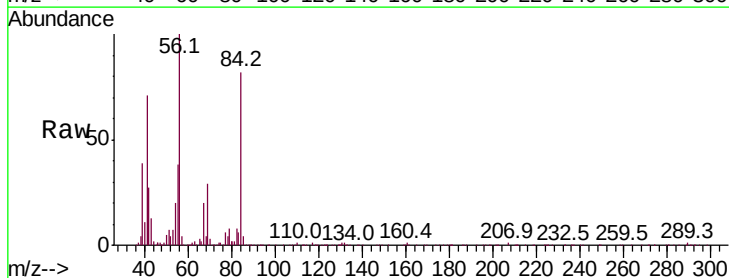

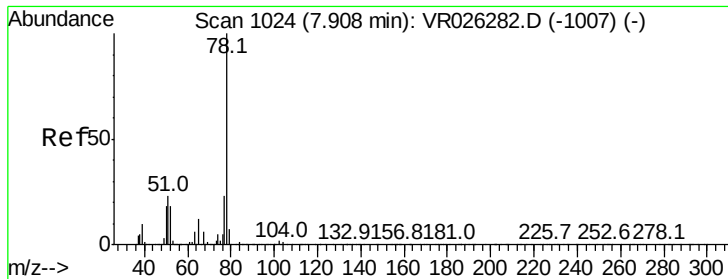

#33

Benzene

Concen: 6.490 ug/L

RT: 7.91 min Scan# 1024





Delta R.T. 0.00 min

Lab File: VR026292.D

Acq: 21 Dec 2018 21:11

Instrument :
MSVOA_R
ClientSampled :

Tgt Ion: 78 Resp: 1164138

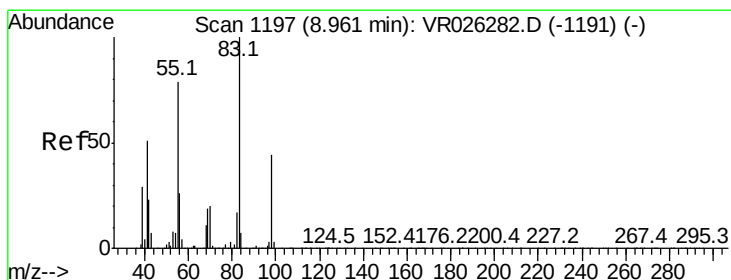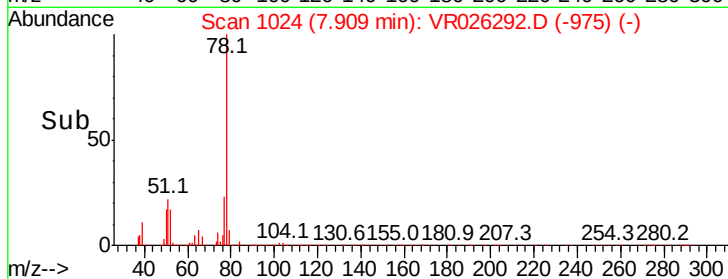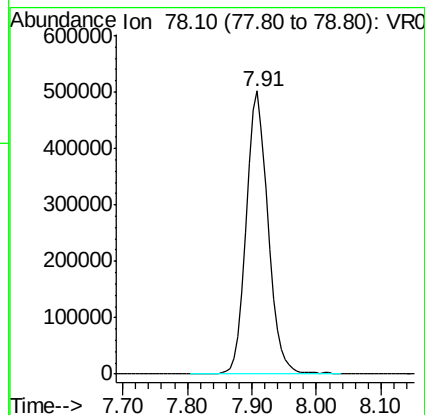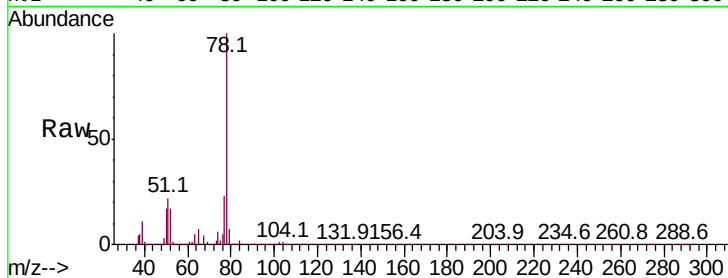

#35

Methylcyclohexane

Concen: 0.621 ug/L

RT: 8.96 min Scan# 1197




Delta R.T. 0.00 min


Lab File: VR026292.D

Acq: 21 Dec 2018 21:11

Tgt Ion: 83 Resp: 42578

Ion	Ratio	Lower	Upper
83	100		
55	97.7	66.6	99.8
98	44.5	35.5	53.3


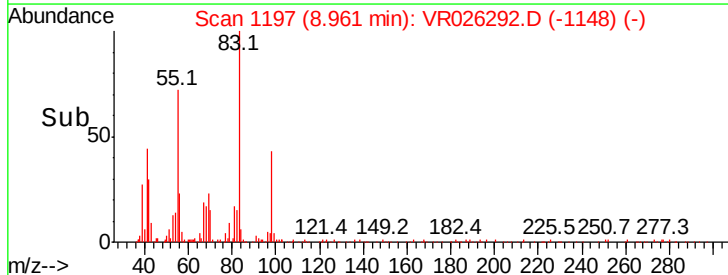
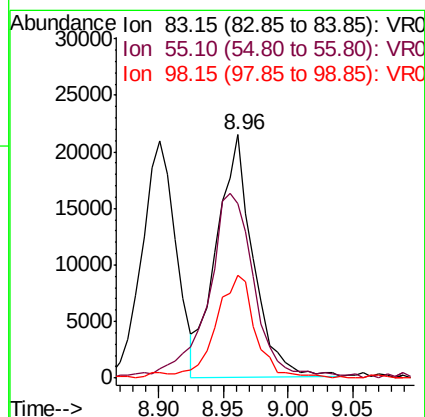
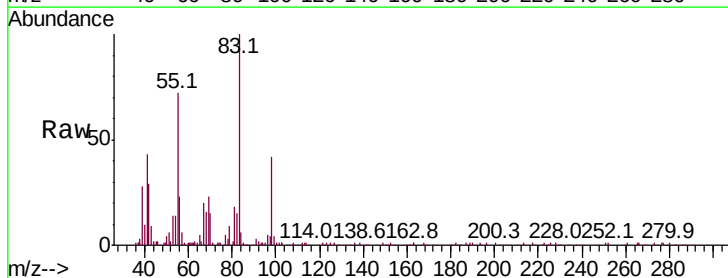


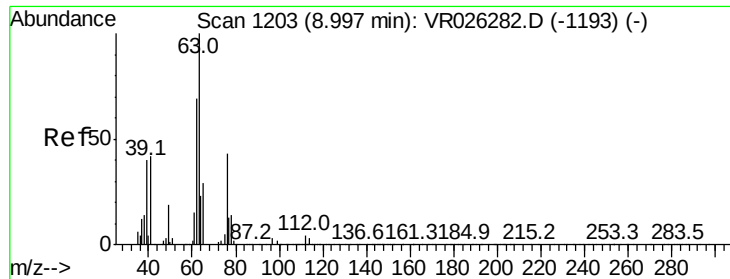

#37
 1,2-Dichloropropane
 Concen: 0.620 ug/L
 RT: 8.89 min Scan# 1186
 Delta R.T. -0.10 min
 Lab File: VR026292.D
 Acq: 21 Dec 2018 21:11




Instrument :
 MSVOA_R
 ClientSampleId :


Tot Ion: 63 Resp: 22770
 Ion Ratio Lower Upper
 63 100
 112 2.5 3.0 4.6#

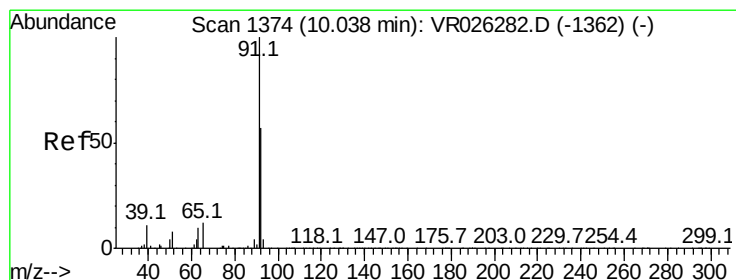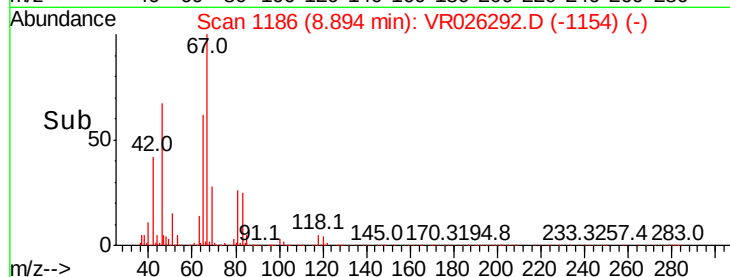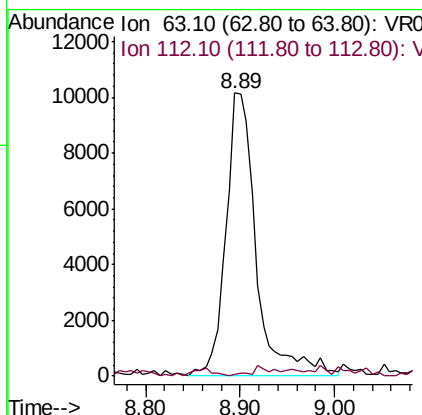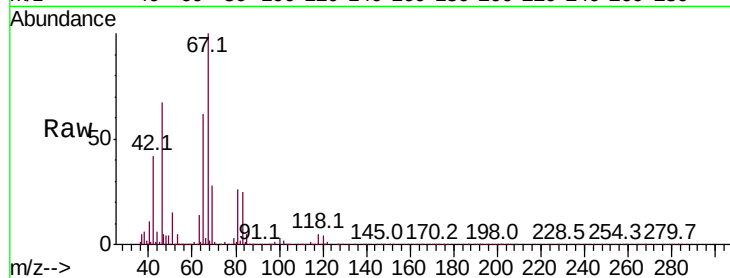

#42
 Toluene
 Concen: 0.138 ug/L
 RT: 10.04 min Scan# 1374
 Delta R.T. 0.00 min
 Lab File: VR026292.D
 Acq: 21 Dec 2018 21:11

Tgt Ion: 91 Resp: 25268
 Ion Ratio Lower Upper
 91 100
 92 53.4 40.0 74.4

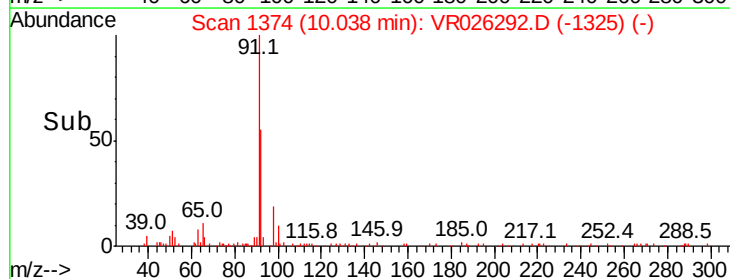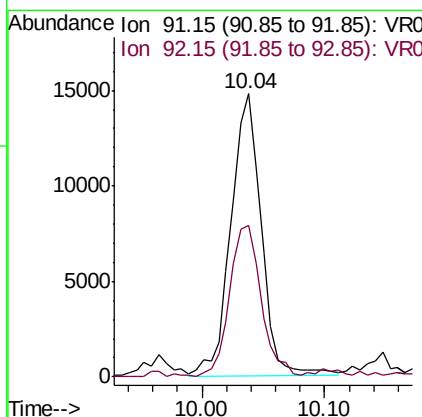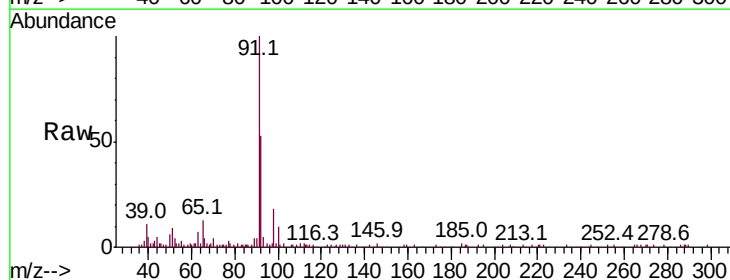

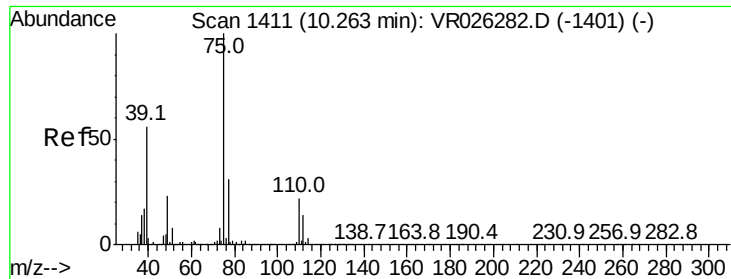

#44

trans-1,3-Dichloropropene

Concen: 0.109 ug/L

RT: 10.24 min Scan# 1407

Delta R.T. -0.02 min

Lab File: VR026292.D

Acq: 21 Dec 2018 21:11

Instrument :

MSVOA_R





ClientSampleId :

Tot Ion: 75 Resp: 3143

Ion Ratio Lower Upper

75 100

77 45.3 21.2 39.4#

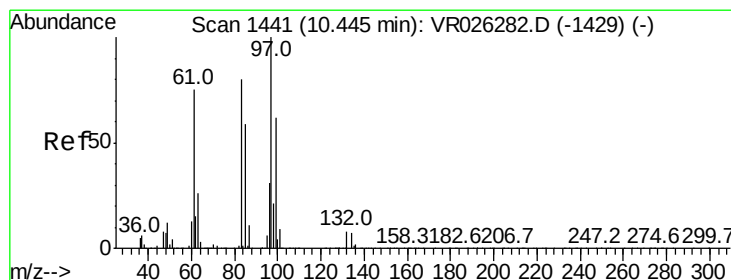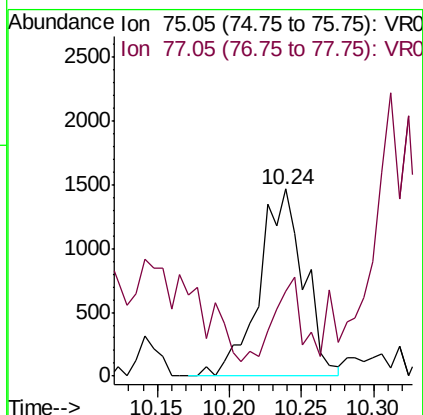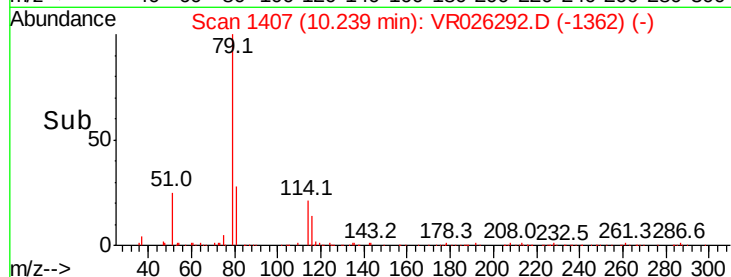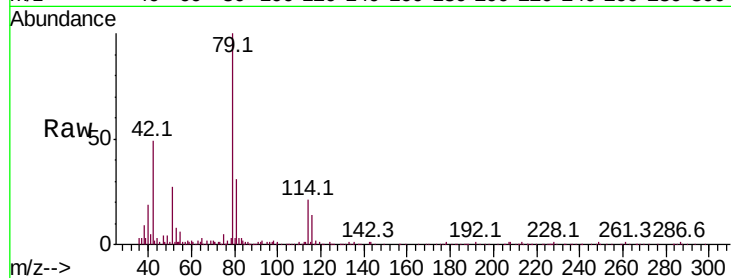

#45

1,1,2-Trichloroethane

Concen: 2.766 ug/L

RT: 10.42 min Scan# 1436

Delta R.T. -0.03 min

Lab File: VR026292.D

Acq: 21 Dec 2018 21:11

Tgt Ion: 97 Resp: 42170




Ion Ratio Lower Upper


97 100

99 0.4 45.0 83.6#

83 7.9 57.9 107.5#

85 1.4 38.9 72.2#


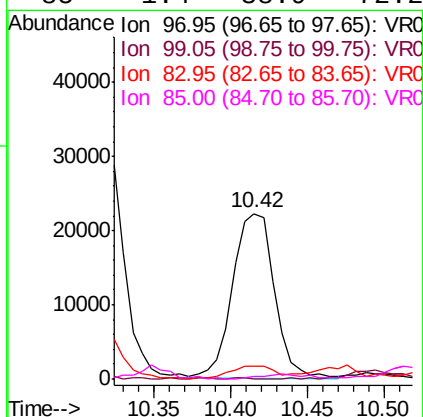
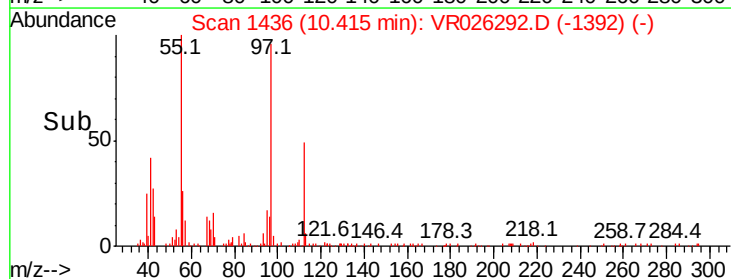
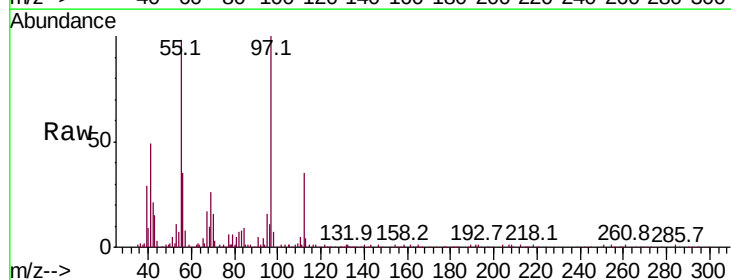


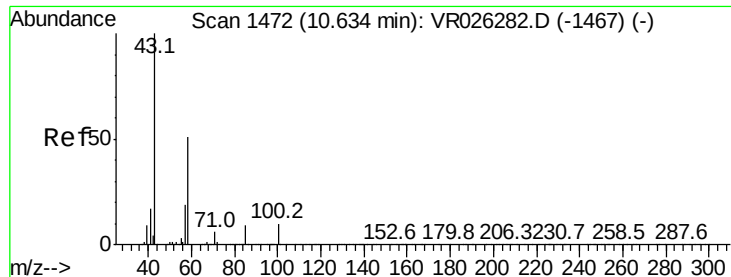

#48
2-Hexanone
Concen: 5.189 ug/L
RT: 10.59 min Scan# 1465
Delta R.T. -0.04 min
Lab File: VR026292.D
Acq: 21 Dec 2018 21:11




Instrument :
MSVOA_R
ClientSampled :


Tot Ion	Ratio	Lower	Upper
43	100		
58	18.6	40.5	60.7#
57	32.4	14.2	21.4#
100	1.5	7.5	11.3#

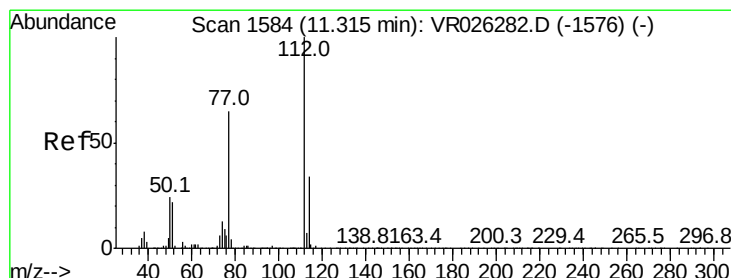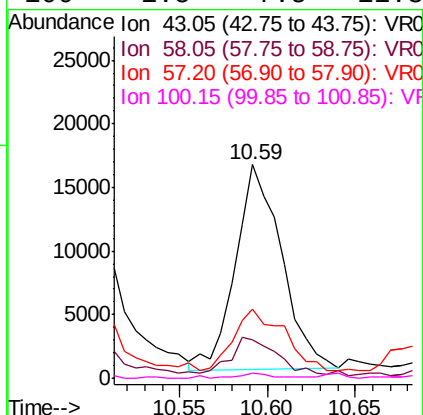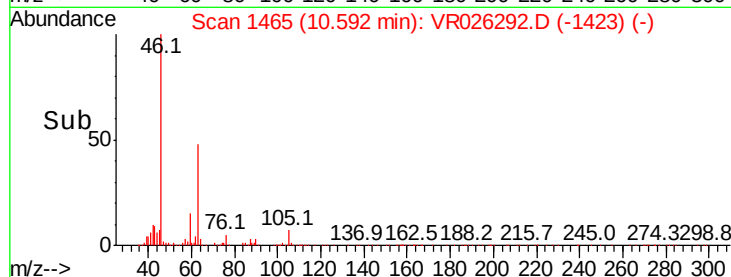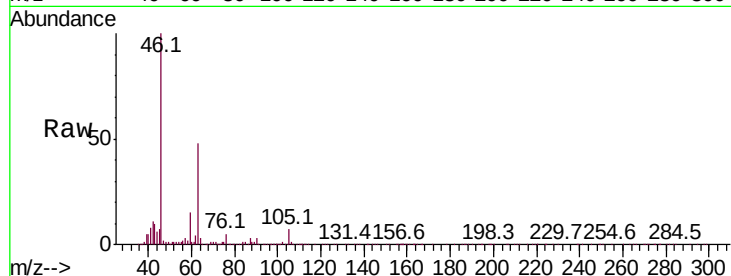

#51
Chlorobenzene
Concen: 0.290 ug/L
RT: 11.32 min Scan# 1584
Delta R.T. 0.00 min
Lab File: VR026292.D
Acq: 21 Dec 2018 21:11

Tgt Ion	Ratio	Lower	Upper
112	100		
114	30.8	21.7	40.3
77	59.4	49.4	74.2

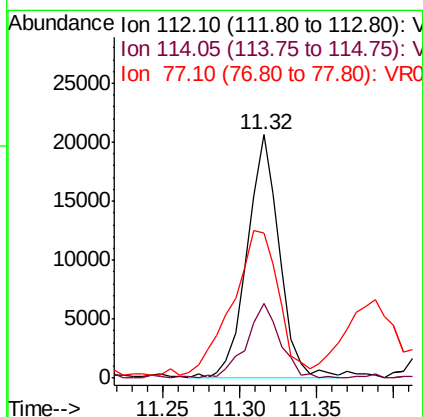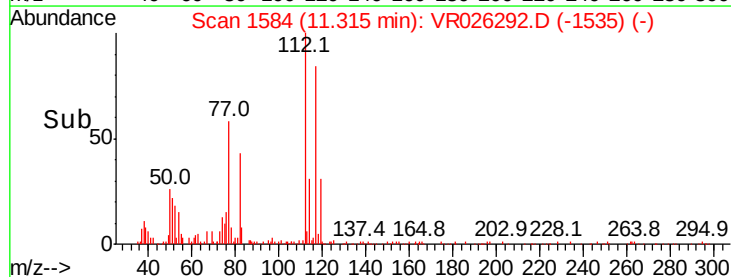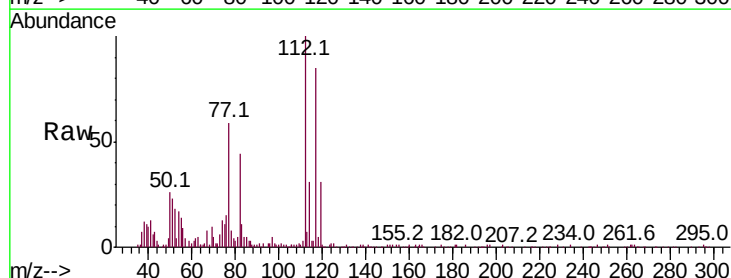

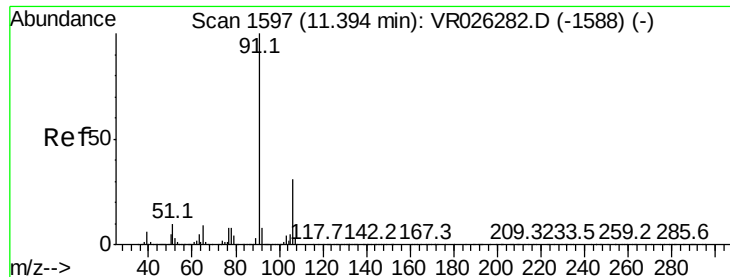

#52

Ethylbenzene

Concen: 0.325 ug/L

RT: 11.39 min Scan# 1597

Delta R.T. 0.00 min

Lab File: VR026292.D

Acq: 21 Dec 2018 21:11

Instrument :

MSVOA_R





ClientSampled :

Tot Ion: 91 Resp: 67308

Ion Ratio Lower Upper

91 100

106 33.2 21.4 39.8

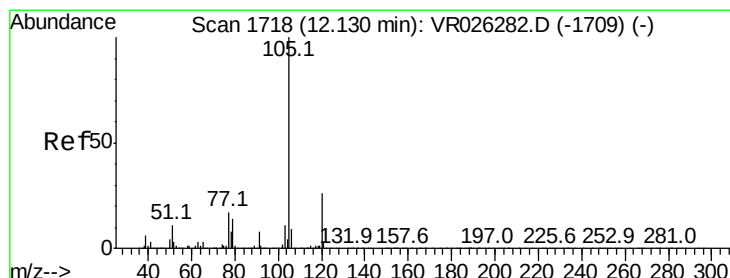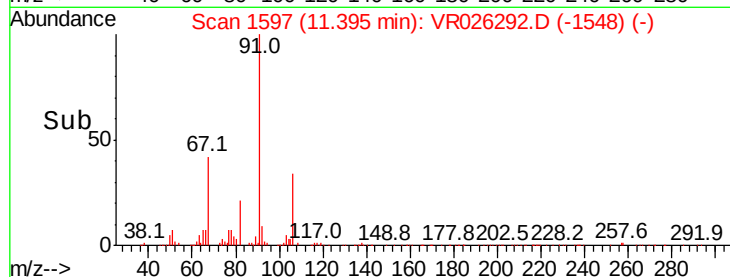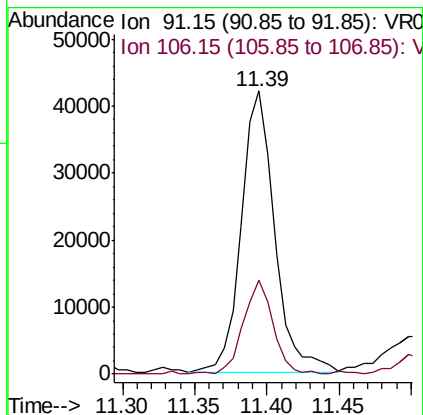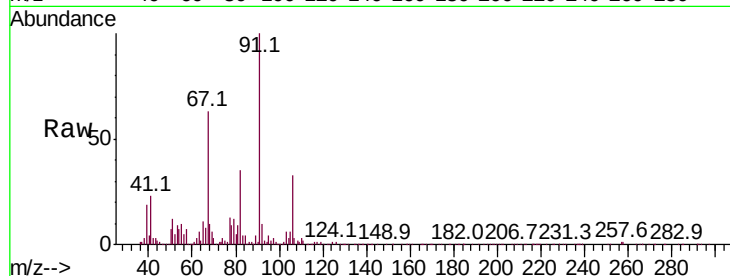

#56

Isopropylbenzene

Concen: 53.382 ug/L

RT: 12.13 min Scan# 1718

Delta R.T. 0.00 min

Lab File: VR026292.D

Acq: 21 Dec 2018 21:11




Tgt Ion: 105 Resp: 10237523


Ion Ratio Lower Upper

105 100

120 37.6 21.2 31.8#

77 23.6 13.6 20.4#

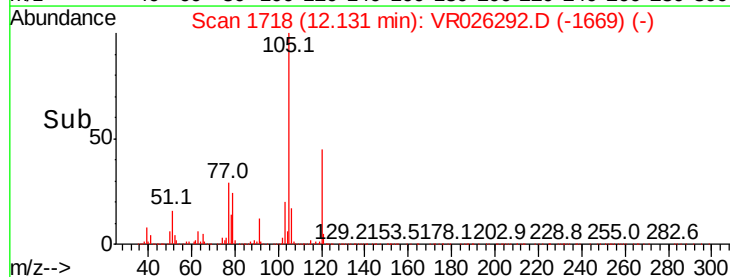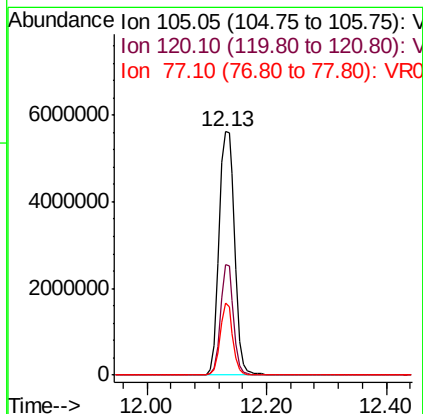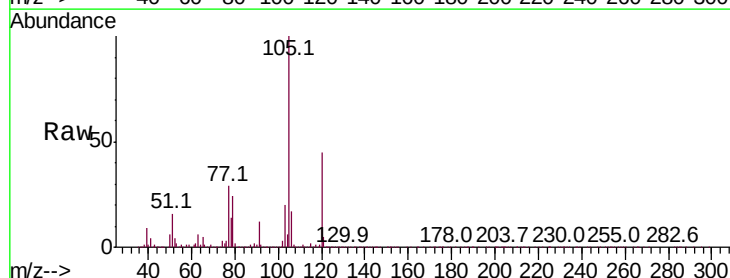

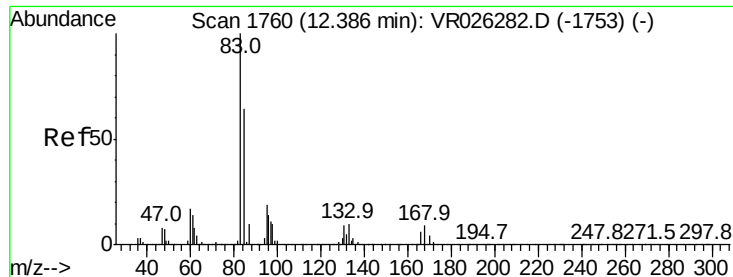

#58

1,1,2,2-Tetrachloroethane

Concen: 1.579 ug/L

RT: 12.35 min Scan# 1754

Delta R.T. -0.04 min

Lab File: VR026292.D

Acq: 21 Dec 2018 21:11

Instrument :

MSVOA_R

ClientSampled :





Tot Ion: 83 Resp: 21264

Ion Ratio Lower Upper

83 100

85 8.8 46.9 87.1#

131 3.5 7.7 11.5#

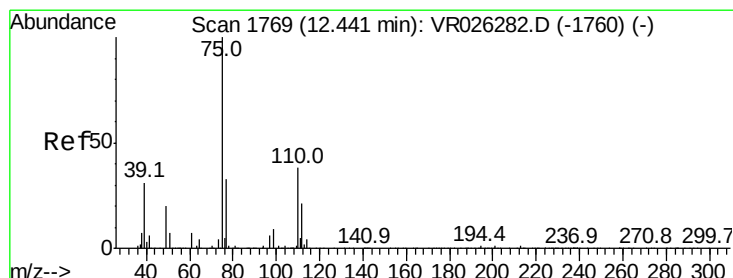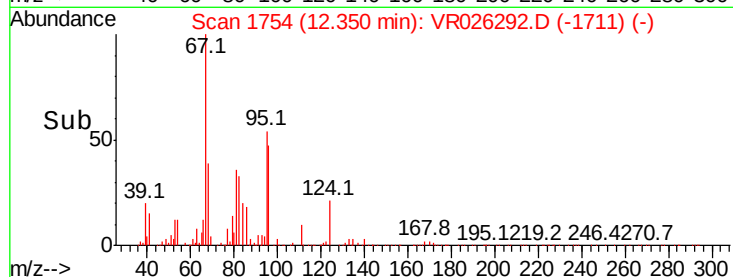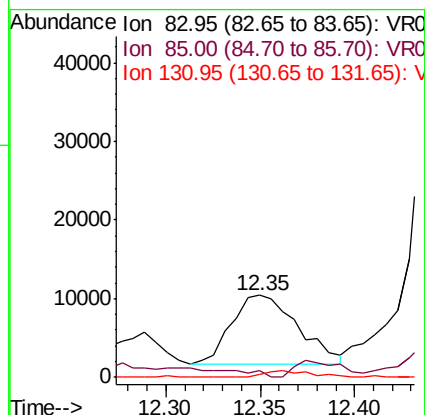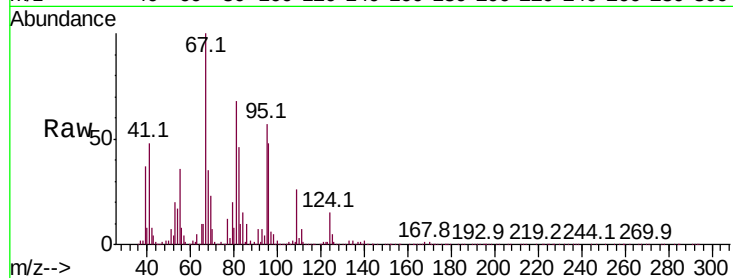

#59

1,2,3-Trichloropropane

Concen: 11.069 ug/L

RT: 12.48 min Scan# 1775

Delta R.T. 0.04 min

Lab File: VR026292.D




Acq: 21 Dec 2018 21:11


Tgt Ion: 75 Resp: 115526

Ion Ratio Lower Upper

75 100

77 639.4 27.0 40.6#


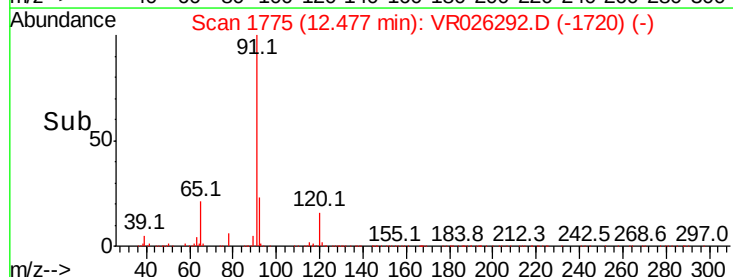
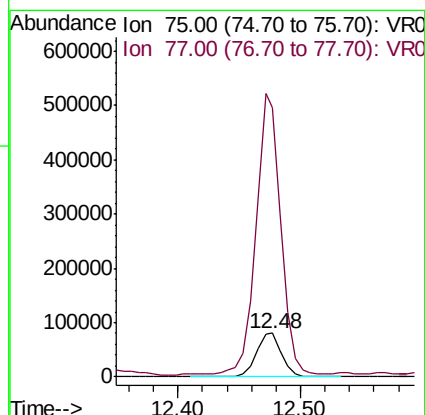
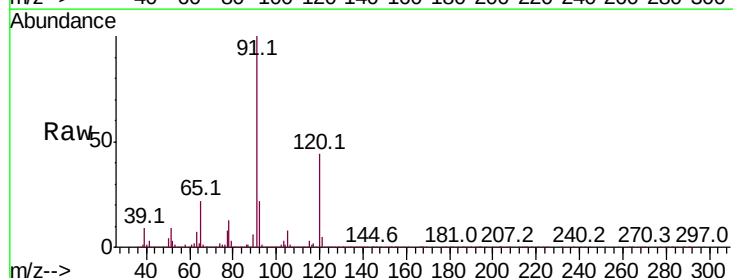


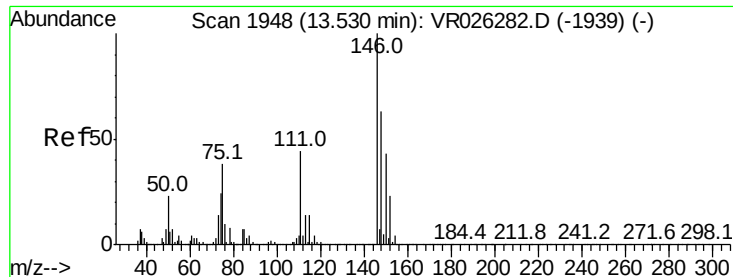

#65
 1,2-Dichlorobenzene
 Concen: 0.387 ug/L
 RT: 13.53 min Scan# 1948
 Delta R.T. 0.00 min
 Lab File: VR026292.D
 Acq: 21 Dec 2018 21:11




Instrument :
 MSVOA_R
 ClientSampled :


Tot Ion	Ratio	Lower	Upper
146	100		
111	58.0	34.6	52.0#
148	57.8	51.0	76.6

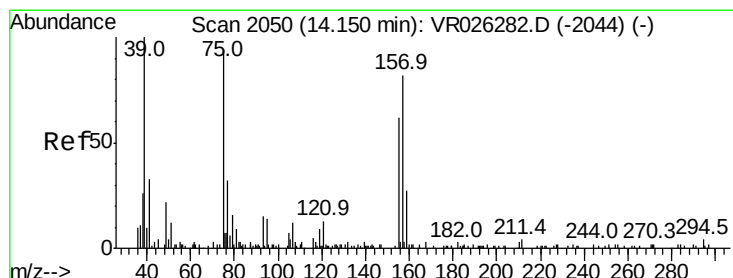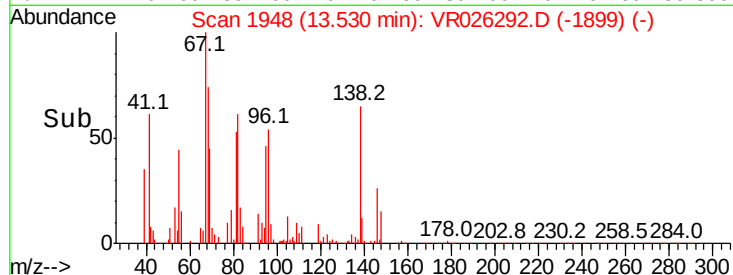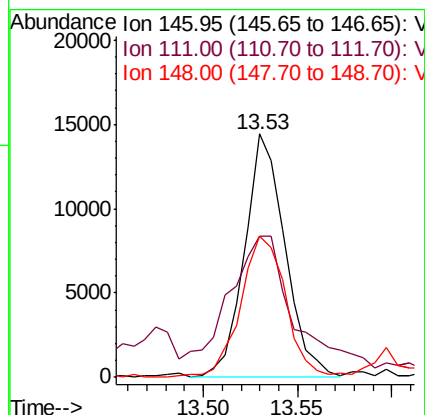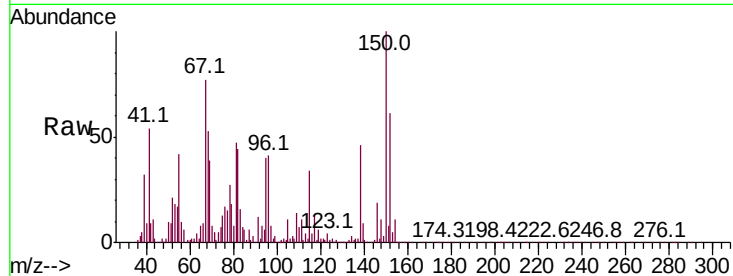

#66
 1,2-Dibromo-3-chloropropane
 Concen: 0.375 ug/L
 RT: 14.17 min Scan# 2053
 Delta R.T. 0.02 min
 Lab File: VR026292.D
 Acq: 21 Dec 2018 21:11

Tgt Ion	Ratio	Lower	Upper
75	100		
155	12.4	44.4	66.6#
157	10.8	66.3	99.5#

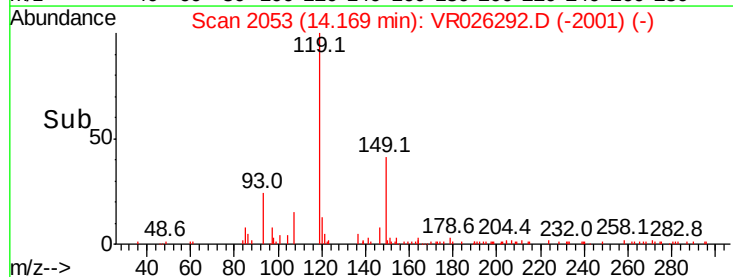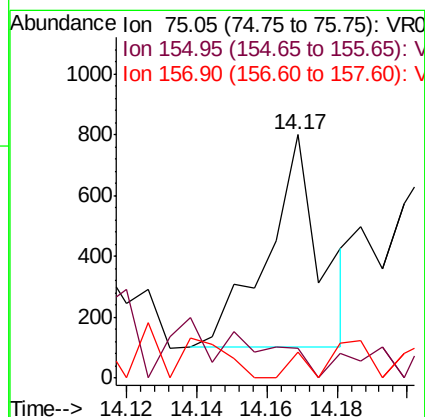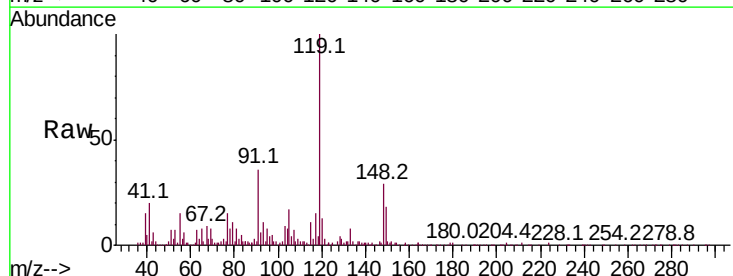

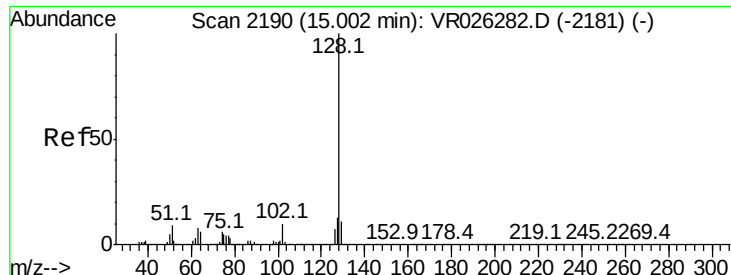

#69

Naphthalene

Concen: 0.278 ug/L

RT: 15.00 min Scan# 2190

Delta R.T. 0.00 min

Lab File: VR026292.D

Acq: 21 Dec 2018 21:11

Instrument :

MSVOA_R

ClientSampleId :


Tot Ion:128 Resp: 5911

Ion Ratio Lower Upper

128 100

127 18.8 11.1 16.7#

129 14.8 8.7 13.1#

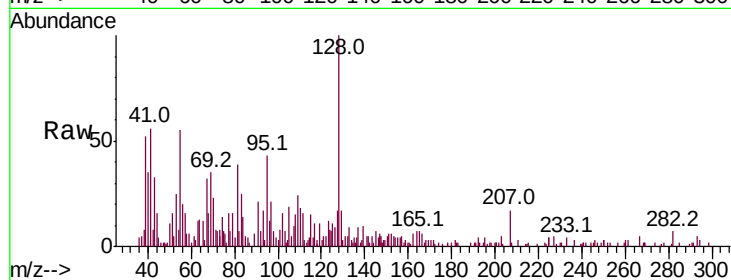

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

