




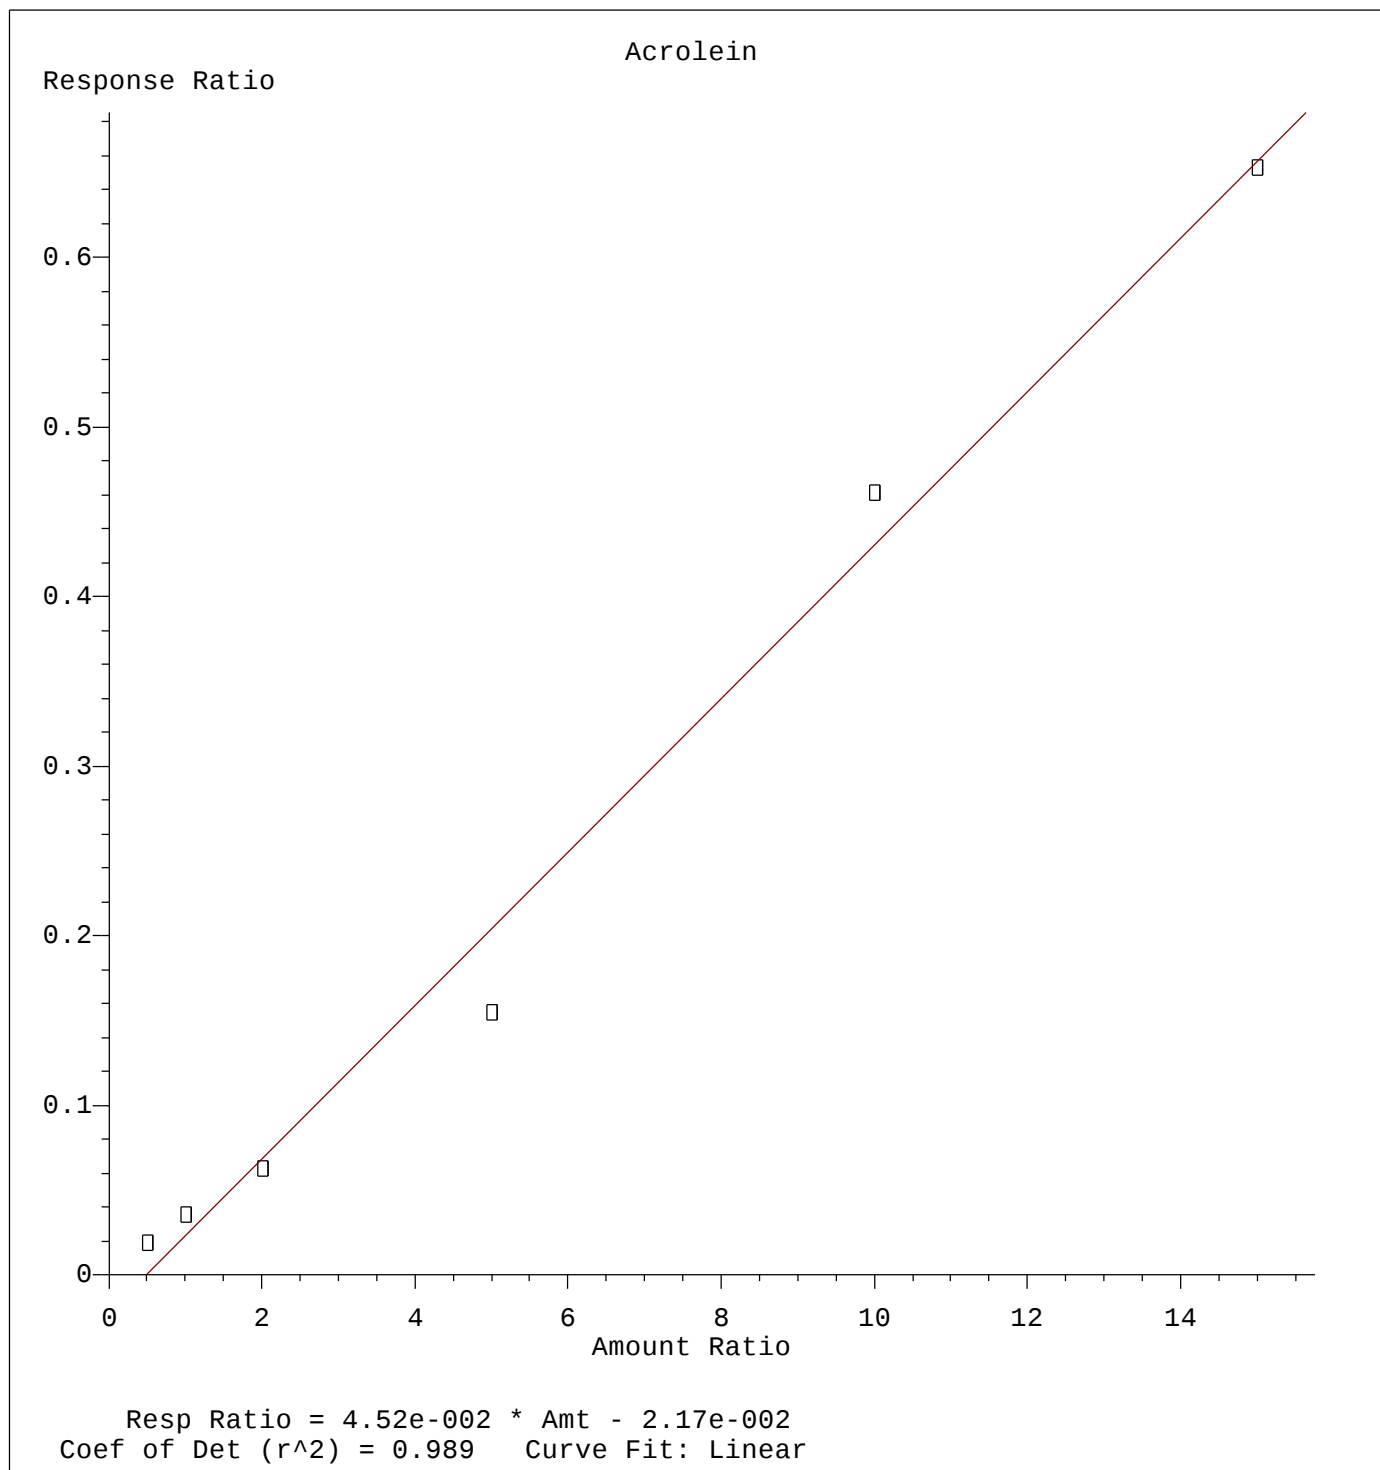


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y010220S.M
Calibration Table Last Updated: Thu Jan 02 13:15:14 2020

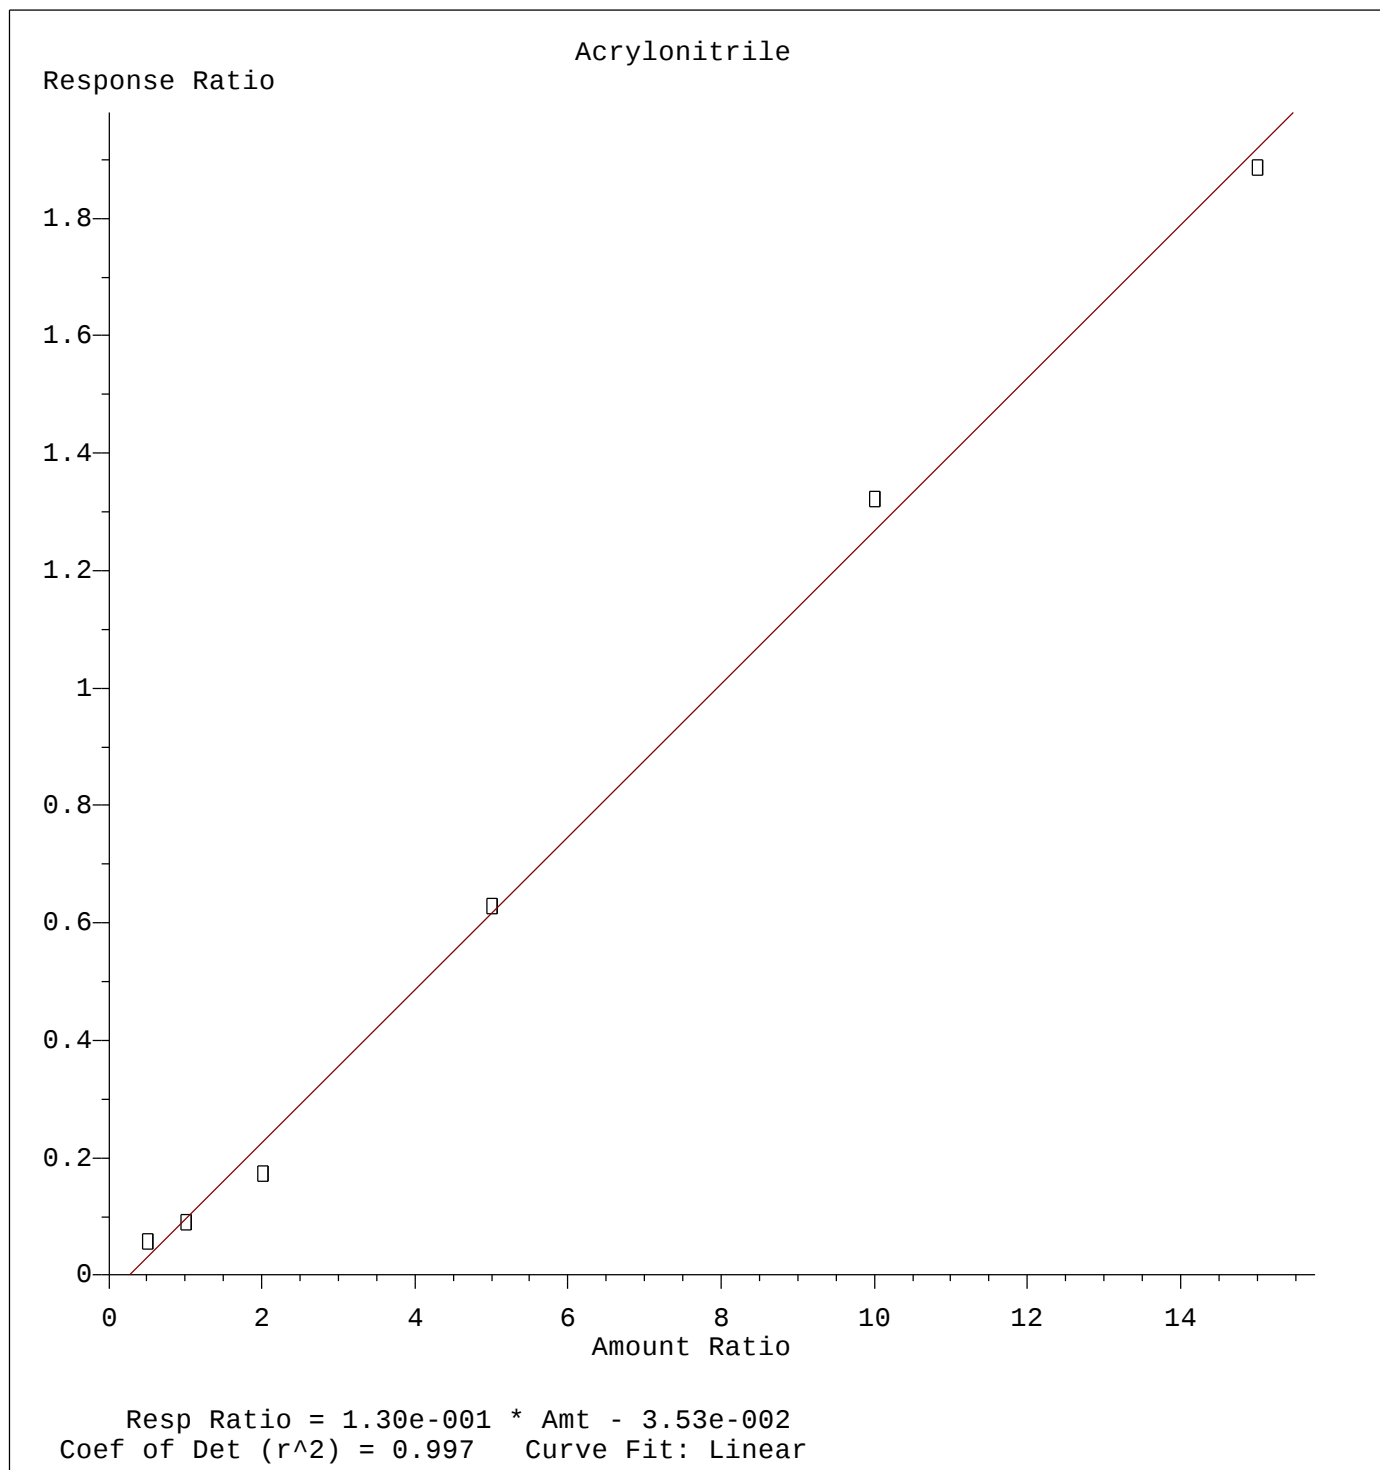


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y010220S.M
Calibration Table Last Updated: Thu Jan 02 13:16:38 2020

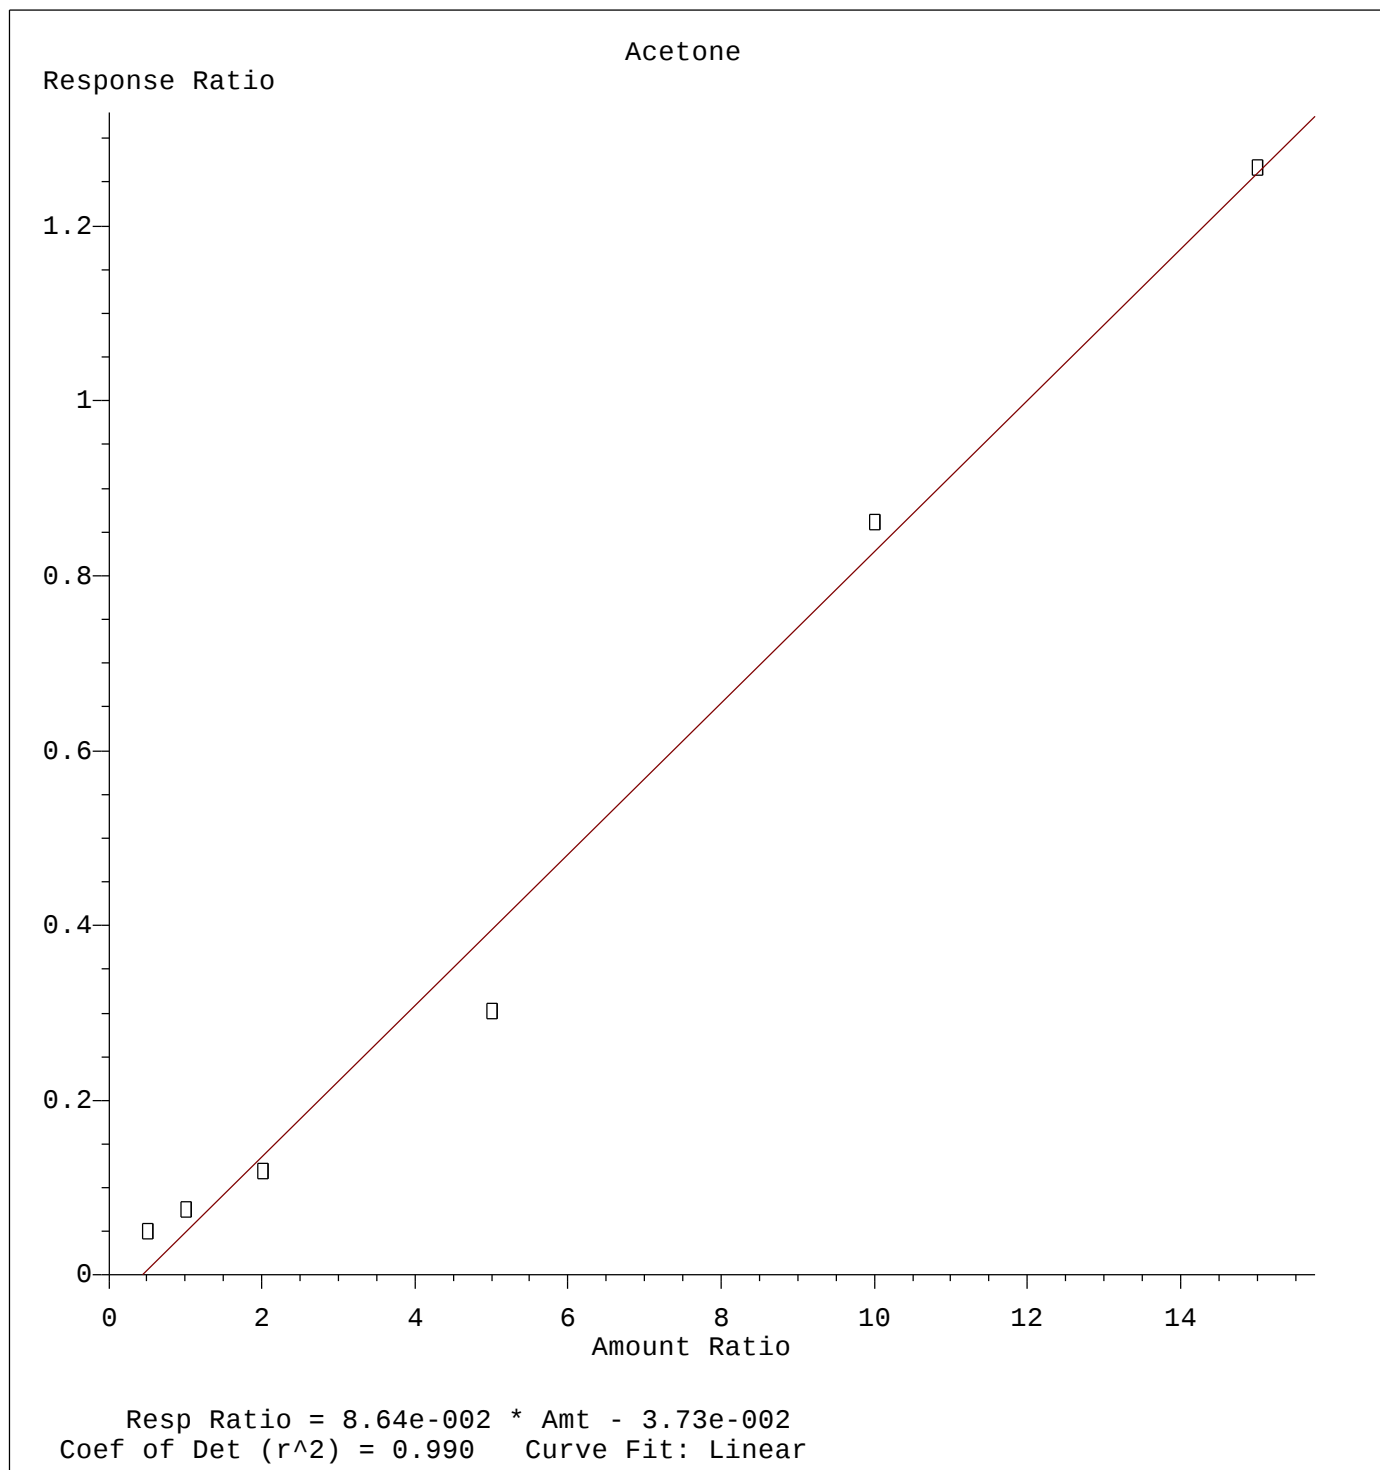


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y010220S.M
Calibration Table Last Updated: Thu Jan 02 13:16:38 2020

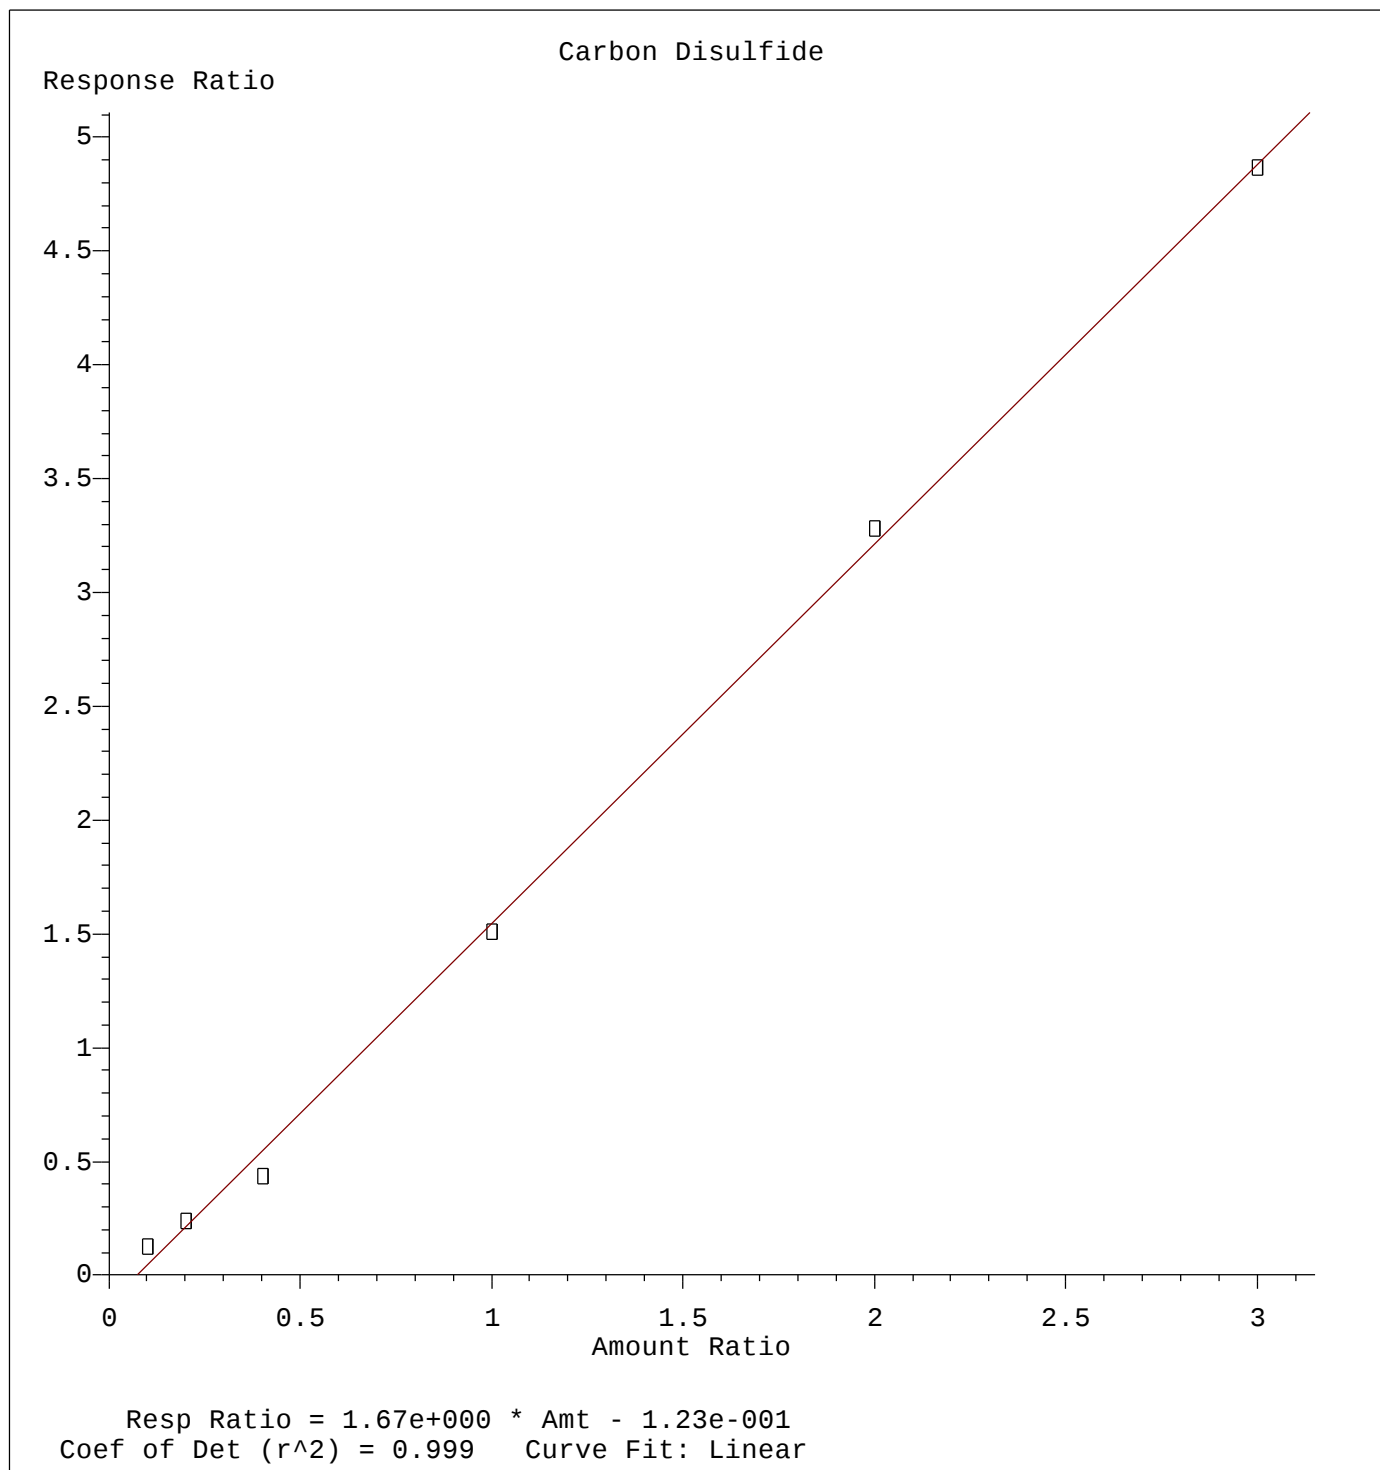


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y010220S.M
Calibration Table Last Updated: Thu Jan 02 13:16:38 2020

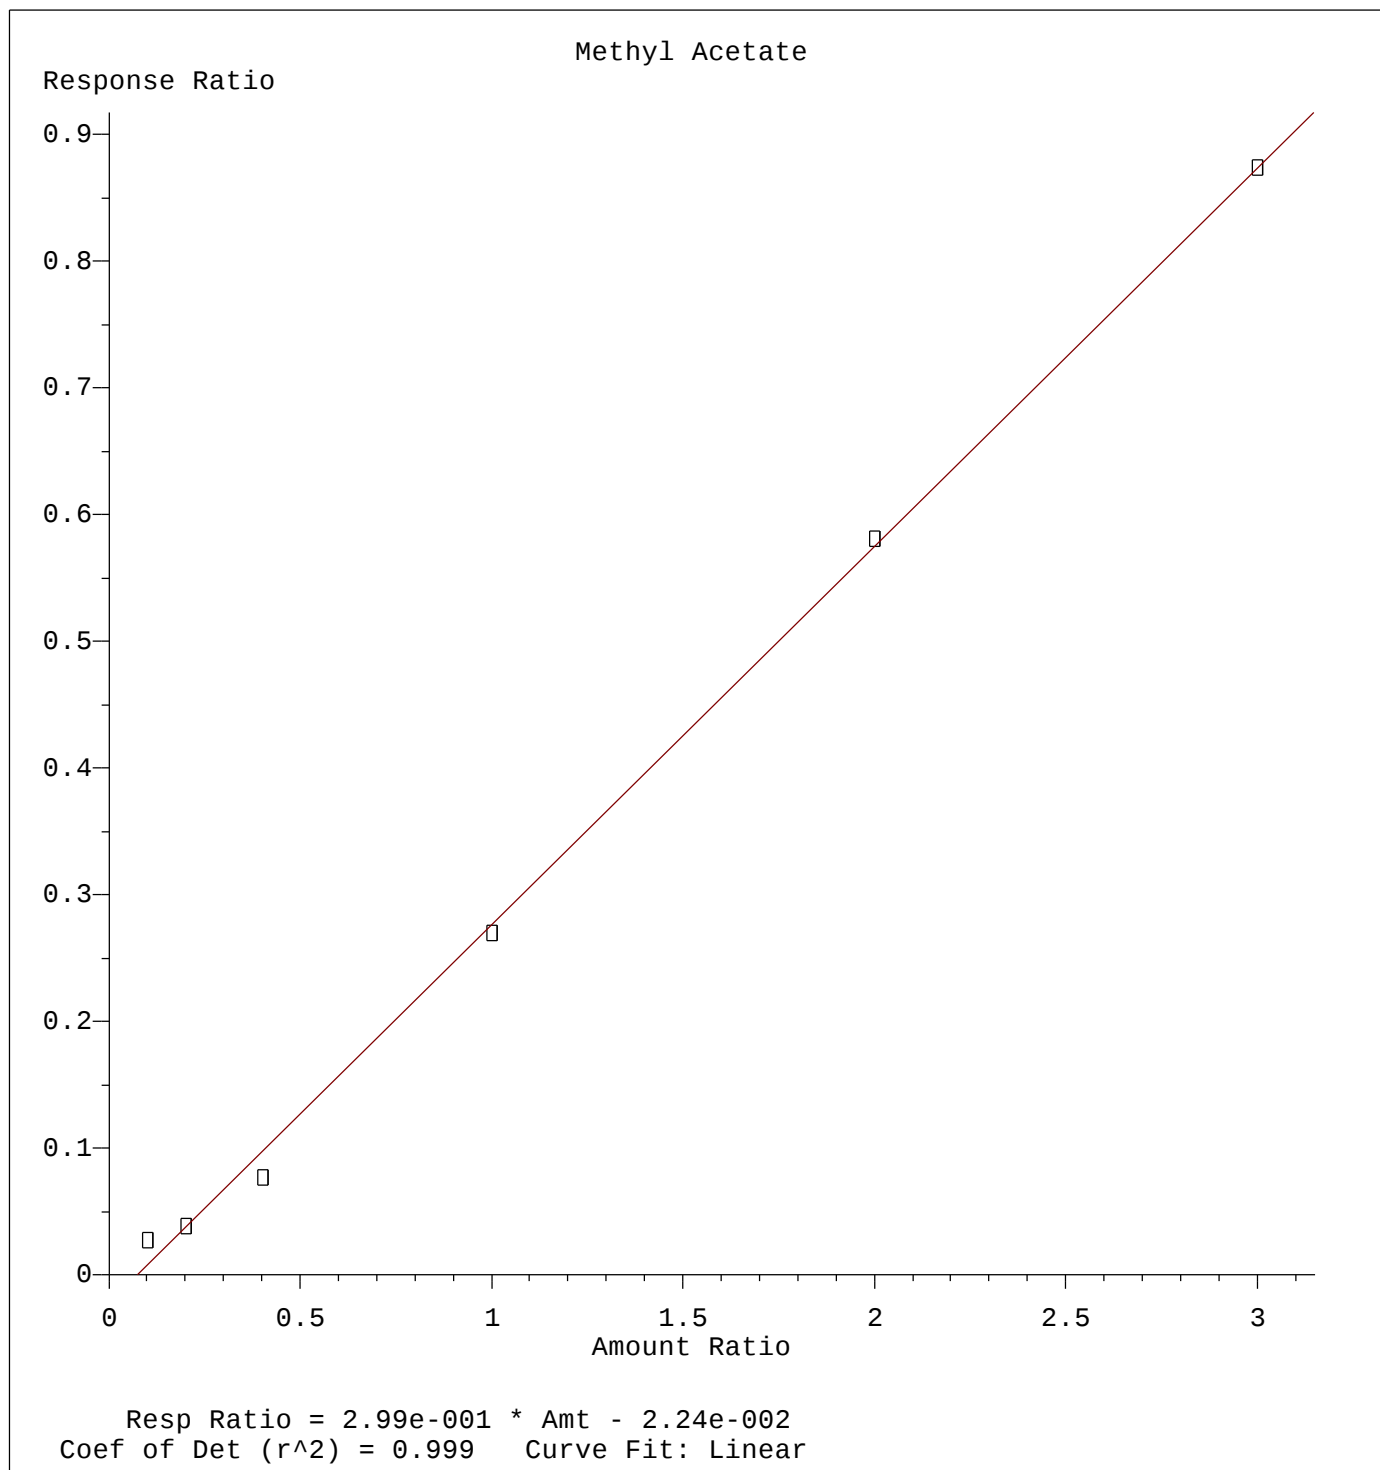

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y010220S.M
Calibration Table Last Updated: Thu Jan 02 13:16:38 2020

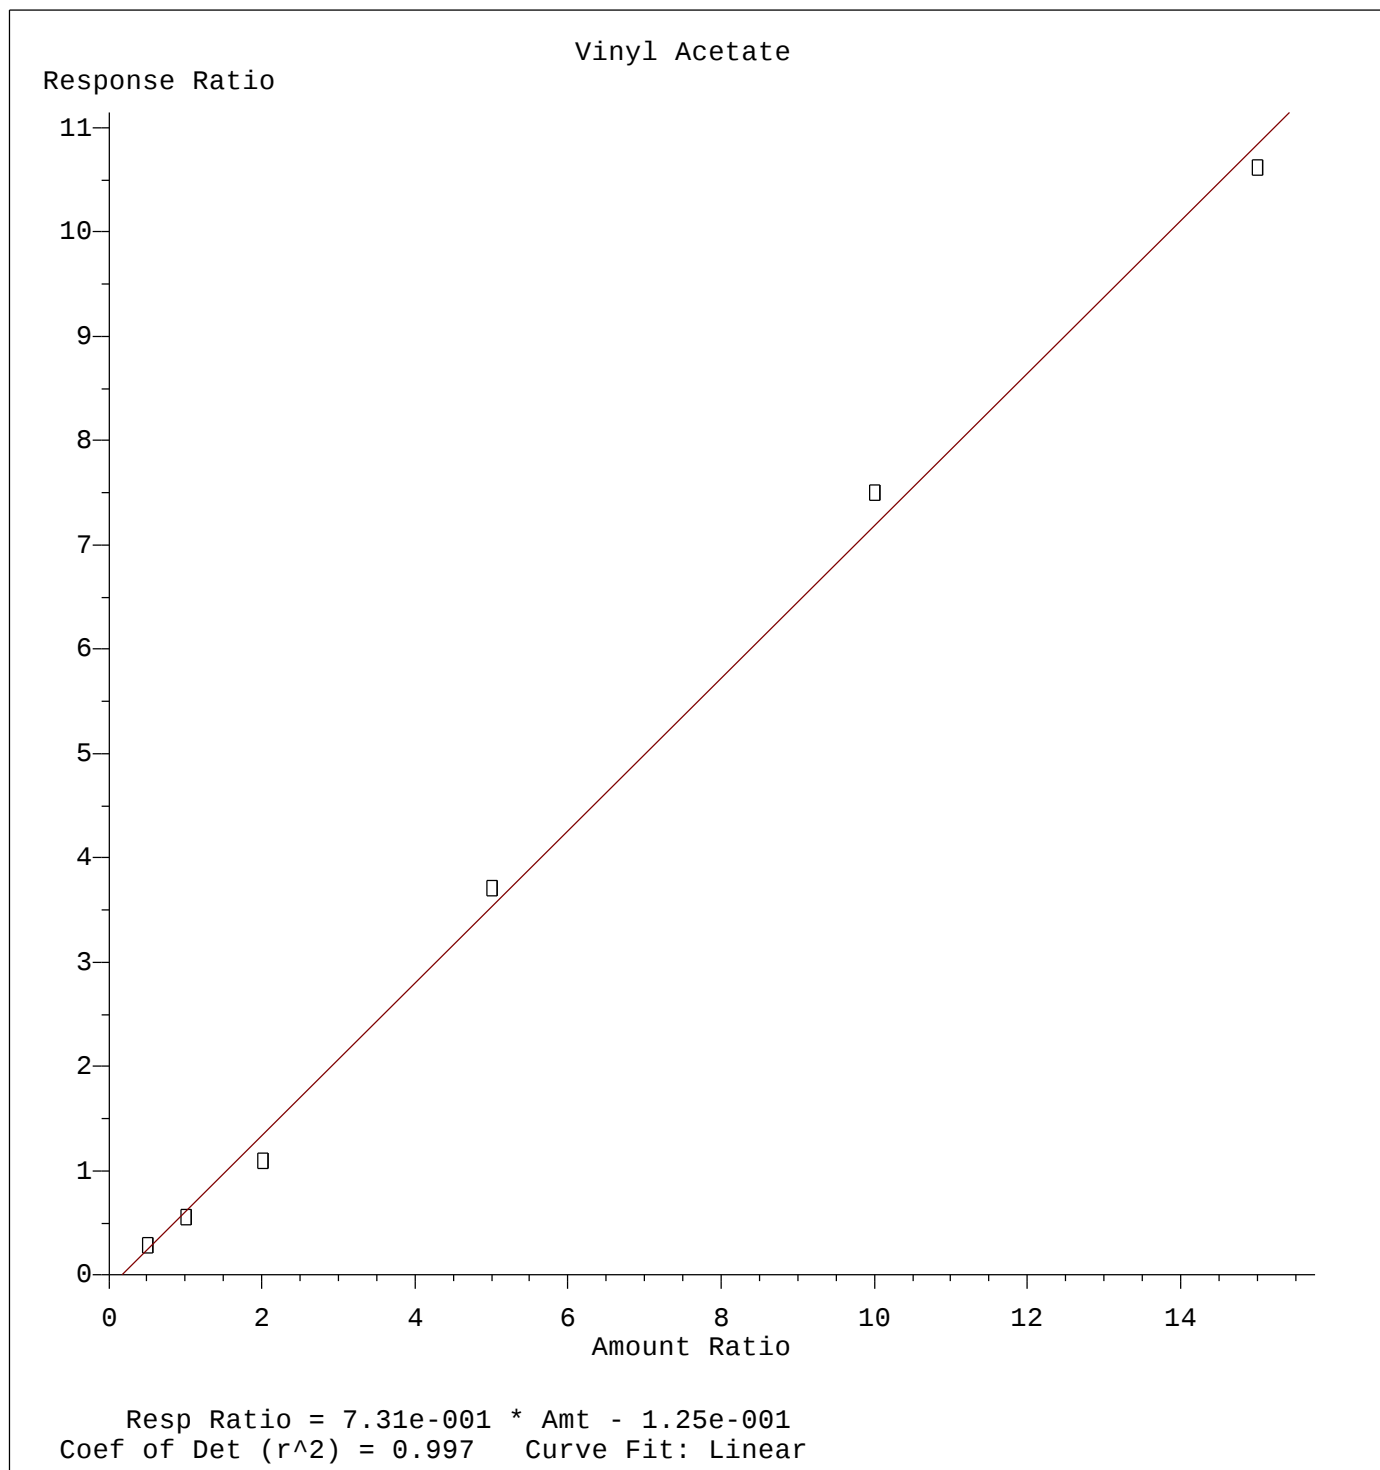


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y010220S.M
Calibration Table Last Updated: Thu Jan 02 13:16:38 2020

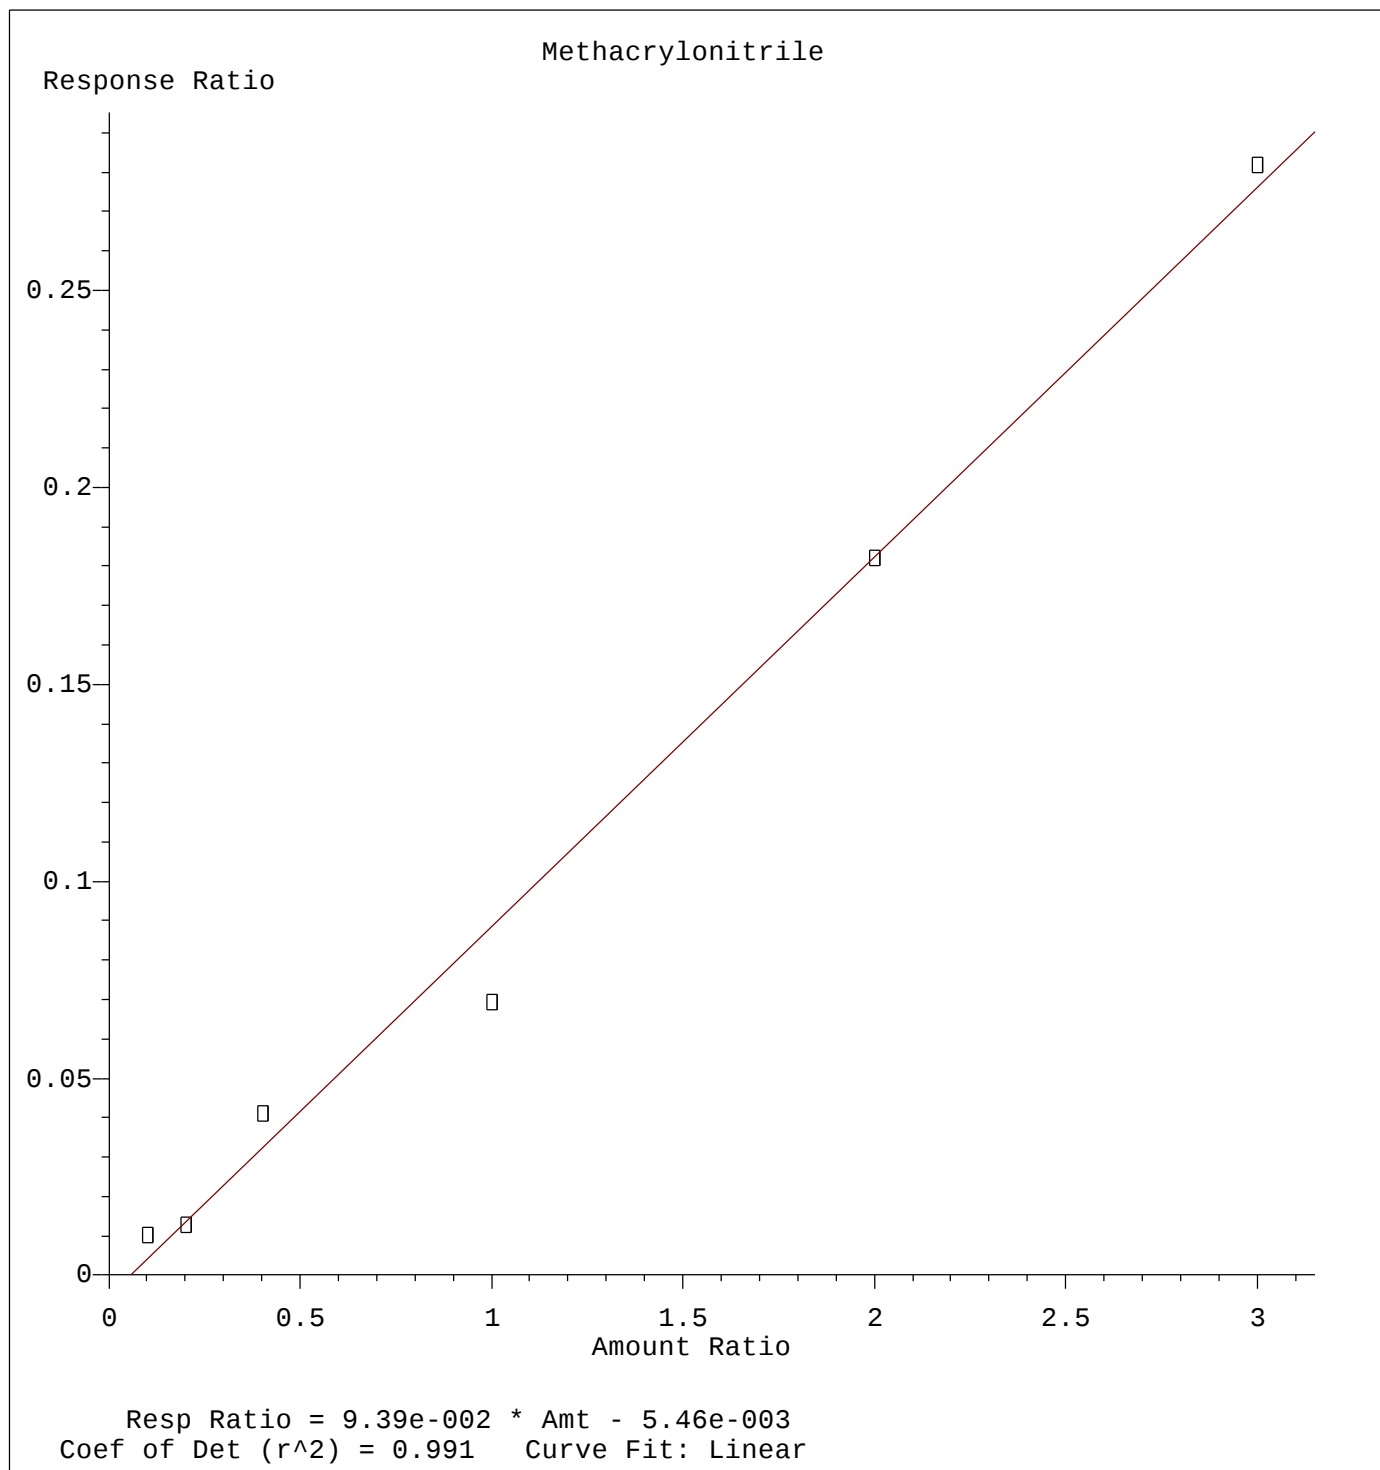

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y010220S.M
Calibration Table Last Updated: Thu Jan 02 13:16:38 2020


Allyl chloride

Response Ratio

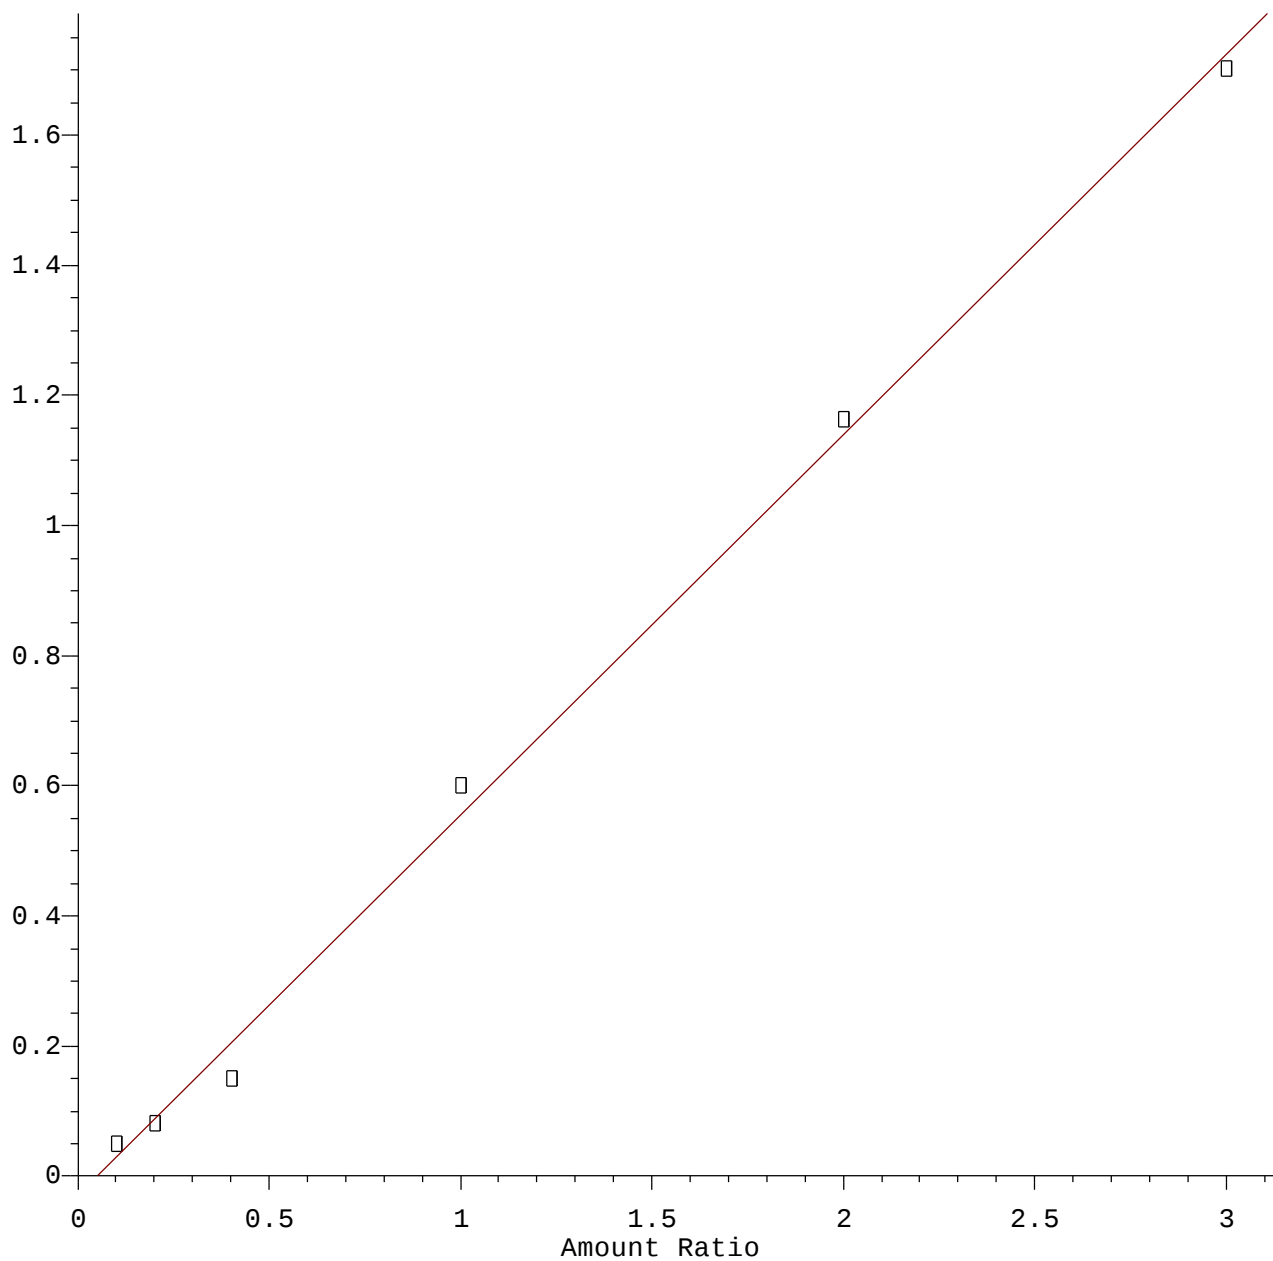


Resp Ratio = $5.84 \times 10^{-1} \times \text{Amt} - 2.84 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y010220S.M
Calibration Table Last Updated: Thu Jan 02 13:16:38 2020

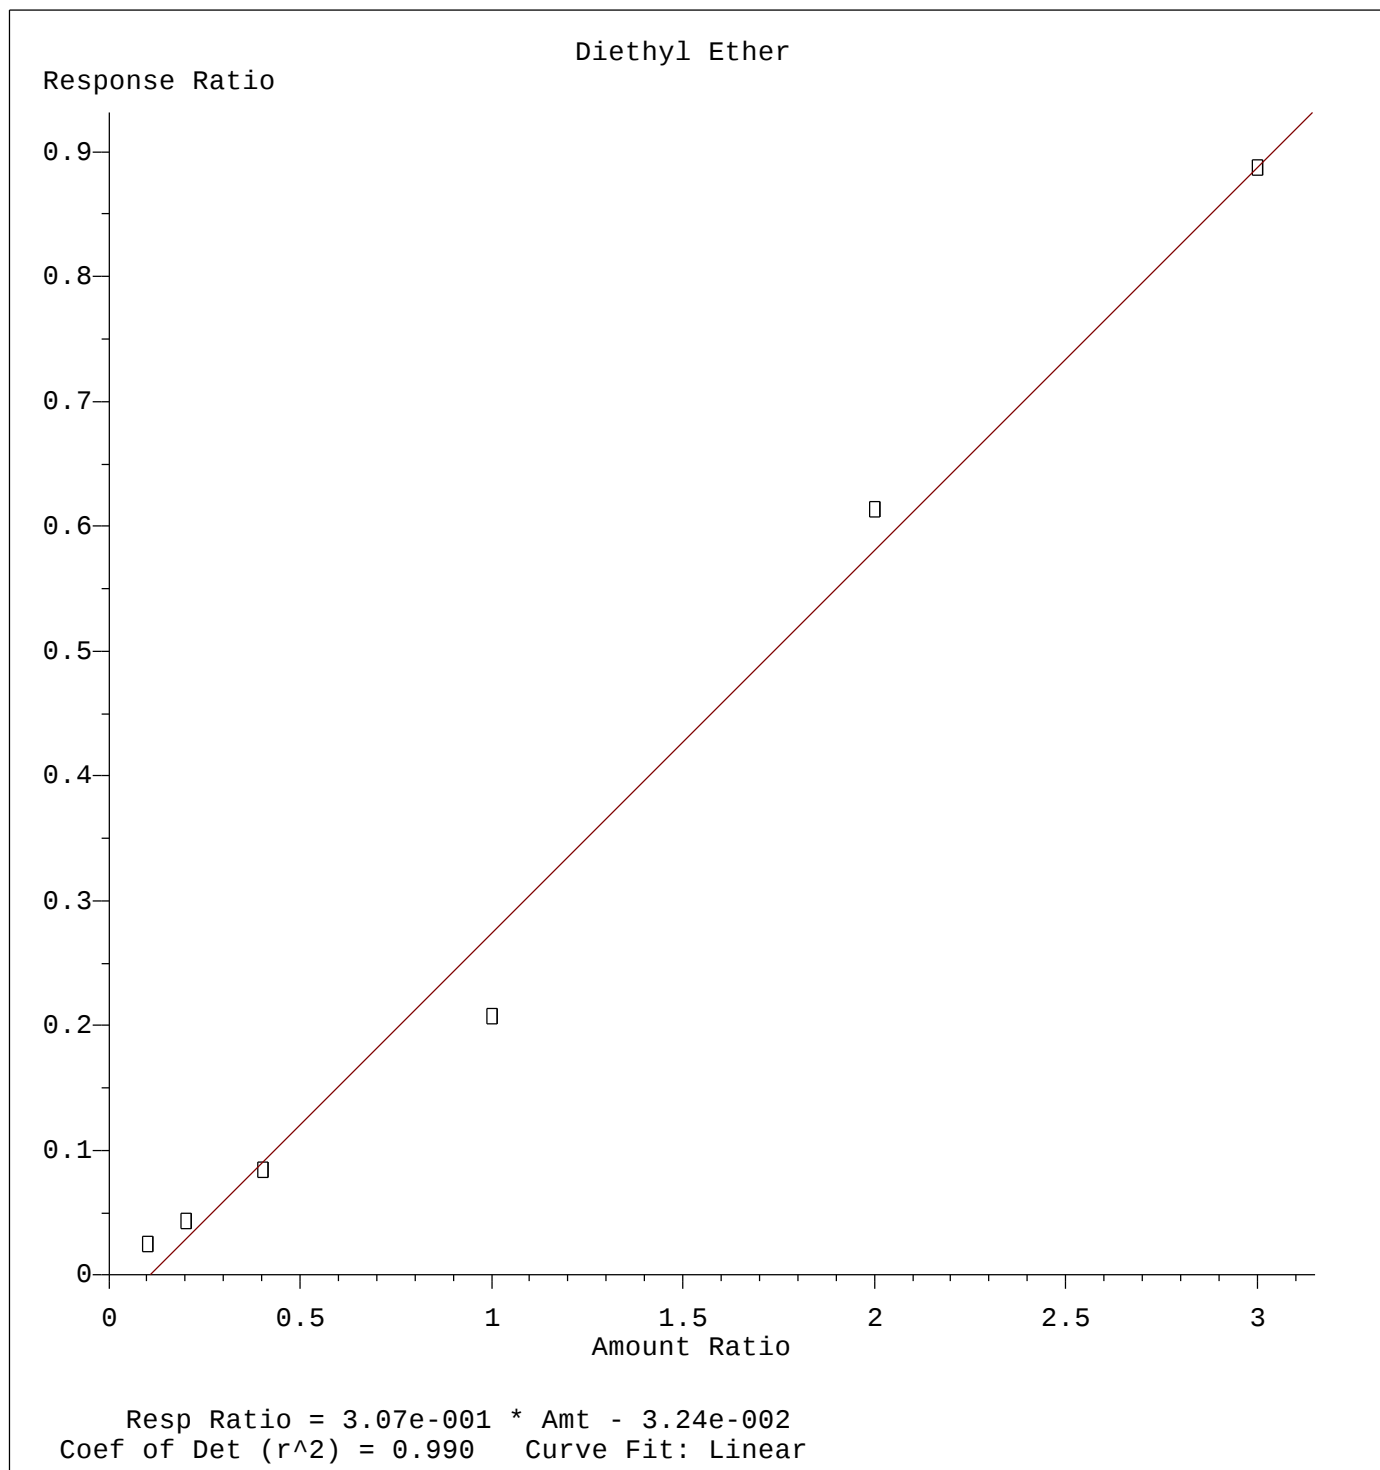

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y010220S.M
Calibration Table Last Updated: Thu Jan 02 13:13:34 2020

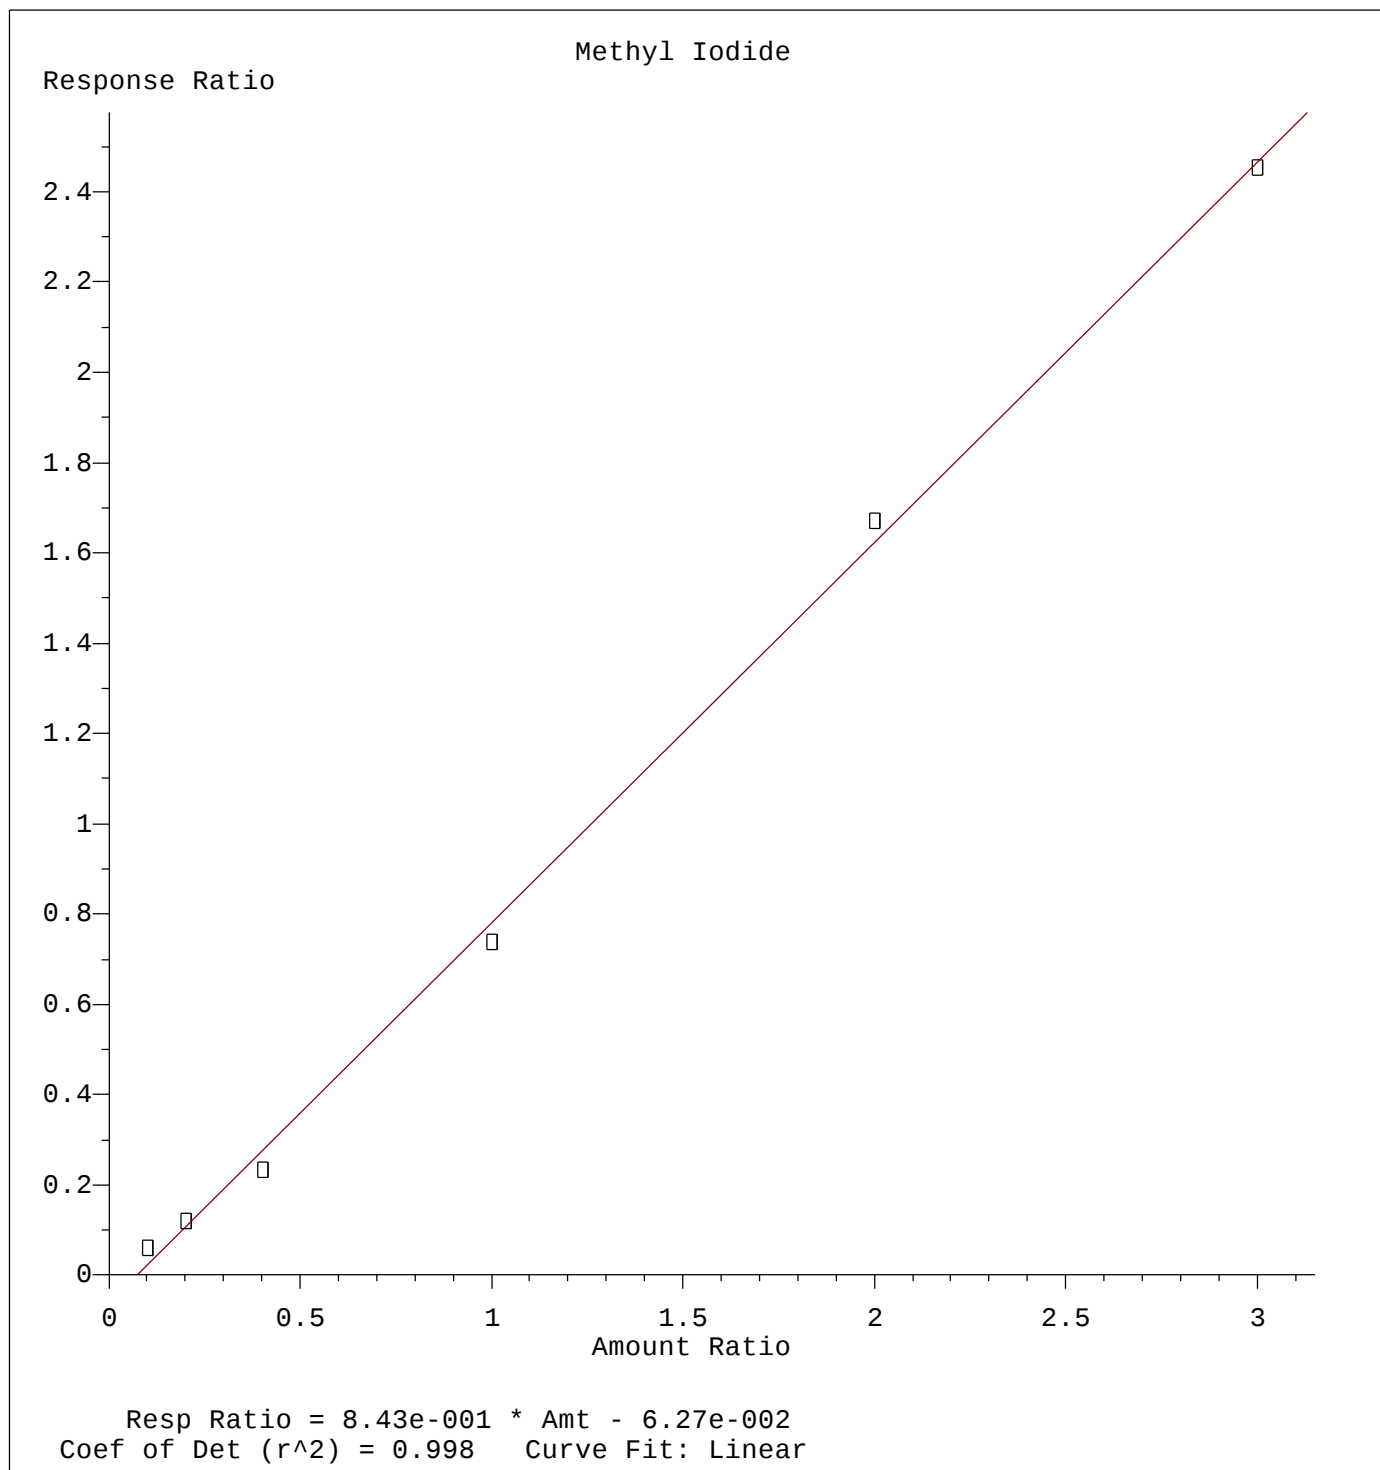

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y010220S.M
Calibration Table Last Updated: Thu Jan 02 13:14:34 2020

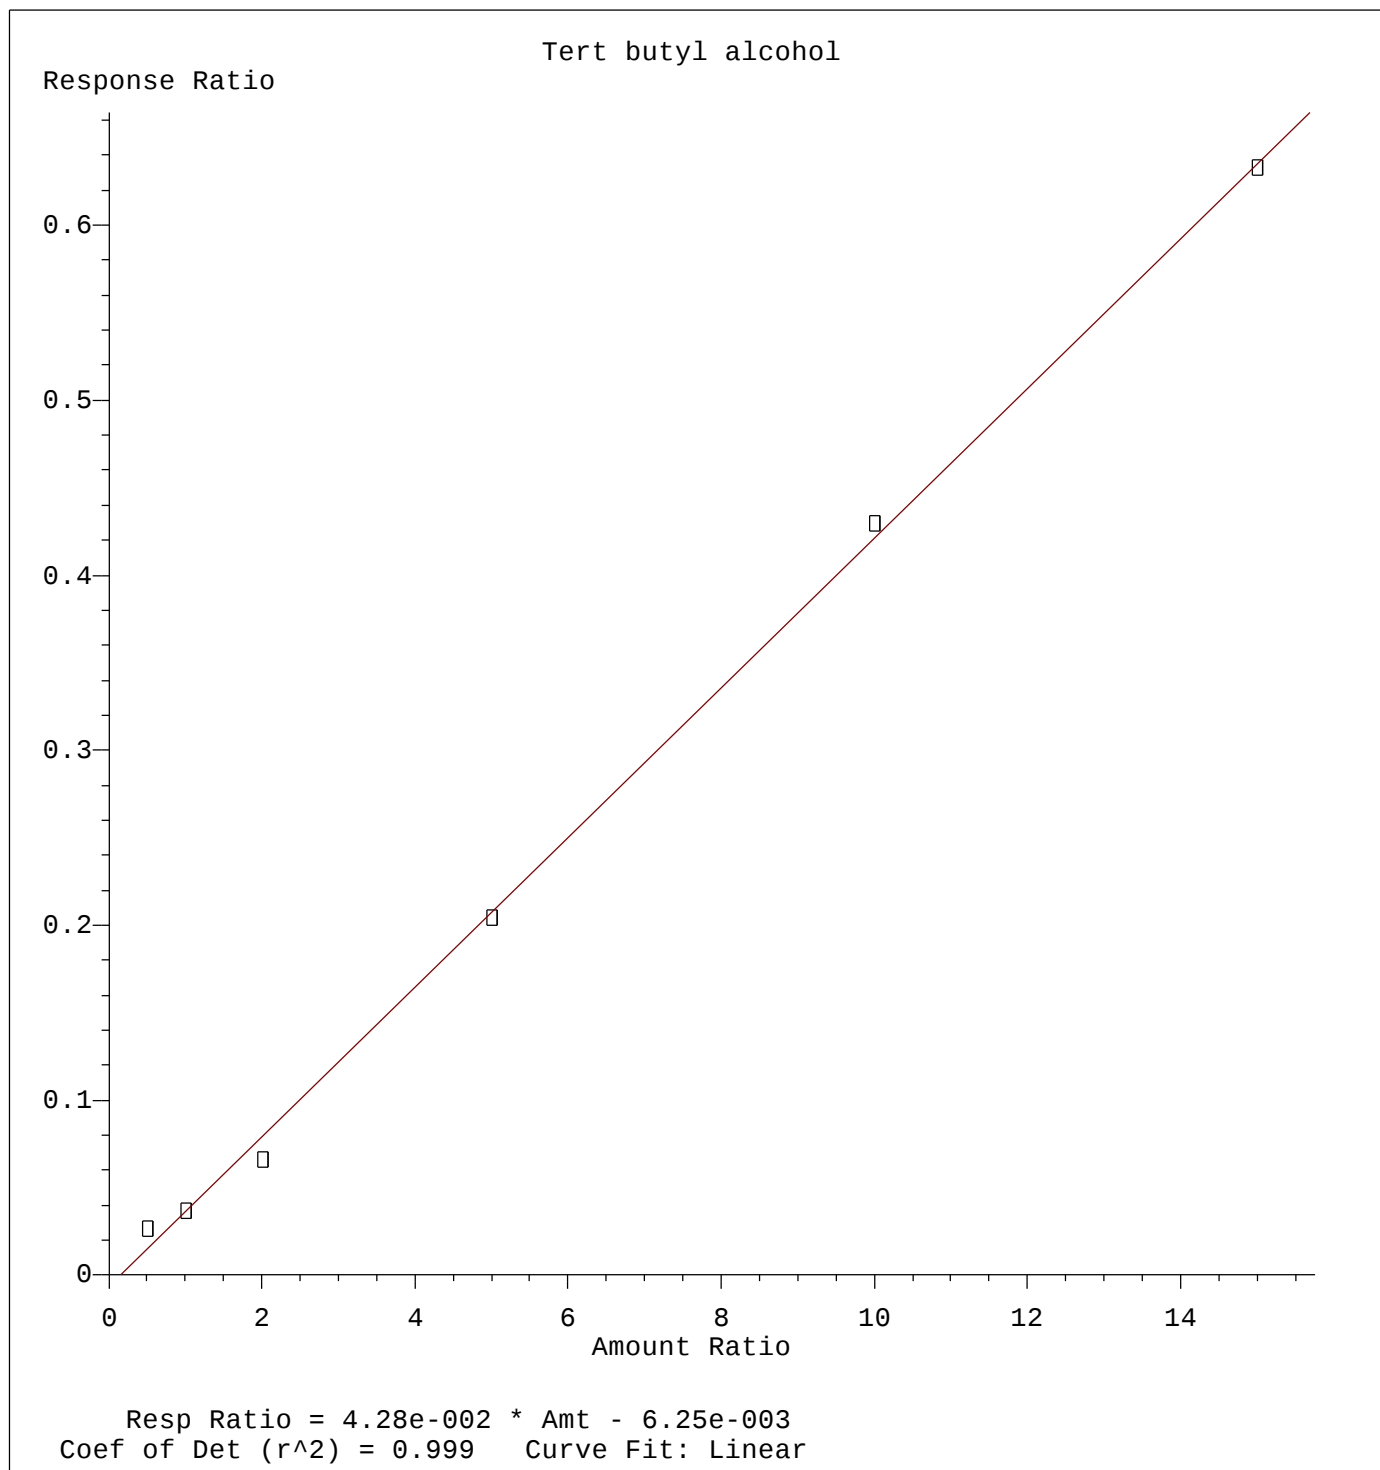

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y010220S.M
Calibration Table Last Updated: Thu Jan 02 13:14:34 2020