


Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY010220\
 Data File : VY001127.D
 Acq On : 02 Jan 2020 09:46
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y010220S.M
 Title : SW846 8260
 Last Update : Thu Jan 02 13:16:38 2020

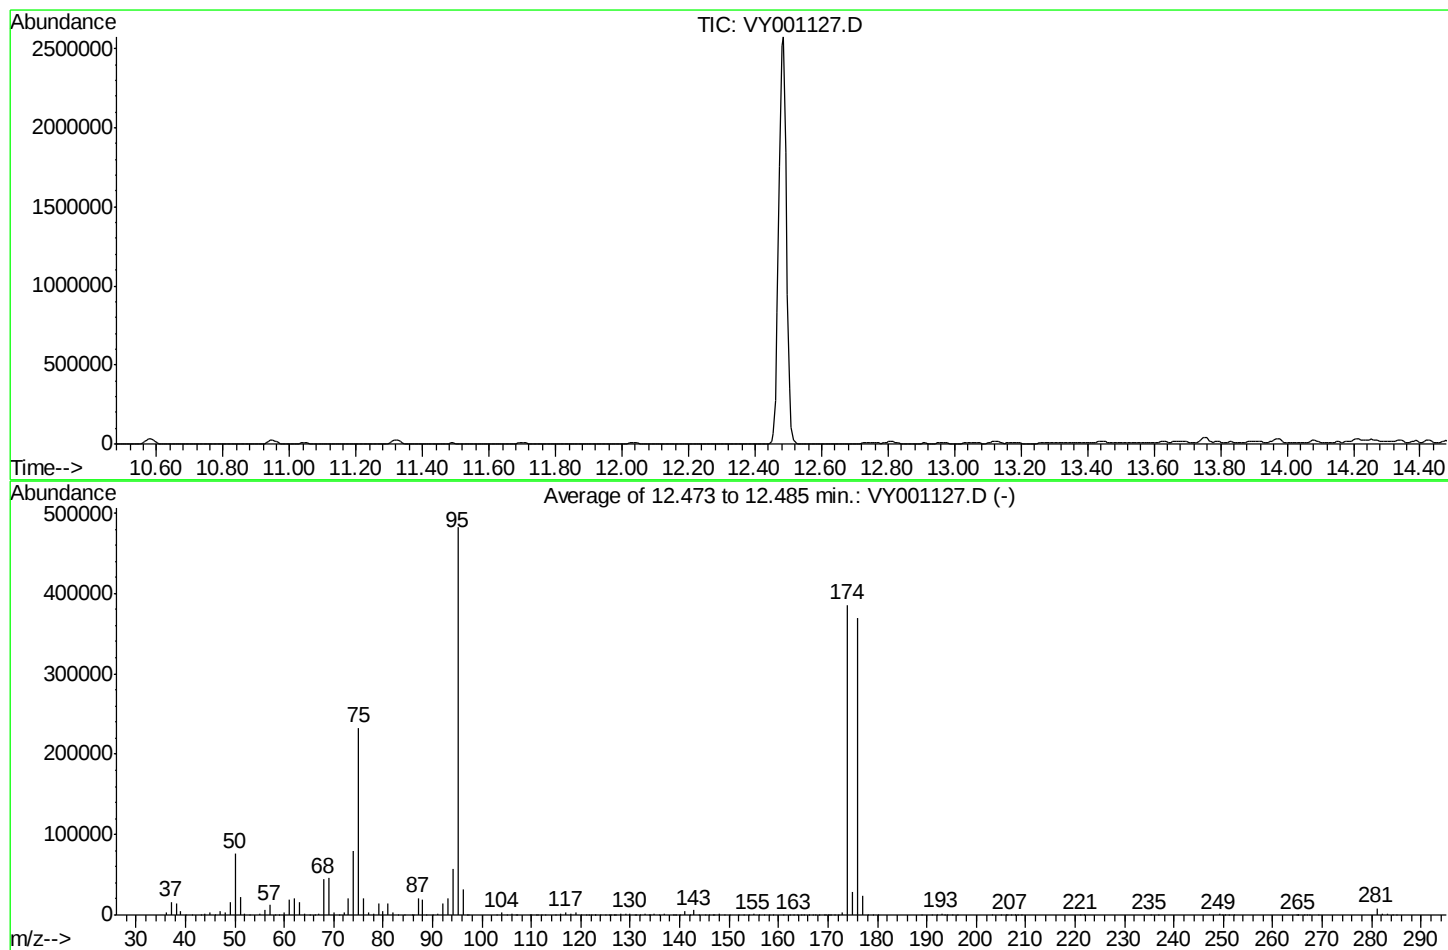

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1752

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	75757	PASS
75	95	30	60	48.2	232533	PASS
95	95	100	100	100.0	482154	PASS
96	95	5	9	6.7	32261	PASS
173	174	0.00	2	0.7	2850	PASS
174	95	50	100	80.0	385770	PASS
175	174	5	9	7.4	28360	PASS
176	174	95	101	95.6	368874	PASS
177	176	5	9	6.4	23648	PASS