
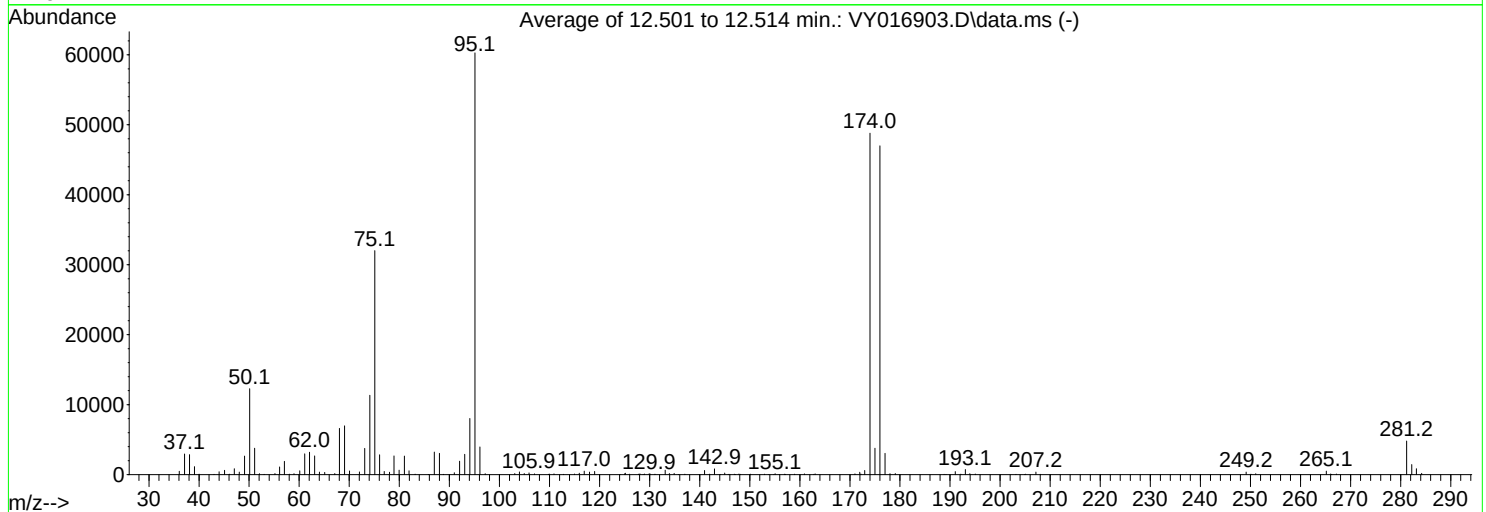


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY010324\
Data File : VY016903.D
Acq On : 03 Jan 2024 08:47
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y010224S.M
Title : SW846 8260
Last Update : Tue Jan 02 14:25:32 2024

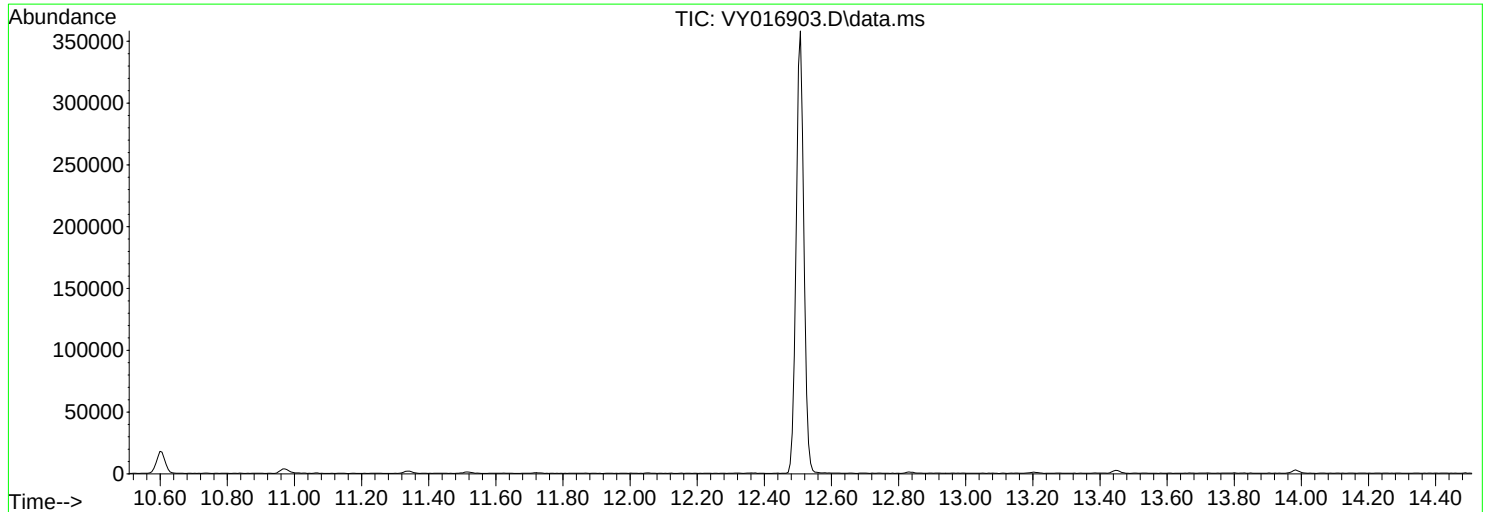

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.4	12285	PASS
75	95	30	60	53.1	32019	PASS
95	95	100	100	100.0	60280	PASS
96	95	5	9	6.6	3966	PASS
173	174	0.00	2	1.2	602	PASS
174	95	50	100	81.0	48808	PASS
175	174	5	9	7.7	3781	PASS
176	174	95	101	96.3	47000	PASS
177	176	5	9	6.5	3036	PASS