
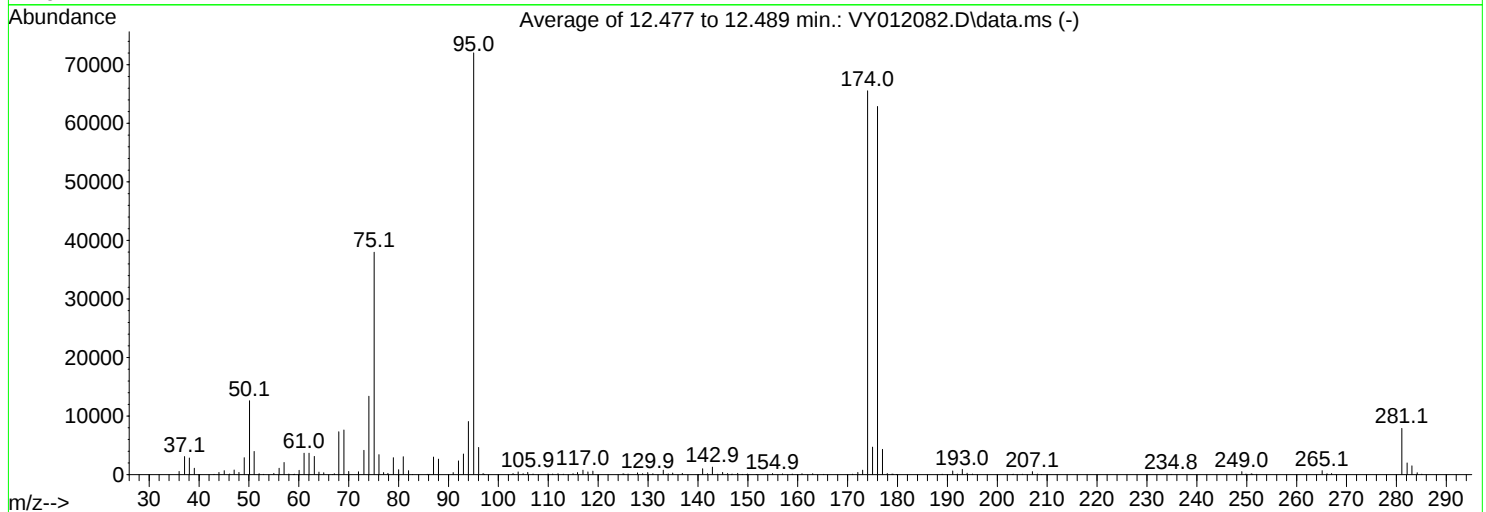


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY010623\
Data File : VY012082.D
Acq On : 06 Jan 2023 09:04
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y010623S.M
Title : SW846 8260
Last Update : Sat Jan 07 01:46:48 2023

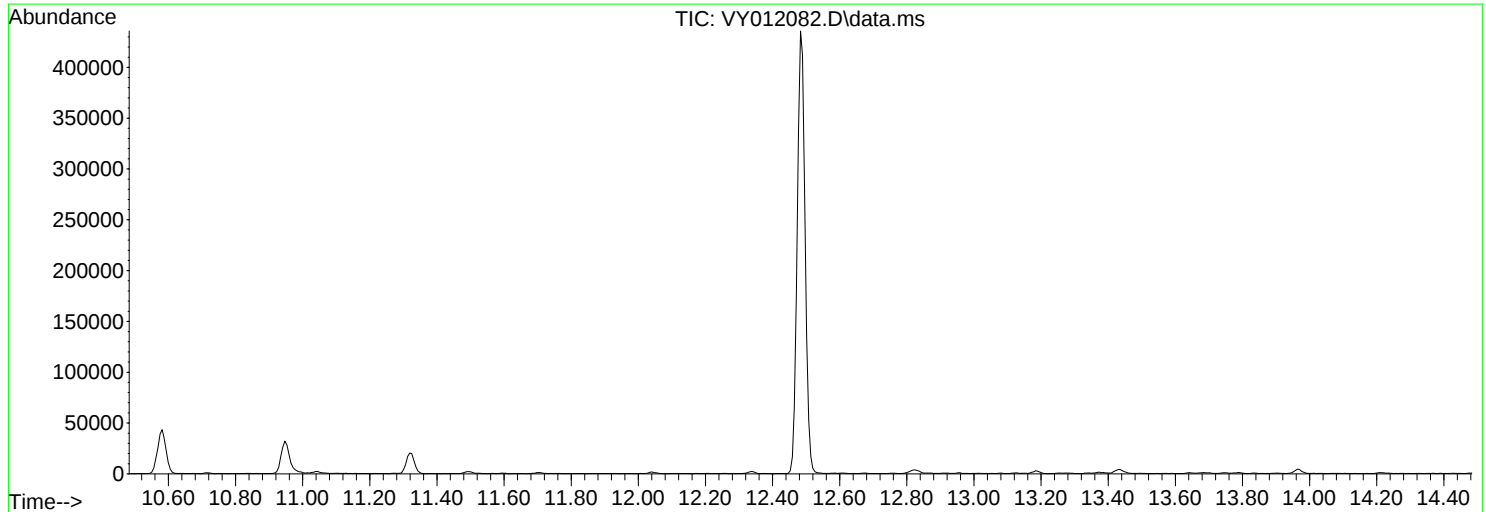

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.5	12632	PASS
75	95	30	60	52.7	37997	PASS
95	95	100	100	100.0	72040	PASS
96	95	5	9	6.4	4642	PASS
173	174	0.00	2	1.2	773	PASS
174	95	50	100	91.0	65544	PASS
175	174	5	9	7.2	4711	PASS
176	174	95	101	95.9	62885	PASS
177	176	5	9	6.9	4317	PASS