


Bromomethane

Response Ratio

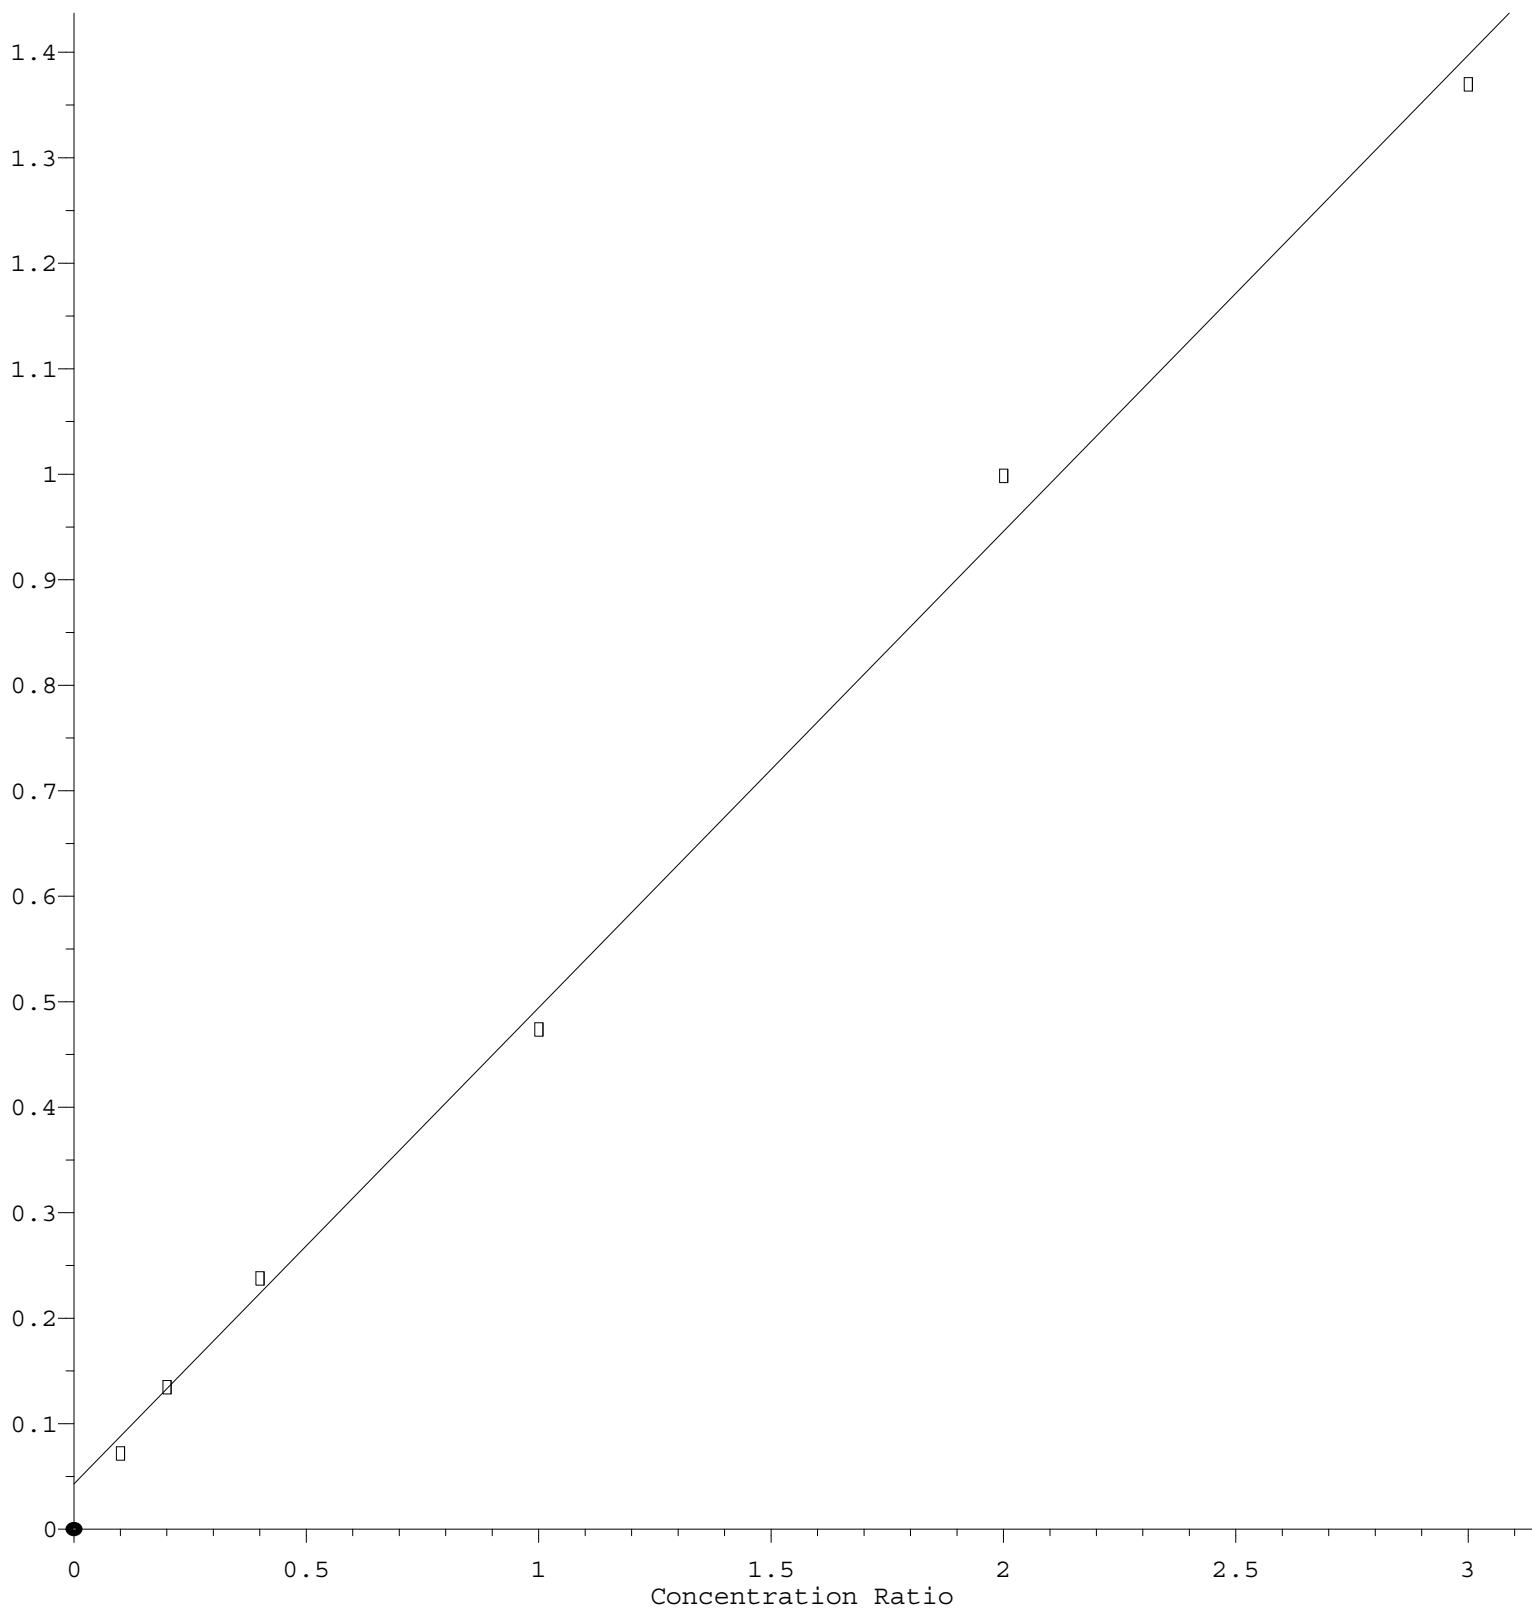

$$\text{Response} = 4.517\text{e-}001 * \text{Amt} + 4.316\text{e-}002$$


Coef of Det (r^2) = 0.996775 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y010721S.M

Calibration Table Last Updated: Fri Jan 08 04:34:36 2021

Methyl Iodide

Response Ratio

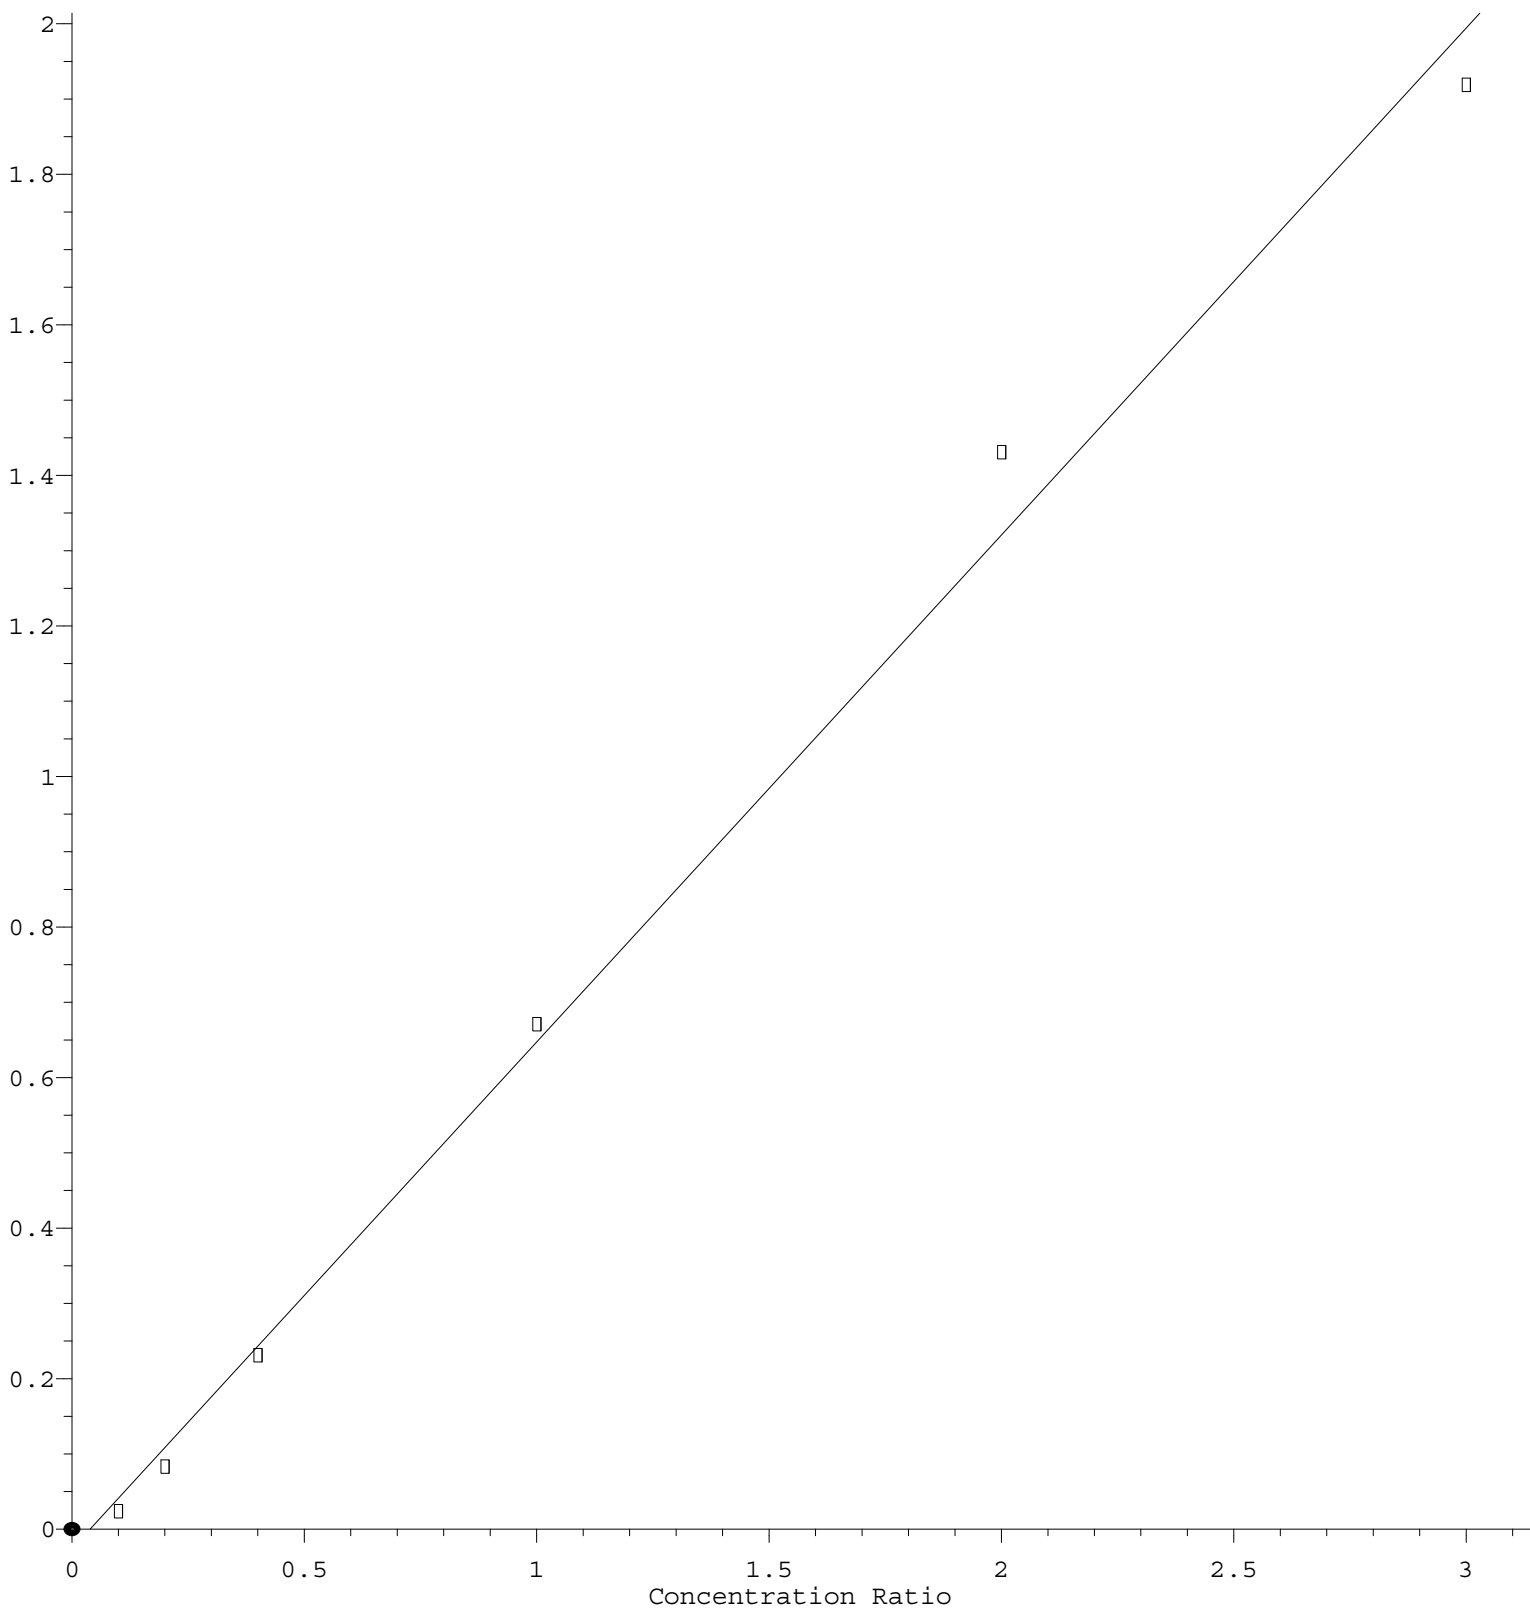

$$\text{Response} = 6.738\text{e-}001 * \text{Amt} - 2.599\text{e-}002$$


Coef of Det (r^2) = 0.993677 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y010721S.M

Calibration Table Last Updated: Fri Jan 08 04:34:36 2021

Methylene Chloride

Response Ratio

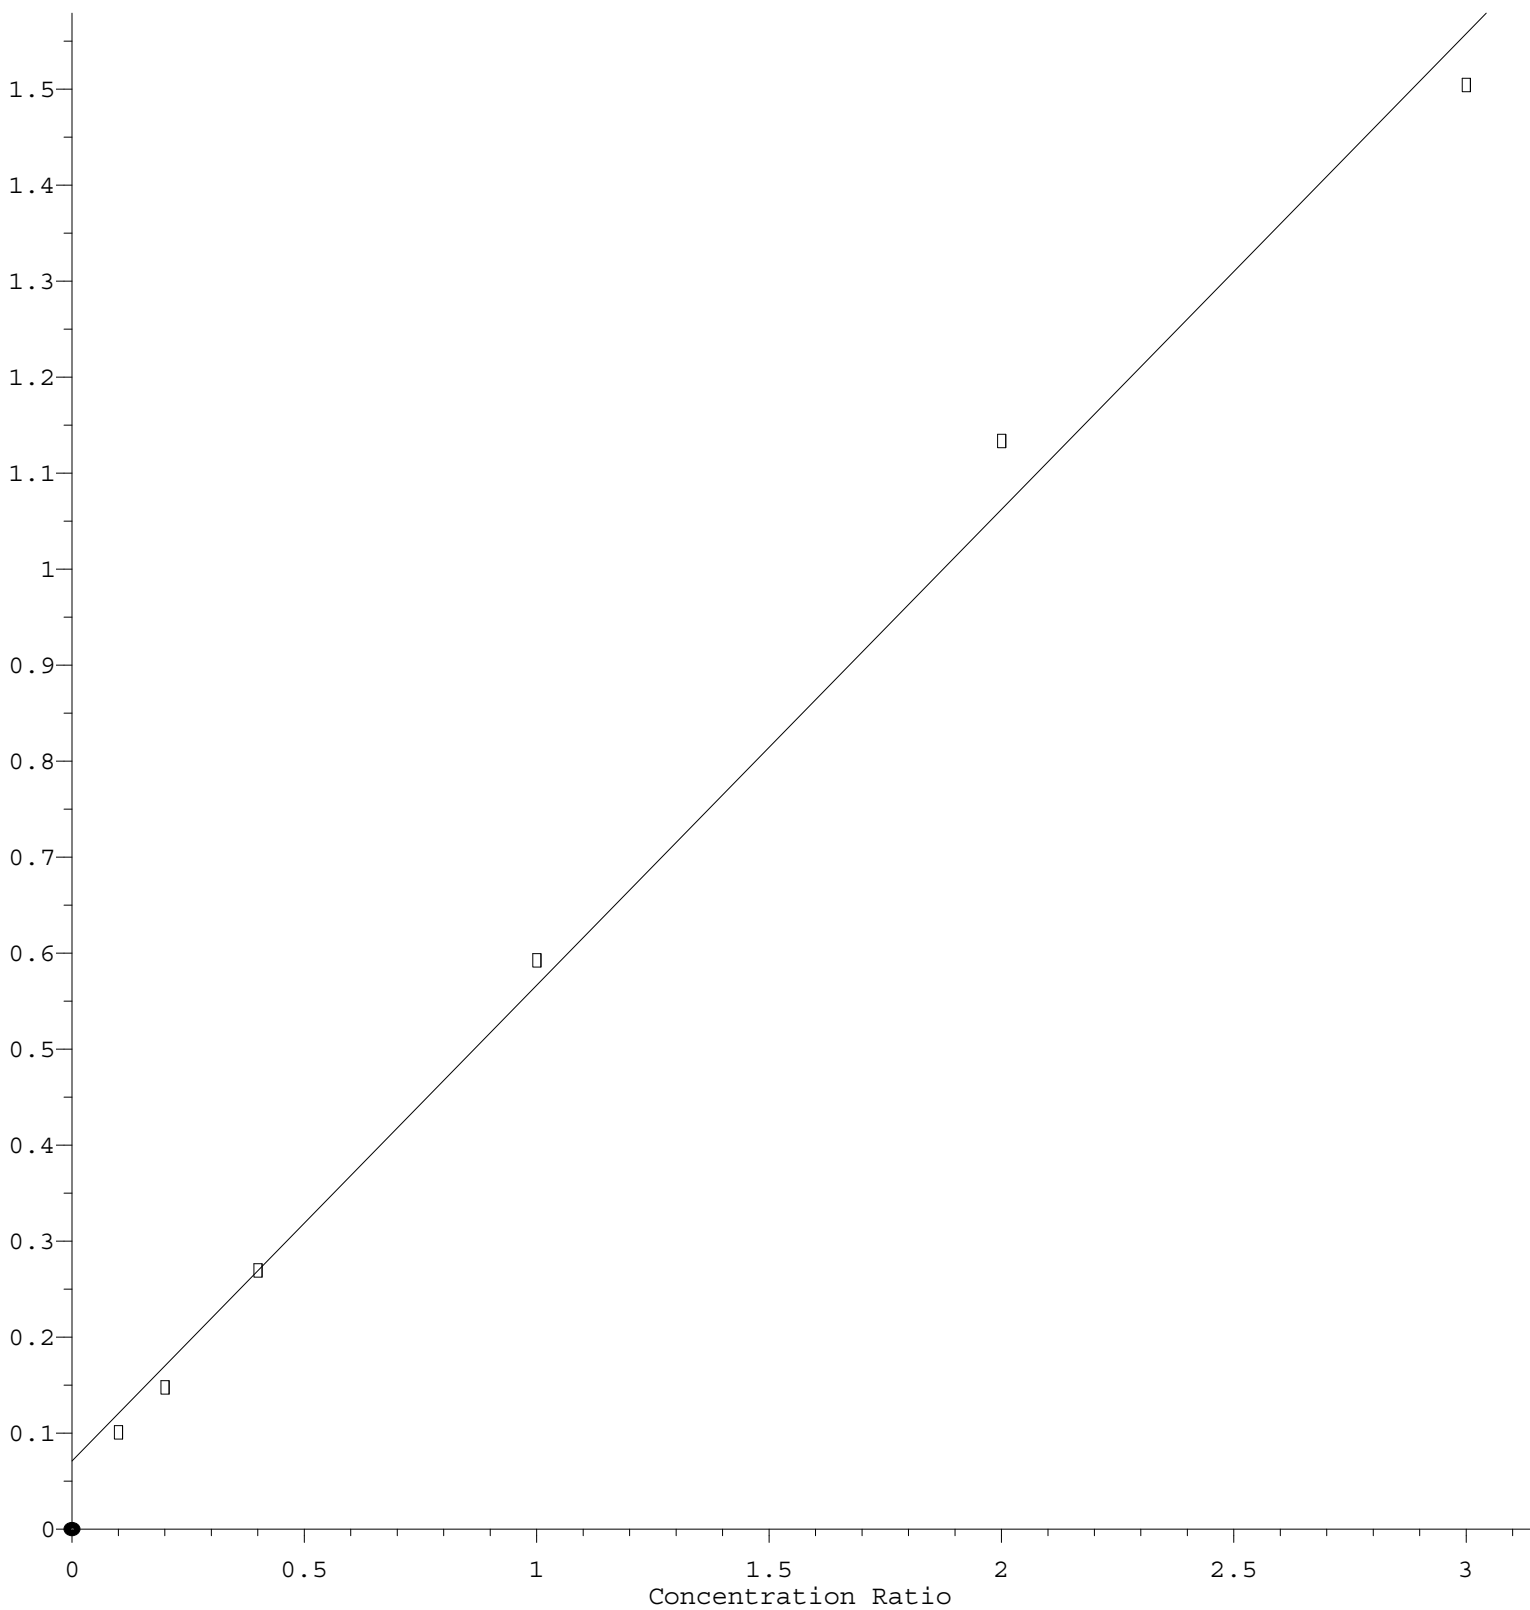

$$\text{Response} = 4.955\text{e-}001 * \text{Amt} + 7.133\text{e-}002$$

Coef of Det (r^2) = 0.994271 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y010721S.M

Calibration Table Last Updated: Fri Jan 08 04:34:36 2021