


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY010722\
 Data File : VY007049.D
 Acq On : 07 Jan 2022 10:52
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y010522S.M
 Title : SW846 8260
 Last Update : Thu Jan 06 04:51:57 2022

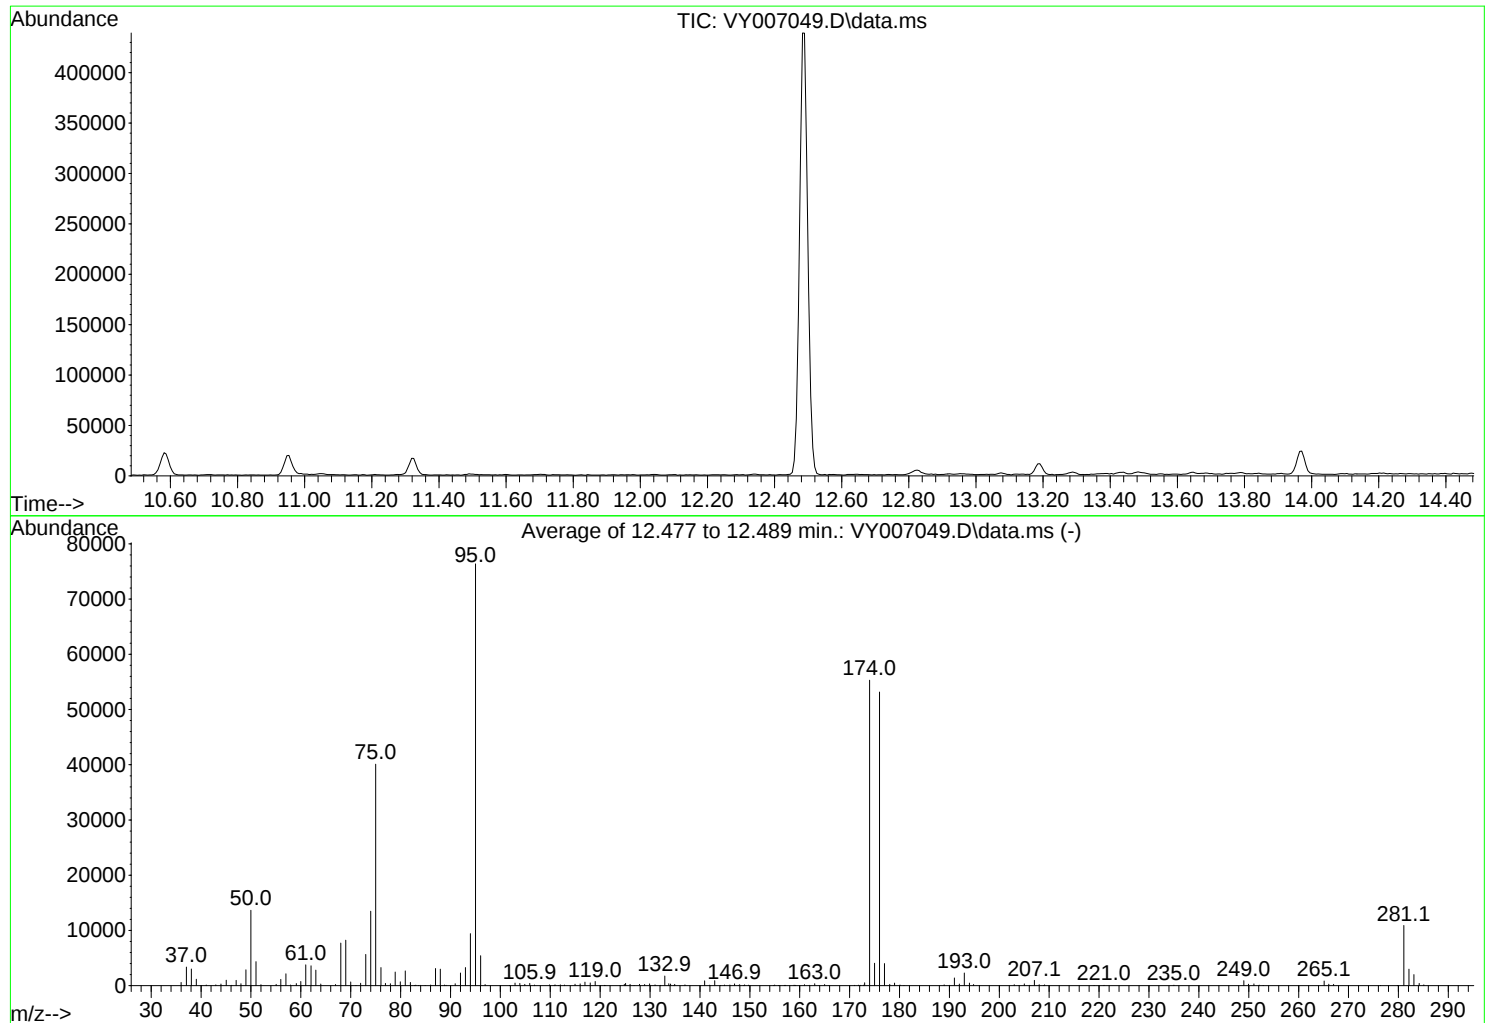

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1741

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	13649	PASS
75	95	30	60	52.5	40088	PASS
95	95	100	100	100.0	76381	PASS
96	95	5	9	7.1	5419	PASS
173	174	0.00	2	0.9	523	PASS
174	95	50	100	72.4	55320	PASS
175	174	5	9	7.3	4058	PASS
176	174	95	101	96.1	53181	PASS
177	176	5	9	7.5	3990	PASS