
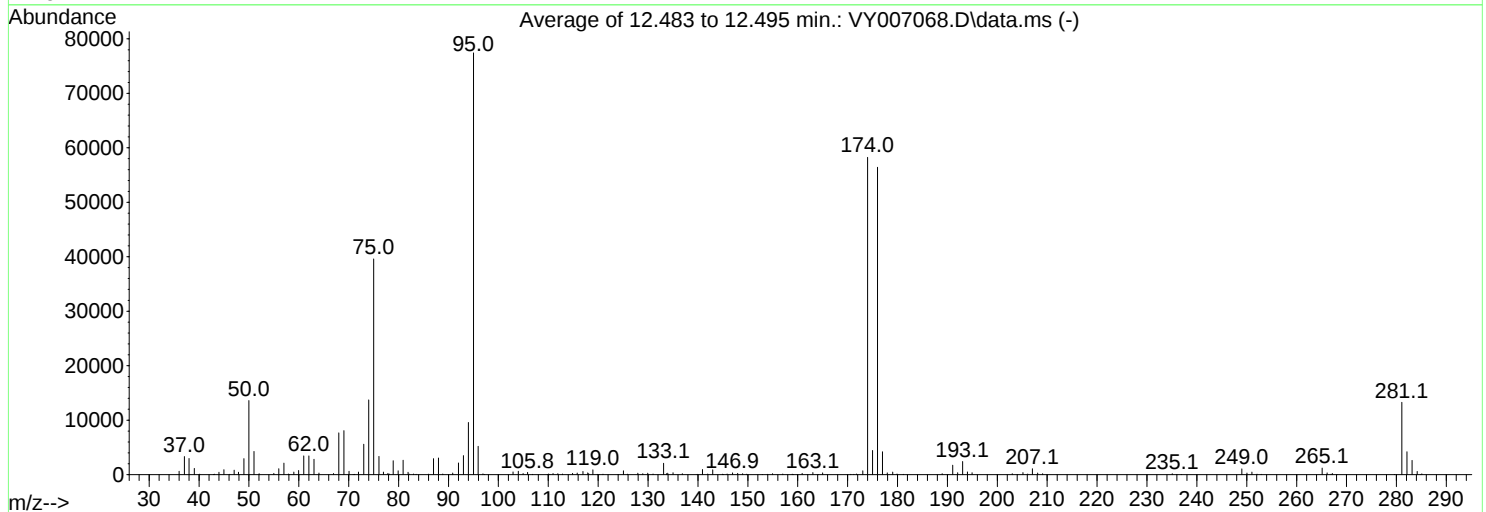


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY010822\
 Data File : VY007068.D
 Acq On : 08 Jan 2022 10:20
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y010822S.M
 Title : SW846 8260
 Last Update : Mon Jan 10 03:29:44 2022

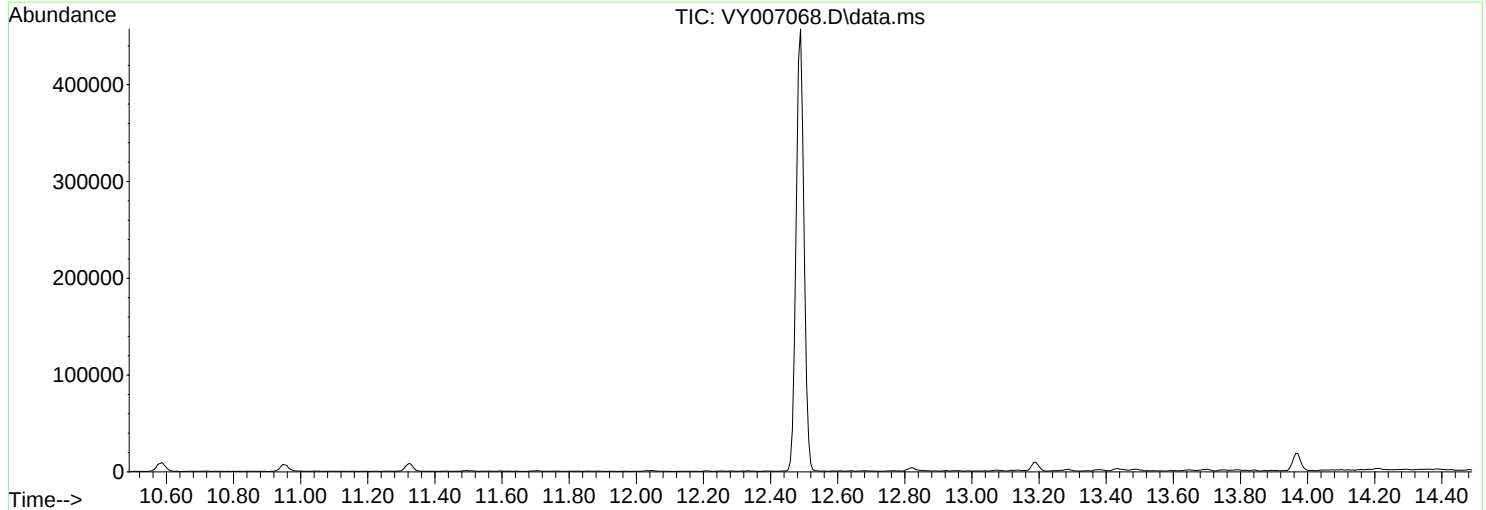

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	13595	PASS
75	95	30	60	51.2	39611	PASS
95	95	100	100	100.0	77435	PASS
96	95	5	9	6.7	5194	PASS
173	174	0.00	2	1.2	712	PASS
174	95	50	100	75.2	58248	PASS
175	174	5	9	7.6	4450	PASS
176	174	95	101	96.9	56435	PASS
177	176	5	9	7.4	4197	PASS