


Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY011020\
 Data File : VY001144.D
 Acq On : 10 Jan 2020 12:27
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y011020S.M
 Title : SW846 8260
 Last Update : Fri Jan 10 16:01:58 2020

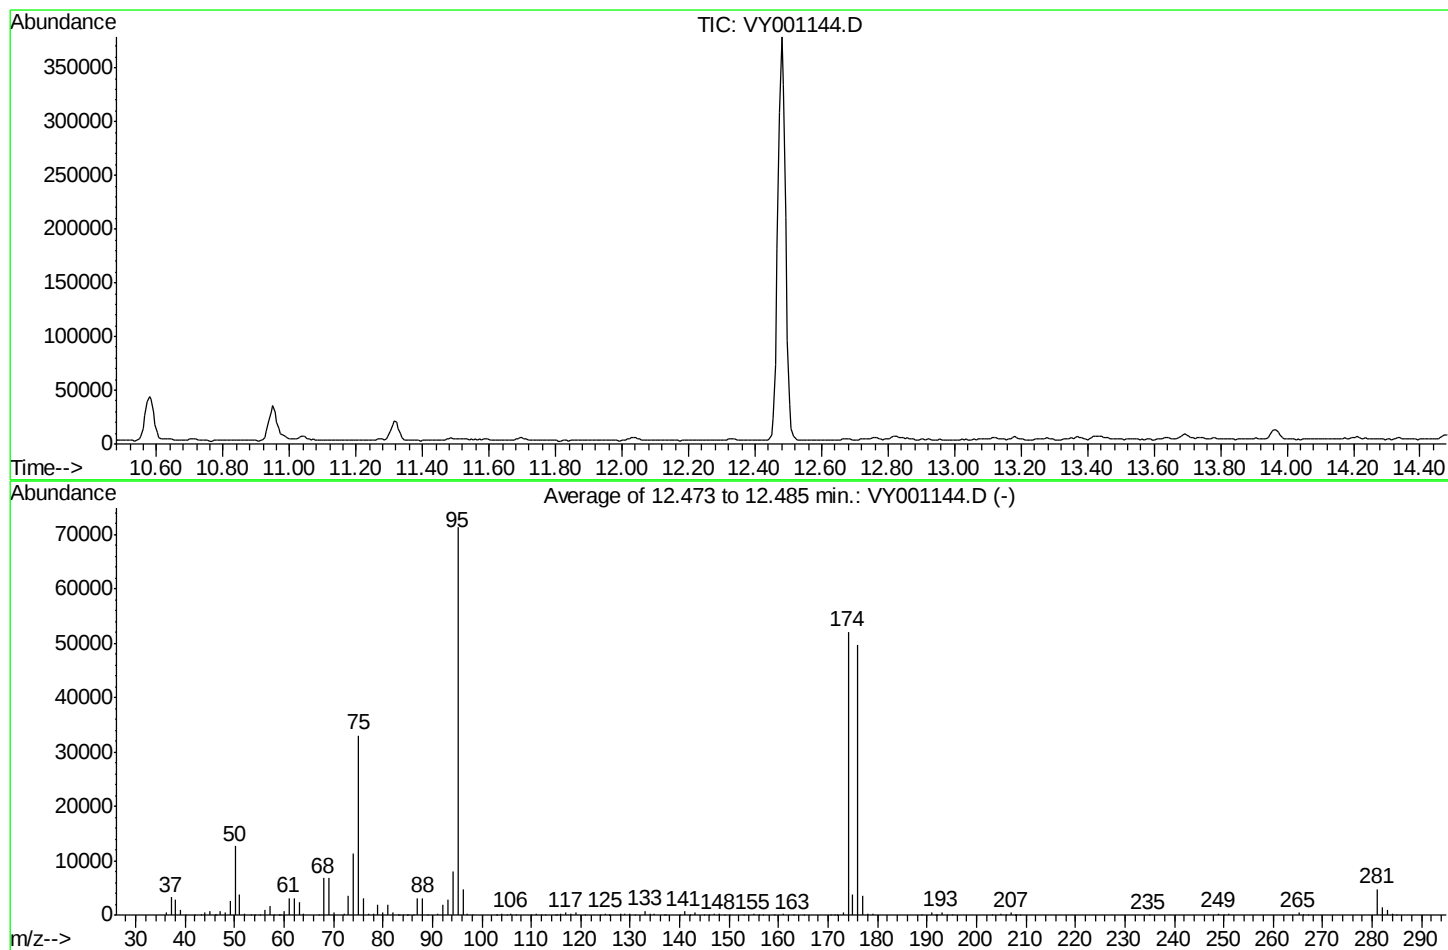

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1752

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	12662	PASS
75	95	30	60	46.3	33053	PASS
95	95	100	100	100.0	71341	PASS
96	95	5	9	6.7	4772	PASS
173	174	0.00	2	0.8	412	PASS
174	95	50	100	73.0	52112	PASS
175	174	5	9	7.3	3790	PASS
176	174	95	101	95.5	49770	PASS
177	176	5	9	7.1	3538	PASS