
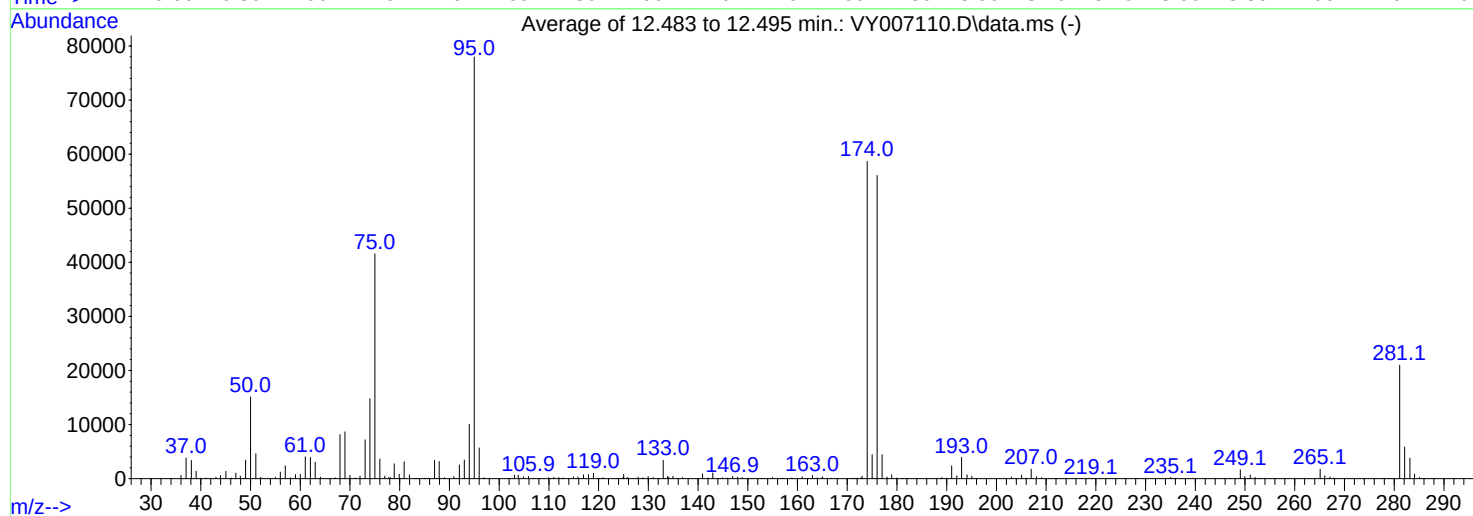


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY011122\
 Data File : VY007110.D
 Acq On : 11 Jan 2022 09:17
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y010822S.M
 Title : SW846 8260
 Last Update : Mon Jan 10 03:29:44 2022

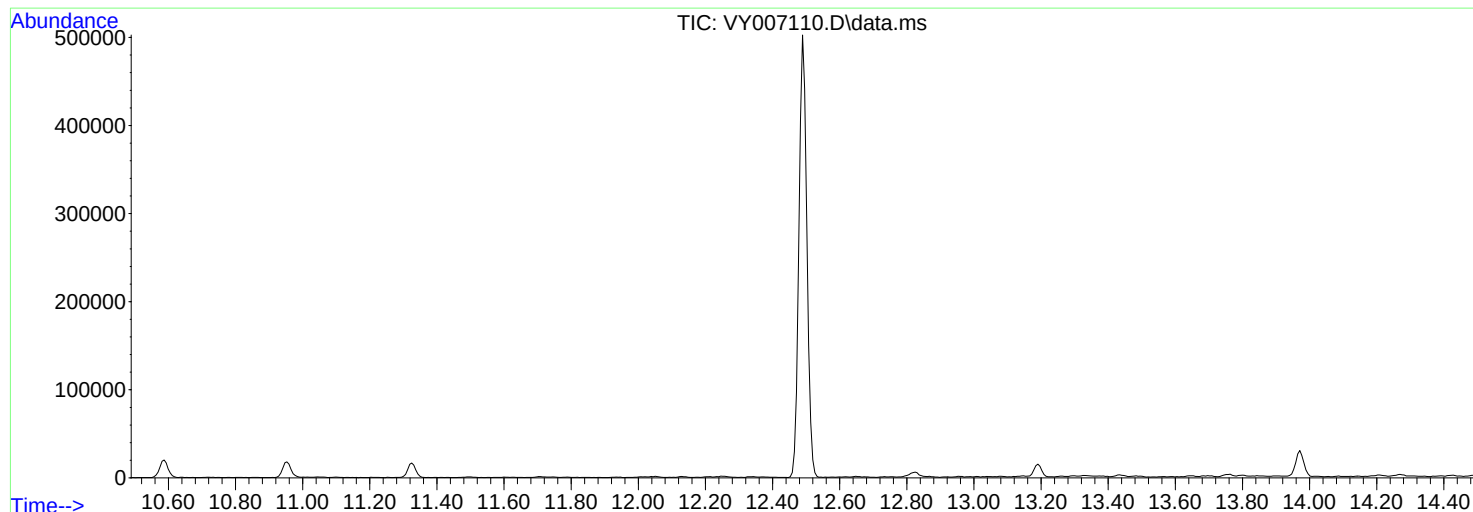

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1741

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	15088	PASS
75	95	30	60	53.3	41552	PASS
95	95	100	100	100.0	77987	PASS
96	95	5	9	7.3	5671	PASS
173	174	0.00	2	0.8	442	PASS
174	95	50	100	75.2	58677	PASS
175	174	5	9	7.5	4430	PASS
176	174	95	101	95.6	56075	PASS
177	176	5	9	7.9	4433	PASS