
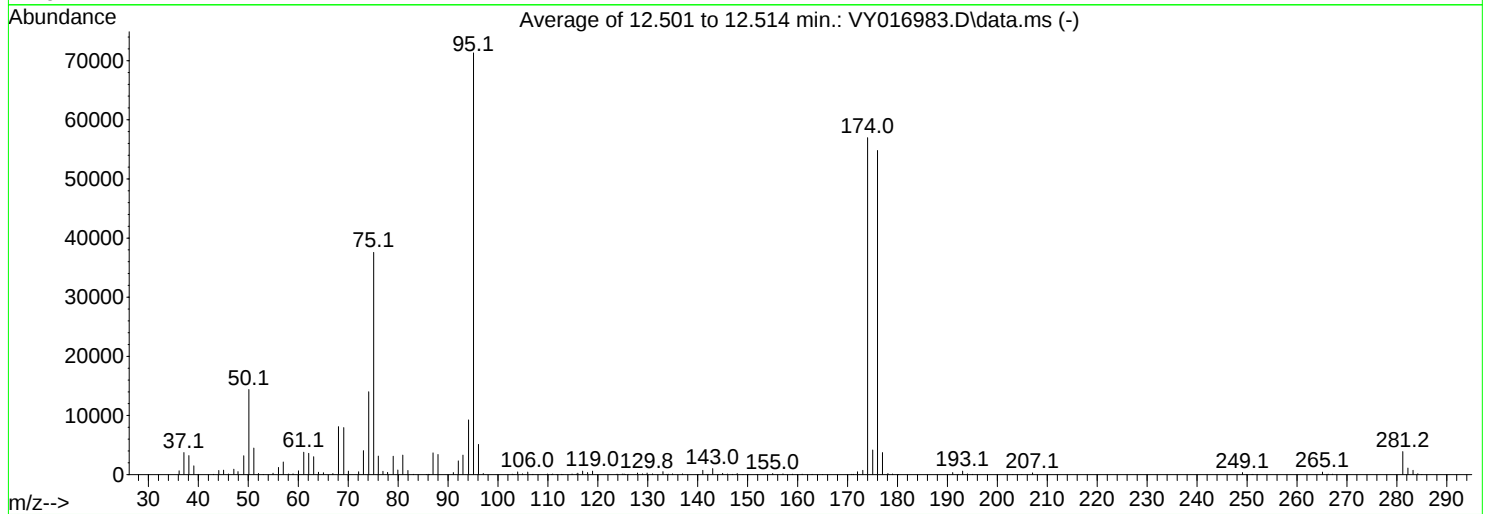


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY011224\
Data File : VY016983.D
Acq On : 12 Jan 2024 08:49
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y010224S.M
Title : SW846 8260
Last Update : Tue Jan 02 14:25:32 2024

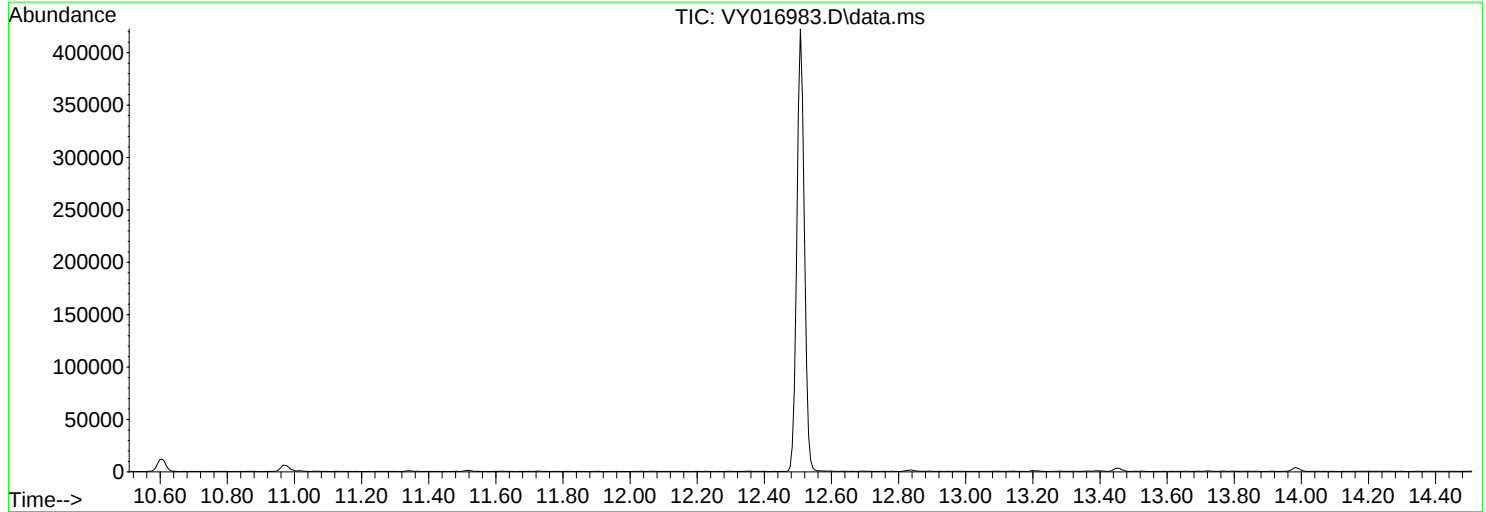

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	14404	PASS
75	95	30	60	52.7	37595	PASS
95	95	100	100	100.0	71323	PASS
96	95	5	9	7.2	5127	PASS
173	174	0.00	2	1.3	725	PASS
174	95	50	100	79.9	56971	PASS
175	174	5	9	7.3	4183	PASS
176	174	95	101	96.2	54813	PASS
177	176	5	9	6.8	3730	PASS