

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_Y\DATA\VY011420\
 Data File : VY001199.D
 Acq On : 14 Jan 2020 13:19
 Operator : SY/MD
 Sample : L1108-05
 Misc : 4.40G/5ML/MSVOA_Y/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 INWOOD-BH-03-A

Quant Time: Jan 15 01:22:32 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y011020S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jan 10 16:01:58 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.80	168	172252	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.70	114	316388	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.49	117	285807	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.42	152	135216	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.15	65	101639	55.87	ug/l	0.00
Spiked Amount	50.000		Recovery	=	111.74%	
35) Dibromofluoromethane	7.73	113	94546	51.04	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.08%	
50) Toluene-d8	10.18	98	371246	52.01	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.02%	
62) 4-Bromofluorobenzene	12.48	95	140693	48.21	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.42%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	2.12	50	1918	1.006	ug/l	99
11) Tert butyl alcohol	4.96	59	2208	12.063	ug/l	98
16) Acetone	3.96	43	3194	7.560	ug/l	96
20) Methylene Chloride	4.74	84	10011	Below Cal		95
25) 2-Butanone	6.99	43	2896	4.404	ug/l #	82
29) Tetrahydrofuran	7.38	42	825	1.831	ug/l #	57
31) Cyclohexane	7.80	56	3718	1.057	ug/l #	1
36) 1,1-Dichloropropene	7.80	75	13362	4.634	ug/l #	48
38) Carbon Tetrachloride	7.80	117	16198	6.129	ug/l #	16
76) 1,2,3-Trichloropropane	12.48	75	67325	46.511	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.48	75	67325	78.873	ug/l #	6
92) 1,2-Dibromo-3-Chloropropan	14.55	75	2128	5.516	ug/l #	16


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_Y\DATA\VY011420\
Data File : VY001199.D
Acq On : 14 Jan 2020 13:19
Operator : SY/MD
Sample : L1108-05
Misc : 4.40G/5ML/MSVOA_Y/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
INWOOD-BH-03-A

Quant Time: Jan 15 01:22:32 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y011020S.M
Quant Title : SW846 8260
QLast Update : Fri Jan 10 16:01:58 2020
Response via : Initial Calibration

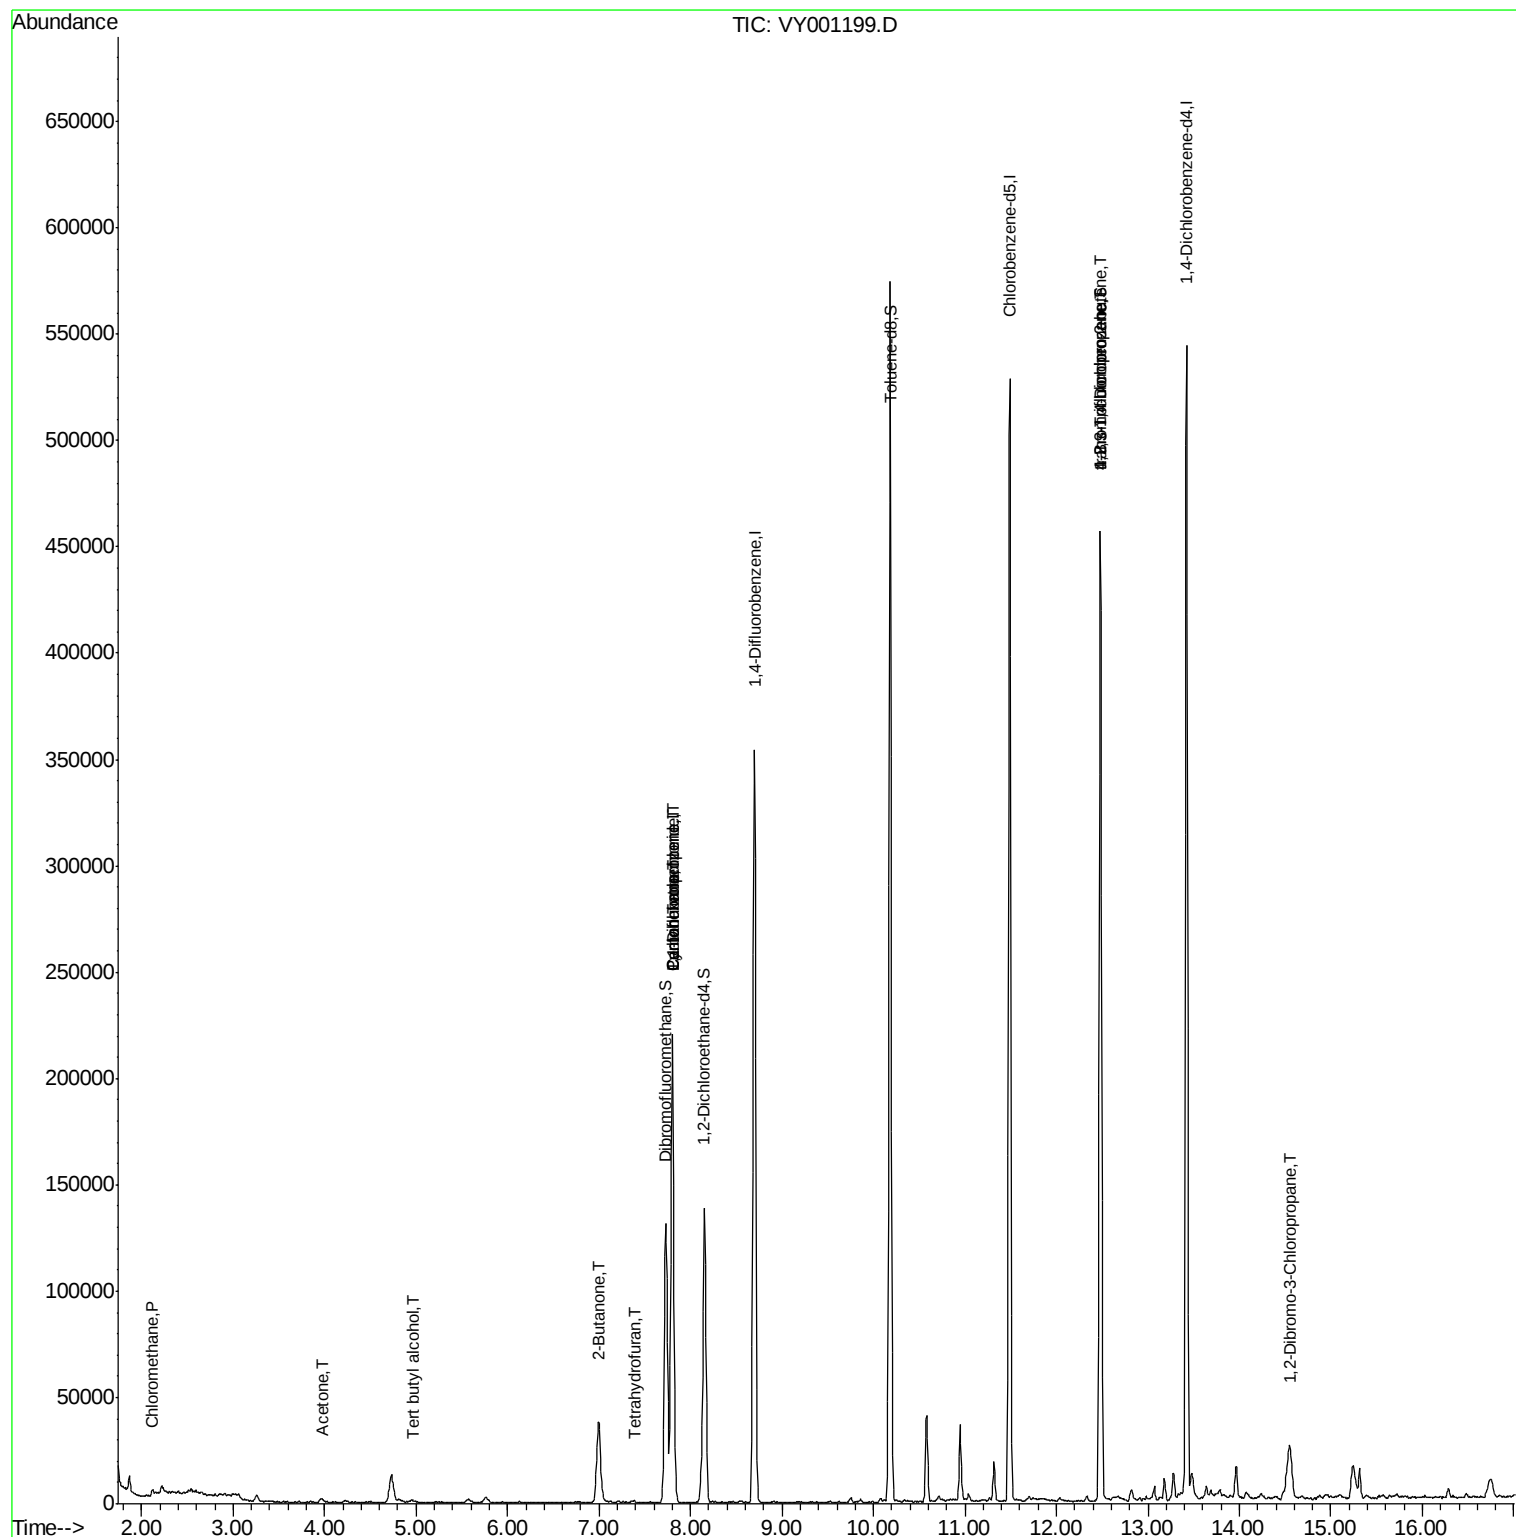

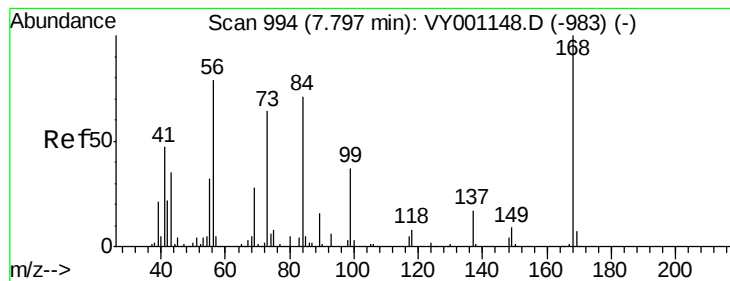

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.80 min Scan# 995

Delta R.T. 0.01 min

Lab File: VY001199.D

Acq: 14 Jan 2020 13:19

Instrument :

MSVOA_Y

ClientSampleId :


INWOOD-BH-03-A

Tgt Ion:168 Resp: 172252

Ion Ratio Lower Upper

168 100

99 55.3 47.9 71.9

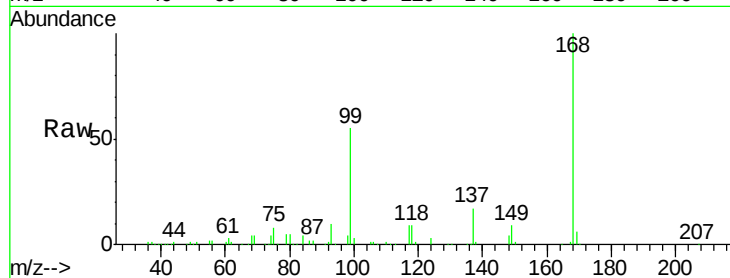

Abundance Ion 167.90 (167.60 to 168.60): VY001148.D (-983) (-)

Ion 98.90 (98.60 to 99.60): VY001148.D (-983) (-)

7.80

80000

60000

40000

20000



0

7.70

7.80

7.90

Time-->

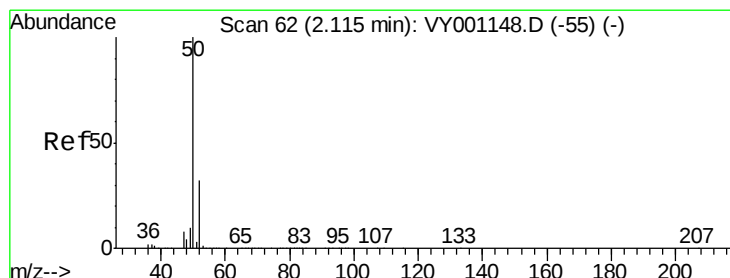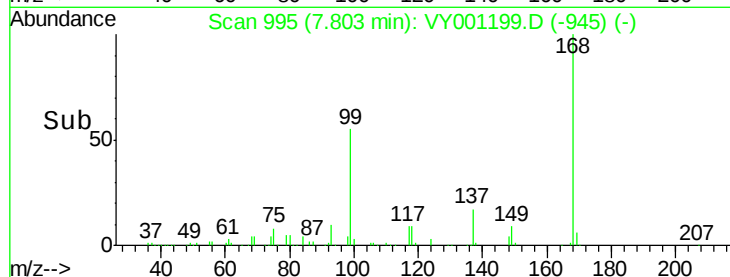

#3

Chloromethane

Concen: 1.006 ug/l

RT: 2.12 min Scan# 62

Delta R.T. -0.00 min

Lab File: VY001199.D


Acq: 14 Jan 2020 13:19

Tgt Ion: 50 Resp: 1918

Ion Ratio Lower Upper

50 100

52 32.6 25.8 38.6

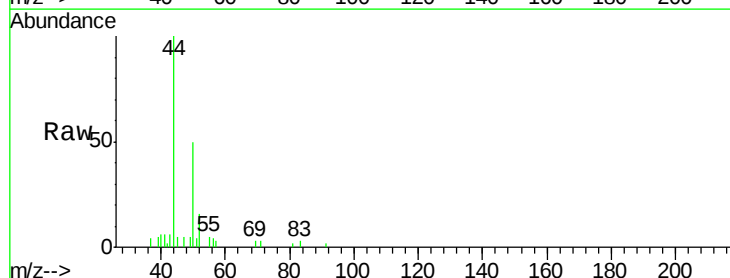

Abundance Ion 49.90 (49.60 to 50.60): VY001148.D (-55) (-)

Ion 51.90 (51.60 to 52.60): VY001148.D (-55) (-)

2.12

1500

1000

500


0


2.05

2.10

2.15

Time-->

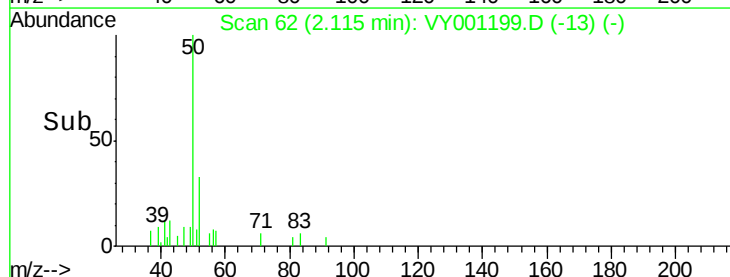




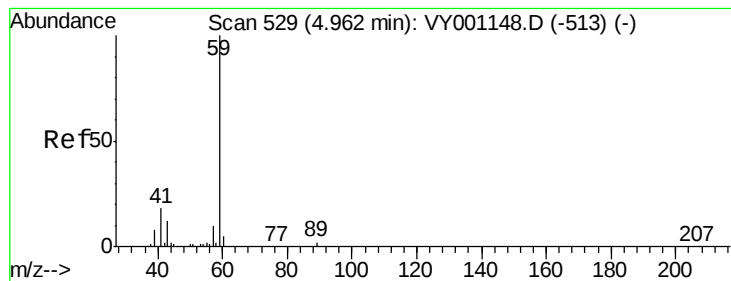


#11

Tert butyl alcohol
 Concen: 12.063 ug/l
 RT: 4.96 min Scan# 529
 Delta R.T. -0.00 min
 Lab File: VY001199.D
 Acq: 14 Jan 2020 13:19

Instrument :
 MSVOA_Y
 ClientSampleId :
 INWOOD-BH-03-A




Tgt Ion: 59 Resp: 2208
 Ion Ratio Lower Upper
 59 100
 57 10.6 7.8 11.8

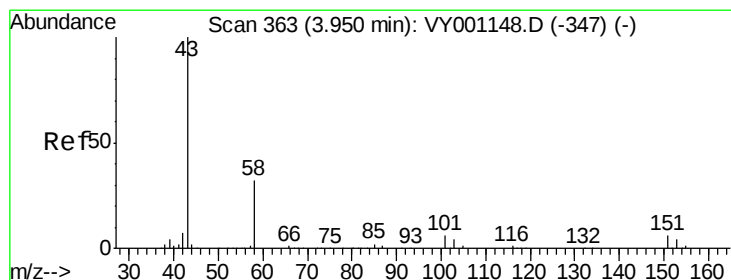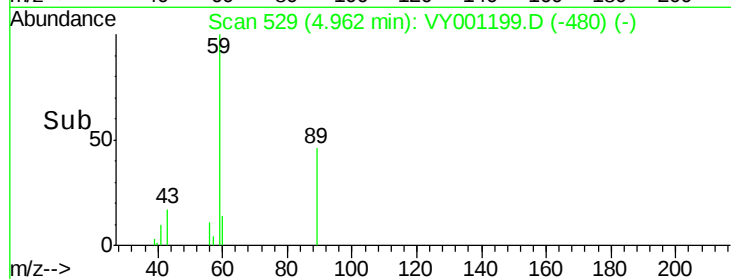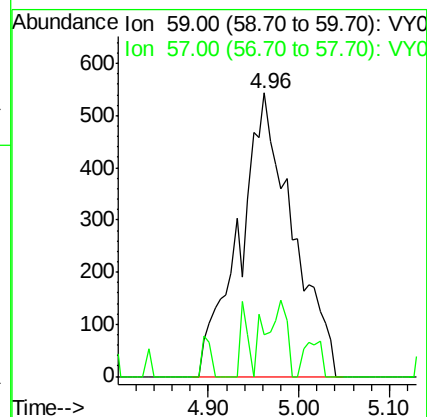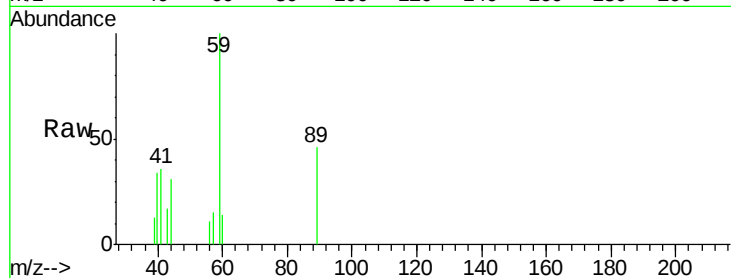


#16

Acetone
 Concen: 7.560 ug/l
 RT: 3.96 min Scan# 365
 Delta R.T. 0.01 min
 Lab File: VY001199.D
 Acq: 14 Jan 2020 13:19

Tgt Ion: 43 Resp: 3194
 Ion Ratio Lower Upper
 43 100
 58 34.4 25.8 38.6

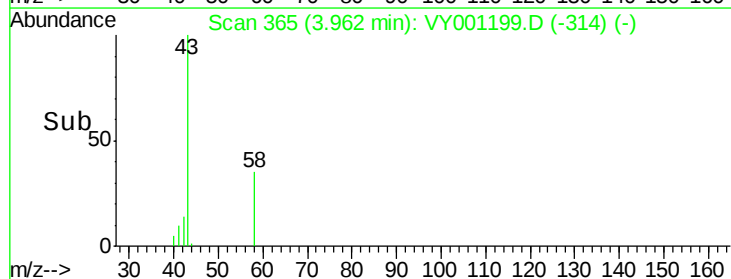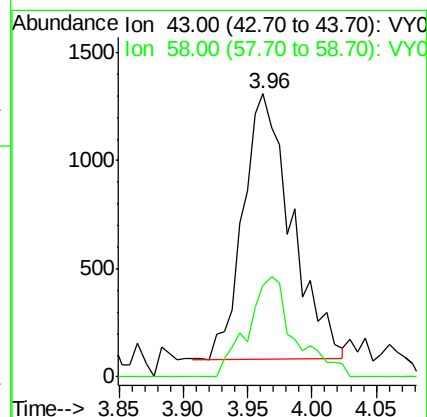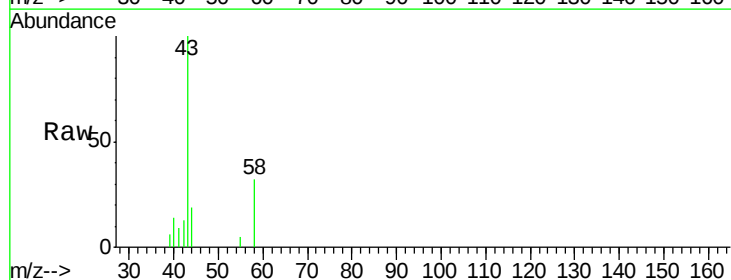

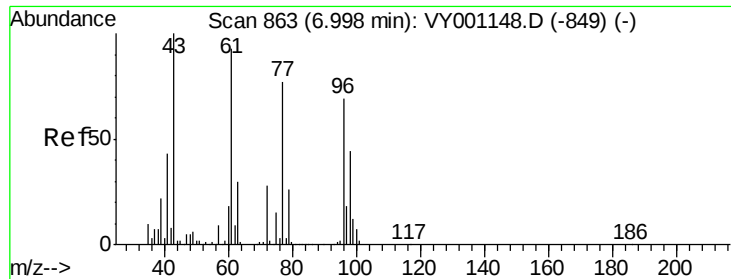

#25

2-Butanone

Concen: 4.404 ug/l

RT: 6.99 min Scan# 862

Delta R.T. -0.01 min

Lab File: VY001199.D

Acq: 14 Jan 2020 13:19

Instrument :

MSVOA_Y

ClientSampleId :





INWOOD-BH-03-A

Tgt Ion: 43 Resp: 2896

Ion Ratio Lower Upper

43 100

72 18.4 22.2 33.2#

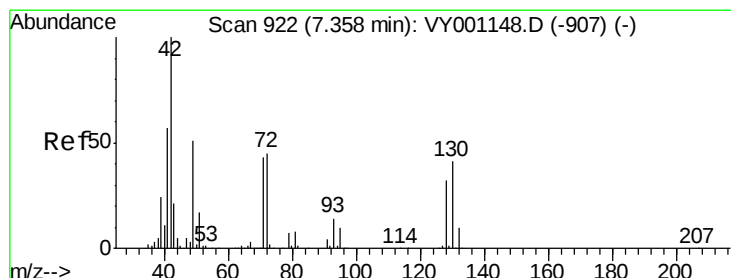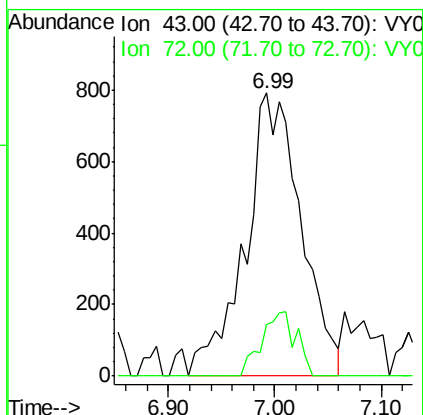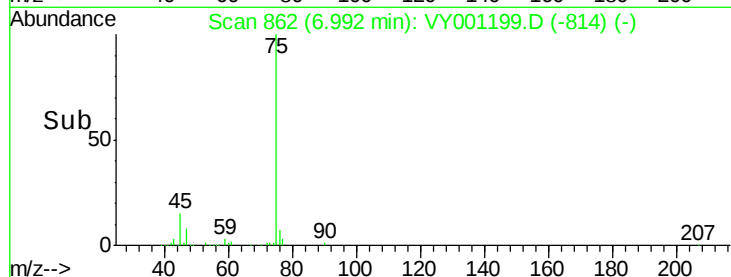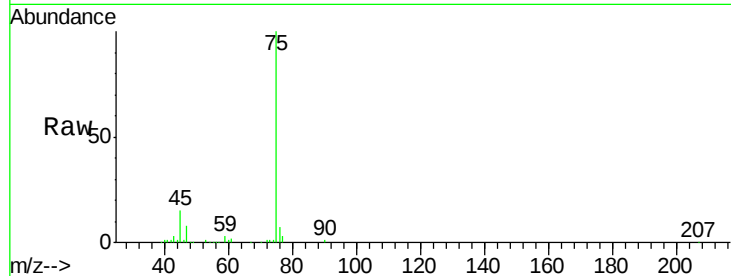

#29

Tetrahydrofuran

Concen: 1.831 ug/l

RT: 7.38 min Scan# 925

Delta R.T. 0.02 min

Lab File: VY001199.D

Acq: 14 Jan 2020 13:19




Tgt Ion: 42 Resp: 825


Ion Ratio Lower Upper

42 100

72 28.0 36.9 55.3#

71 4.4 34.0 51.0#

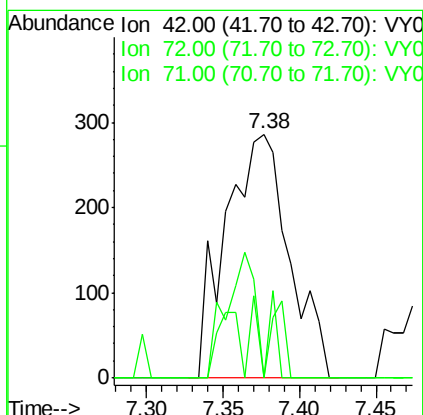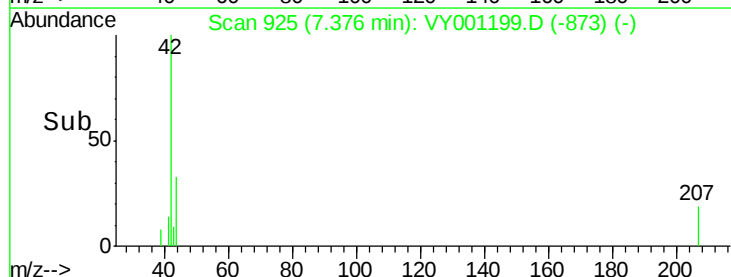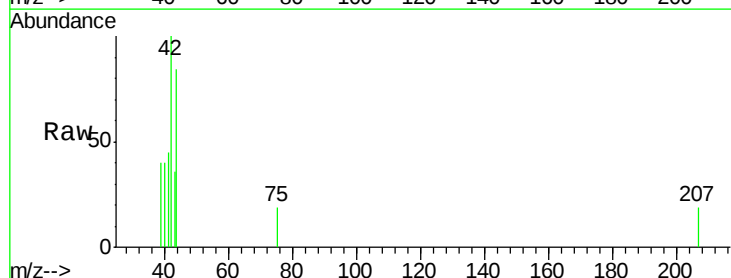

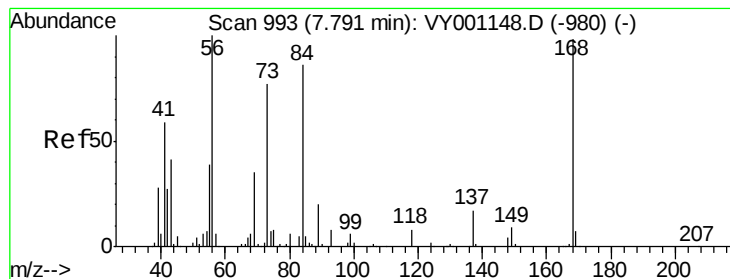

#31

Cyclohexane

Concen: 1.057 ug/l

RT: 7.80 min Scan# 995

Delta R.T. 0.01 min

Lab File: VY001199.D

Acq: 14 Jan 2020 13:19

Instrument :

MSVOA_Y

ClientSampleId :

INWOOD-BH-03-A


Tgt Ion: 56 Resp: 3718

Ion Ratio Lower Upper

56 100

69 150.6 27.8 41.8#




84 156.5 68.9 103.3#

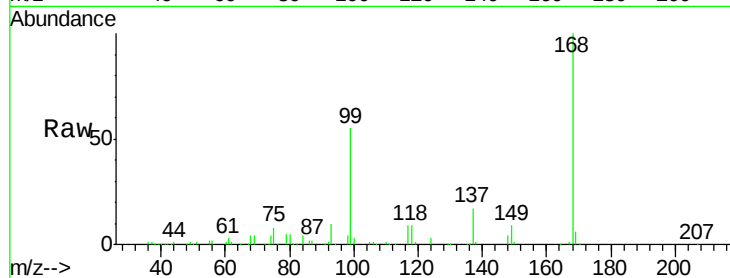

Abundance Ion 56.00 (55.70 to 56.70): VY0

Ion 69.00 (68.70 to 69.70): VY0

Ion 84.00 (83.70 to 84.70): VY0

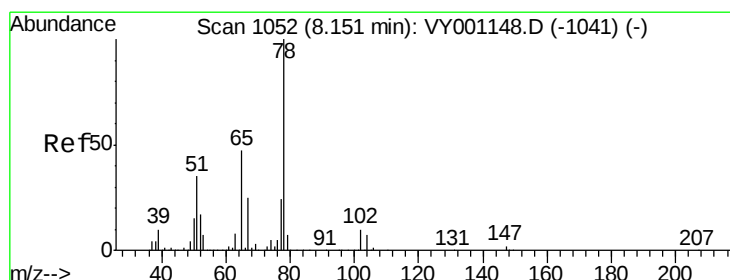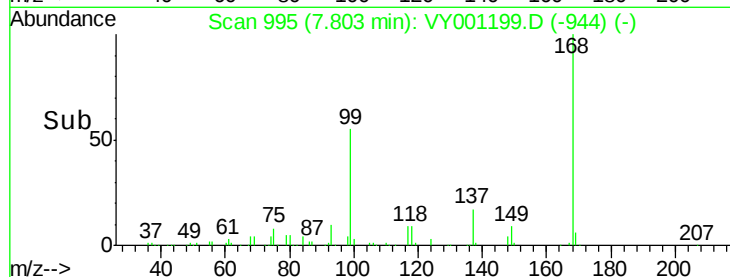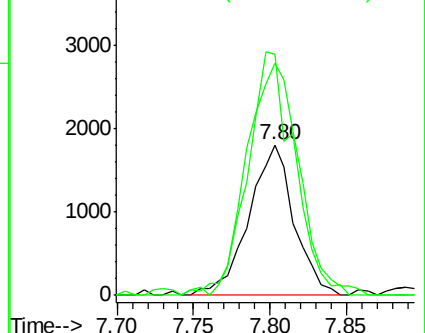

#33

1,2-Dichloroethane-d4

Concen: 55.868 ug/l

RT: 8.15 min Scan# 1052

Delta R.T. -0.00 min

Lab File: VY001199.D


Acq: 14 Jan 2020 13:19

Tgt Ion: 65 Resp: 101639

Ion Ratio Lower Upper



65 100


67 54.8 0.0 105.2

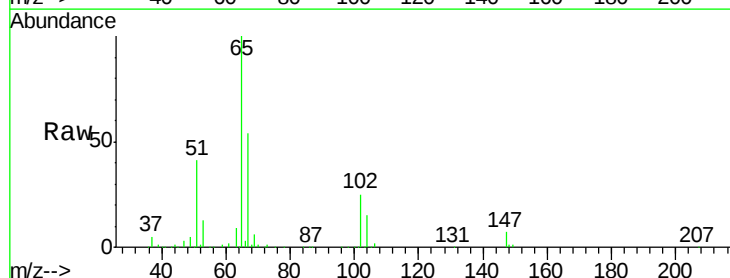

Abundance Ion 64.90 (64.60 to 65.60): VY0

Ion 66.90 (66.60 to 67.60): VY0

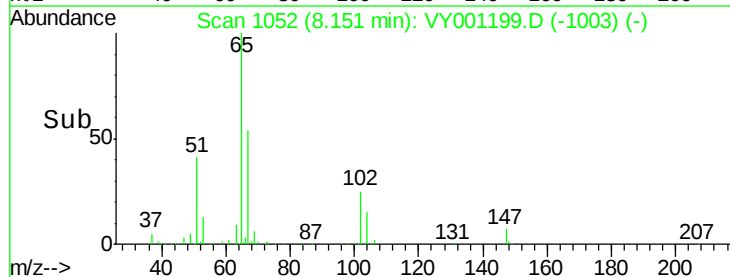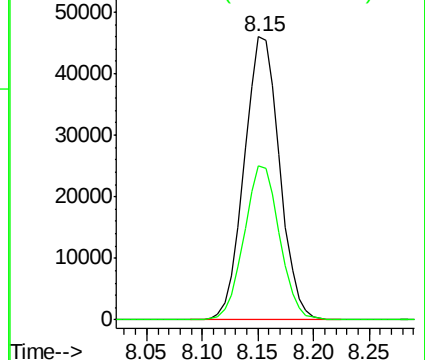

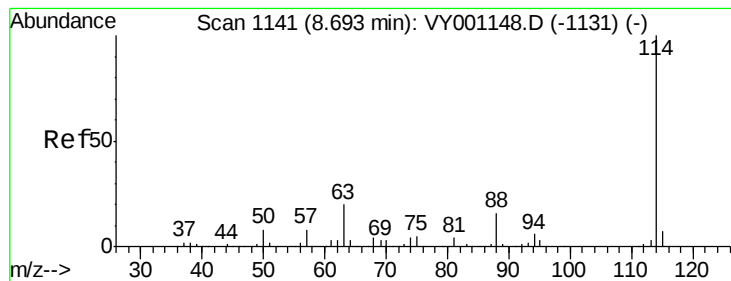

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.70 min Scan# 1142

Delta R.T. 0.01 min

Lab File: VY001199.D

Acq: 14 Jan 2020 13:19

Instrument :

MSVOA_Y

ClientSampleId :

INWOOD-BH-03-A


Tgt Ion:114 Resp: 316388

Ion Ratio Lower Upper

114 100

63 19.1 0.0 40.8




88 15.2 0.0 32.4

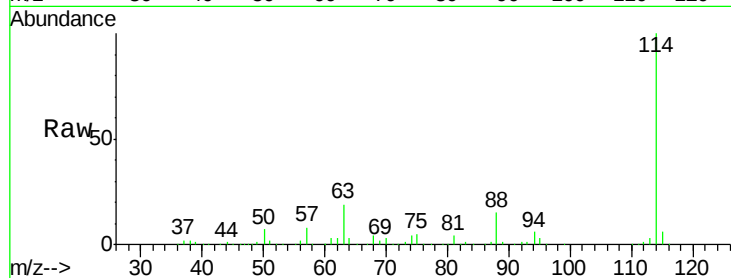

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VY0

Ion 87.90 (87.60 to 88.60): VY0

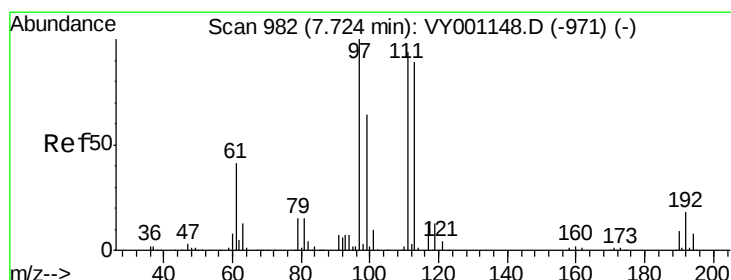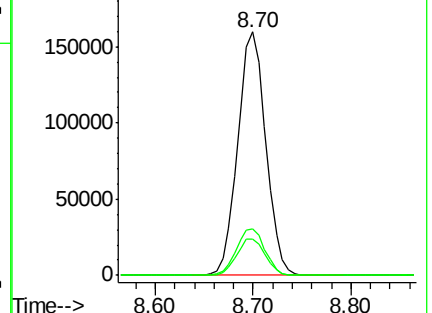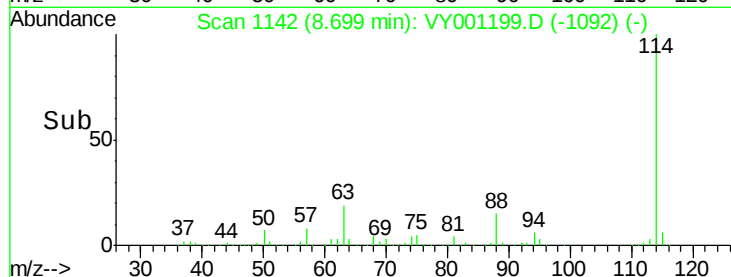

#35

Dibromofluoromethane

Concen: 51.038 ug/l

RT: 7.73 min Scan# 983

Delta R.T. 0.01 min

Lab File: VY001199.D

Acq: 14 Jan 2020 13:19


Tgt Ion:113 Resp: 94546

Ion Ratio Lower Upper

113 100

111 103.5 82.9 124.3



192 19.7 15.4 23.2

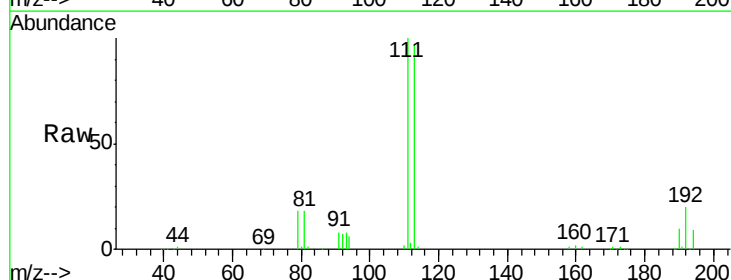


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



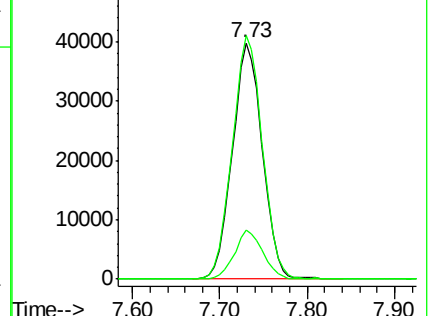
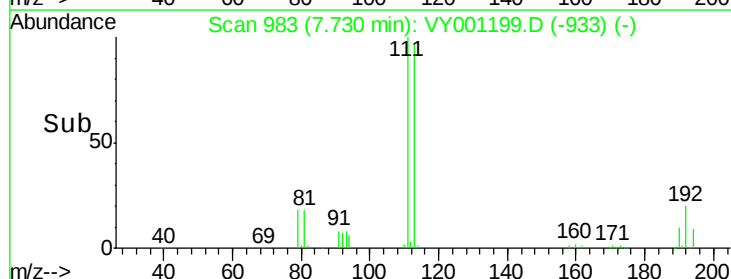


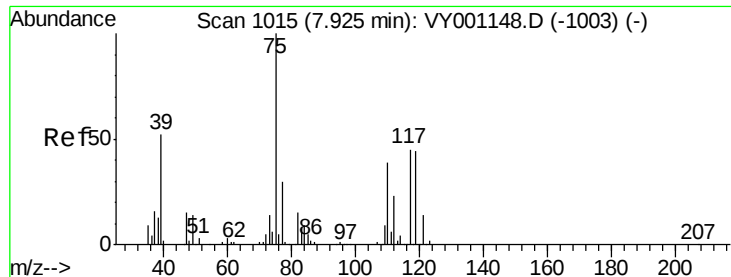

#36
 1,1-Dichloropropene
 Concen: 4.634 ug/l
 RT: 7.80 min Scan# 995
 Delta R.T. -0.12 min
 Lab File: VY001199.D
 Acq: 14 Jan 2020 13:19




Instrument :
 MSVOA_Y
 ClientSampleId :
 INWOOD-BH-03-A


Tgt Ion: 75 Resp: 13362
 Ion Ratio Lower Upper
 75 100
 110 8.5 18.3 54.8#
 77 0.0 25.1 37.7#

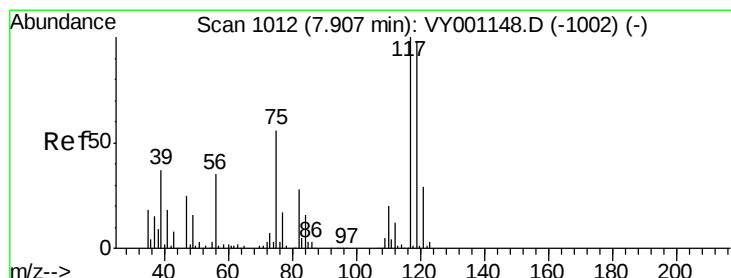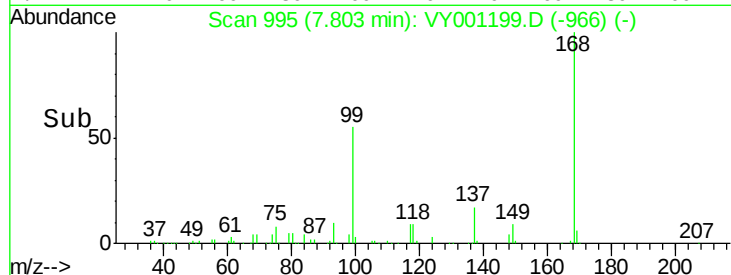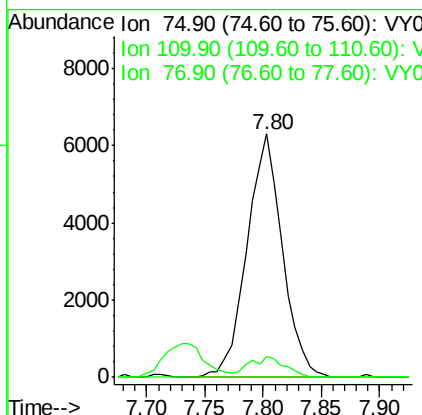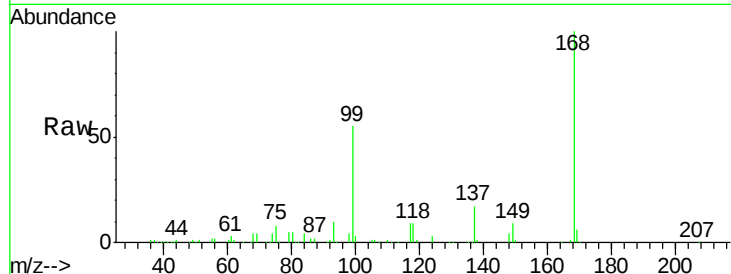

#38
 Carbon Tetrachloride
 Concen: 6.129 ug/l
 RT: 7.80 min Scan# 995
 Delta R.T. -0.10 min
 Lab File: VY001199.D
 Acq: 14 Jan 2020 13:19

Tgt Ion: 117 Resp: 16198
 Ion Ratio Lower Upper
 117 100
 119 5.8 78.3 117.5#
 121 0.0 23.5 35.3#

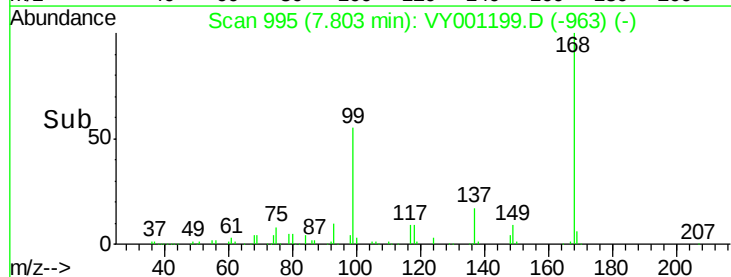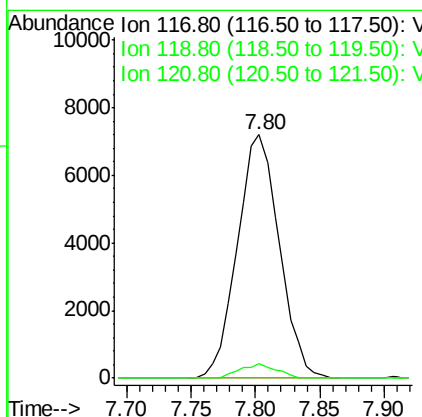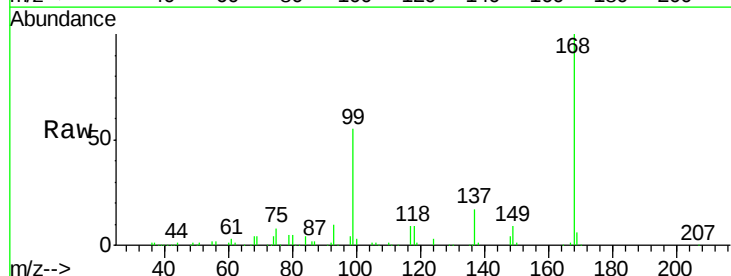

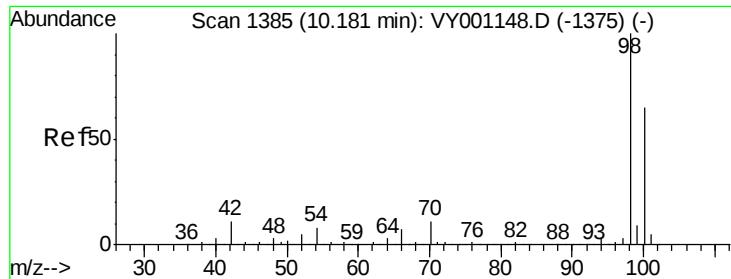

#50

Toluene-d8

Concen: 52.012 ug/l

RT: 10.18 min Scan# 1385

Delta R.T. -0.00 min

Lab File: VY001199.D

Acq: 14 Jan 2020 13:19

Instrument :

MSVOA_Y

ClientSampleId :





INWOOD-BH-03-A

Tgt Ion: 98 Resp: 371246

Ion Ratio Lower Upper

98 100

100 66.2 53.1 79.7

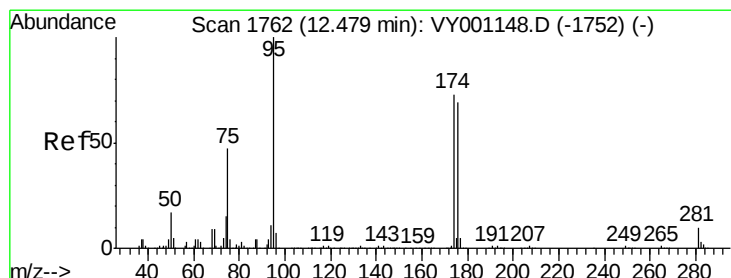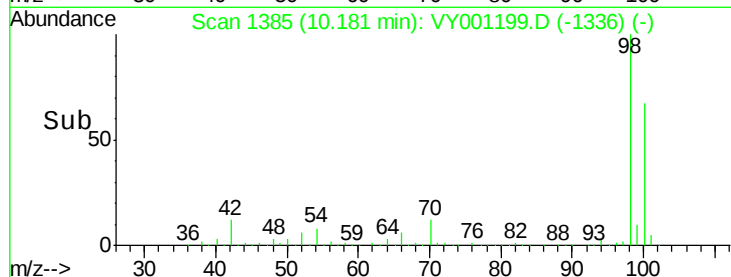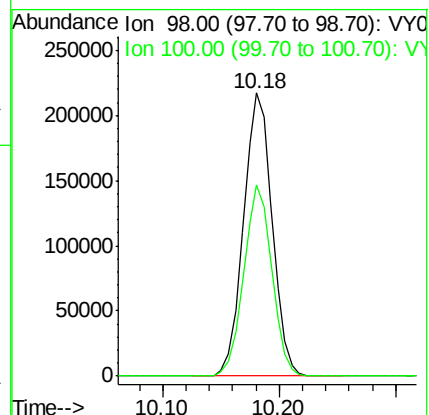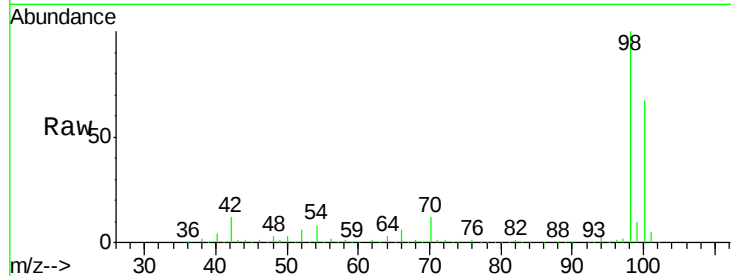

#62

4-Bromofluorobenzene

Concen: 48.213 ug/l

RT: 12.48 min Scan# 1762

Delta R.T. -0.00 min

Lab File: VY001199.D

Acq: 14 Jan 2020 13:19




Tgt Ion: 95 Resp: 140693


Ion Ratio Lower Upper

95 100

174 74.6 0.0 143.2

176 71.8 0.0 136.0

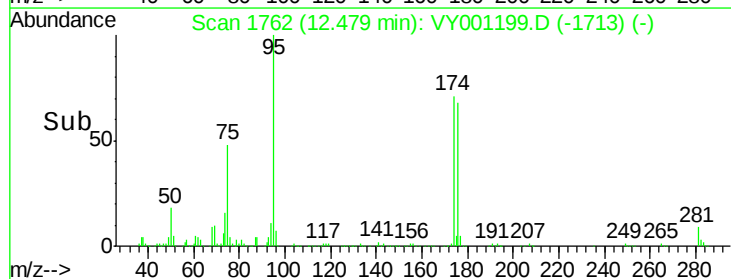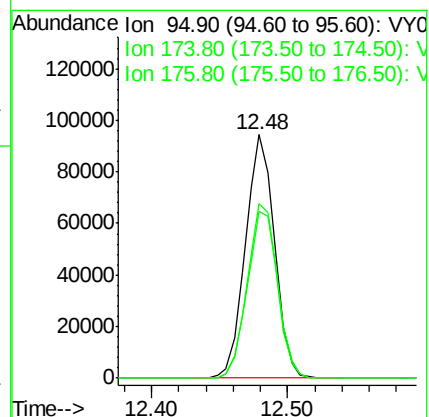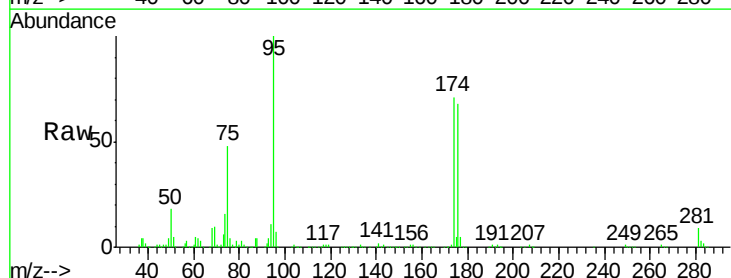


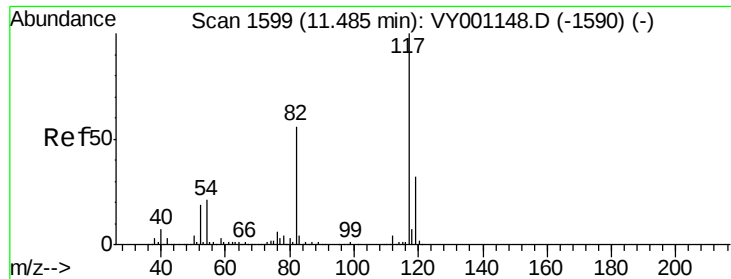




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.49 min Scan# 1600
Delta R.T. 0.01 min
Lab File: VY001199.D
Acq: 14 Jan 2020 13:19

Instrument :
MSVOA_Y
ClientSampleId :
INWOOD-BH-03-A

Tgt Ion:117 Resp: 285807
Ion Ratio Lower Upper
117 100
82 53.8 44.9 67.3
119 32.3 25.7 38.5

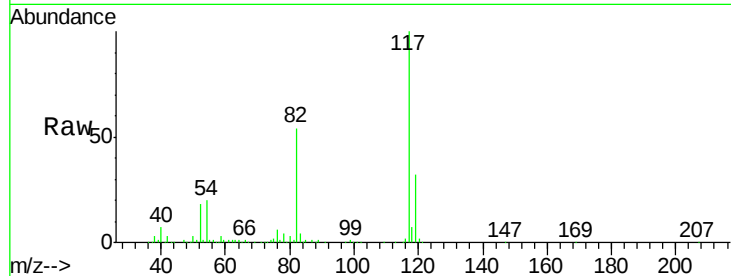


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VY0
Ion 118.90 (118.60 to 119.60): V

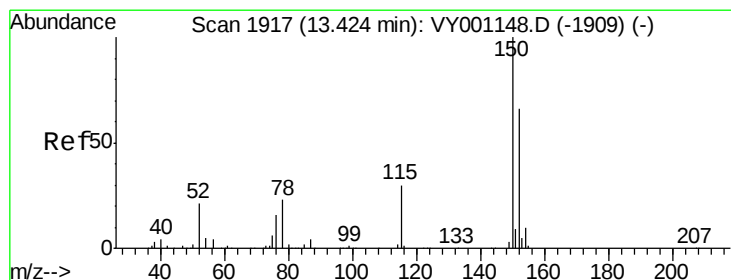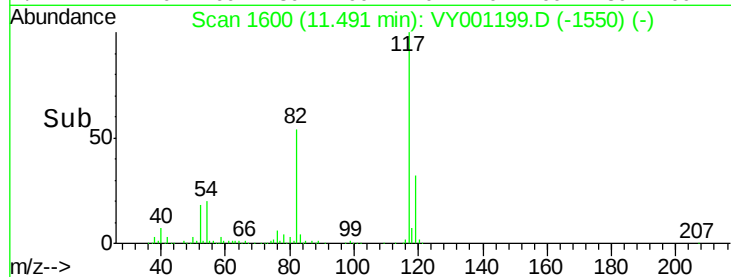
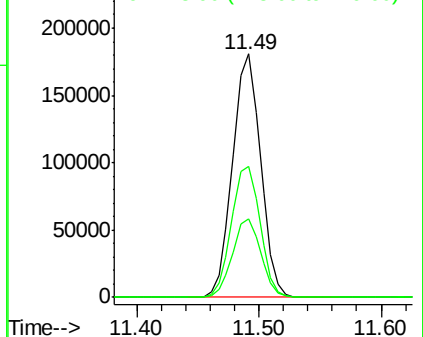



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.42 min Scan# 1917
Delta R.T. -0.00 min
Lab File: VY001199.D
Acq: 14 Jan 2020 13:19

Tgt Ion:152 Resp: 135216
Ion Ratio Lower Upper
152 100
115 59.3 30.9 92.5
150 157.8 0.0 346.8

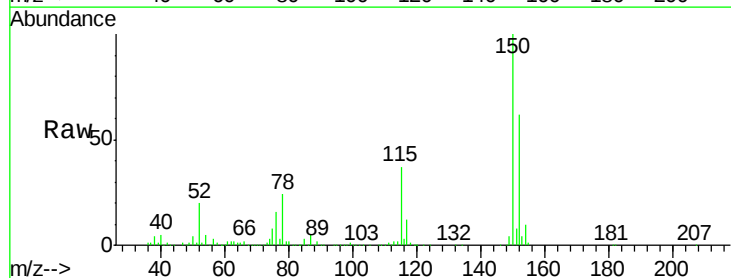

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V



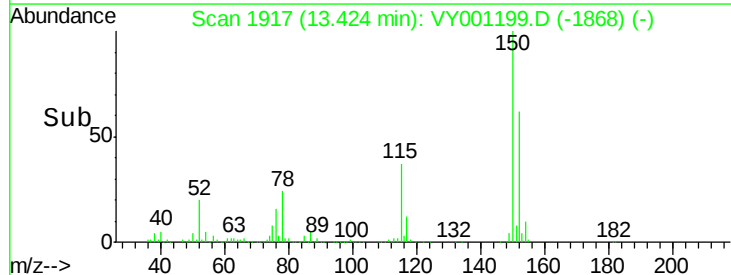
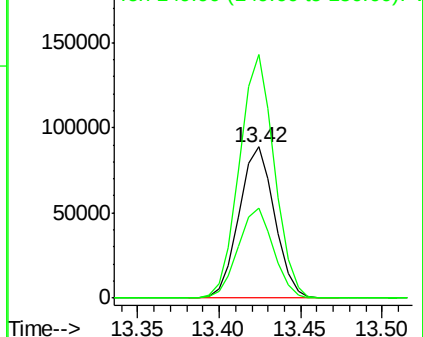


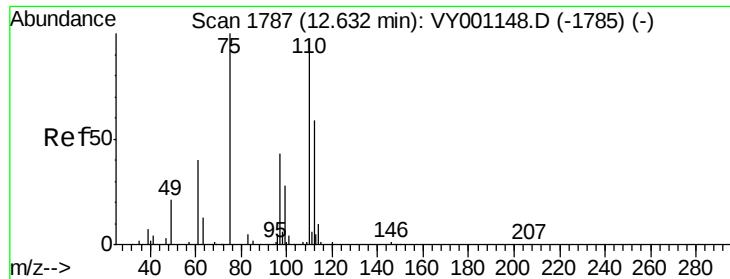

#76
 1,2,3-Trichloropropane
 Concen: 46.511 ug/l
 RT: 12.48 min Scan# 1762
 Delta R.T. -0.15 min
 Lab File: VY001199.D
 Acq: 14 Jan 2020 13:19




Instrument :
 MSVOA_Y
 ClientSampleId :
 INWOOD-BH-03-A


Tgt Ion: 75 Resp: 67325
 Ion Ratio Lower Upper
 75 100
 77 2.0 0.0 0.0#

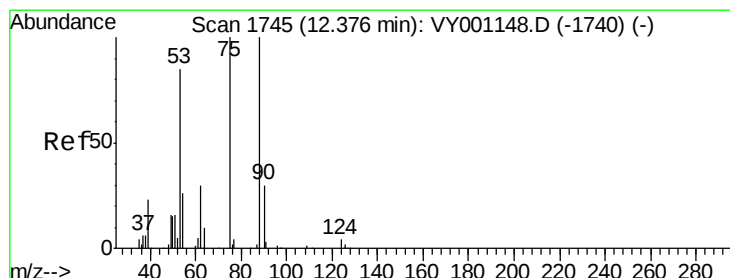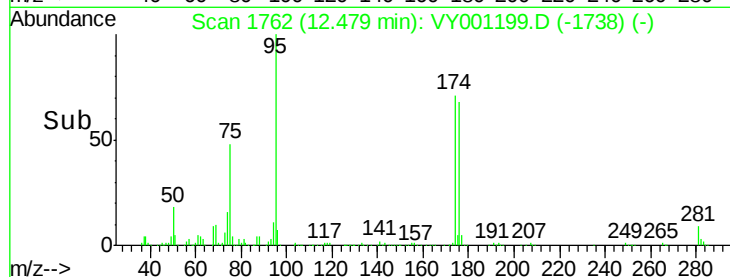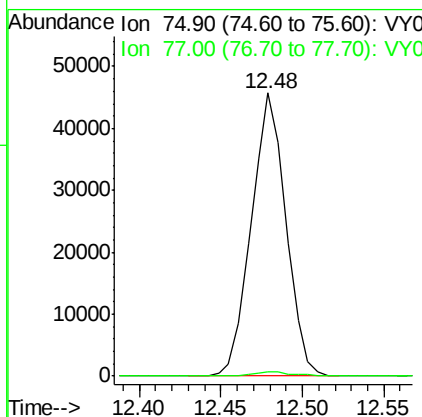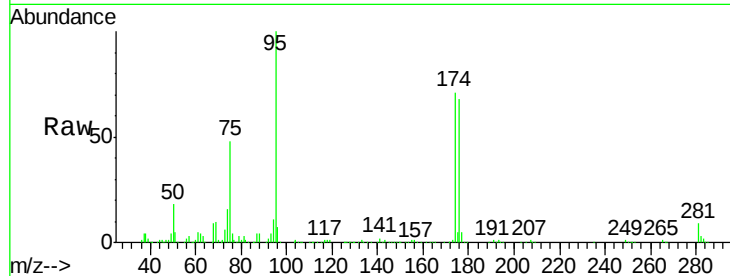

#81
 trans-1,4-Dichloro-2-butene
 Concen: 78.873 ug/l
 RT: 12.48 min Scan# 1762
 Delta R.T. 0.10 min
 Lab File: VY001199.D
 Acq: 14 Jan 2020 13:19

Tgt Ion: 75 Resp: 67325
 Ion Ratio Lower Upper
 75 100
 53 0.1 69.4 104.2#
 89 0.1 0.0 0.0#

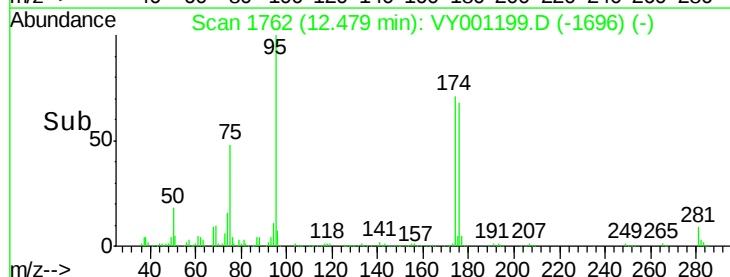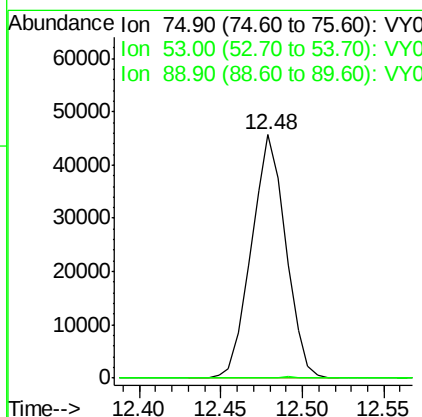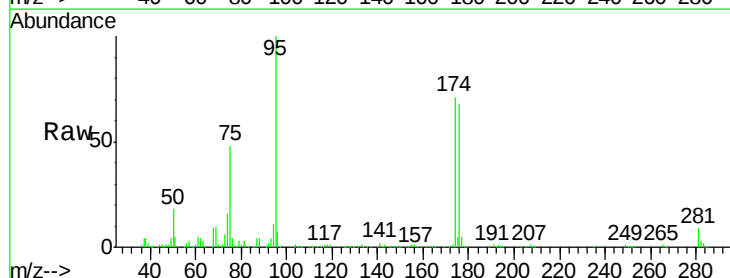

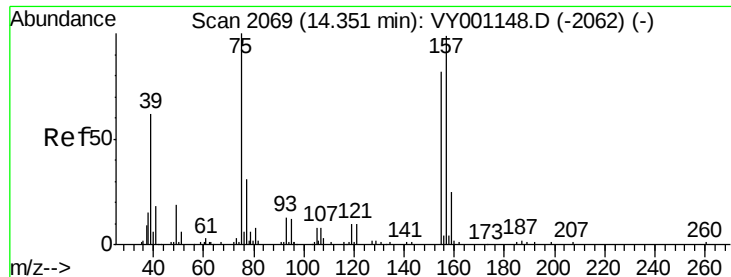

#92

1,2-Dibromo-3-Chloropropane

Concen: 5.516 ug/l

RT: 14.55 min Scan# 2102

Delta R.T. 0.20 min

Lab File: VY001199.D

Acq: 14 Jan 2020 13:19

Instrument :

MSVOA_Y

ClientSampleId :

INWOOD-BH-03-A


Tgt Ion: 75 Resp: 2128

Ion Ratio Lower Upper

75 100

155 137.4 41.2 123.6#

157 0.0 52.8 158.4#

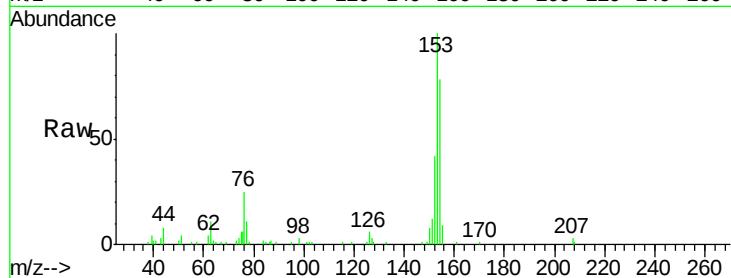

Abundance Ion 74.90 (74.60 to 75.60): VY0

Ion 154.80 (154.50 to 155.50): V

Ion 156.80 (156.50 to 157.50): V

