

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY011520\
 Data File : VY001218.D
 Acq On : 15 Jan 2020 15:17
 Operator : SY/MD
 Sample : L1125-04
 Misc : 7.58G/5ML/MSVOA Y/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 FESB-21A-(2.5-3)

Quant Time: Jan 16 05:31:47 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y011020S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jan 10 16:01:58 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.80	168	167934	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.69	114	297052	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.49	117	266321	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.42	152	119098	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.15	65	90859	51.23	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.46%	
35) Dibromofluoromethane	7.73	113	87169	50.12	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.24%	
50) Toluene-d8	10.18	98	351019	52.38	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.76%	
62) 4-Bromofluorobenzene	12.48	95	126022	46.00	ug/l	0.00
Spiked Amount	50.000		Recovery	=	92.00%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY011520\
Data File : VY001218.D
Acq On : 15 Jan 2020 15:17
Operator : SY/MD
Sample : L1125-04
Misc : 7.58G/5ML/MSVOA Y/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
FESB-21A-(2.5-3)

Quant Time: Jan 16 05:31:47 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y011020S.M
Quant Title : SW846 8260
QLast Update : Fri Jan 10 16:01:58 2020
Response via : Initial Calibration

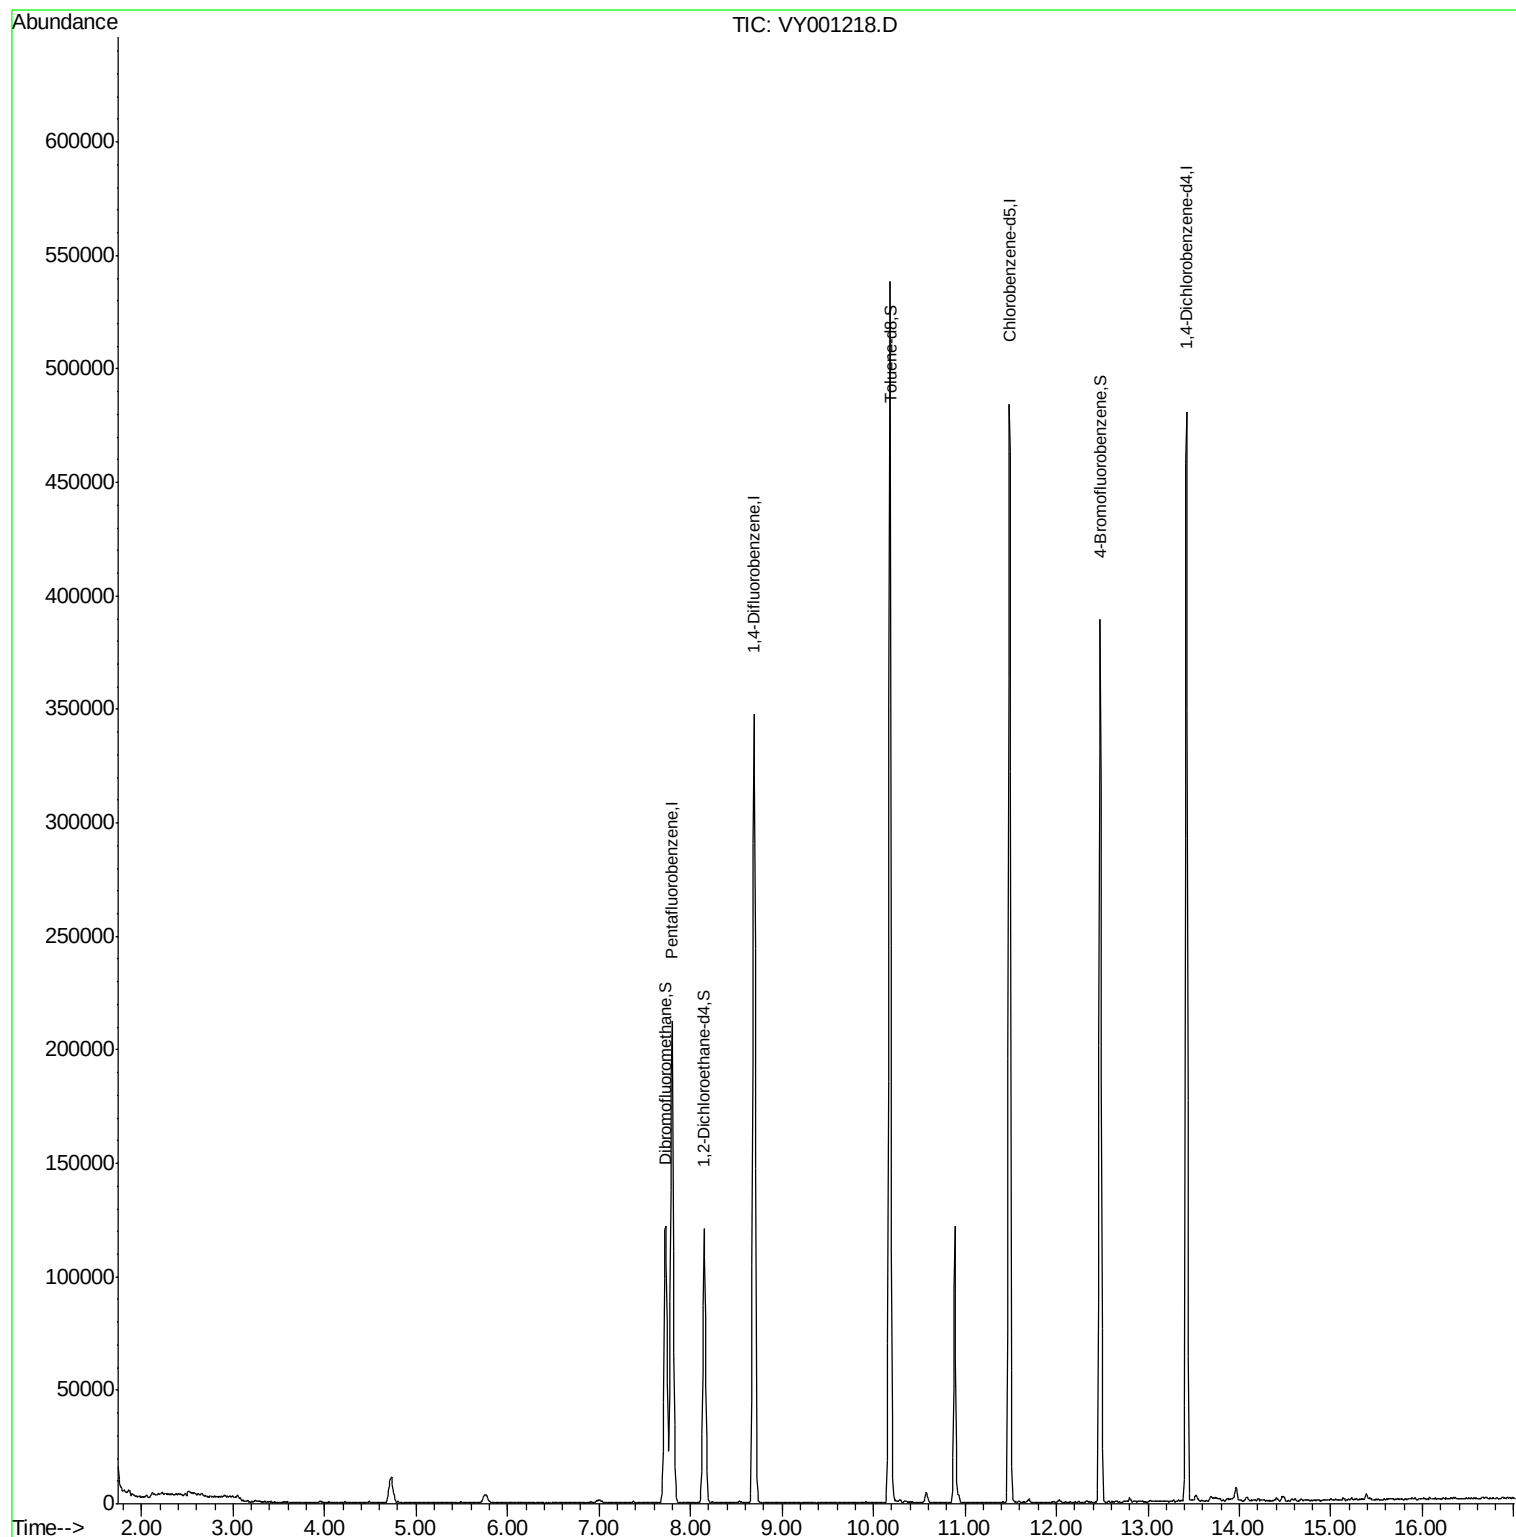

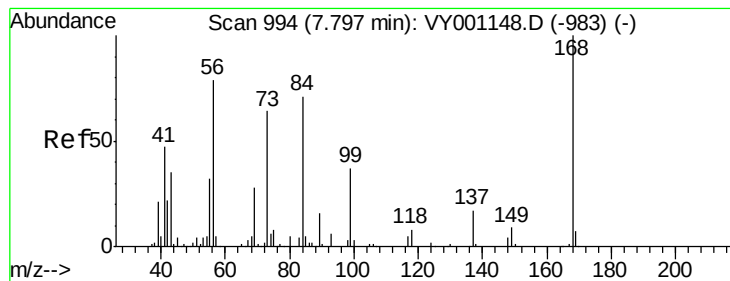

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.80 min Scan# 994

Delta R.T. -0.00 min

Lab File: VY001218.D

Acq: 15 Jan 2020 15:17

Instrument :

MSVOA_Y

ClientSampleId :


FESB-21A-(2.5-3)

Tot Ion:168 Resp: 167934

Ion Ratio Lower Upper




168 100

99 54.7 47.9 71.9

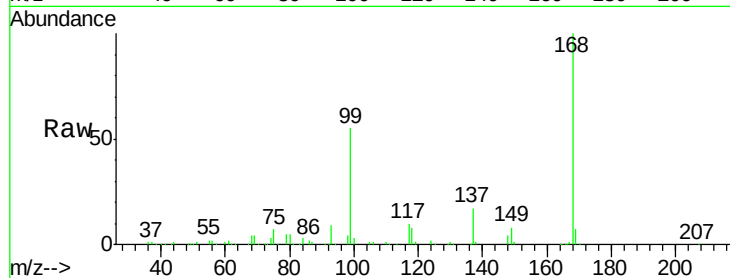

Abundance Ion 167.90 (167.60 to 168.60): VY001148.D (-983) (-)

Ion 98.90 (98.60 to 99.60): VY001148.D (-983) (-)

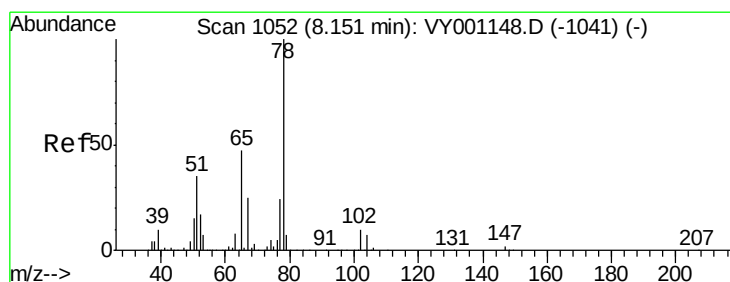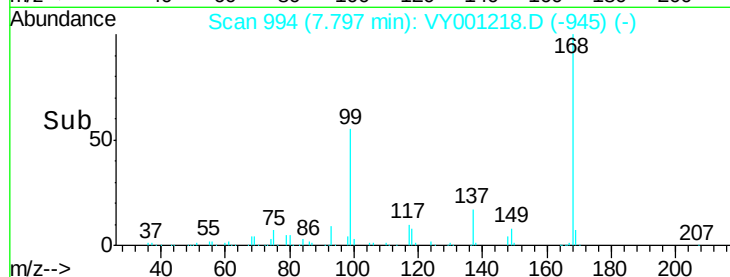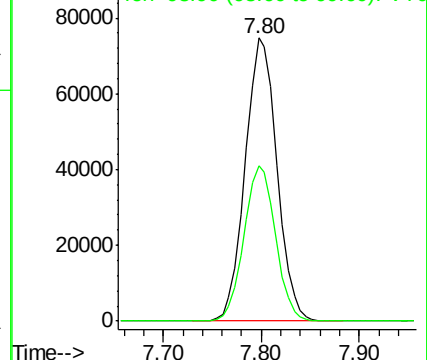

#33

1,2-Dichloroethane-d4

Concen: 51.226 ug/l

RT: 8.15 min Scan# 1052

Delta R.T. -0.00 min

Lab File: VY001218.D


Acq: 15 Jan 2020 15:17

Tgt Ion: 65 Resp: 90859

Ion Ratio Lower Upper



65 100


67 54.2 0.0 105.2

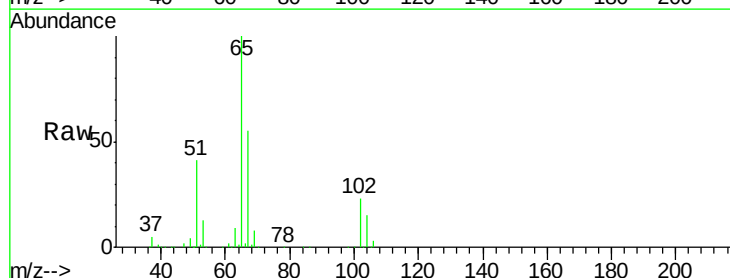

Abundance Ion 64.90 (64.60 to 65.60): VY001148.D (-1041) (-)

Ion 66.90 (66.60 to 67.60): VY001148.D (-1041) (-)

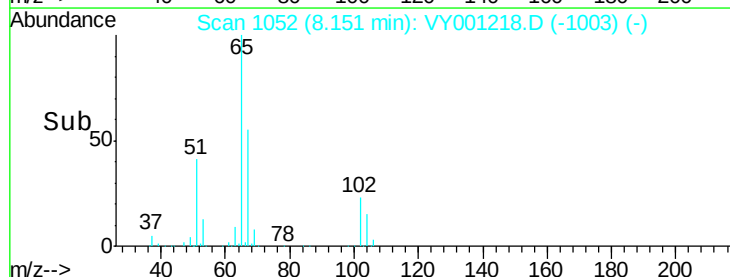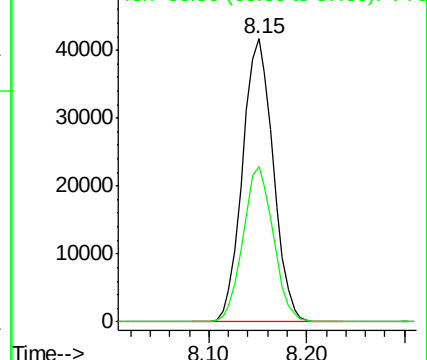

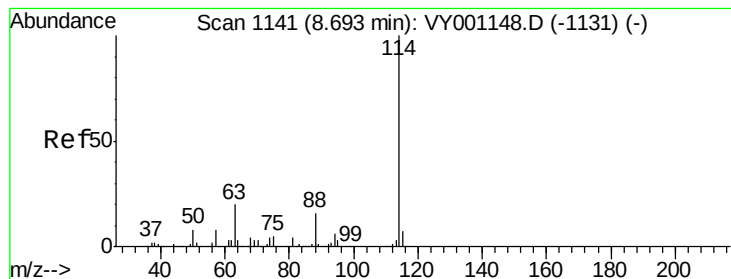

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.69 min Scan# 1141

Delta R.T. -0.00 min

Lab File: VY001218.D

Acq: 15 Jan 2020 15:17

Instrument :

MSVOA_Y

ClientSampleId :

FESB-21A-(2.5-3)


Tot Ion:114 Resp: 297052

Ion Ratio Lower Upper

114 100

63 20.7 0.0 40.8




88 16.2 0.0 32.4

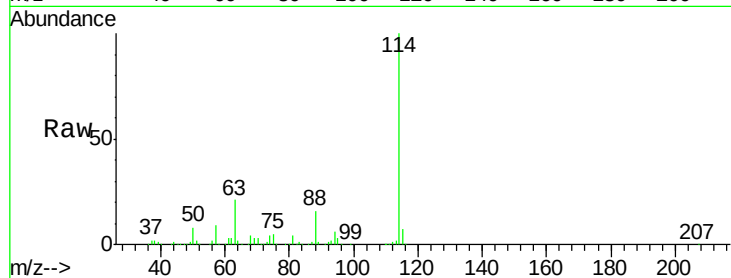

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VY0

Ion 87.90 (87.60 to 88.60): VY0

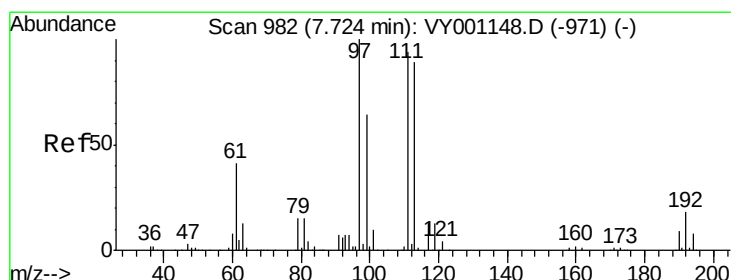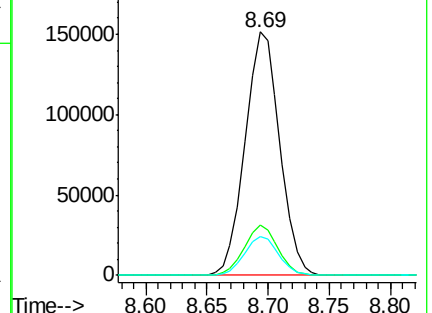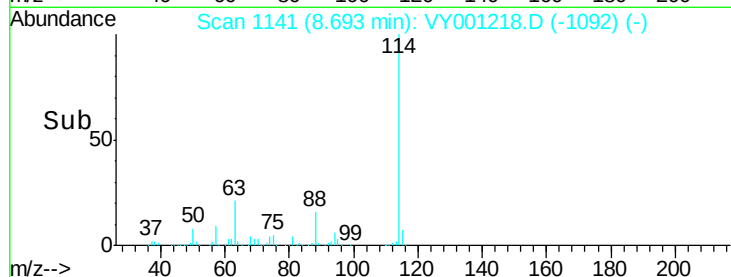

#35

Dibromofluoromethane

Concen: 50.119 ug/l

RT: 7.73 min Scan# 983

Delta R.T. 0.01 min

Lab File: VY001218.D

Acq: 15 Jan 2020 15:17


Tgt Ion:113 Resp: 87169

Ion Ratio Lower Upper

113 100

111 104.2 82.9 124.3



192 20.5 15.4 23.2

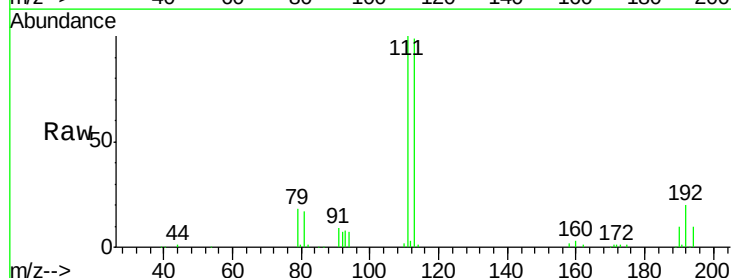


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

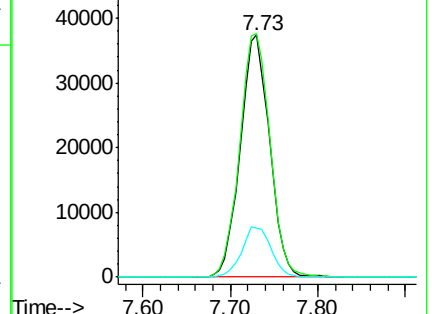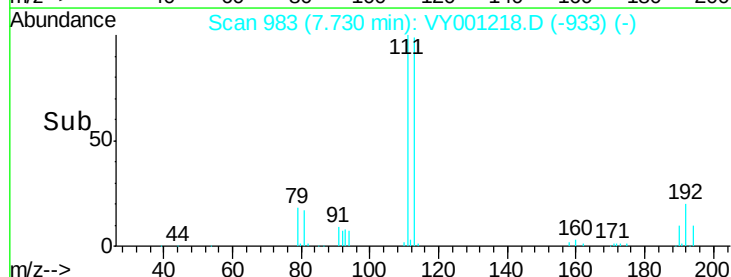

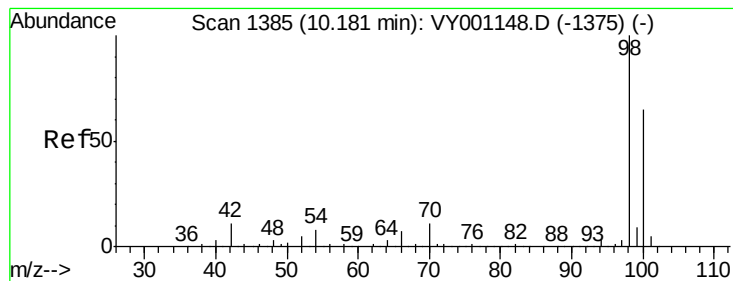

#50

Toluene-d8

Concen: 52.379 ug/l

RT: 10.18 min Scan# 1385

Delta R.T. -0.00 min

Lab File: VY001218.D

Acq: 15 Jan 2020 15:17

Instrument :

MSVOA_Y

ClientSampleId :


FESB-21A-(2.5-3)

Tot Ion: 98 Resp: 351019

Ion Ratio Lower Upper




98 100

100 65.8 53.1 79.7

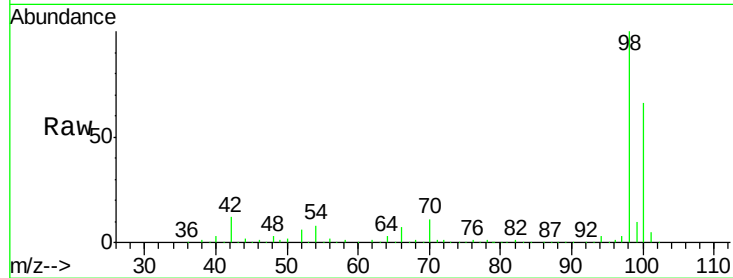

Abundance Ion 98.00 (97.70 to 98.70): VY0

Ion 100.00 (99.70 to 100.70): VY0

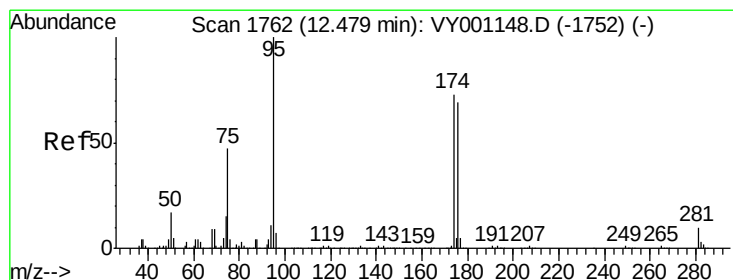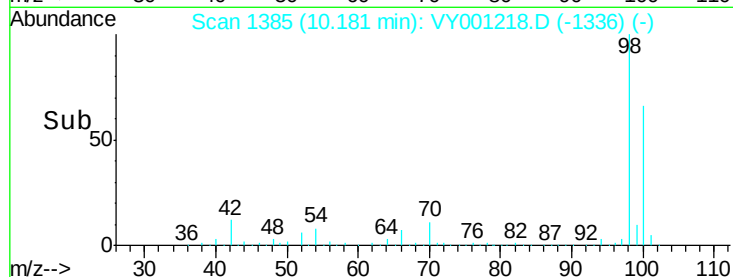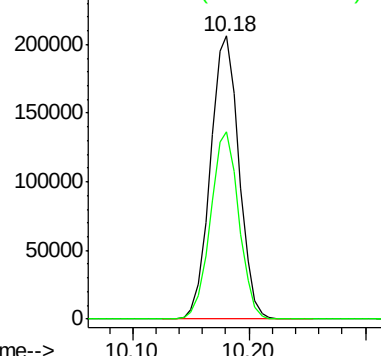

#62

4-Bromofluorobenzene

Concen: 45.997 ug/l

RT: 12.48 min Scan# 1762

Delta R.T. -0.00 min

Lab File: VY001218.D

Acq: 15 Jan 2020 15:17


Tgt Ion: 95 Resp: 126022

Ion Ratio Lower Upper

95 100

174 76.0 0.0 143.2



176 73.0 0.0 136.0

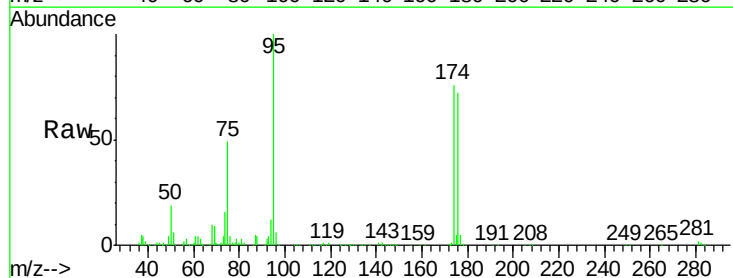


Abundance Ion 94.90 (94.60 to 95.60): VY0

Ion 173.80 (173.50 to 174.50): VY0

Ion 175.80 (175.50 to 176.50): VY0

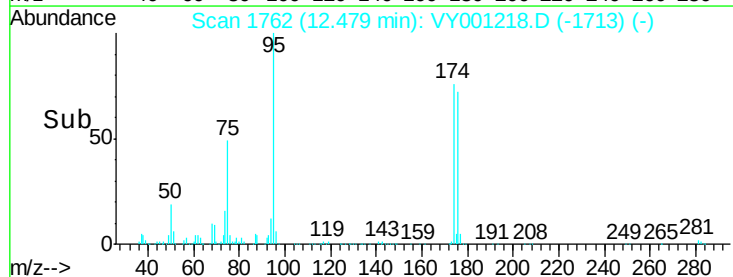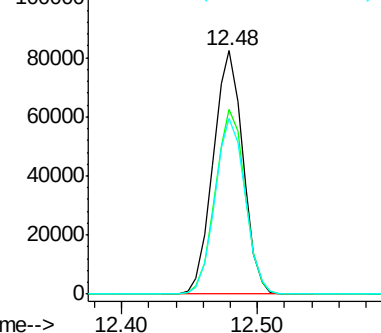


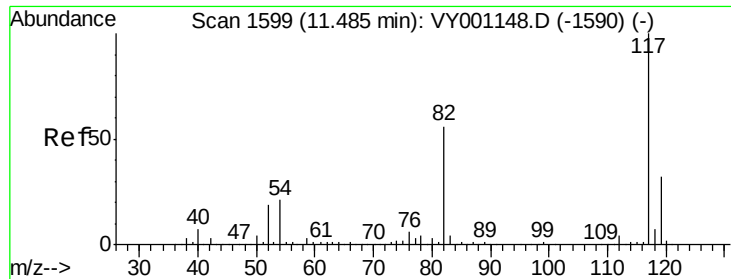




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.49 min Scan# 1600
Delta R.T. 0.01 min
Lab File: VY001218.D
Acq: 15 Jan 2020 15:17

Instrument :
MSVOA_Y
ClientSampleId :
FESB-21A-(2.5-3)

Tot Ion:117 Resp: 266321
Ion Ratio Lower Upper
117 100
82 53.3 44.9 67.3
119 32.0 25.7 38.5

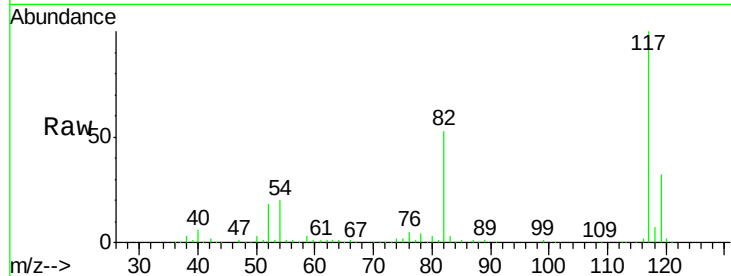


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VY0
Ion 118.90 (118.60 to 119.60): V

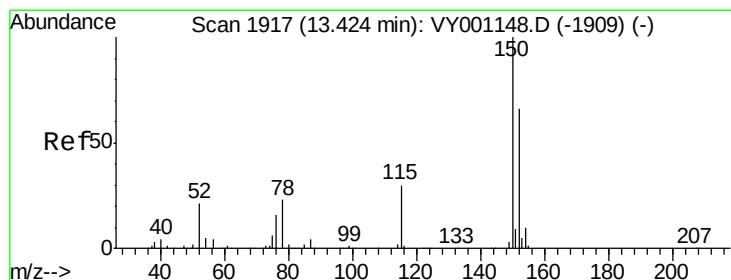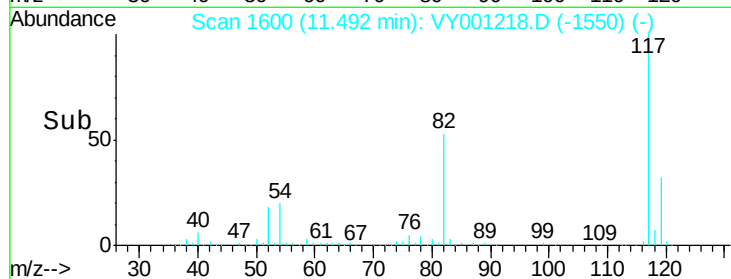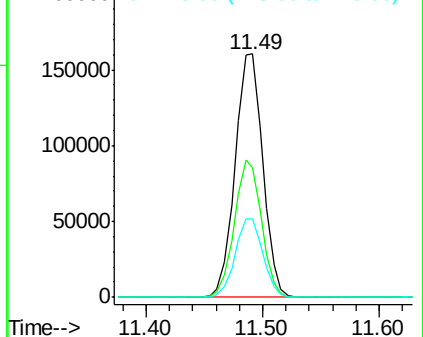

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.42 min Scan# 1917
Delta R.T. -0.00 min
Lab File: VY001218.D
Acq: 15 Jan 2020 15:17

Tgt Ion:152 Resp: 119098
Ion Ratio Lower Upper
152 100
115 60.3 30.9 92.5
150 158.0 0.0 346.8

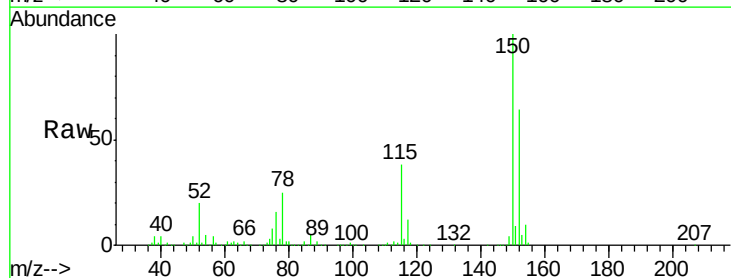

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

