

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY011520\
 Data File : VY001226.D
 Acq On : 15 Jan 2020 18:15
 Operator : SY/MD
 Sample : L1127-04
 Misc : 6.90G/5ML/MSVOA Y/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 QVD-SB-102-2-2.5

Quant Time: Jan 16 05:58:47 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y011020S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jan 10 16:01:58 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.80	168	164530	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.69	114	294920	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.49	117	255302	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.42	152	99381	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.15	65	90346	51.99	ug/l	0.00
Spiked Amount	50.000		Recovery	=	103.98%	
35) Dibromofluoromethane	7.73	113	86361	50.01	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.02%	
50) Toluene-d8	10.18	98	342499	51.48	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.96%	
62) 4-Bromofluorobenzene	12.48	95	113585	41.76	ug/l	0.00
Spiked Amount	50.000		Recovery	=	83.52%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY011520\
Data File : VY001226.D
Acq On : 15 Jan 2020 18:15
Operator : SY/MD
Sample : L1127-04
Misc : 6.90G/5ML/MSVOA Y/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
QVD-SB-102-2-2.5

Quant Time: Jan 16 05:58:47 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y011020S.M
Quant Title : SW846 8260
QLast Update : Fri Jan 10 16:01:58 2020
Response via : Initial Calibration

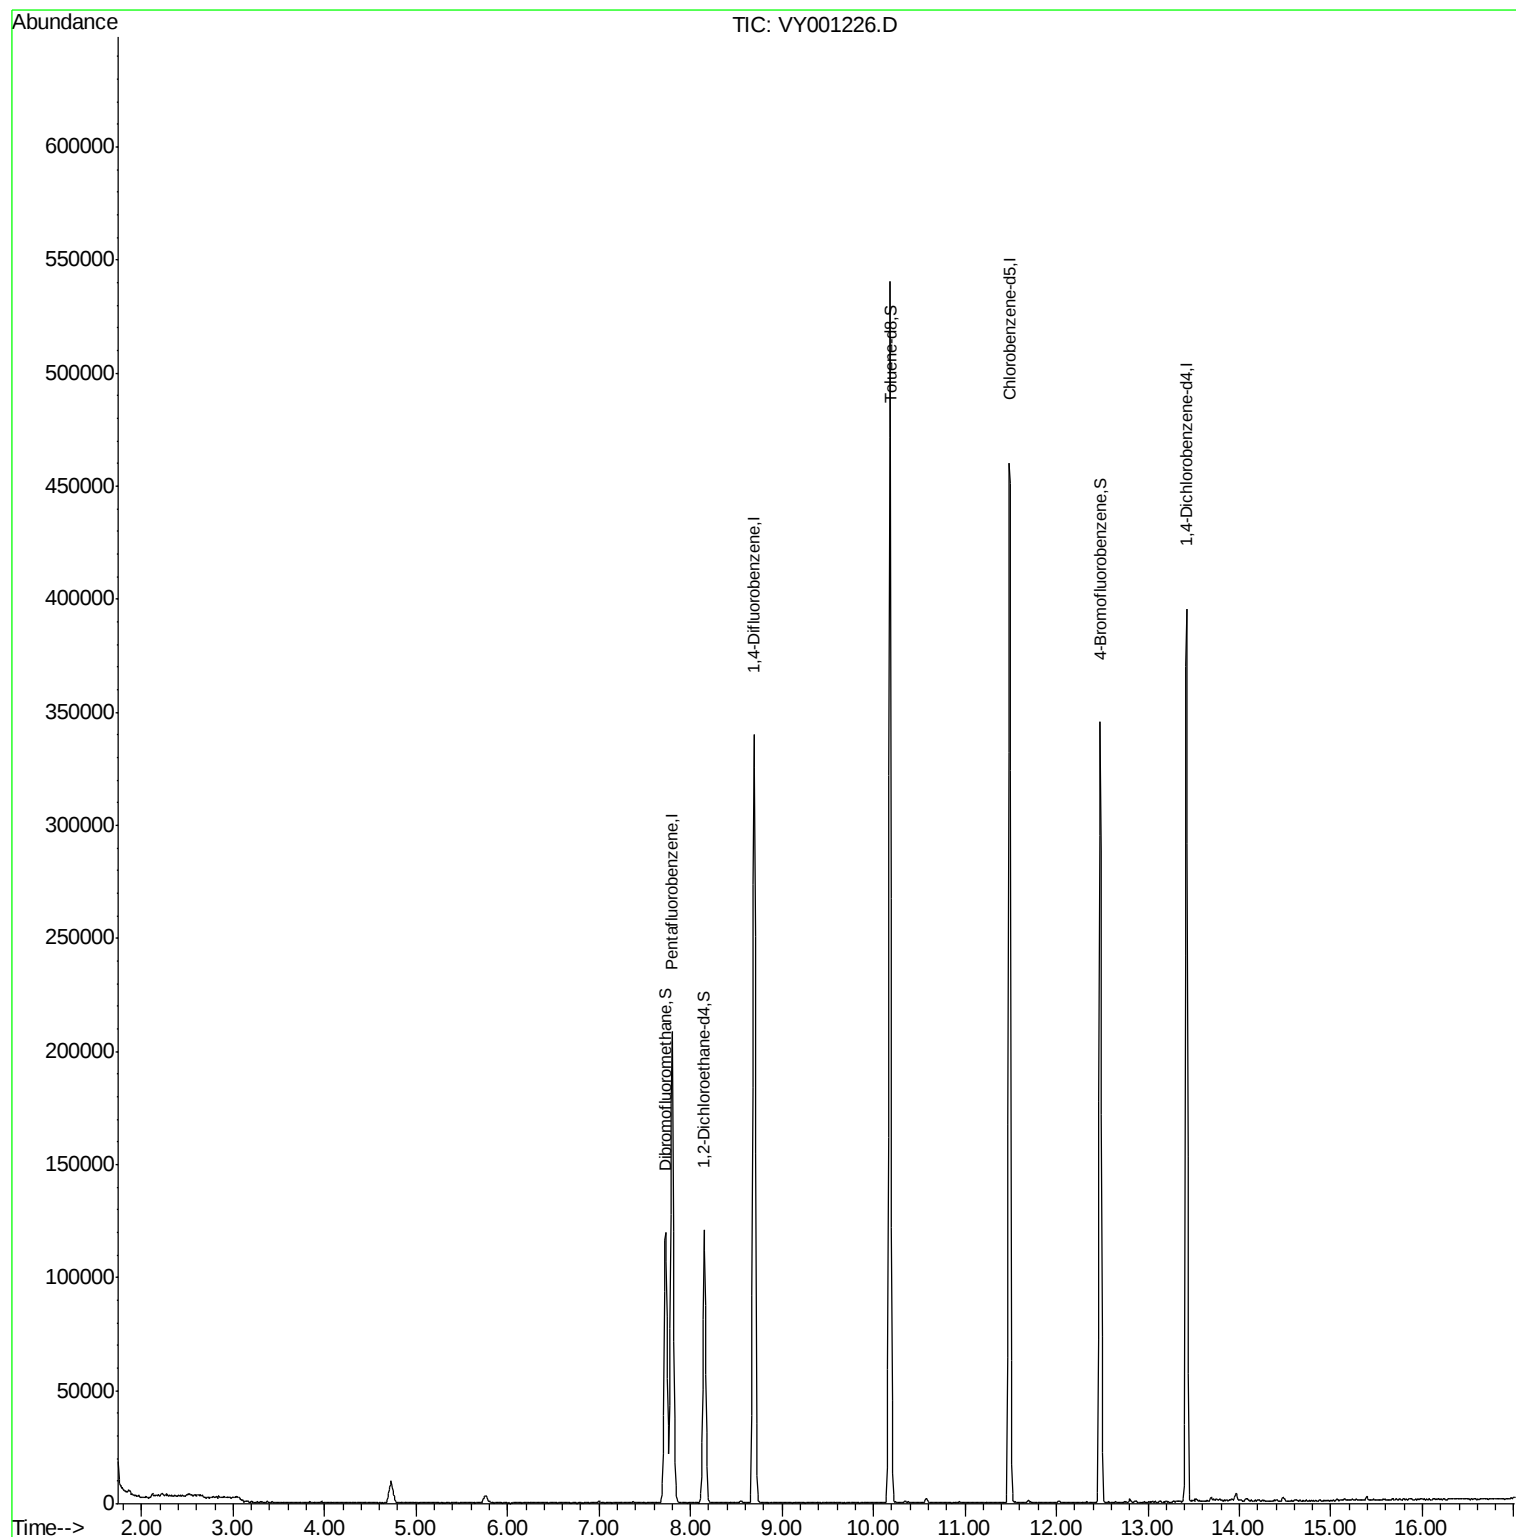

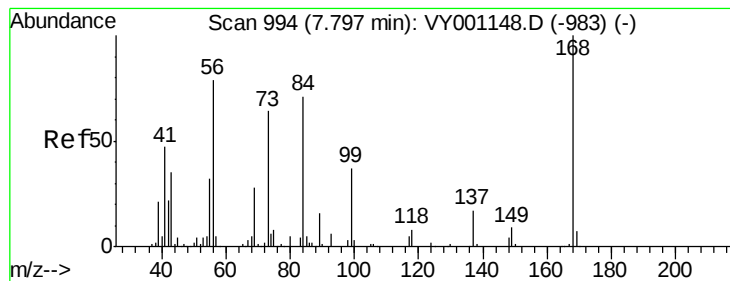

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.80 min Scan# 995

Delta R.T. 0.01 min

Lab File: VY001226.D

Acq: 15 Jan 2020 18:15

Instrument :

MSVOA_Y

ClientSampleId :


QVD-SB-102-2-2.5

Tot Ion:168 Resp: 164530

Ion Ratio Lower Upper

168 100

99 53.8 47.9 71.9

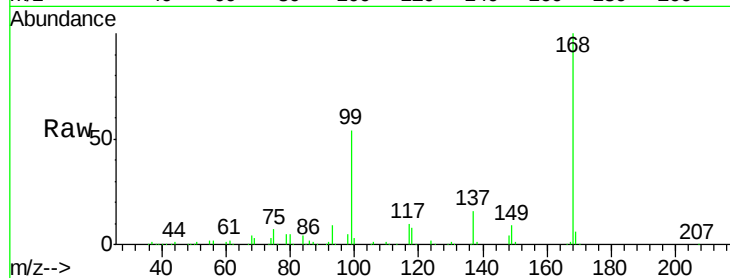

Abundance Ion 167.90 (167.60 to 168.60): VY001148.D (-983) (-)

Ion 98.90 (98.60 to 99.60): VY001148.D (-983) (-)

7.80

80000

60000



40000

20000

0

7.70 7.80 7.90

Time-->

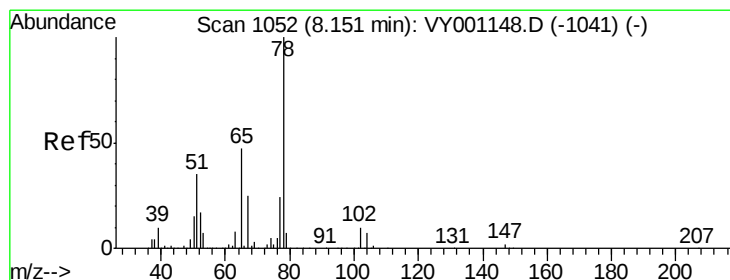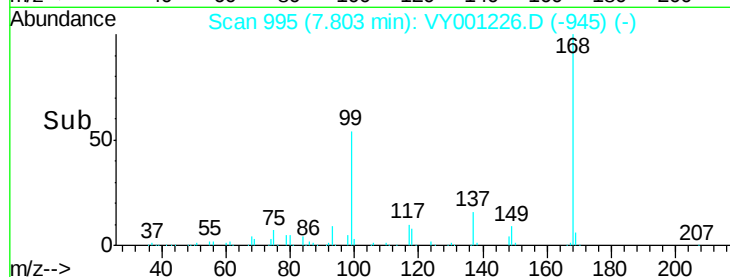

#33

1,2-Dichloroethane-d4

Concen: 51.991 ug/l

RT: 8.15 min Scan# 1052

Delta R.T. -0.00 min

Lab File: VY001226.D


Acq: 15 Jan 2020 18:15

Tgt Ion: 65 Resp: 90346

Ion Ratio Lower Upper

65 100

67 53.8 0.0 105.2

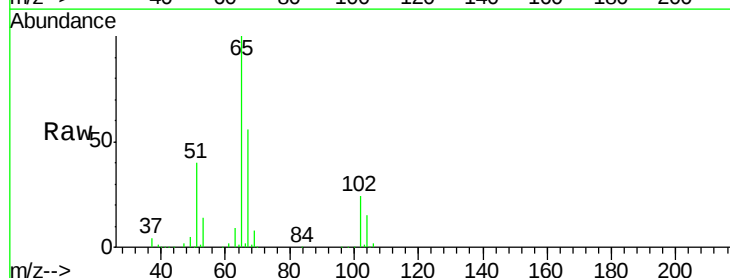

Abundance Ion 64.90 (64.60 to 65.60): VY001148.D (-1041) (-)

Ion 66.90 (66.60 to 67.60): VY001148.D (-1041) (-)

8.15

50000

40000

30000


20000


10000

0

8.10 8.20

Time-->

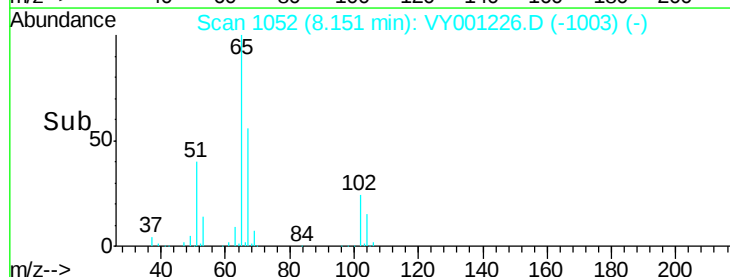


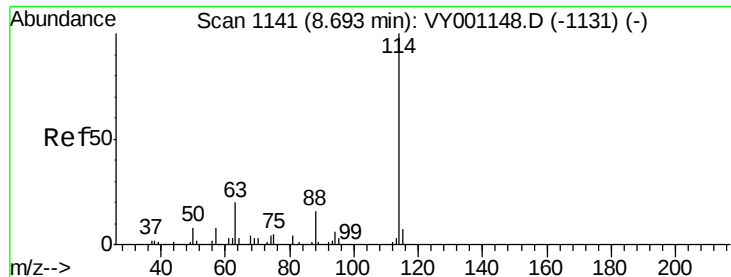




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.69 min Scan# 1141
Delta R.T. -0.00 min
Lab File: VY001226.D
Acq: 15 Jan 2020 18:15

Instrument :
MSVOA_Y
ClientSampleId :
QVD-SB-102-2-2.5

Tot Ion	Ratio	Lower	Upper
114	100		
63	18.8	0.0	40.8
88	15.8	0.0	32.4

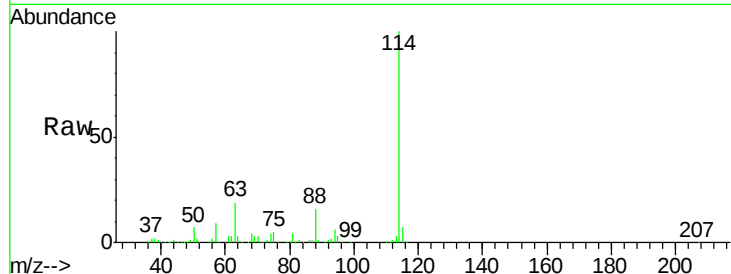


Abundance Ion 113.90 (113.60 to 114.60): V
Ion 63.00 (62.70 to 63.70): VY0
Ion 87.90 (87.60 to 88.60): VY0

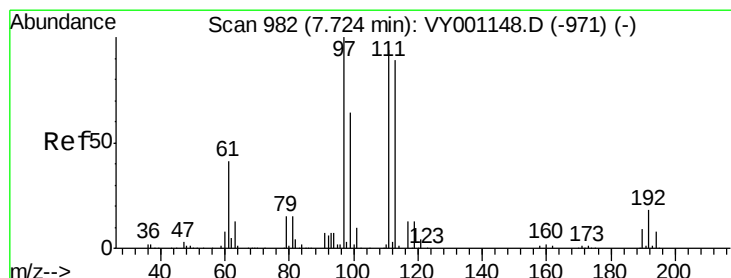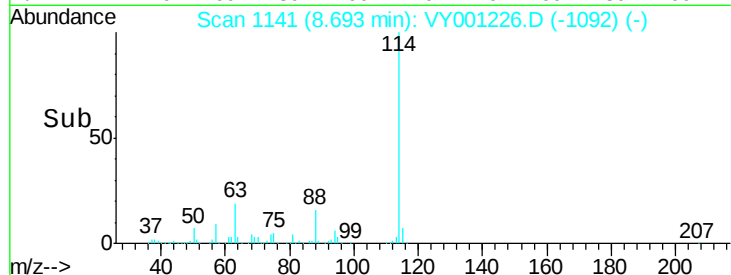
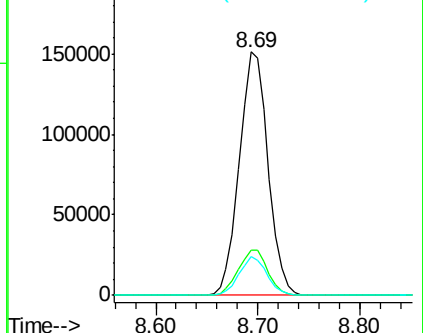



#35
Dibromofluoromethane
Concen: 50.014 ug/l
RT: 7.73 min Scan# 983
Delta R.T. 0.01 min
Lab File: VY001226.D
Acq: 15 Jan 2020 18:15

Tgt Ion	Ratio	Lower	Upper
113	100		
111	102.9	82.9	124.3
192	19.5	15.4	23.2

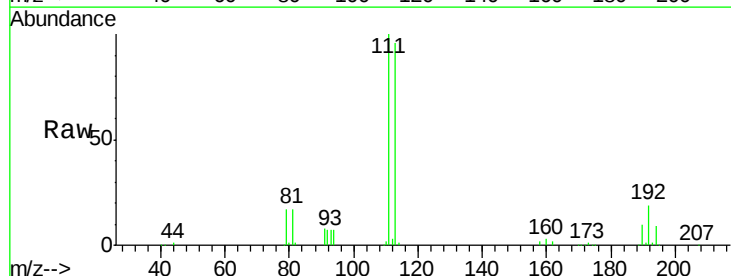

Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V

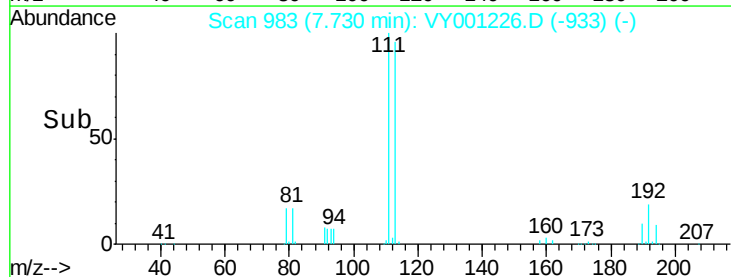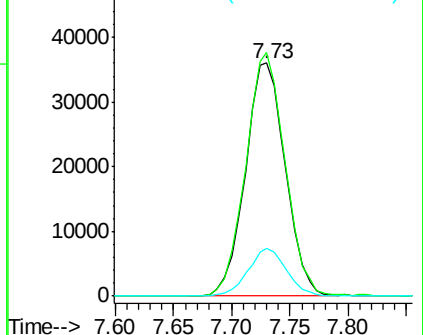

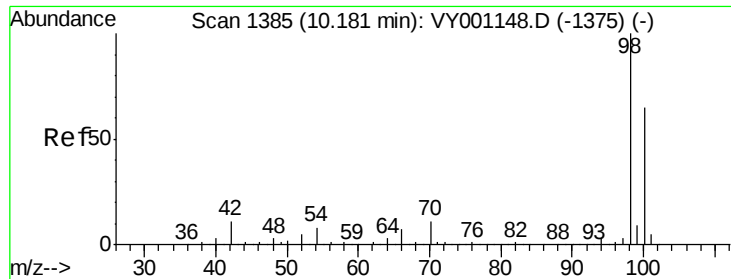

#50

Toluene-d8

Concen: 51.477 ug/l

RT: 10.18 min Scan# 1385

Delta R.T. -0.00 min

Lab File: VY001226.D

Acq: 15 Jan 2020 18:15

Instrument :

MSVOA_Y

ClientSampleId :


QVD-SB-102-2-2.5

Tot Ion: 98 Resp: 342499

Ion Ratio Lower Upper

98 100

100 66.5 53.1 79.7

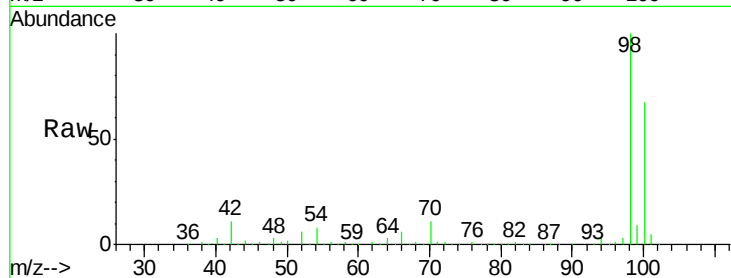

Abundance Ion 98.00 (97.70 to 98.70): VY001148.D (-1375) (-)

Ion 100.00 (99.70 to 100.70): VY001148.D (-1375) (-)

10.18

200000

150000



100000

50000

0

10.10 10.20 10.30

Time-->

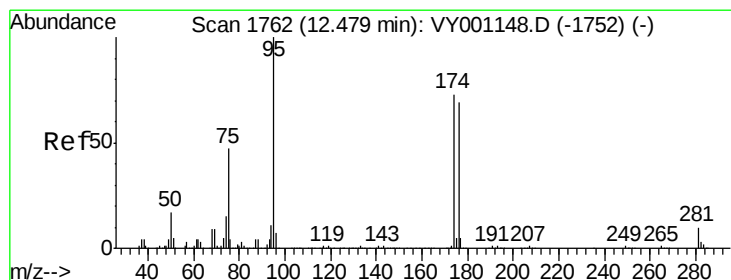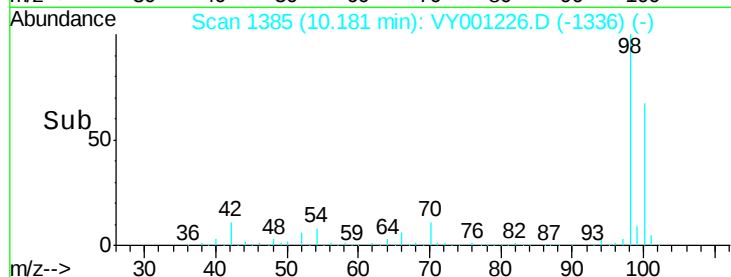

#62

4-Bromofluorobenzene

Concen: 41.757 ug/l

RT: 12.48 min Scan# 1762

Delta R.T. -0.00 min

Lab File: VY001226.D

Acq: 15 Jan 2020 18:15


Tgt Ion: 95 Resp: 113585

Ion Ratio Lower Upper

95 100

174 75.8 0.0 143.2

176 74.3 0.0 136.0

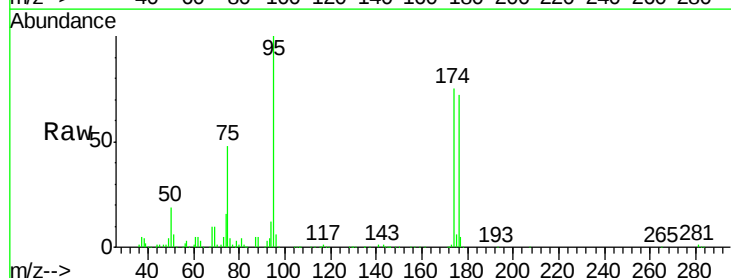

Abundance Ion 94.90 (94.60 to 95.60): VY001148.D (-1752) (-)

Ion 173.80 (173.50 to 174.50): VY001148.D (-1752) (-)

Ion 175.80 (175.50 to 176.50): VY001148.D (-1752) (-)

12.48

100000

80000

60000


40000


20000

0

12.40 12.50

Time-->

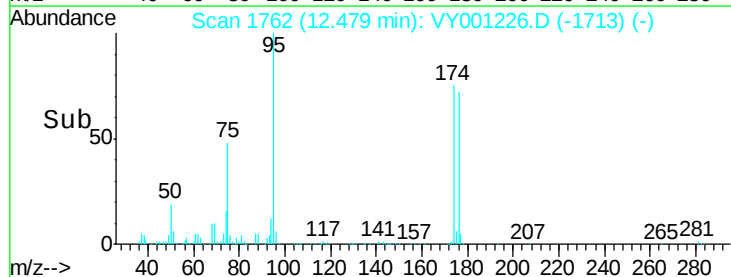


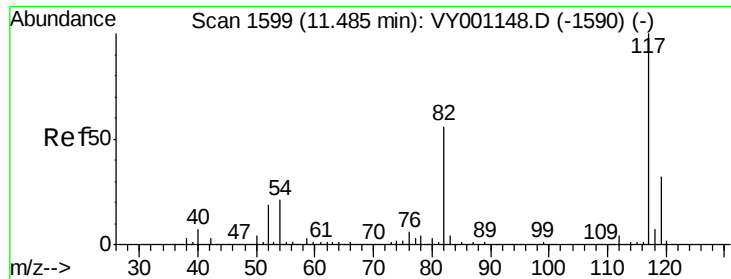




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.49 min Scan# 1600
Delta R.T. 0.01 min
Lab File: VY001226.D
Acq: 15 Jan 2020 18:15

Instrument :
MSVOA_Y
ClientSampleId :
QVD-SB-102-2-2.5

Tot Ion:117 Resp: 255302
Ion Ratio Lower Upper
117 100
82 53.9 44.9 67.3
119 32.1 25.7 38.5

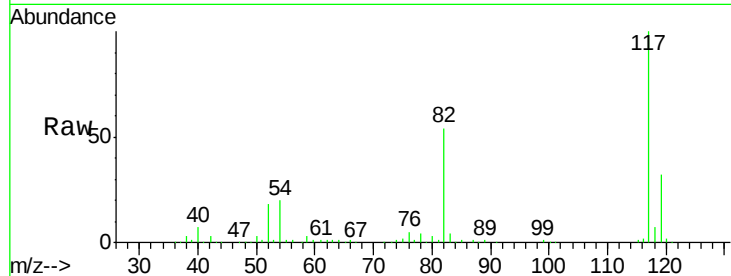


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VY0
Ion 118.90 (118.60 to 119.60): V

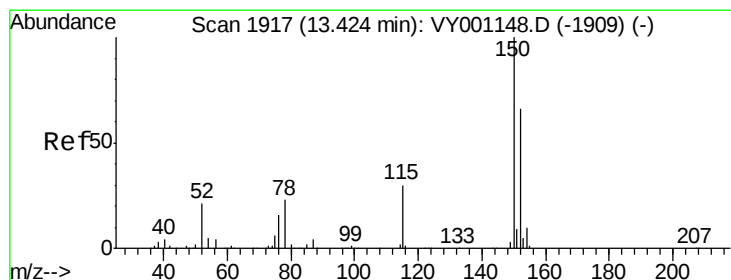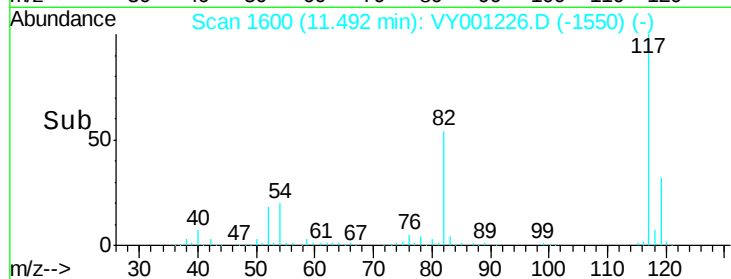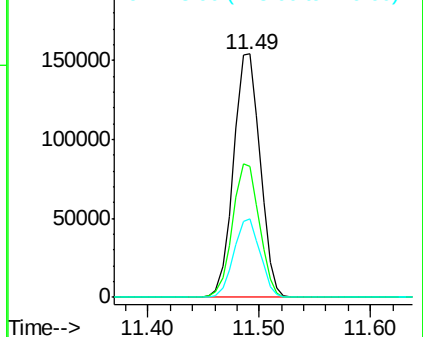

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.42 min Scan# 1917
Delta R.T. -0.00 min
Lab File: VY001226.D
Acq: 15 Jan 2020 18:15

Tgt Ion:152 Resp: 99381
Ion Ratio Lower Upper
152 100
115 57.2 30.9 92.5
150 157.4 0.0 346.8

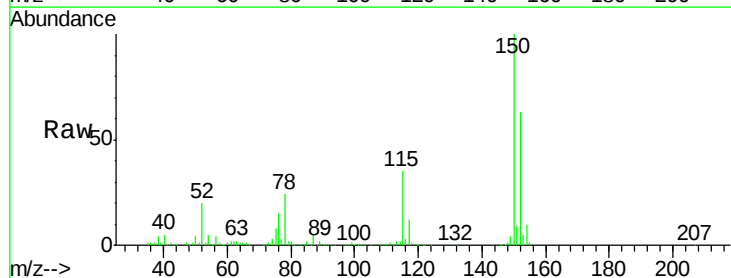

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

