


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\VY011520\
Data File : VY001234.D
Acq On : 15 Jan 2020 21:54
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA Y/SOIL
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y011020S.M
Title : SW846 8260
Last Update : Fri Jan 10 16:01:58 2020

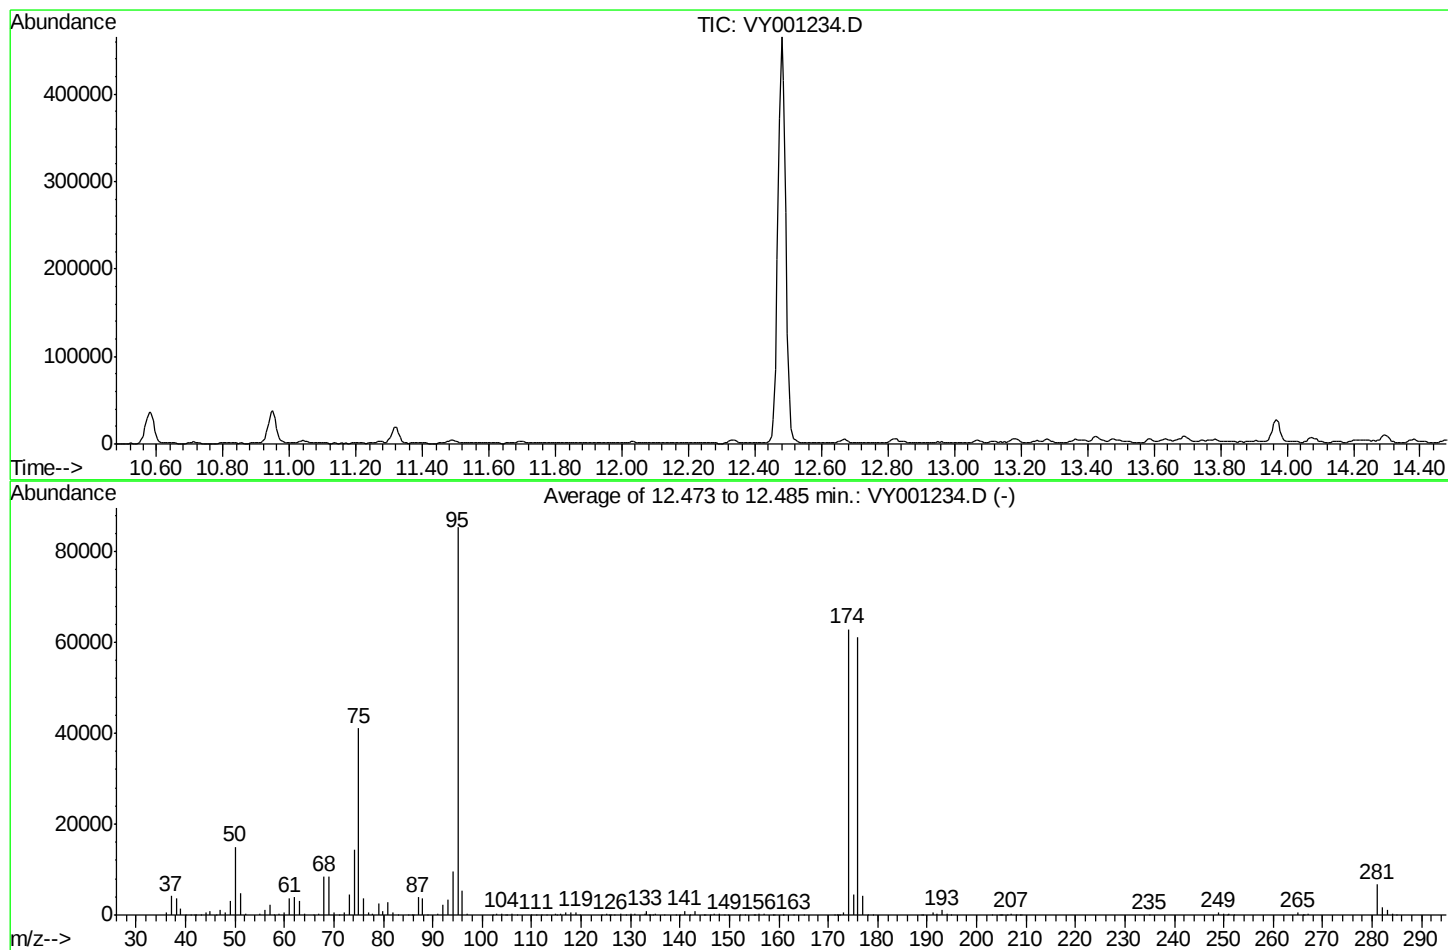

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1753

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	14982	PASS
75	95	30	60	48.2	41106	PASS
95	95	100	100	100.0	85333	PASS
96	95	5	9	6.4	5453	PASS
173	174	0.00	2	0.9	540	PASS
174	95	50	100	73.8	62936	PASS
175	174	5	9	7.3	4606	PASS
176	174	95	101	97.1	61117	PASS
177	176	5	9	6.7	4096	PASS