
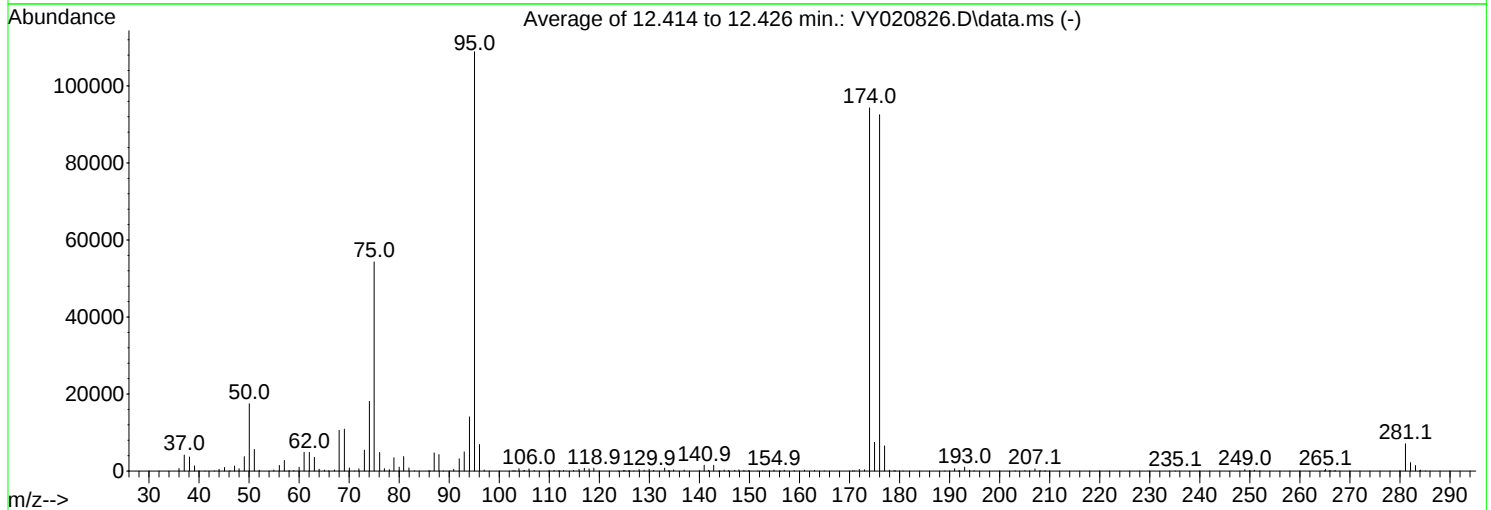


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY011525\
Data File : VY020826.D
Acq On : 15 Jan 2025 09:11
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y010625S.M
Title : SW846 8260
Last Update : Tue Jan 07 01:31:46 2025

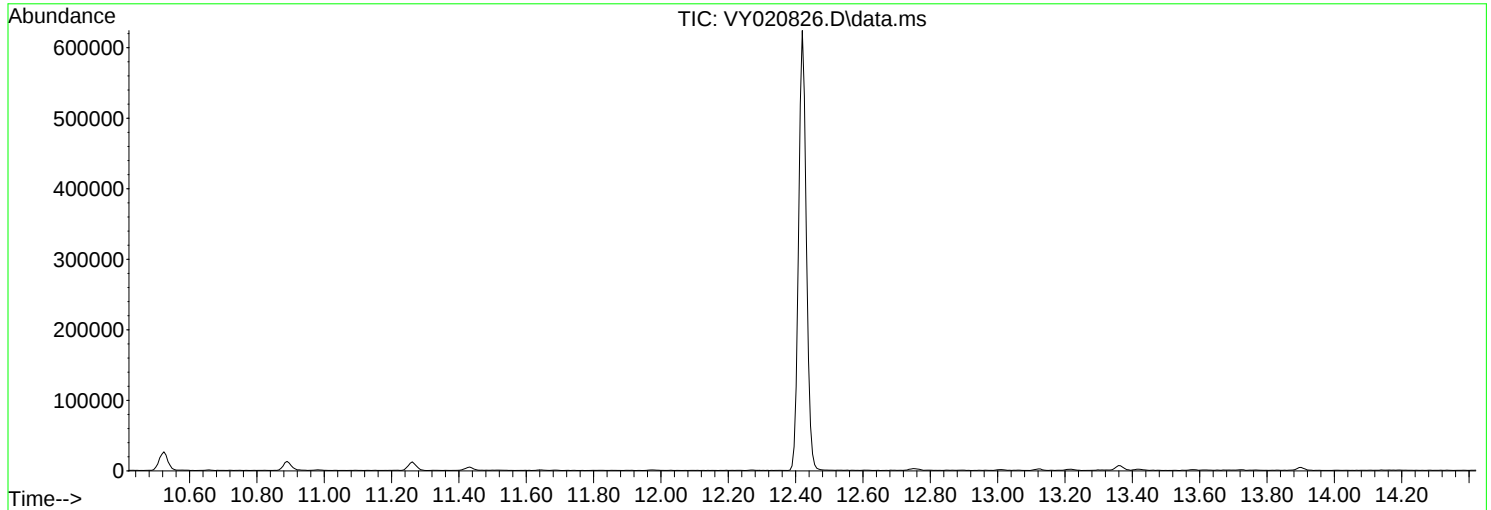

AutoFind: Scans 1754, 1755, 1756; Background Corrected with Scan 1746

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	17473	PASS
75	95	30	60	49.9	54315	PASS
95	95	100	100	100.0	108883	PASS
96	95	5	9	6.3	6894	PASS
173	174	0.00	2	0.4	351	PASS
174	95	50	100	86.6	94315	PASS
175	174	5	9	7.9	7483	PASS
176	174	95	101	98.1	92531	PASS
177	176	5	9	7.1	6550	PASS