


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\VY011720\
 Data File : VY001265.D
 Acq On : 17 Jan 2020 14:57
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA Y/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y011020S.M
 Title : SW846 8260
 Last Update : Fri Jan 10 16:01:58 2020

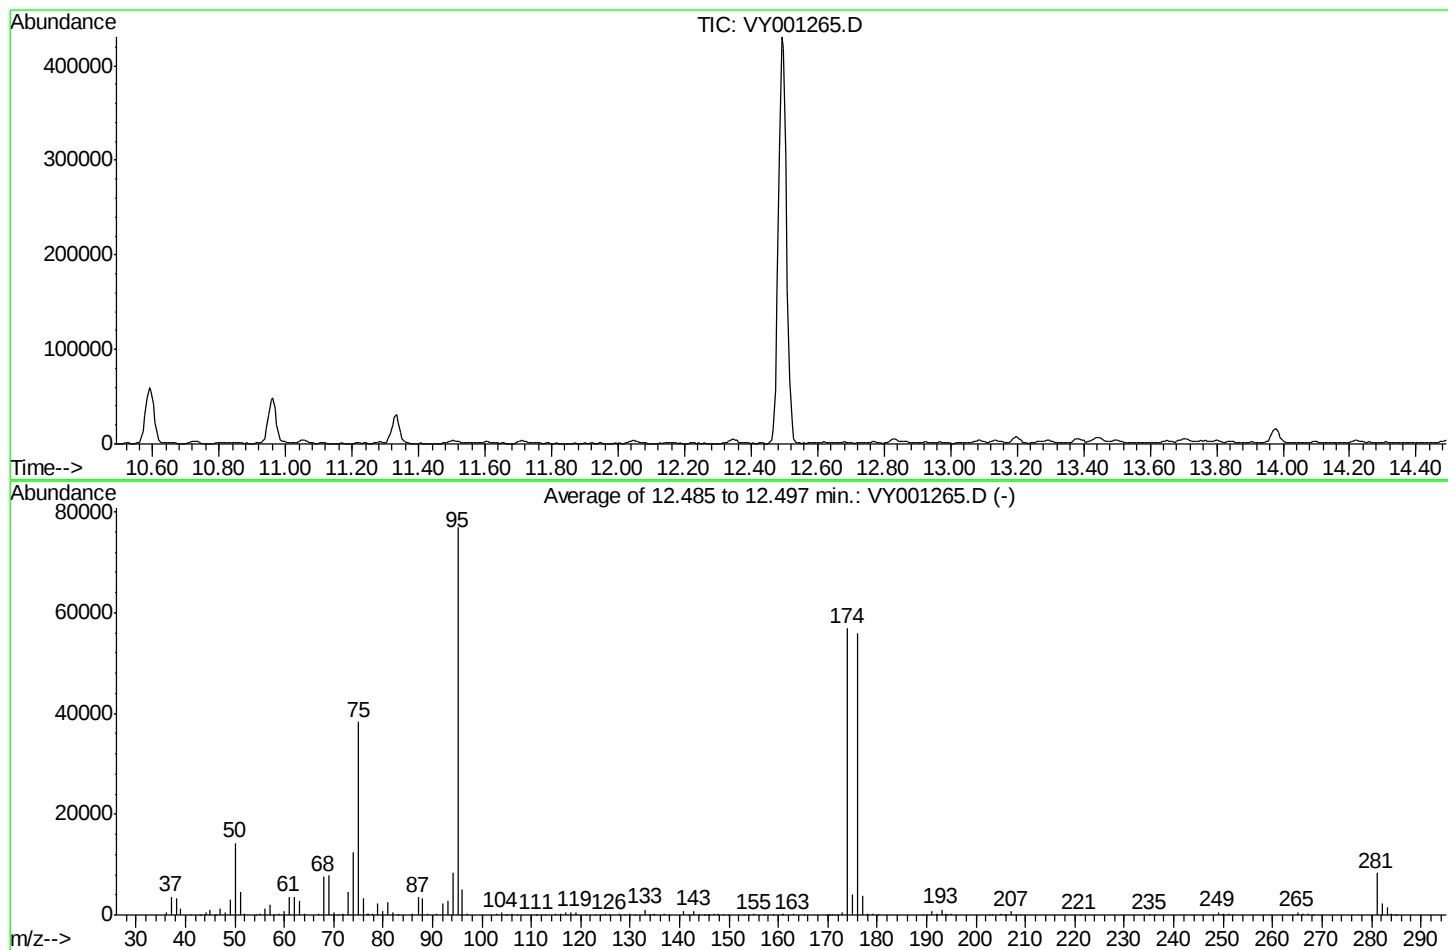

AutoFind: Scans 1763, 1764, 1765; Background Corrected with Scan 1755

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	14262	PASS
75	95	30	60	49.7	38258	PASS
95	95	100	100	100.0	76933	PASS
96	95	5	9	6.6	5060	PASS
173	174	0.00	2	0.8	480	PASS
174	95	50	100	73.9	56890	PASS
175	174	5	9	7.4	4197	PASS
176	174	95	101	98.1	55789	PASS
177	176	5	9	6.9	3870	PASS