
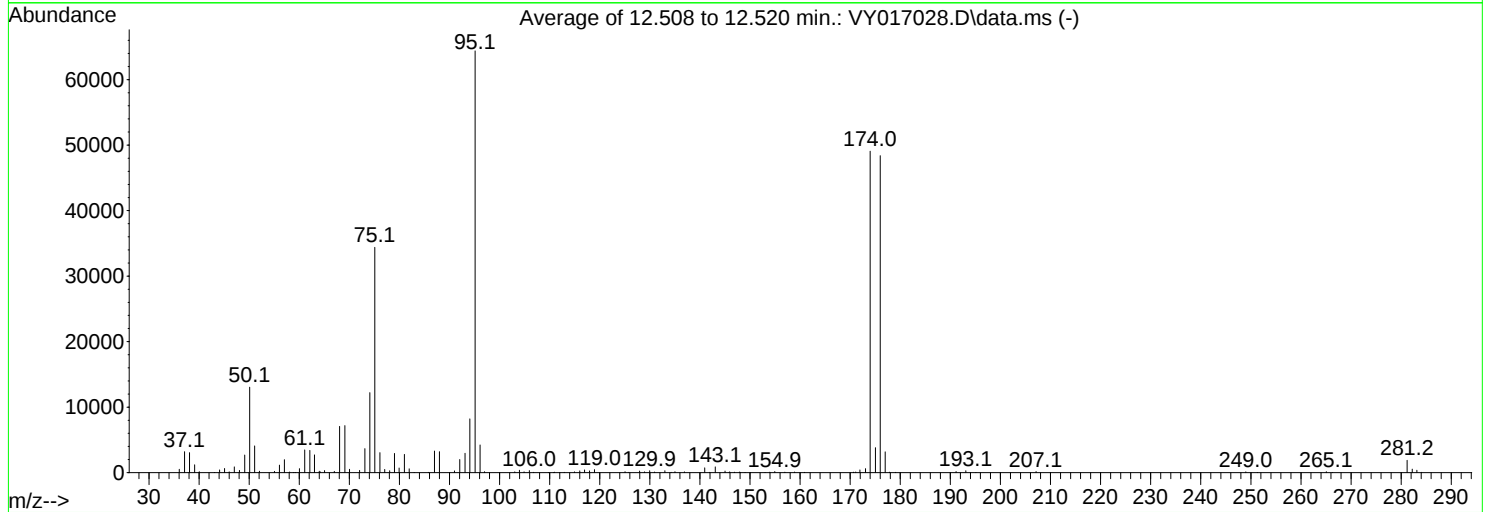


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY011824\
Data File : VY017028.D
Acq On : 18 Jan 2024 08:51
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y010224S.M
Title : SW846 8260
Last Update : Tue Jan 02 14:25:32 2024

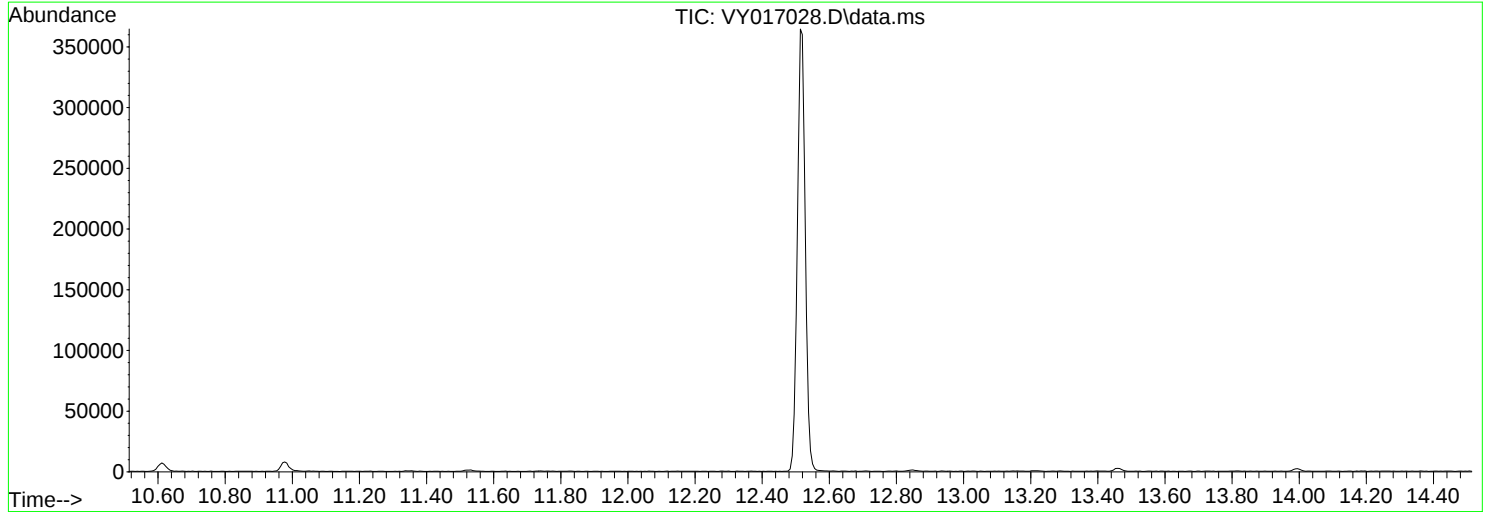

AutoFind: Scans 1753, 1754, 1755; Background Corrected with Scan 1745

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.3	13051	PASS
75	95	30	60	53.4	34405	PASS
95	95	100	100	100.0	64395	PASS
96	95	5	9	6.6	4224	PASS
173	174	0.00	2	1.2	603	PASS
174	95	50	100	76.2	49075	PASS
175	174	5	9	7.8	3807	PASS
176	174	95	101	98.6	48384	PASS
177	176	5	9	6.6	3170	PASS