

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY012020\
 Data File : VY001302.D
 Acq On : 20 Jan 2020 17:45
 Operator : SY/MD
 Sample : L1164-04
 Misc : 6.56G/5ML/MSVOA Y/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 QVD-SB-03-6-7

Quant Time: Jan 21 07:43:27 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y011020S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 21 06:54:04 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.82	168	190031	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.71	114	344530	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.50	117	294598	50.00	ug/l	-0.01
72) 1,4-Dichlorobenzene-d4	13.43	152	108020	50.00	ug/l	-0.01
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.17	65	107162	53.39	ug/l	0.00
Spiked Amount 50.000			Recovery	=	106.78%	
35) Dibromofluoromethane	7.75	113	101580	50.36	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.72%	
50) Toluene-d8	10.19	98	402997	51.85	ug/l	-0.01
Spiked Amount 50.000			Recovery	=	103.70%	
62) 4-Bromofluorobenzene	12.49	95	129659	40.80	ug/l	-0.01
Spiked Amount 50.000			Recovery	=	81.60%	
Target Compounds						
16) Acetone	3.98	43	8334	17.879	ug/l	95
68) m/p-Xylenes	11.70	106	11616	2.860	ug/l	100
69) o-Xylene	12.03	106	7501	1.926	ug/l	100
80) 1,3,5-Trimethylbenzene	12.82	105	7762	1.146	ug/l	99
84) 1,2,4-Trimethylbenzene	13.13	105	25314	3.762	ug/l	100
95) Naphthalene	15.25	128	14524	3.002	ug/l	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY012020\
Data File : VY001302.D
Acq On : 20 Jan 2020 17:45
Operator : SY/MD
Sample : L1164-04
Misc : 6.56G/5ML/MSVOA Y/SOIL
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
QVD-SB-03-6-7

Quant Time: Jan 21 07:43:27 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y011020S.M
Quant Title : SW846 8260
QLast Update : Tue Jan 21 06:54:04 2020
Response via : Initial Calibration

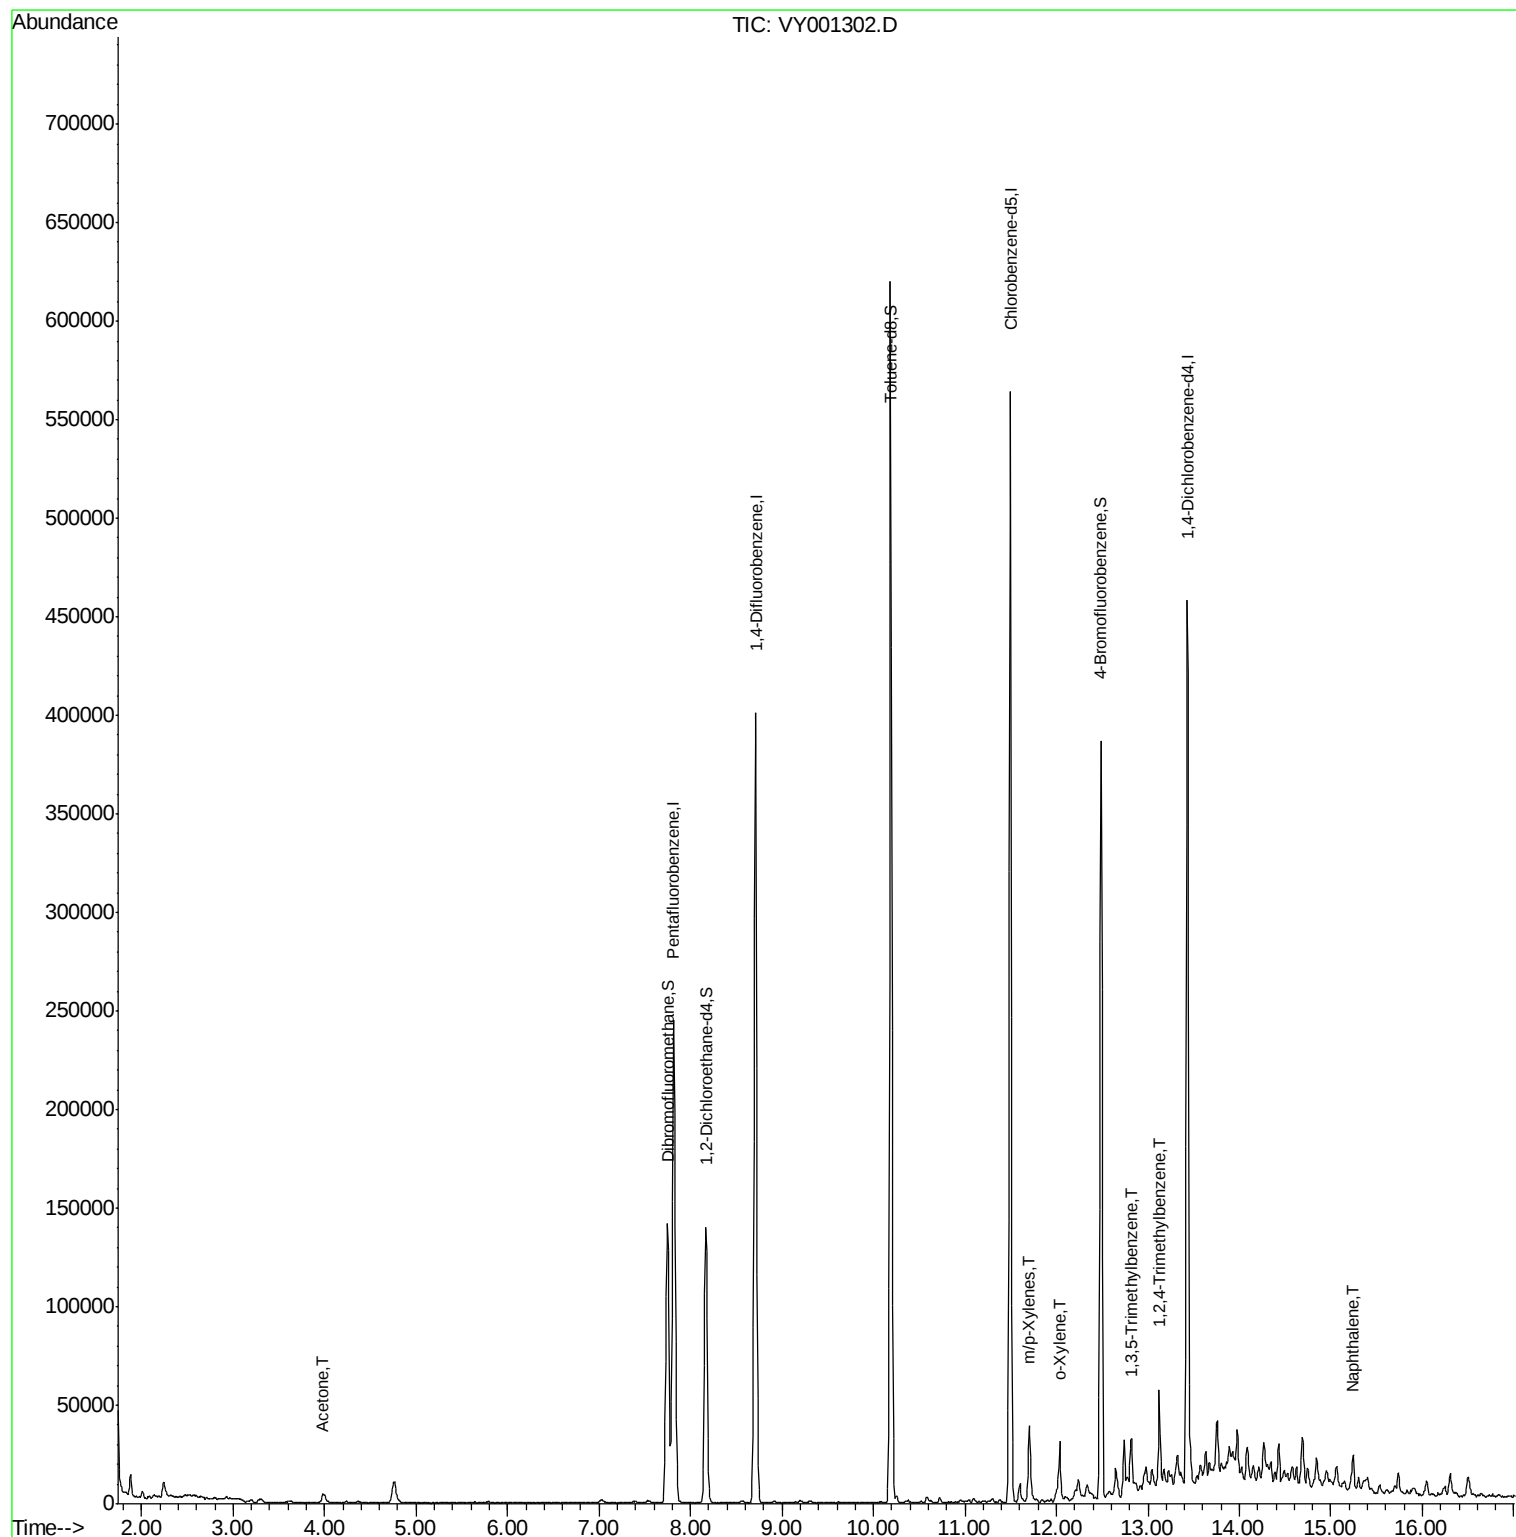

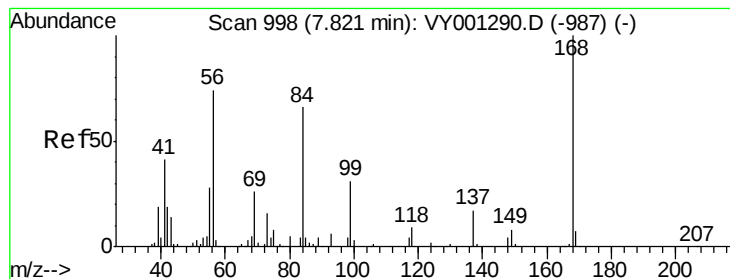

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.82 min Scan# 998

Delta R.T. 0.00 min

Lab File: VY001302.D

Acq: 20 Jan 2020 17:45

Instrument :

MSVOA_Y

ClientSampleId :


QVD-SB-03-6-7

Tot Ion:168 Resp: 190031




Ion Ratio Lower Upper

168 100

99 53.8 47.9 71.9

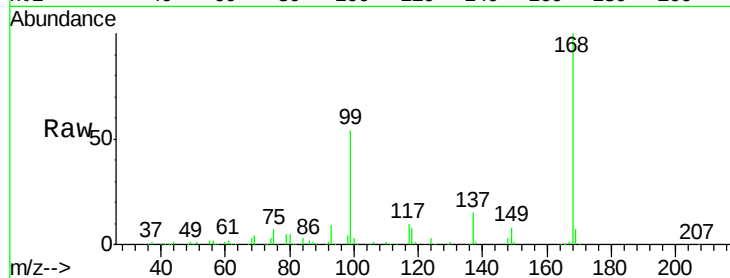

Abundance Ion 167.90 (167.60 to 168.60): VY001302.D (-949) (-)

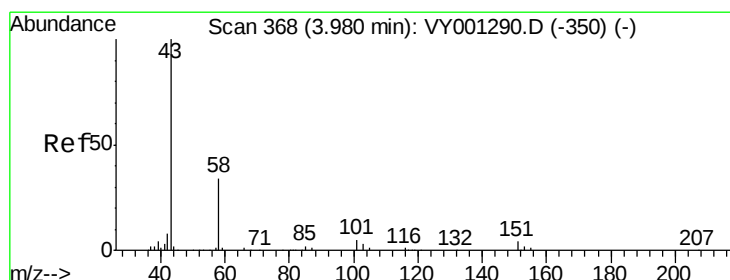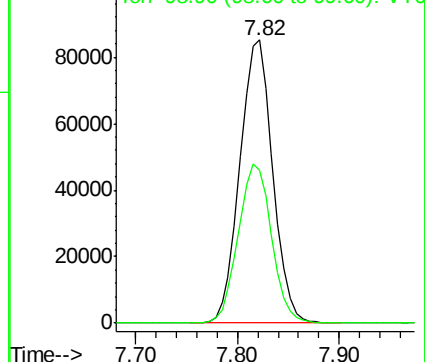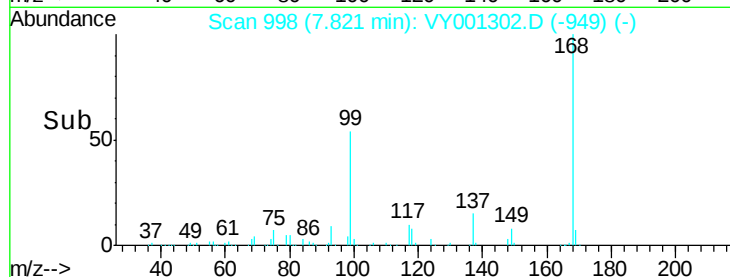

#16

Acetone

Concen: 17.879 ug/l

RT: 3.98 min Scan# 368

Delta R.T. 0.00 min

Lab File: VY001302.D


Acq: 20 Jan 2020 17:45

Tgt Ion: 43 Resp: 8334



Ion Ratio Lower Upper


43 100

58 34.9 25.8 38.6

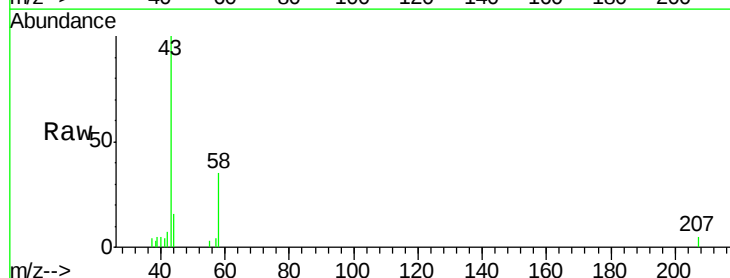

Abundance Ion 43.00 (42.70 to 43.70): VY001302.D (-319) (-)



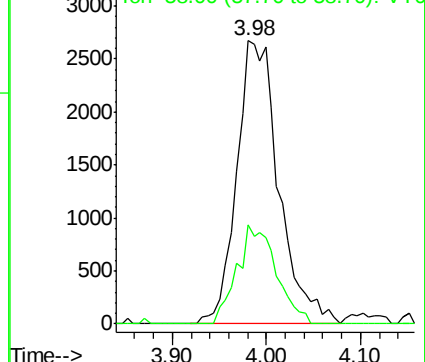
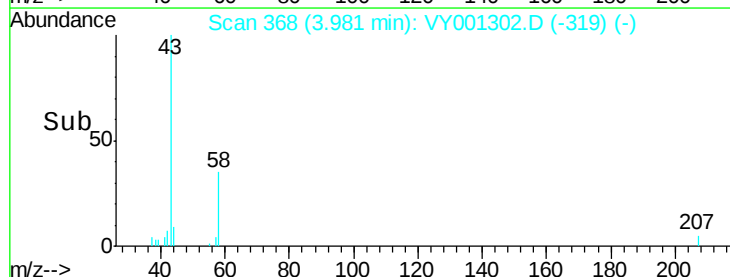




#33
 1,2-Dichloroethane-d4
 Concen: 53.393 ug/l
 RT: 8.17 min Scan# 1055
 Delta R.T. -0.01 min
 Lab File: VY001302.D
 Acq: 20 Jan 2020 17:45




Instrument :
 MSVOA_Y
 ClientSampleId :
 QVD-SB-03-6-7


Tot Ion: 65 Resp: 107162
 Ion Ratio Lower Upper
 65 100
 67 54.0 0.0 105.2

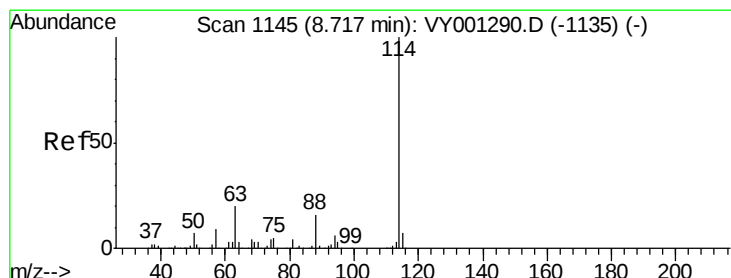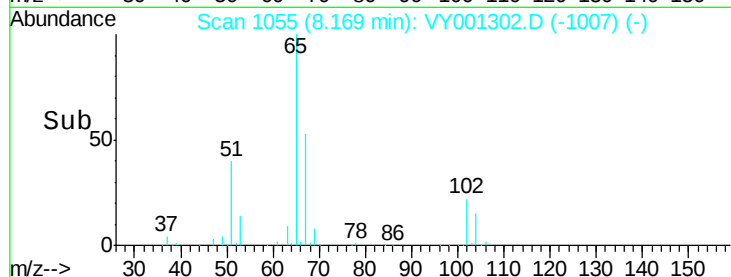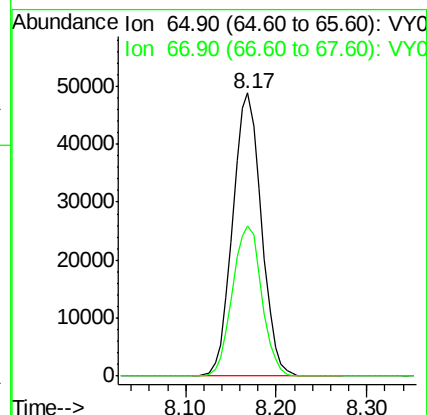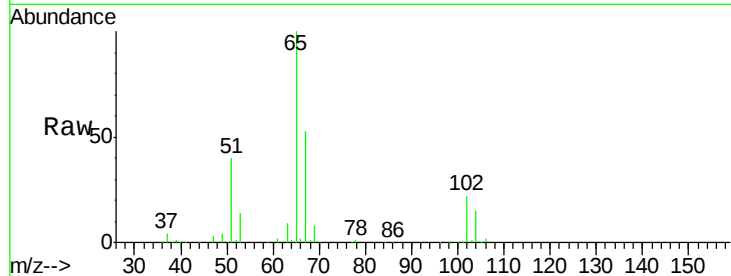

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.71 min Scan# 1144
 Delta R.T. -0.01 min
 Lab File: VY001302.D
 Acq: 20 Jan 2020 17:45

Tgt Ion: 114 Resp: 344530
 Ion Ratio Lower Upper
 114 100
 63 20.2 0.0 40.8
 88 15.8 0.0 32.4

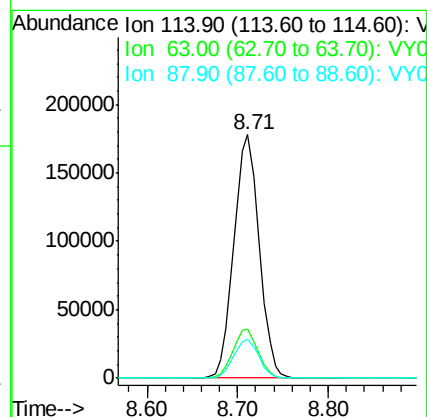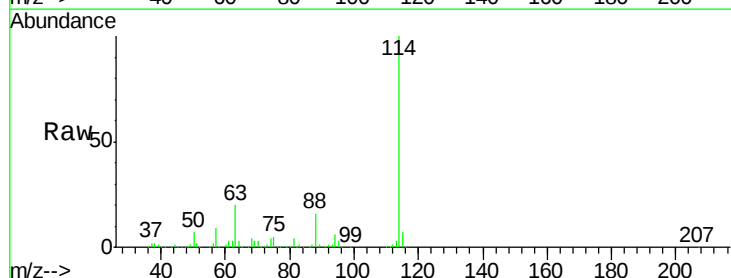







#35
Dibromofluoromethane
Concen: 50.356 ug/l
RT: 7.75 min Scan# 986
Delta R.T. -0.01 min
Lab File: VY001302.D
Acq: 20 Jan 2020 17:45

Instrument :
MSVOA_Y
ClientSampleId :
QVD-SB-03-6-7

Tot Ion	Ratio	Lower	Upper
113	100		
111	101.7	82.9	124.3
192	19.4	15.4	23.2

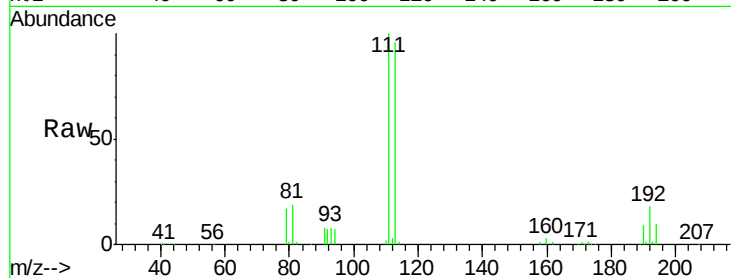


Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V

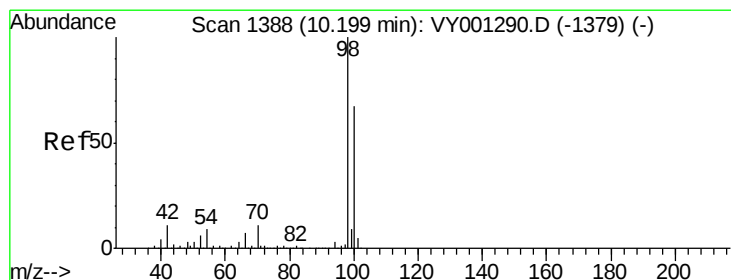
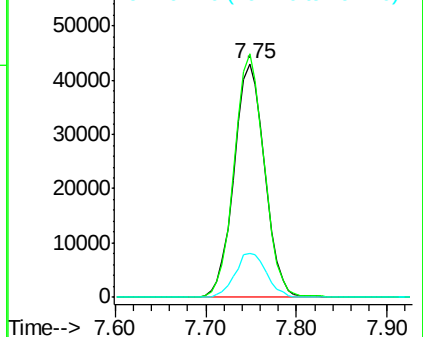



#50
Toluene-d8
Concen: 51.848 ug/l
RT: 10.19 min Scan# 1386
Delta R.T. -0.01 min
Lab File: VY001302.D
Acq: 20 Jan 2020 17:45

Tgt Ion	Ratio	Lower	Upper
98	100		
100	66.3	53.1	79.7

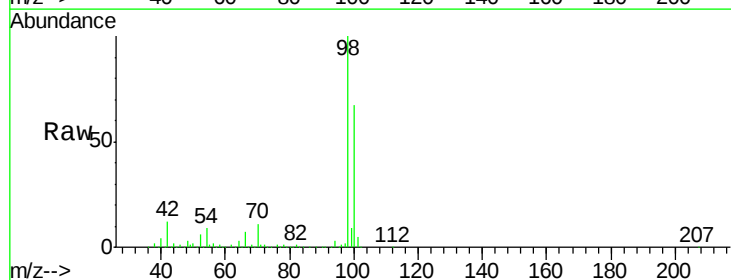

Abundance Ion 98.00 (97.70 to 98.70): VY0
Ion 100.00 (99.70 to 100.70): VY




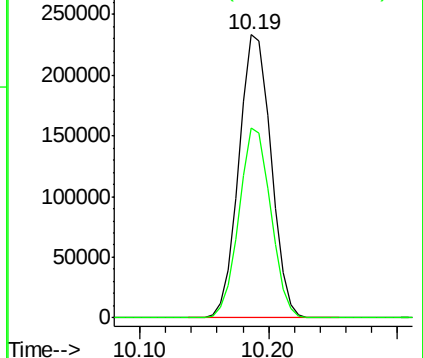




#62
4-Bromofluorobenzene
Concen: 40.803 ug/l
RT: 12.49 min Scan# 1763
Delta R.T. -0.01 min
Lab File: VY001302.D
Acq: 20 Jan 2020 17:45




Instrument :
MSVOA_Y
ClientSampleId :
QVD-SB-03-6-7


Tot Ion	95	Resp	129659
Ion Ratio	Lower	Upper	
95	100		
174	74.8	0.0	143.2
176	71.5	0.0	136.0

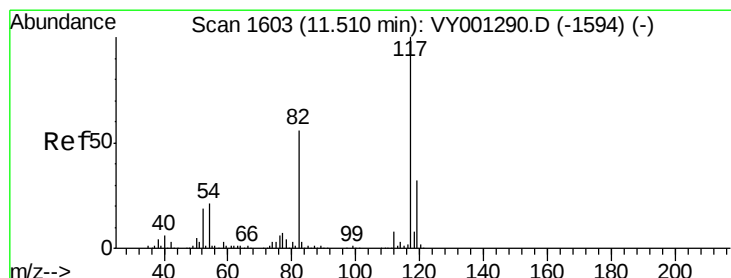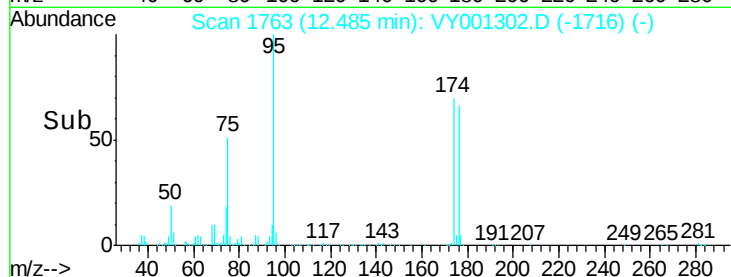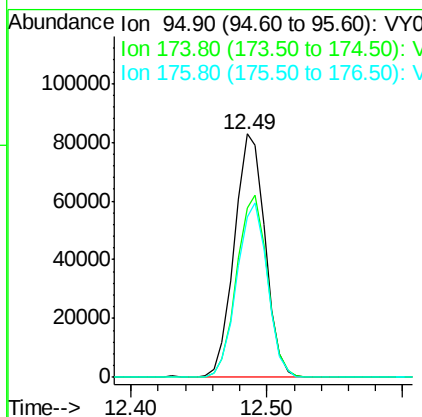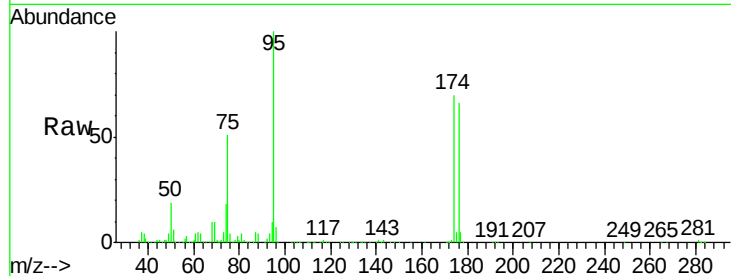

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.50 min Scan# 1601
Delta R.T. -0.01 min
Lab File: VY001302.D
Acq: 20 Jan 2020 17:45

Tgt Ion	117	Resp	294598
Ion Ratio	Lower	Upper	
117	100		
82	55.3	44.9	67.3
119	32.6	25.7	38.5


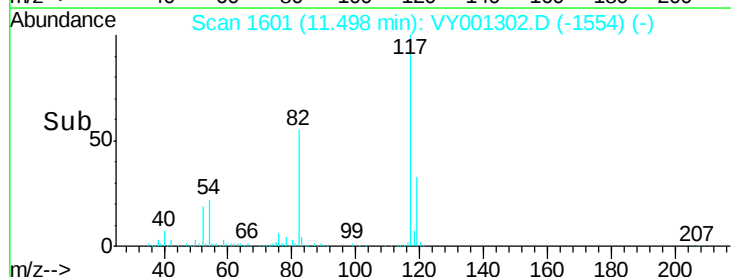
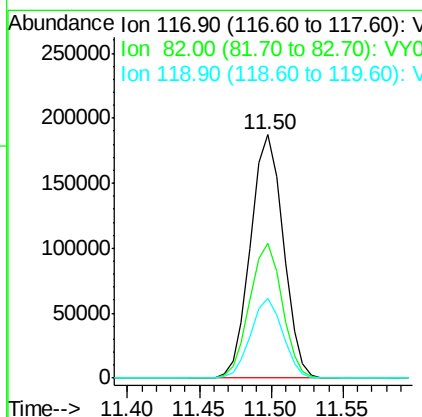
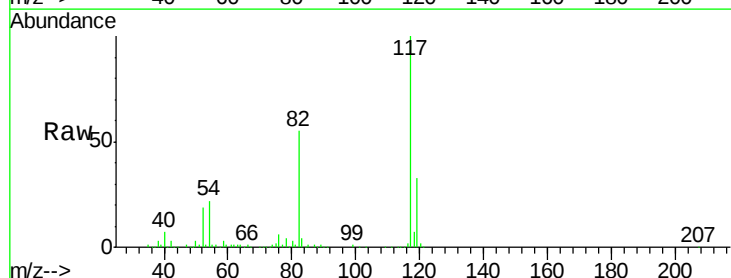




#68
m/p-Xylenes
Concen: 2.860 ug/l
RT: 11.70 min Scan# 1635
Delta R.T. -0.01 min
Lab File: VY001302.D
Acq: 20 Jan 2020 17:45




Instrument :
MSVOA_Y
ClientSampleId :
QVD-SB-03-6-7


Tot Ion:106 Resp: 11616
Ion Ratio Lower Upper
106 100
91 201.4 161.4 242.2

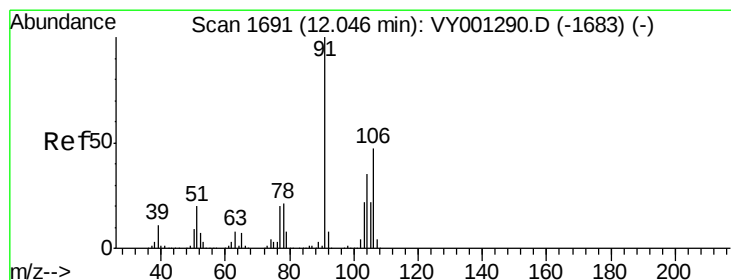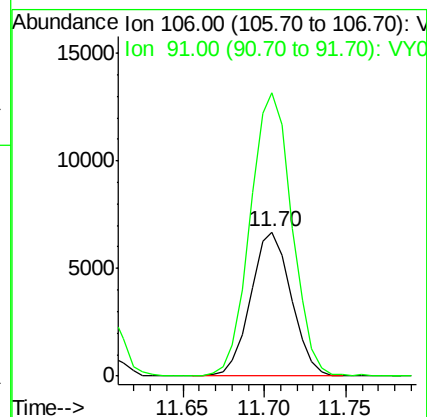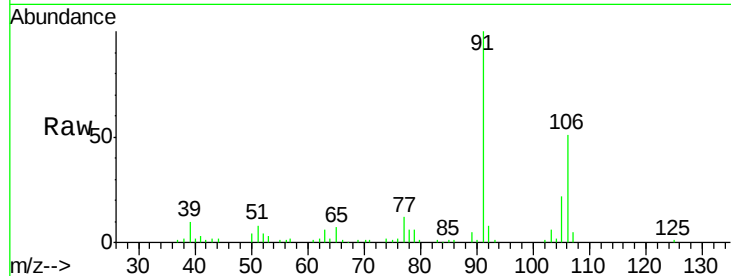

#69
o-Xylene
Concen: 1.926 ug/l
RT: 12.03 min Scan# 1689
Delta R.T. -0.01 min
Lab File: VY001302.D
Acq: 20 Jan 2020 17:45

Tgt Ion:106 Resp: 7501
Ion Ratio Lower Upper
106 100
91 212.9 106.3 318.8

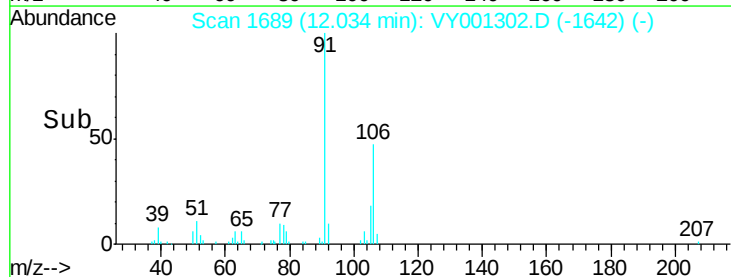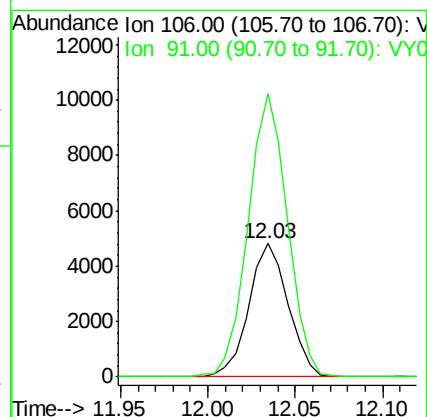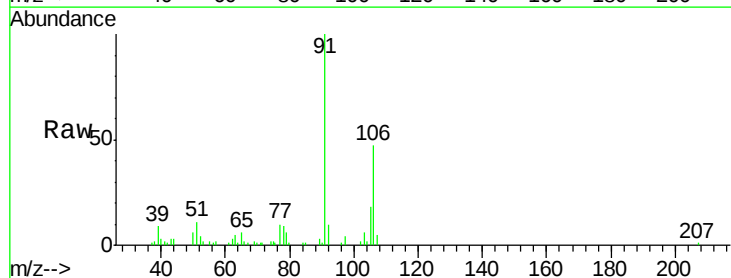

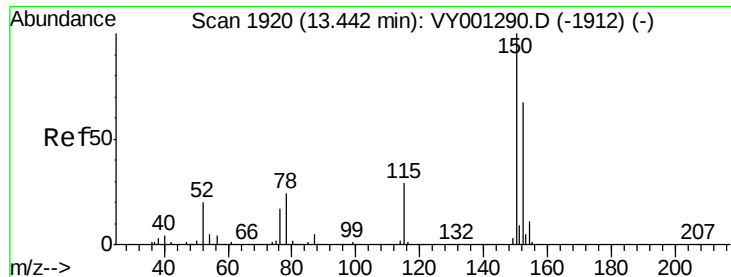

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.43 min Scan# 1918

Delta R.T. -0.01 min

Lab File: VY001302.D

Acq: 20 Jan 2020 17:45

Instrument :

MSVOA_Y

ClientSampleId :

QVD-SB-03-6-7


Tot Ion:152 Resp: 108020

Ion Ratio Lower Upper

152 100

115 61.3 30.9 92.5




150 160.2 0.0 346.8

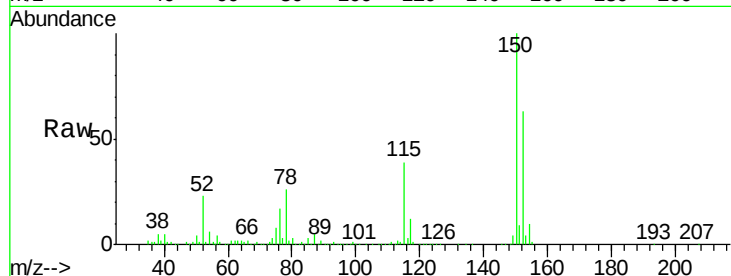

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

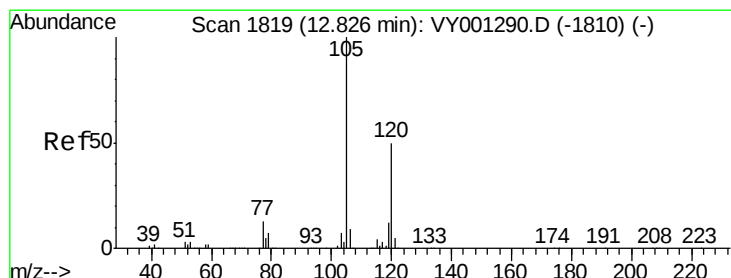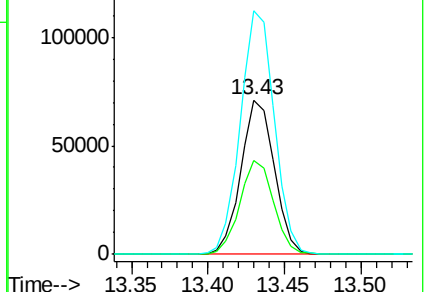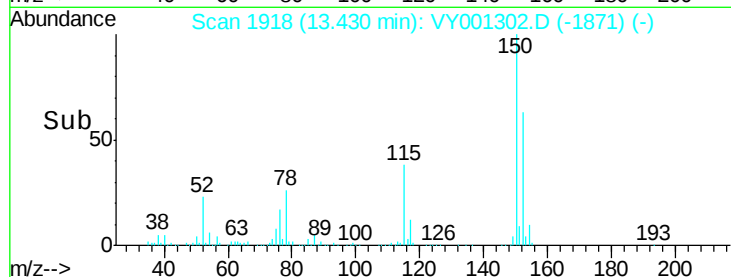

#80

1,3,5-Trimethylbenzene

Concen: 1.146 ug/l

RT: 12.82 min Scan# 1818

Delta R.T. -0.01 min

Lab File: VY001302.D


Acq: 20 Jan 2020 17:45

Tgt Ion:105 Resp: 7762

Ion Ratio Lower Upper



105 100


120 49.2 24.2 72.6

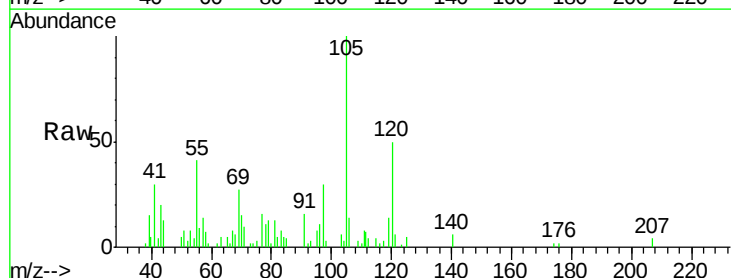

Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

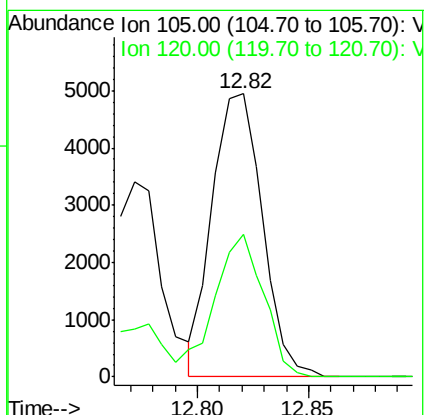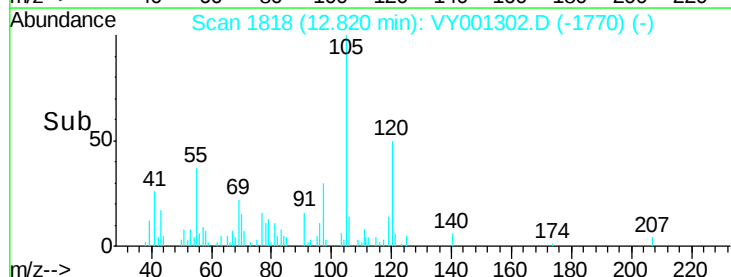



#84

1,2,4-Trimethylbenzene

Concen: 3.762 ug/l

RT: 13.13 min Scan# 1868

Delta R.T. -0.01 min

Lab File: VY001302.D

Acq: 20 Jan 2020 17:45

Instrument :

MSVOA_Y

ClientSampleId :





QVD-SB-03-6-7

Tot Ion:105 Resp: 25314

Ion Ratio Lower Upper

105 100

120 45.8 22.8 68.3

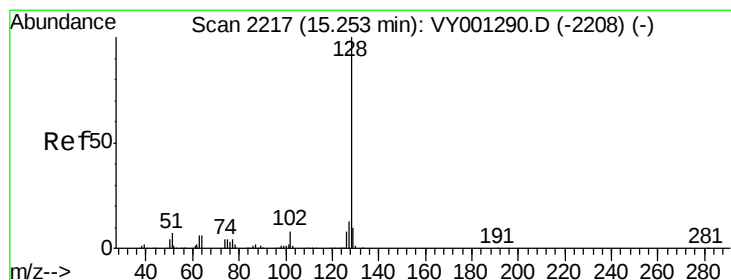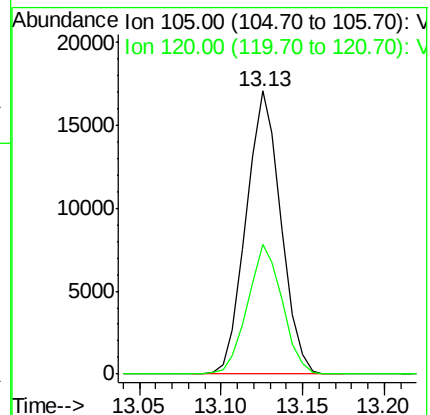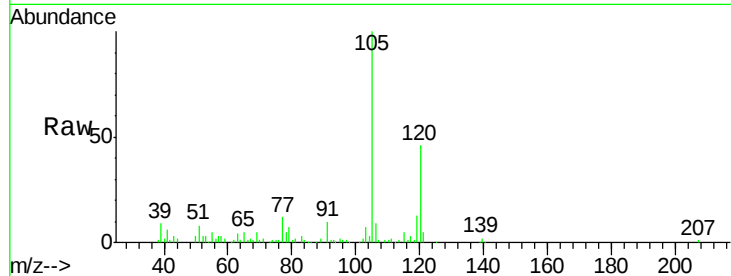

#95

Naphthalene

Concen: 3.002 ug/l

RT: 15.25 min Scan# 2216

Delta R.T. -0.01 min

Lab File: VY001302.D

Acq: 20 Jan 2020 17:45

Tgt Ion:128 Resp: 14524

Ion Ratio Lower Upper

128 100

127 13.8 10.2 15.4

129 12.4 8.5 12.7

