

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY012023\
 Data File : VY012304.D
 Acq On : 20 Jan 2023 20:30
 Operator : KP/MD
 Sample : 01237-02
 Misc : 5.06g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 3A

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y011623S.M

Title : SW846 8260

Signal : TIC: VY012304.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.479	106	108	111	rBV2	244	370	7.10%	1.058%
2	2.747	149	152	155	rBV	246	262	5.03%	0.749%
3	2.839	164	167	168	rBV	183	179	3.44%	0.512%
4	3.015	193	196	201	rBV	184	286	5.49%	0.818%
5	3.326	243	247	249	rBV2	232	274	5.26%	0.784%
6	4.107	372	375	376	rBV	115	145	2.78%	0.415%
7	4.302	405	407	408	rVB	200	135	2.59%	0.386%
8	4.332	408	412	413	rBV	165	170	3.26%	0.486%
9	4.540	444	446	449	rVB	143	153	2.94%	0.438%
10	4.655	462	465	466	rBV	202	167	3.20%	0.478%
11	4.716	471	475	479	rVB2	251	326	6.26%	0.932%
12	4.820	489	492	495	rBV	171	173	3.32%	0.495%
13	4.972	515	517	520	rVB2	145	175	3.36%	0.500%
14	5.509	602	605	608	rBV	141	175	3.36%	0.500%
15	5.631	622	625	629	rVB	134	137	2.63%	0.392%
16	6.192	713	717	720	rVB	139	194	3.72%	0.555%
17	6.509	766	769	770	rVB	174	164	3.15%	0.469%
18	6.527	770	772	776	rBV2	172	240	4.61%	0.686%
19	6.966	842	844	851	rVB2	410	763	14.64%	2.182%
20	7.289	896	897	900	rBV	215	283	5.43%	0.809%
21	7.466	924	926	930	rVB	161	233	4.47%	0.666%
22	7.716	963	967	974	rVB2	455	855	16.41%	2.445%
23	7.789	974	979	982	rBV2	921	1667	31.99%	4.767%
24	7.856	988	990	992	rVB	199	133	2.55%	0.380%
25	7.905	996	998	1001	rBV	204	270	5.18%	0.772%
26	8.057	1021	1023	1024	rBV2	173	144	2.76%	0.412%
27	8.143	1031	1037	1043	rBV3	1011	2224	42.68%	6.360%
28	8.222	1046	1050	1053	rBV	143	161	3.09%	0.460%
29	8.600	1110	1112	1116	rBV	156	195	3.74%	0.558%
30	8.691	1121	1127	1133	rVB	1763	3185	61.12%	9.109%
31	9.051	1183	1186	1187	rBV	148	146	2.80%	0.418%
32	9.209	1209	1212	1215	rBV	170	180	3.45%	0.515%
33	9.429	1245	1248	1251	rVB	120	156	2.99%	0.446%
34	9.606	1275	1277	1280	rBV	172	165	3.17%	0.472%
35	9.715	1293	1295	1299	rVB	135	145	2.78%	0.415%
36	10.179	1367	1371	1378	rVB	3288	5211	100.00%	14.903%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY012023\
 Data File : VY012304.D
 Acq On : 20 Jan 2023 20:30
 Operator : KP/MD
 Sample : 01237-02
 Misc : 5.06g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 3A

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y011623S.M
 Title : SW846 8260

37	10.289	1387	1389	1391	rVB	281	165	3.17%	0.472%
38	10.386	1403	1405	1407	rBV	160	160	3.07%	0.458%
39	10.575	1432	1436	1438	rBV2	277	408	7.83%	1.167%
40	10.776	1464	1469	1470	rBV2	143	239	4.59%	0.684%
41	10.849	1478	1481	1483	rVB	113	153	2.94%	0.438%
42	10.880	1484	1486	1489	rVV	151	161	3.09%	0.460%
43	10.953	1493	1498	1502	rVV3	406	643	12.34%	1.839%
44	11.014	1506	1508	1511	rVV	164	212	4.07%	0.606%
45	11.081	1515	1519	1521	rVB3	180	184	3.53%	0.526%
46	11.179	1531	1535	1536	rBV	126	144	2.76%	0.412%
47	11.362	1561	1565	1569	rBV2	160	337	6.47%	0.964%
48	11.496	1581	1587	1592	rBV	3021	5042	96.76%	14.419%
49	11.611	1605	1606	1608	rBV	182	164	3.15%	0.469%
50	11.874	1647	1649	1651	rBV	215	161	3.09%	0.460%
51	11.910	1653	1655	1658	rVV	201	170	3.26%	0.486%
52	11.959	1661	1663	1665	rBV2	137	147	2.82%	0.420%
53	12.252	1709	1711	1713	rBV	222	203	3.90%	0.581%
54	12.331	1722	1724	1726	rBV2	216	184	3.53%	0.526%
55	12.392	1732	1734	1737	rBV2	194	217	4.16%	0.621%
56	12.483	1745	1749	1755	rVB4	1475	2652	50.89%	7.584%
57	12.752	1791	1793	1795	rBV2	194	170	3.26%	0.486%
58	13.111	1849	1852	1853	rBV2	190	214	4.11%	0.612%
59	13.428	1900	1904	1909	rBV5	1375	1954	37.50%	5.588%
60	13.642	1937	1939	1942	rBV2	175	159	3.05%	0.455%
61	14.129	2017	2019	2021	rBV2	177	202	3.88%	0.578%
62	14.885	2141	2143	2146	rVB3	322	274	5.26%	0.784%
63	15.080	2173	2175	2178	rVB2	500	407	7.81%	1.164%


Sum of corrected areas: 34967

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY012023\
Data File : VY012304.D
Acq On : 20 Jan 2023 20:30
Operator : KP/MD
Sample : 01237-02
Misc : 5.06g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
3A

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y011623S.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

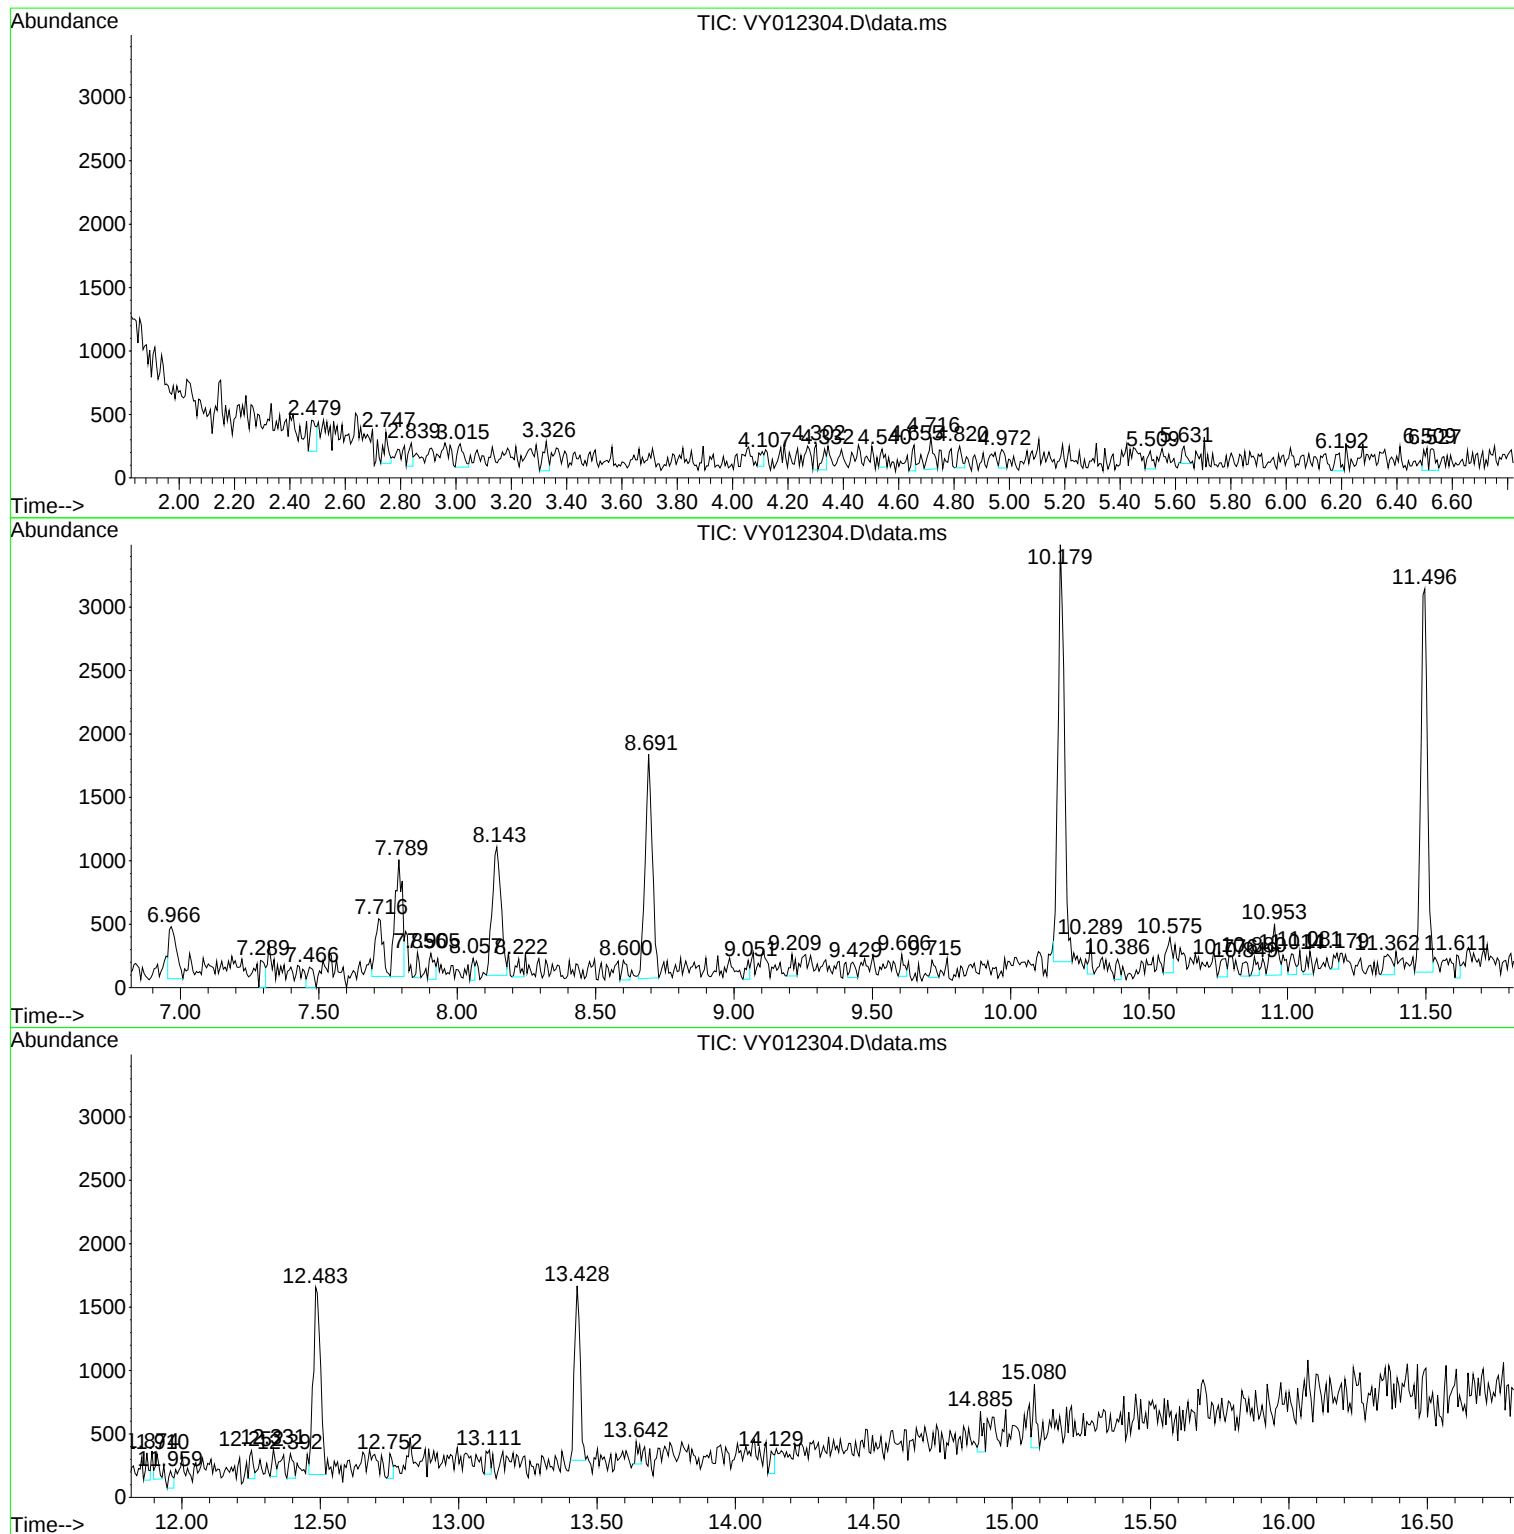

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY012023\
Data File : VY012304.D
Acq On : 20 Jan 2023 20:30
Operator : KP/MD
Sample : 01237-02
Misc : 5.06g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
3A

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y011623S.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY012023\
Data File : VY012304.D
Acq On : 20 Jan 2023 20:30
Operator : KP/MD
Sample : 01237-02
Misc : 5.06g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
3A

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y011623S.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------