


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\VY012120\
 Data File : VY001318.D
 Acq On : 21 Jan 2020 12:21
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y012120S.M
 Title : SW846 8260
 Last Update : Tue Jan 21 16:48:50 2020

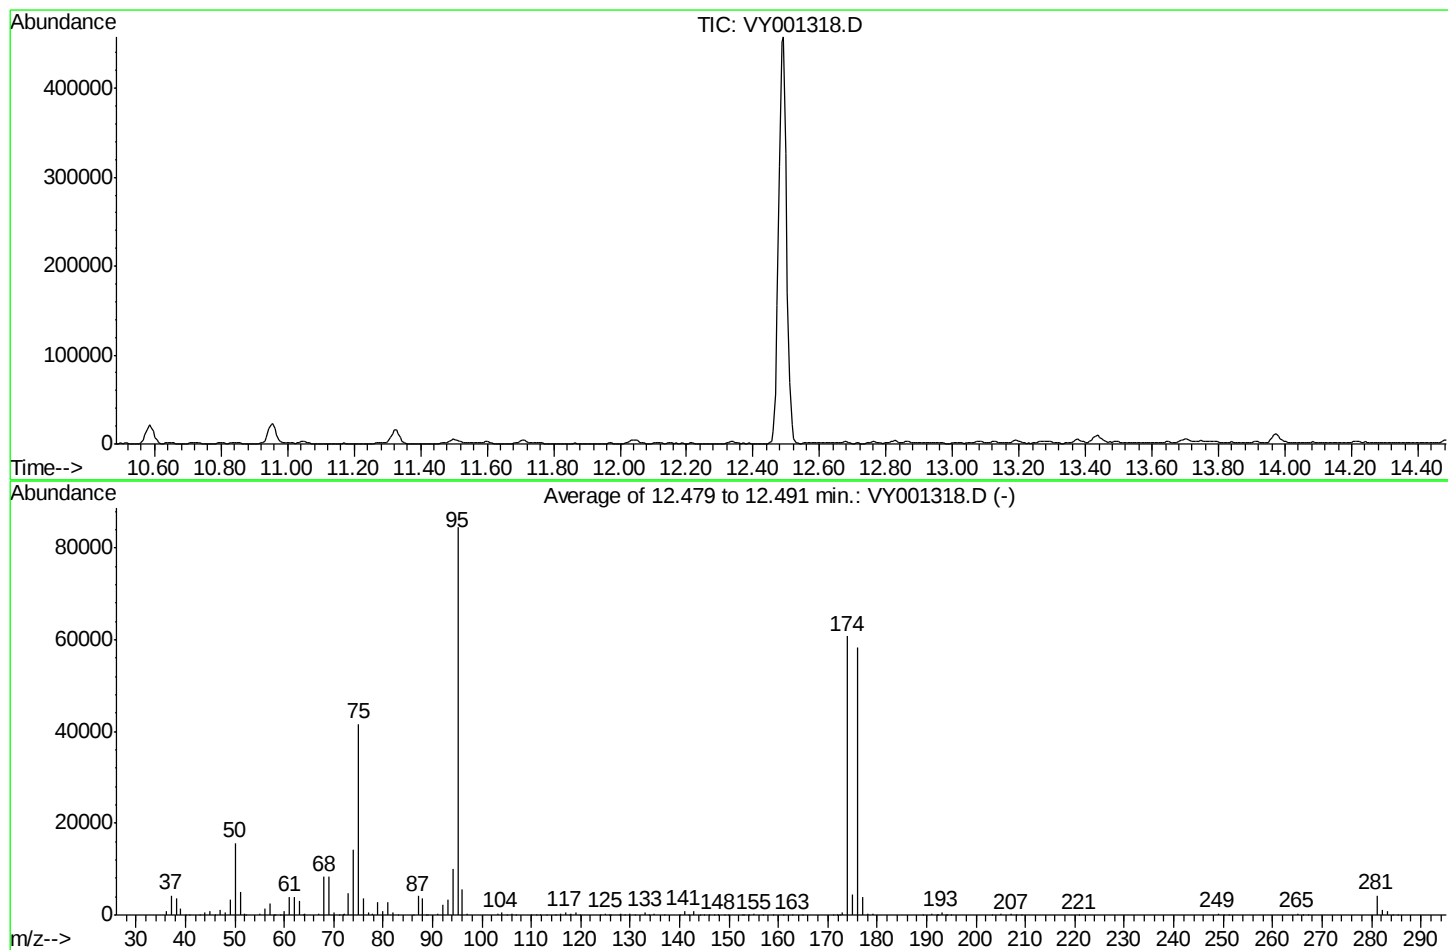

AutoFind: Scans 1762, 1763, 1764; Background Corrected with Scan 1755

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	15689	PASS
75	95	30	60	49.3	41725	PASS
95	95	100	100	100.0	84554	PASS
96	95	5	9	6.7	5677	PASS
173	174	0.00	2	0.8	488	PASS
174	95	50	100	71.9	60778	PASS
175	174	5	9	7.2	4368	PASS
176	174	95	101	96.1	58413	PASS
177	176	5	9	6.9	4030	PASS