


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv012220\
Data File : VY001327.D
Acq On : 22 Jan 2020 12:43
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y012120S.M
Title : SW846 8260
Last Update : Thu Jan 23 01:21:47 2020

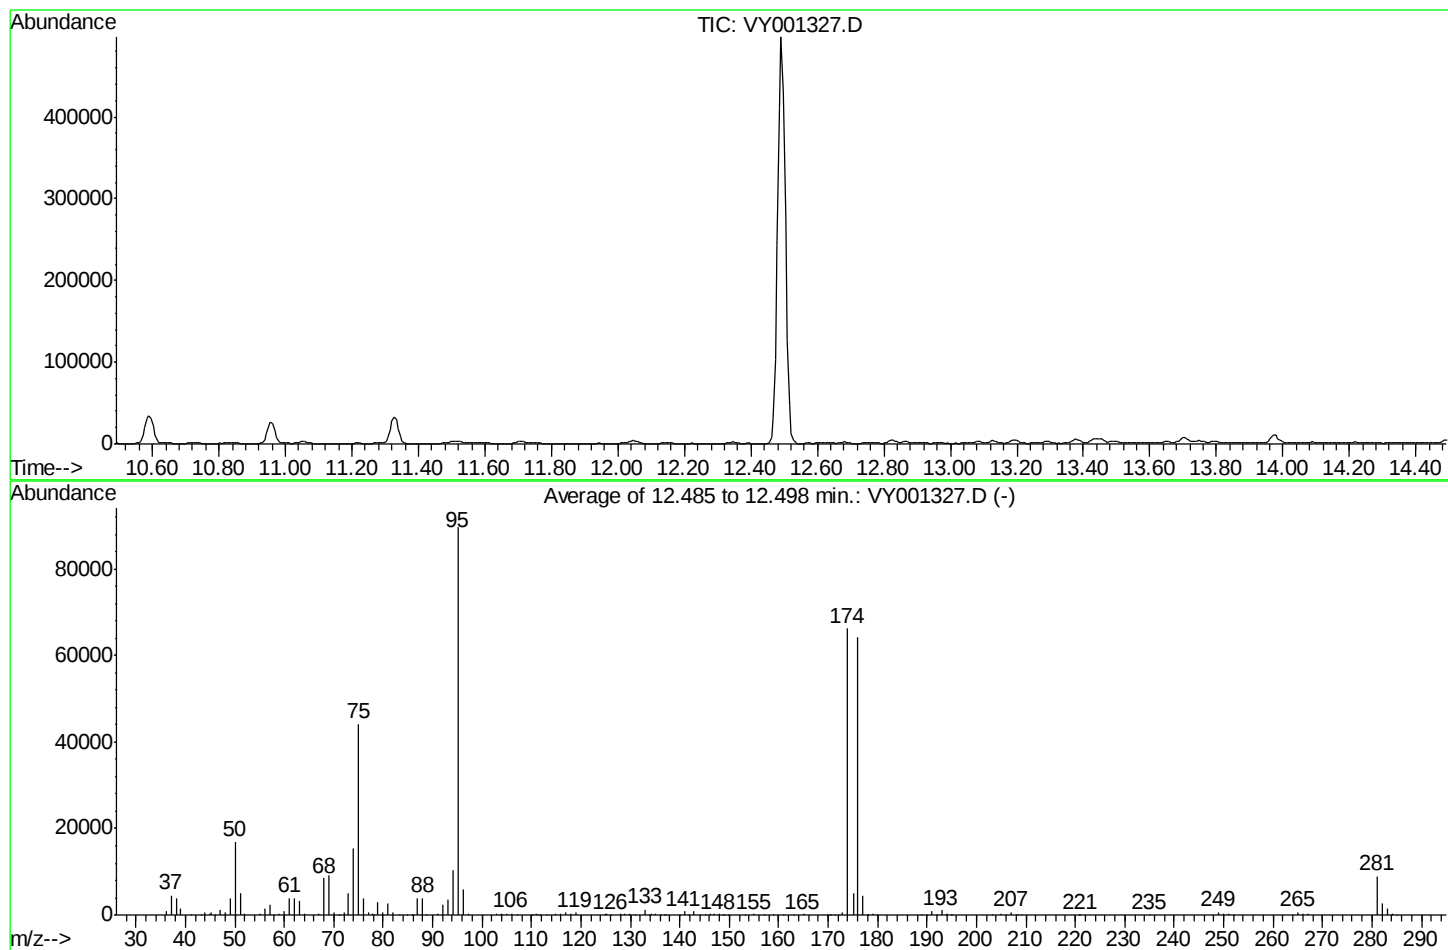

AutoFind: Scans 1763, 1764, 1765; Background Corrected with Scan 1755

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	16915	PASS
75	95	30	60	49.3	44256	PASS
95	95	100	100	100.0	89685	PASS
96	95	5	9	6.7	6028	PASS
173	174	0.00	2	0.9	592	PASS
174	95	50	100	73.9	66274	PASS
175	174	5	9	7.5	4969	PASS
176	174	95	101	96.8	64125	PASS
177	176	5	9	6.9	4447	PASS