
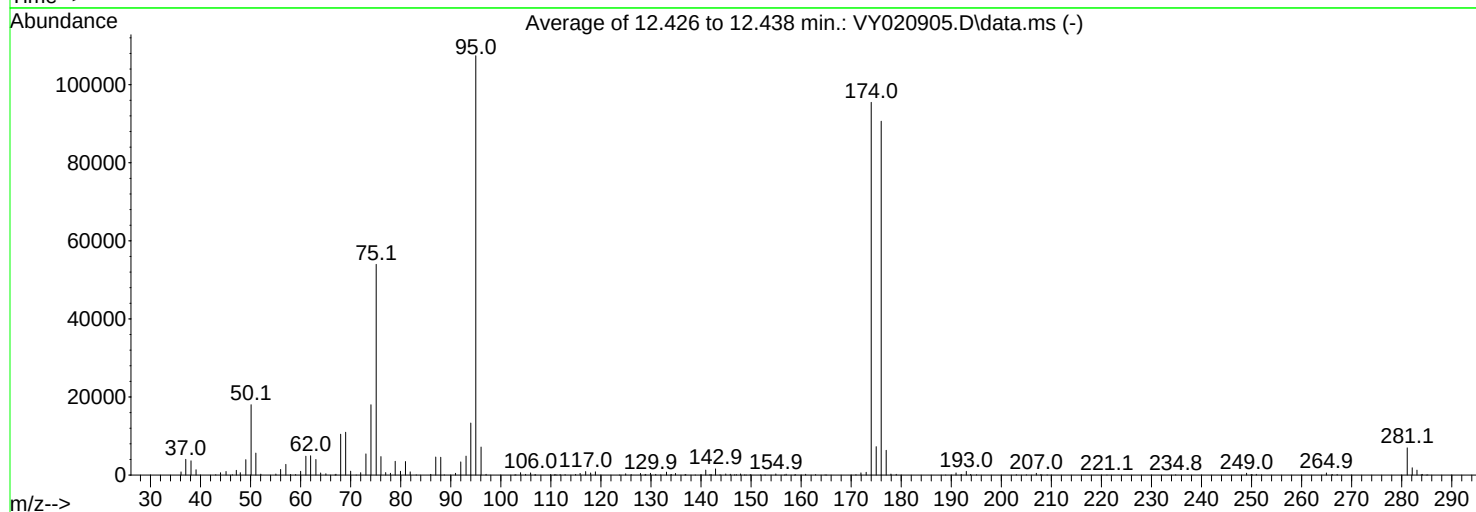


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY012325\
Data File : VY020905.D
Acq On : 23 Jan 2025 08:29
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y010625S.M
Title : SW846 8260
Last Update : Thu Jan 23 00:38:42 2025

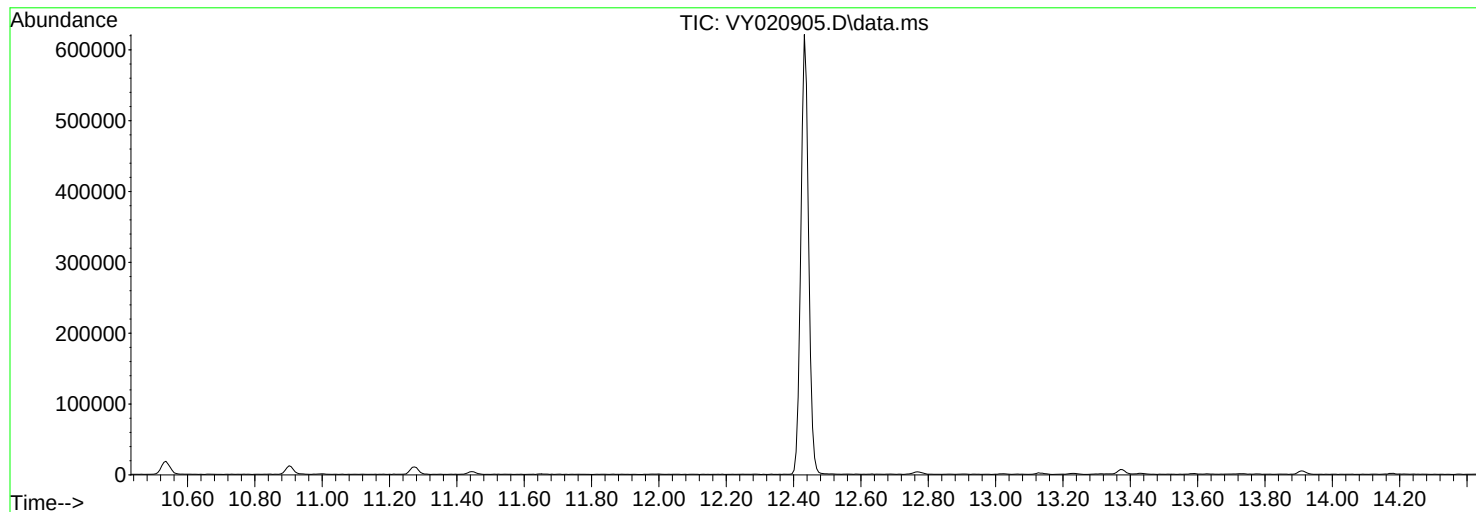

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	18024	PASS
75	95	30	60	50.2	53976	PASS
95	95	100	100	100.0	107416	PASS
96	95	5	9	6.7	7182	PASS
173	174	0.00	2	0.7	709	PASS
174	95	50	100	88.9	95477	PASS
175	174	5	9	7.6	7277	PASS
176	174	95	101	94.9	90640	PASS
177	176	5	9	7.0	6346	PASS