

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY012422\
 Data File : VY007277.D
 Acq On : 24 Jan 2022 18:32
 Operator : SY/MD
 Sample : N1245-04
 Misc : 4.84g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SB-2(2.5-3)

Quant Time: Jan 25 00:34:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y011322S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jan 14 05:48:29 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.795	168	86389	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	161286	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	155747	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	68991	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	56716	53.505	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	107.020%
35) Dibromofluoromethane	7.722	113	54090	49.597	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	99.200%
50) Toluene-d8	10.185	98	201238	50.499	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	101.000%
62) 4-Bromofluorobenzene	12.483	95	72595	51.213	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	102.420%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY012422\
Data File : VY007277.D
Acq On : 24 Jan 2022 18:32
Operator : SY/MD
Sample : N1245-04
Misc : 4.84g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SB-2(2.5-3)

Quant Time: Jan 25 00:34:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y011322S.M
Quant Title : SW846 8260
QLast Update : Fri Jan 14 05:48:29 2022
Response via : Initial Calibration




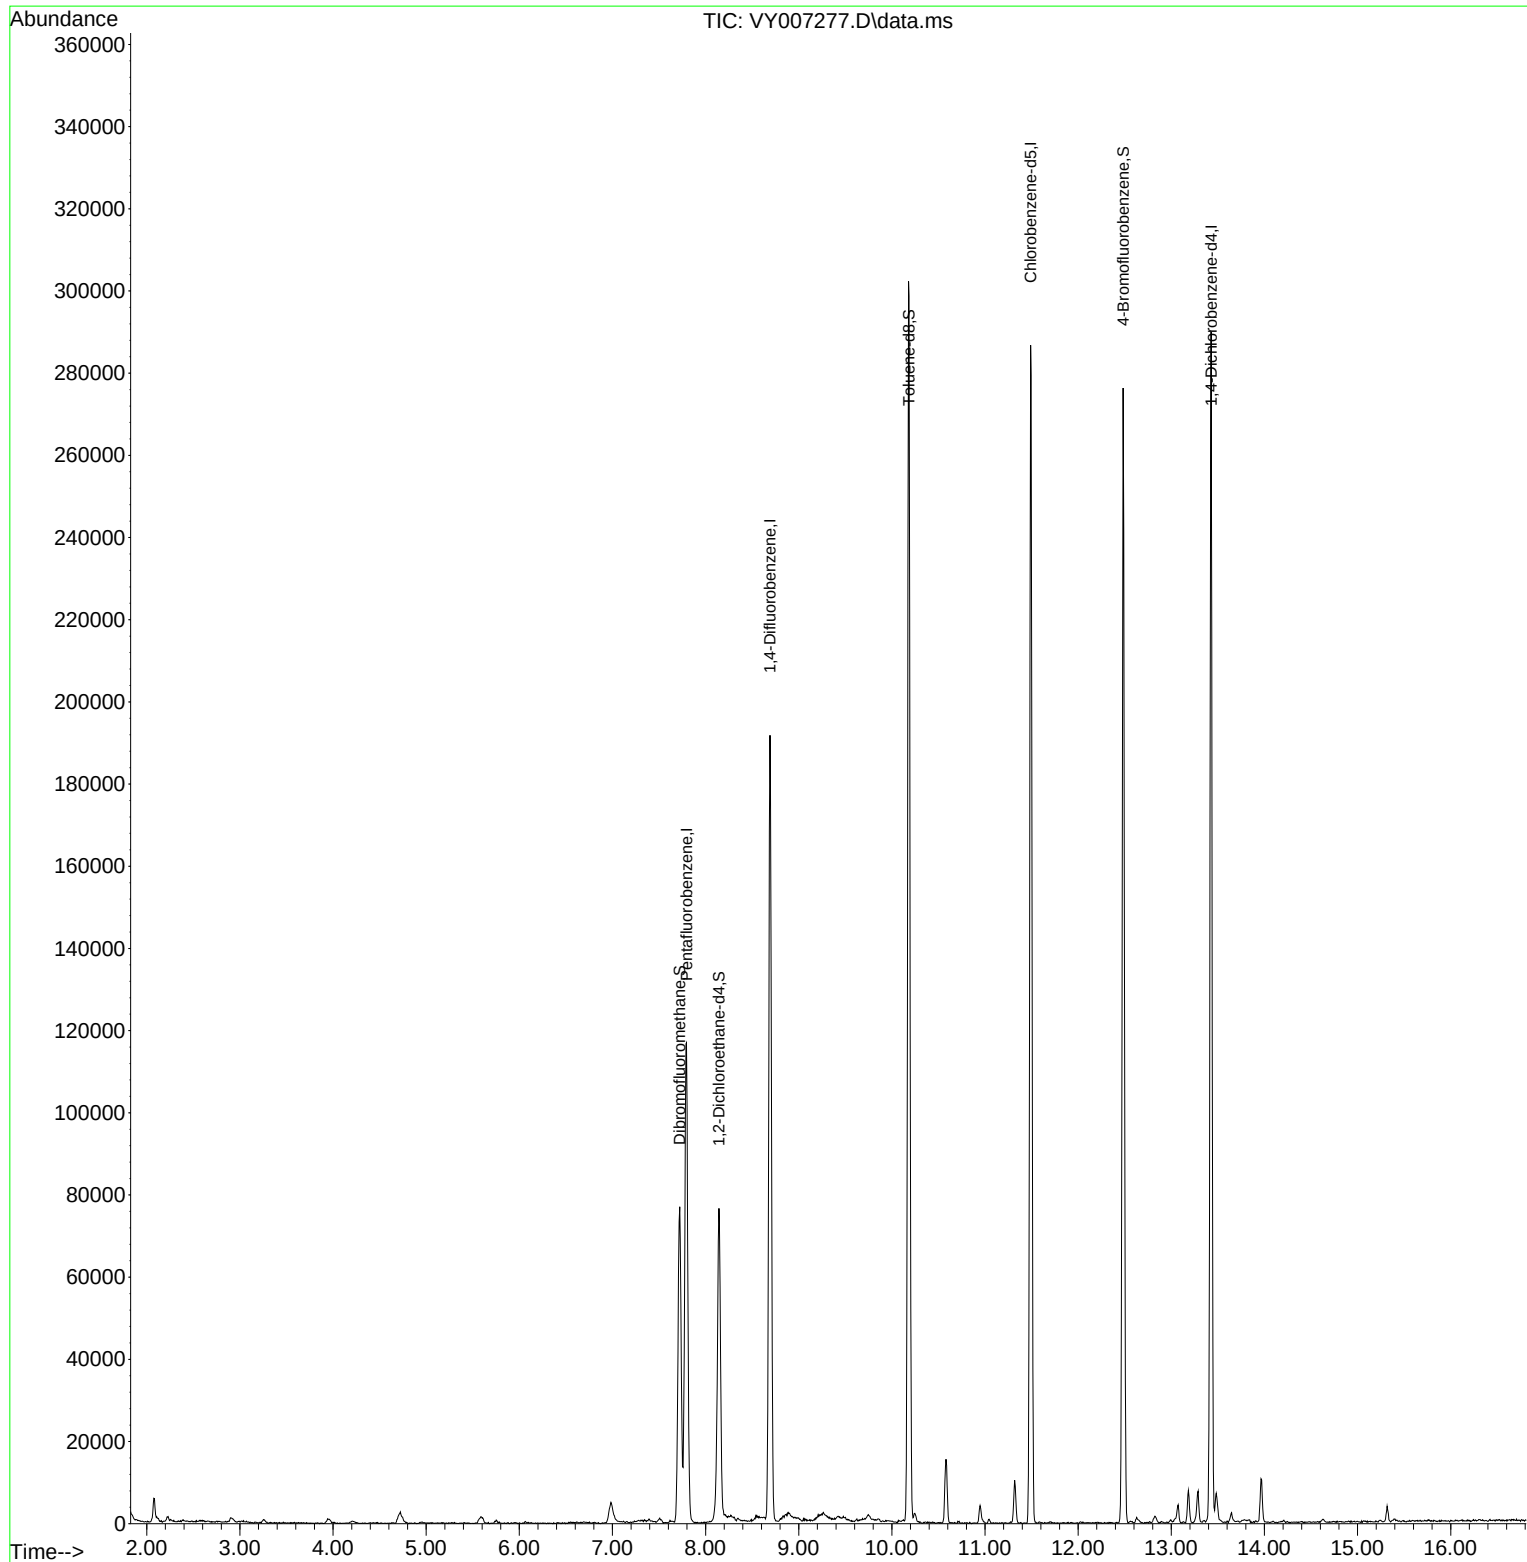


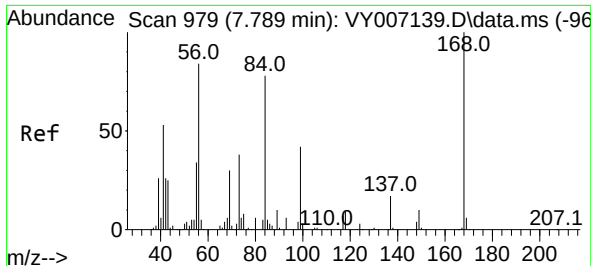

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.795 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY007277.D
Acq: 24 Jan 2022 18:32




Instrument :
MSVOA_Y
ClientSampleId :
SB-2(2.5-3)


Tgt Ion:168 Resp: 86389
Ion Ratio Lower Upper
168 100
99 60.5 49.1 73.7

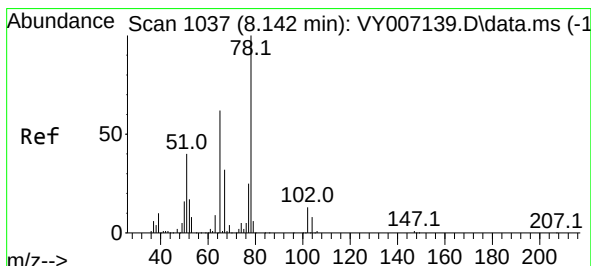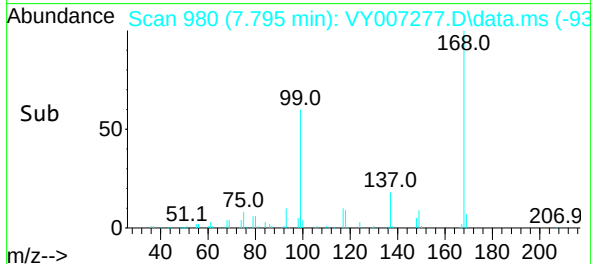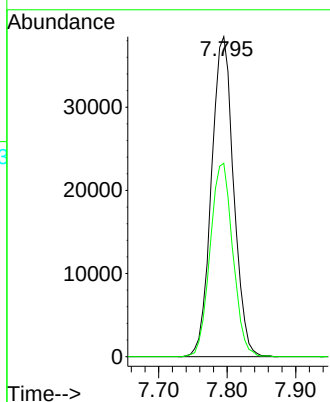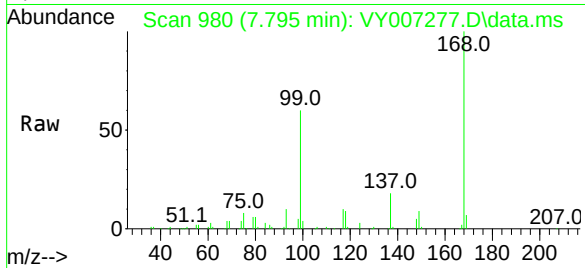

#33
1,2-Dichloroethane-d4
Concen: 53.505 ug/l
RT: 8.143 min Scan# 1037
Delta R.T. 0.000 min
Lab File: VY007277.D
Acq: 24 Jan 2022 18:32

Tgt Ion: 65 Resp: 56716
Ion Ratio Lower Upper
65 100
67 52.7 0.0 105.6


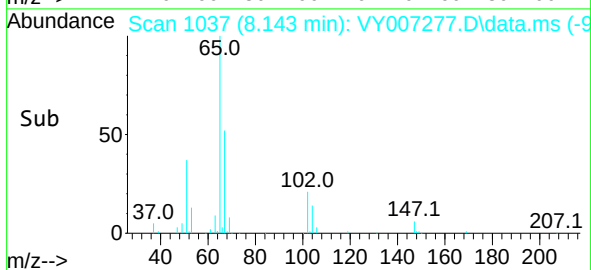
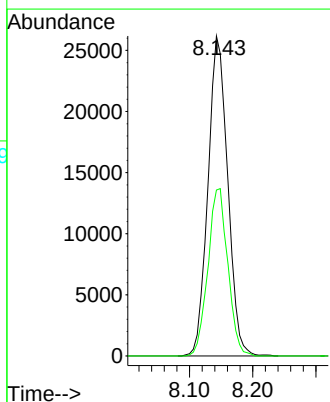
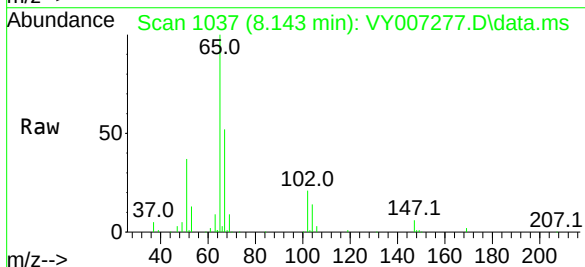


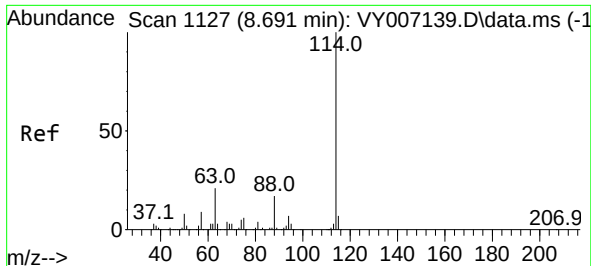

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.691 min Scan# 1127
Delta R.T. 0.000 min
Lab File: VY007277.D
Acq: 24 Jan 2022 18:32




Instrument :
MSVOA_Y
ClientSampleId :
SB-2(2.5-3)


Tgt Ion:114 Resp: 161286
Ion Ratio Lower Upper
114 100
63 21.0 0.0 39.2
88 16.7 0.0 31.0

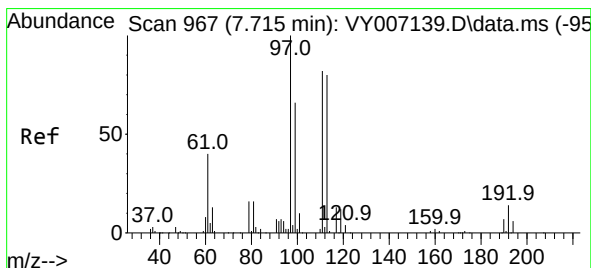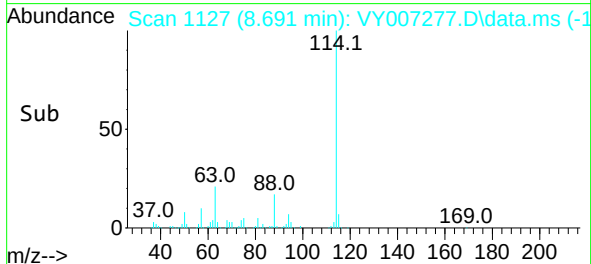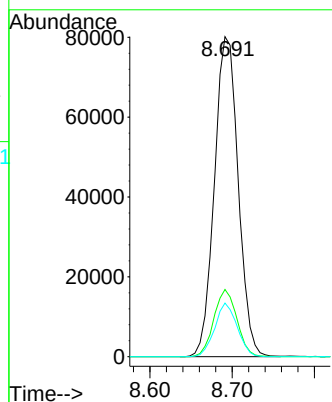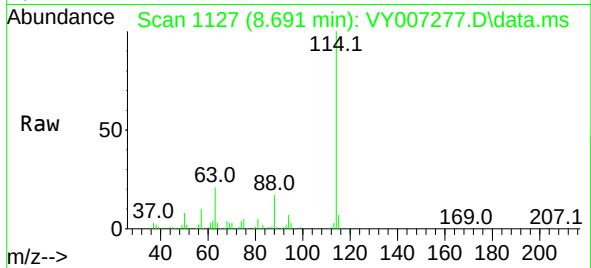

#35
Dibromofluoromethane
Concen: 49.597 ug/l
RT: 7.722 min Scan# 968
Delta R.T. 0.007 min
Lab File: VY007277.D
Acq: 24 Jan 2022 18:32

Tgt Ion:113 Resp: 54090
Ion Ratio Lower Upper
113 100
111 104.0 82.2 123.4
192 17.7 14.2 21.4


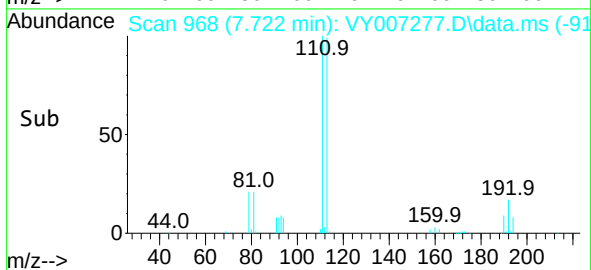
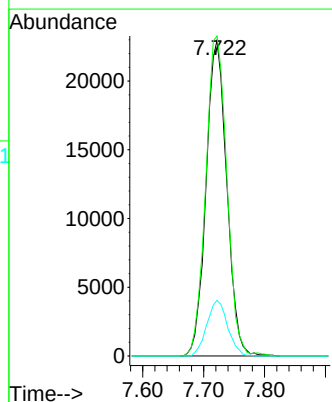
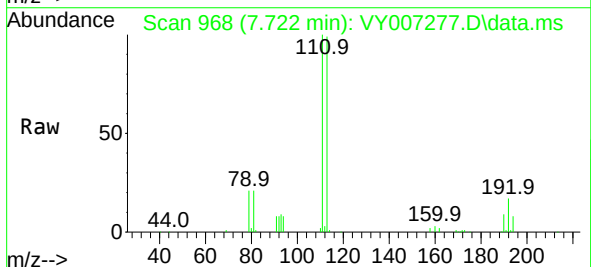


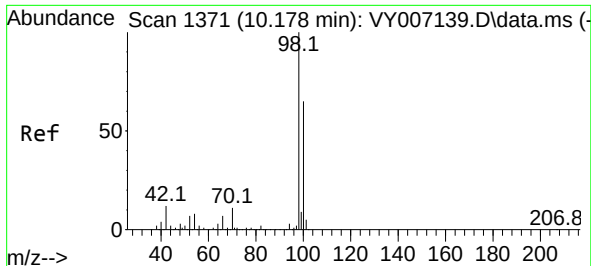

#50
Toluene-d8
Concen: 50.499 ug/l
RT: 10.185 min Scan# 11
Delta R.T. 0.007 min
Lab File: VY007277.D
Acq: 24 Jan 2022 18:32




Instrument :
MSVOA_Y
ClientSampleId :
SB-2(2.5-3)


Tgt Ion: 98 Resp: 201238
Ion Ratio Lower Upper
98 100
100 63.7 52.2 78.2

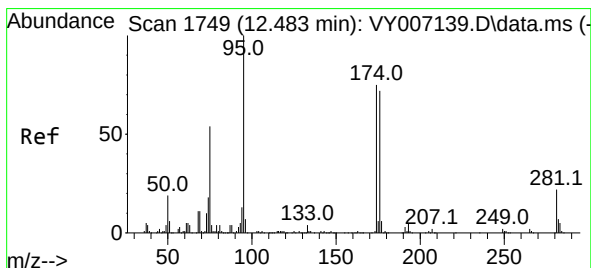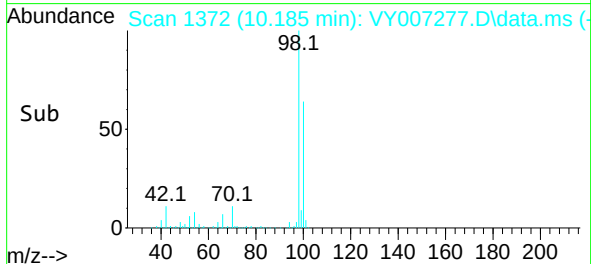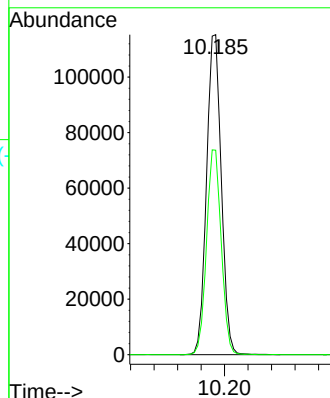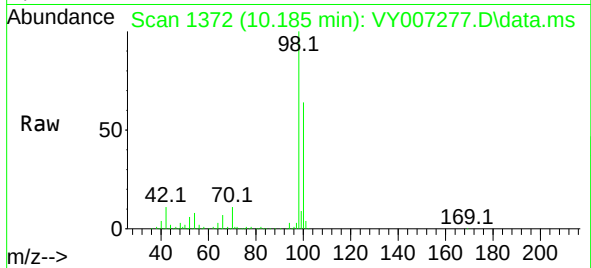

#62
4-Bromofluorobenzene
Concen: 51.213 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY007277.D
Acq: 24 Jan 2022 18:32

Tgt Ion: 95 Resp: 72595
Ion Ratio Lower Upper
95 100
174 76.1 0.0 148.4
176 74.6 0.0 146.6

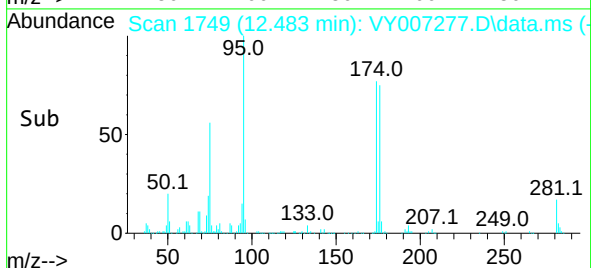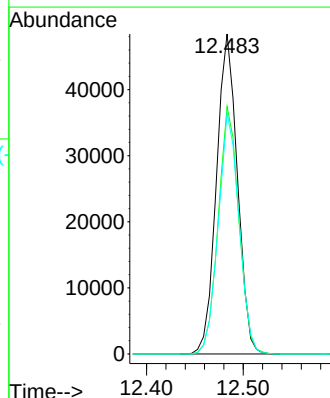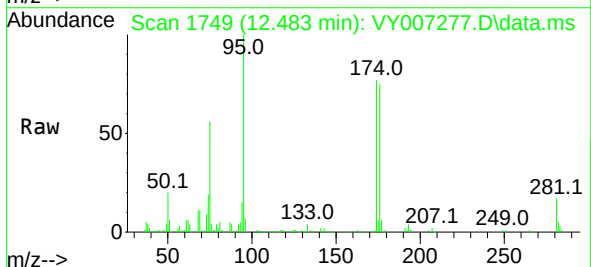

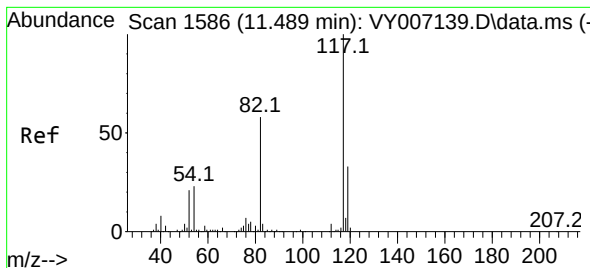

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.490 min Scan# 11

Delta R.T. 0.000 min

Lab File: VY007277.D

Acq: 24 Jan 2022 18:32

Instrument :

MSVOA_Y

ClientSampleId :

SB-2(2.5-3)





Tgt Ion:117 Resp: 155747

Ion Ratio Lower Upper

117 100

82 56.2 45.4 68.0

119 31.4 26.4 39.6

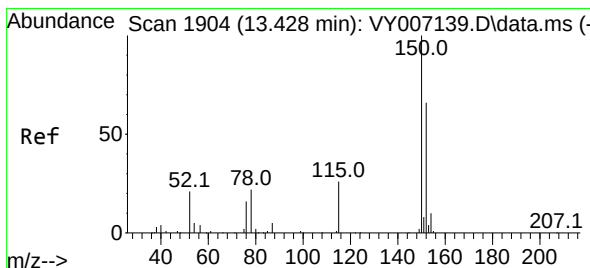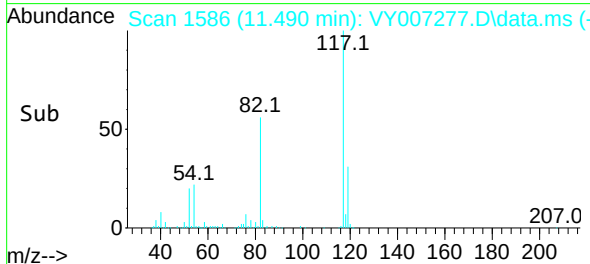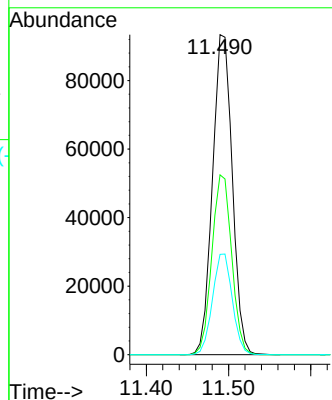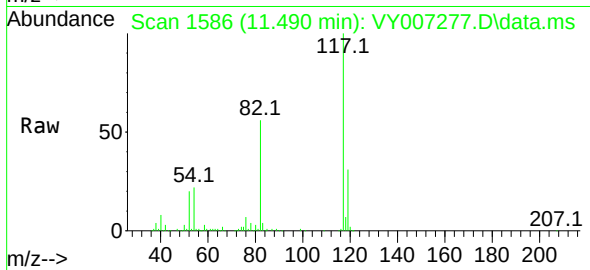

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.428 min Scan# 1904

Delta R.T. 0.000 min

Lab File: VY007277.D

Acq: 24 Jan 2022 18:32

Tgt Ion:152 Resp: 68991

Ion Ratio Lower Upper

152 100

115 61.9 31.4 94.0

150 156.1 0.0 348.4

