
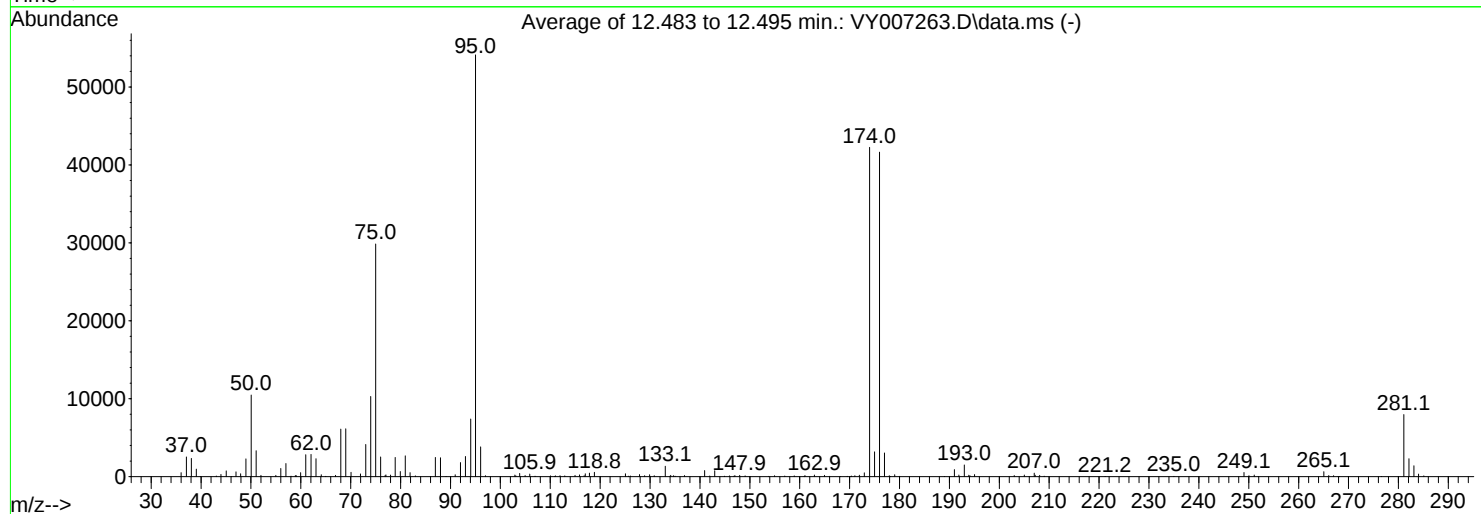


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY012422\
 Data File : VY007263.D
 Acq On : 24 Jan 2022 09:42
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y011322S.M
 Title : SW846 8260
 Last Update : Fri Jan 14 05:48:29 2022

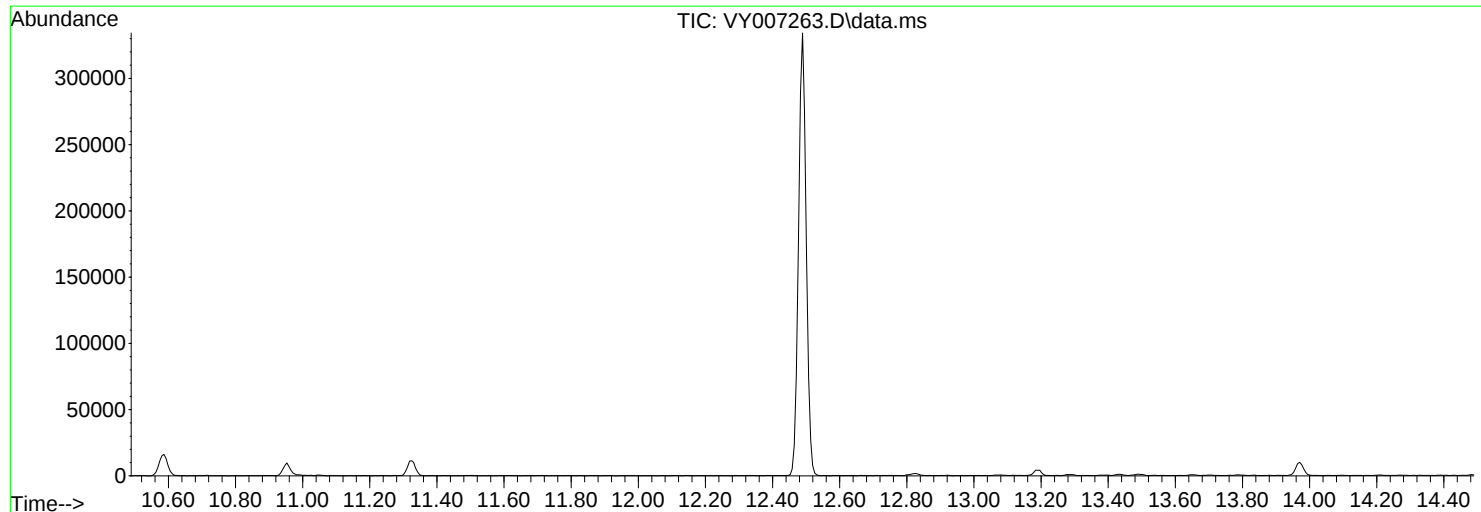

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1741

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	10473	PASS
75	95	30	60	55.1	29851	PASS
95	95	100	100	100.0	54128	PASS
96	95	5	9	7.0	3815	PASS
173	174	0.00	2	1.1	485	PASS
174	95	50	100	78.1	42253	PASS
175	174	5	9	7.5	3179	PASS
176	174	95	101	98.6	41645	PASS
177	176	5	9	7.3	3047	PASS