
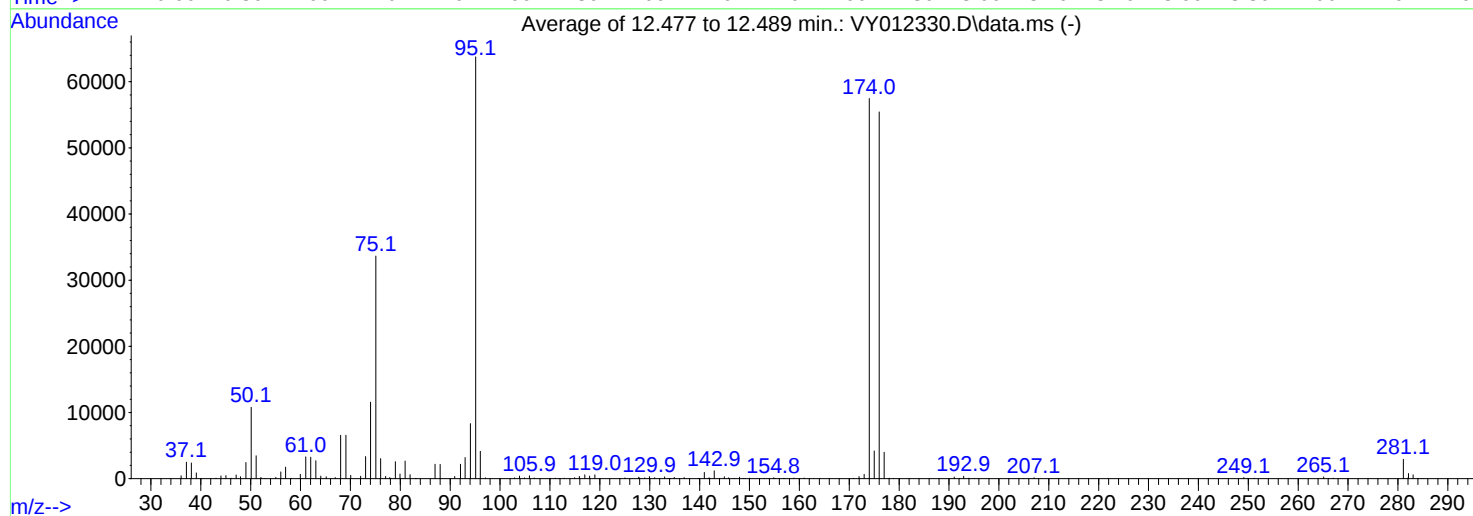


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY012423\
Data File : VY012330.D
Acq On : 24 Jan 2023 09:24
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y011623S.M
Title : SW846 8260
Last Update : Tue Jan 17 04:31:47 2023

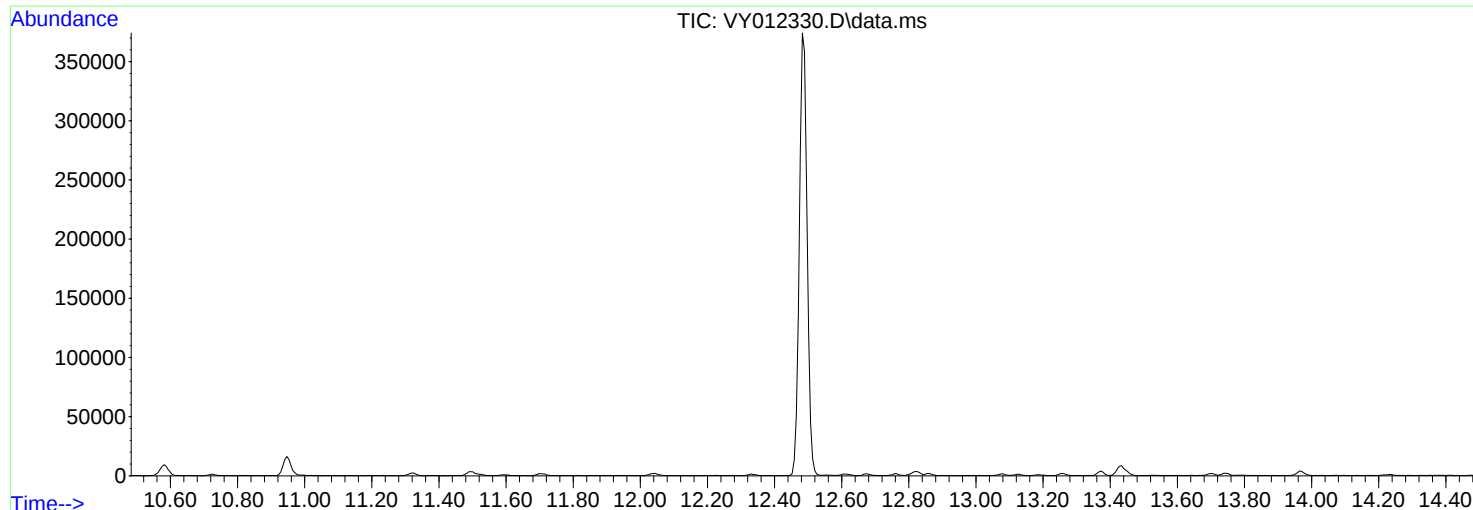

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	10797	PASS
75	95	30	60	52.8	33643	PASS
95	95	100	100	100.0	63763	PASS
96	95	5	9	6.5	4151	PASS
173	174	0.00	2	1.2	666	PASS
174	95	50	100	90.1	57469	PASS
175	174	5	9	7.3	4187	PASS
176	174	95	101	96.5	55437	PASS
177	176	5	9	7.2	3986	PASS