
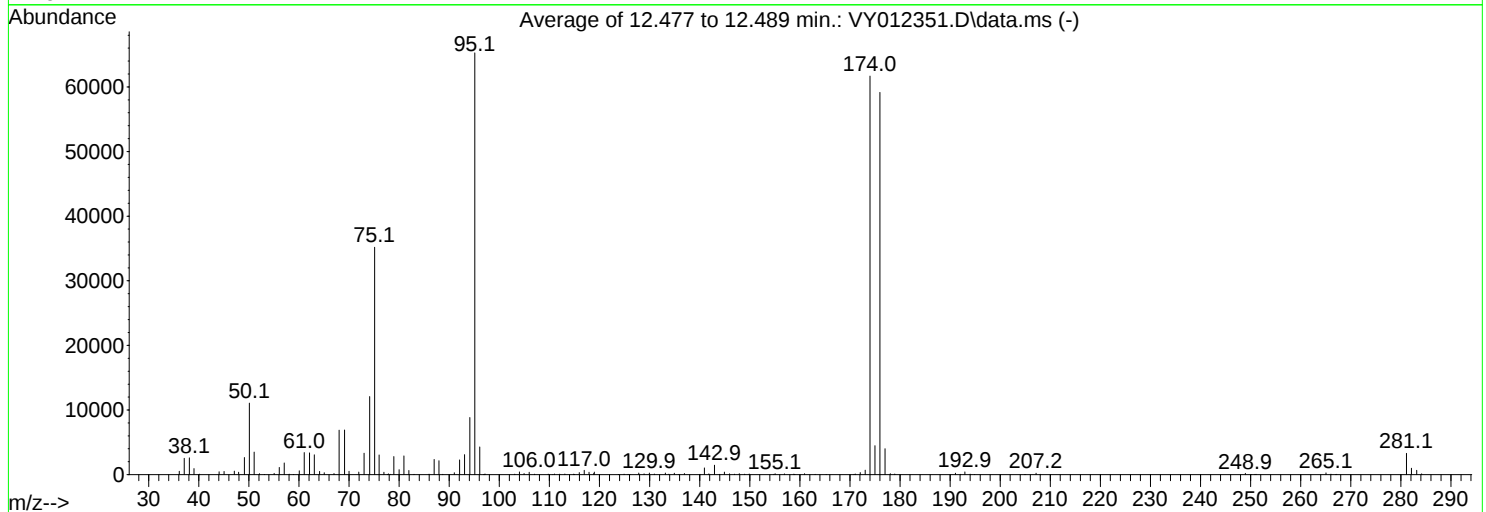


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY012523\
Data File : VY012351.D
Acq On : 25 Jan 2023 09:15
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y011623S.M
Title : SW846 8260
Last Update : Tue Jan 17 04:31:47 2023

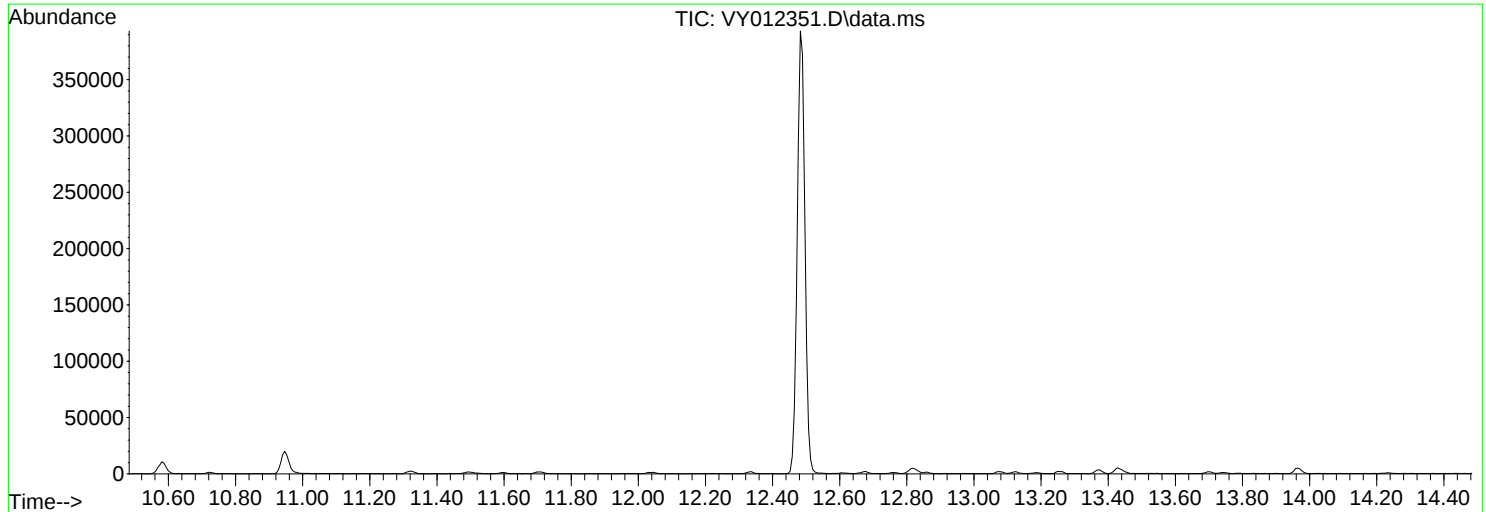

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	11070	PASS
75	95	30	60	53.9	35176	PASS
95	95	100	100	100.0	65275	PASS
96	95	5	9	6.6	4287	PASS
173	174	0.00	2	1.1	701	PASS
174	95	50	100	94.5	61672	PASS
175	174	5	9	7.3	4481	PASS
176	174	95	101	95.9	59149	PASS
177	176	5	9	6.8	4003	PASS